


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX120419\
 Data File : VX013743.D
 Acq On : 04 Dec 2019 09:19
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112619W.M
 Title : SW846 8260
 Last Update : Tue Nov 26 15:53:00 2019

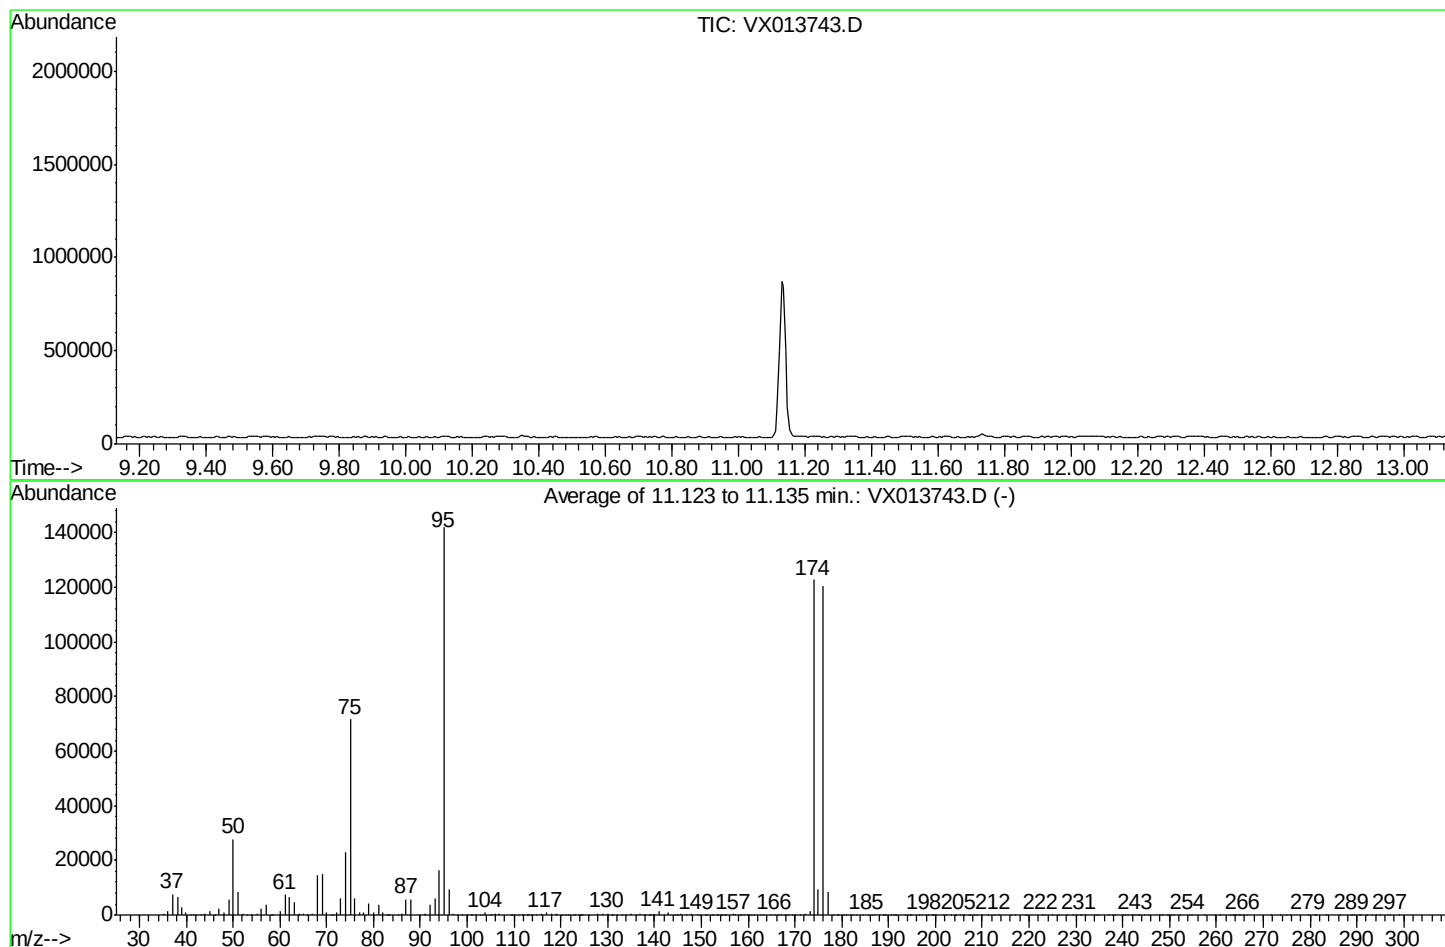

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1670

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	27857	PASS
75	95	30	60	50.5	71672	PASS
95	95	100	100	100.0	142029	PASS
96	95	5	9	6.7	9457	PASS
173	174	0.00	2	1.1	1408	PASS
174	95	50	100	86.5	122858	PASS
175	174	5	9	7.8	9525	PASS
176	174	95	101	98.2	120669	PASS
177	176	5	9	6.9	8325	PASS