


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX120420\
 Data File : VX019708.D
 Acq On : 04 Dec 2020 09:14
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
 Title : SW846 8260
 Last Update : Fri Dec 04 15:32:53 2020

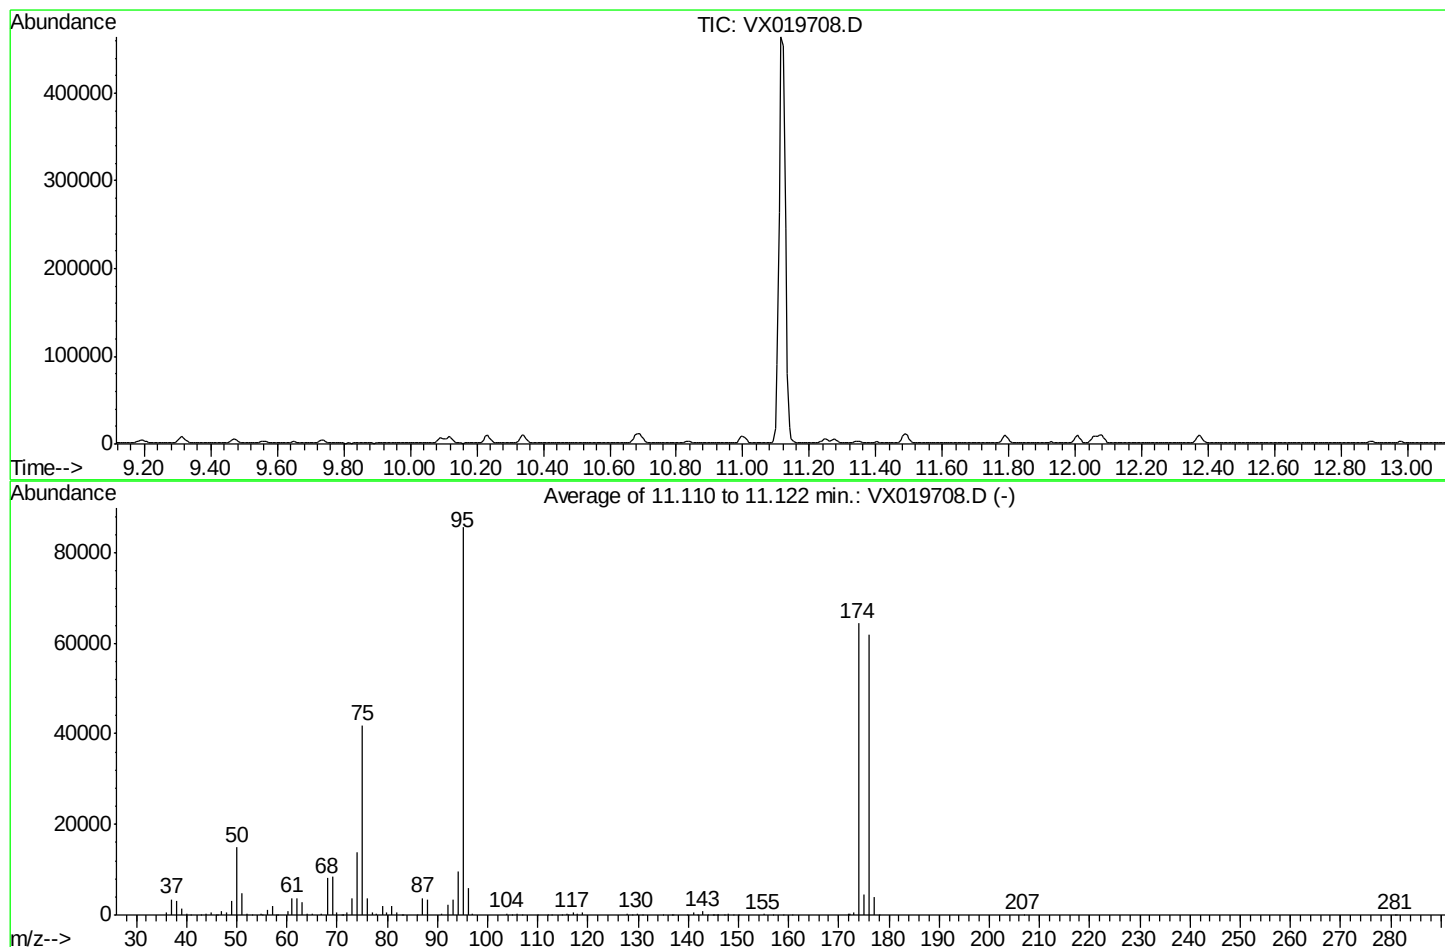

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	14935	PASS
75	95	30	60	48.7	41701	PASS
95	95	100	100	100.0	85586	PASS
96	95	5	9	7.0	5990	PASS
173	174	0.00	2	0.8	501	PASS
174	95	50	100	75.2	64381	PASS
175	174	5	9	7.1	4571	PASS
176	174	95	101	96.2	61954	PASS
177	176	5	9	6.5	4027	PASS