

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
 Data File : VX025521.D
 Acq On : 04 Dec 2021 14:57
 Operator : JC/MD
 Sample : M4923-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB01-20211201

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M

Title : SW846 8260

Signal : TIC: VX025521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	22	27	32	rBV	10273	14199	2.87%	0.545%
2	1.563	69	78	81	rBV5	2705	5295	1.07%	0.203%
3	2.538	230	238	246	rBV	3445	6432	1.30%	0.247%
4	5.391	694	706	719	rBV	58916	171131	34.59%	6.569%
5	5.556	721	733	746	rVV2	97510	274167	55.41%	10.524%
6	5.958	789	799	811	rBV	60596	164065	33.16%	6.298%
7	6.763	921	931	945	rBV	154417	363211	73.41%	13.942%
8	8.653	1234	1241	1253	rBV	318943	494800	100.00%	18.993%
9	10.055	1465	1471	1485	rBV	317589	426805	86.26%	16.383%
10	11.085	1634	1640	1650	rVB	241224	315083	63.68%	12.095%
11	12.024	1789	1794	1804	rBV	298805	369976	74.77%	14.202%




Sum of corrected areas: 2605164

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
Data File : VX025521.D
Acq On : 04 Dec 2021 14:57
Operator : JC/MD
Sample : M4923-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB01-20211201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

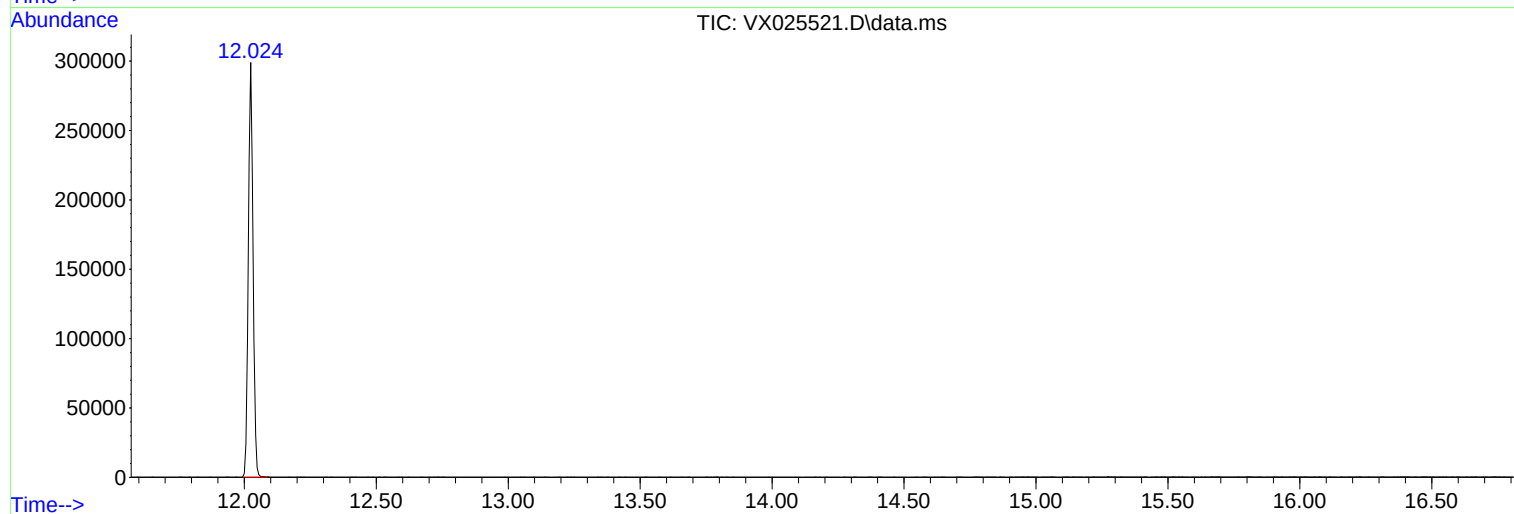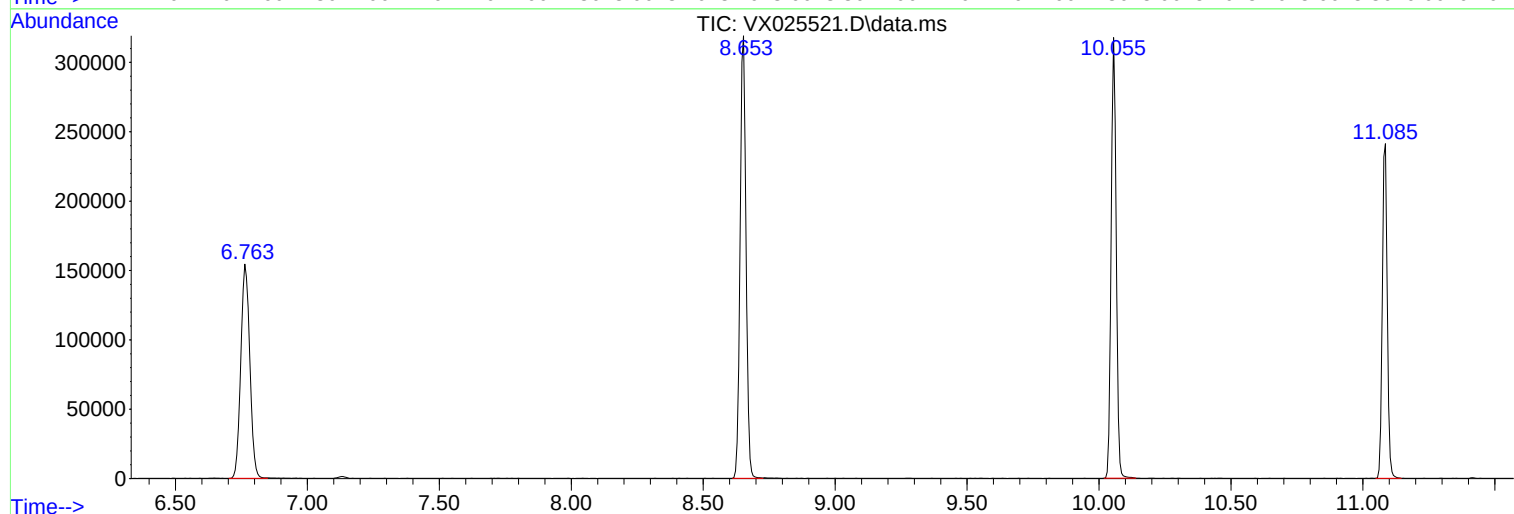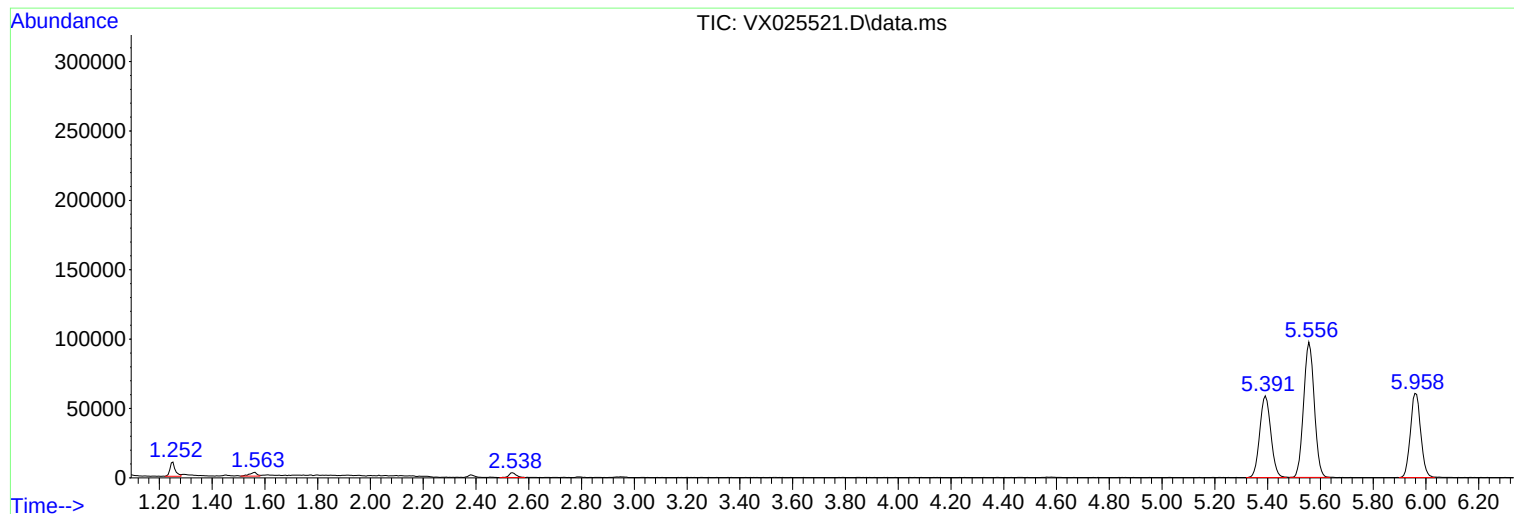

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
Data File : VX025521.D
Acq On : 04 Dec 2021 14:57
Operator : JC/MD
Sample : M4923-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB01-20211201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
Data File : VX025521.D
Acq On : 04 Dec 2021 14:57
Operator : JC/MD
Sample : M4923-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB01-20211201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------