

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
 Data File : VX025522.D
 Acq On : 04 Dec 2021 15:20
 Operator : JC/MD
 Sample : M4923-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB02-20211202

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
 Title : SW846 8260

Signal : TIC: VX025522.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	22	27	32	rBV	9410	12336	2.50%	0.467%
2	2.538	231	238	252	rBV	16950	29586	5.99%	1.120%
3	2.953	297	306	312	rBV2	2882	6118	1.24%	0.232%
4	5.391	695	706	722	rBV	59144	170655	34.53%	6.463%
5	5.556	722	733	747	rVB	97283	273486	55.34%	10.357%
6	5.958	789	799	815	rBV	61497	165623	33.52%	6.272%
7	6.763	921	931	949	rBV	150787	364914	73.84%	13.820%
8	8.653	1234	1241	1254	rBV	312567	494167	100.00%	18.715%
9	10.055	1465	1471	1488	rBV	316486	426264	86.26%	16.143%
10	11.085	1634	1640	1652	rVB	243191	318960	64.54%	12.080%
11	12.024	1789	1794	1808	rBV	305094	378361	76.57%	14.329%




Sum of corrected areas: 2640470

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
Data File : VX025522.D
Acq On : 04 Dec 2021 15:20
Operator : JC/MD
Sample : M4923-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB02-20211202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

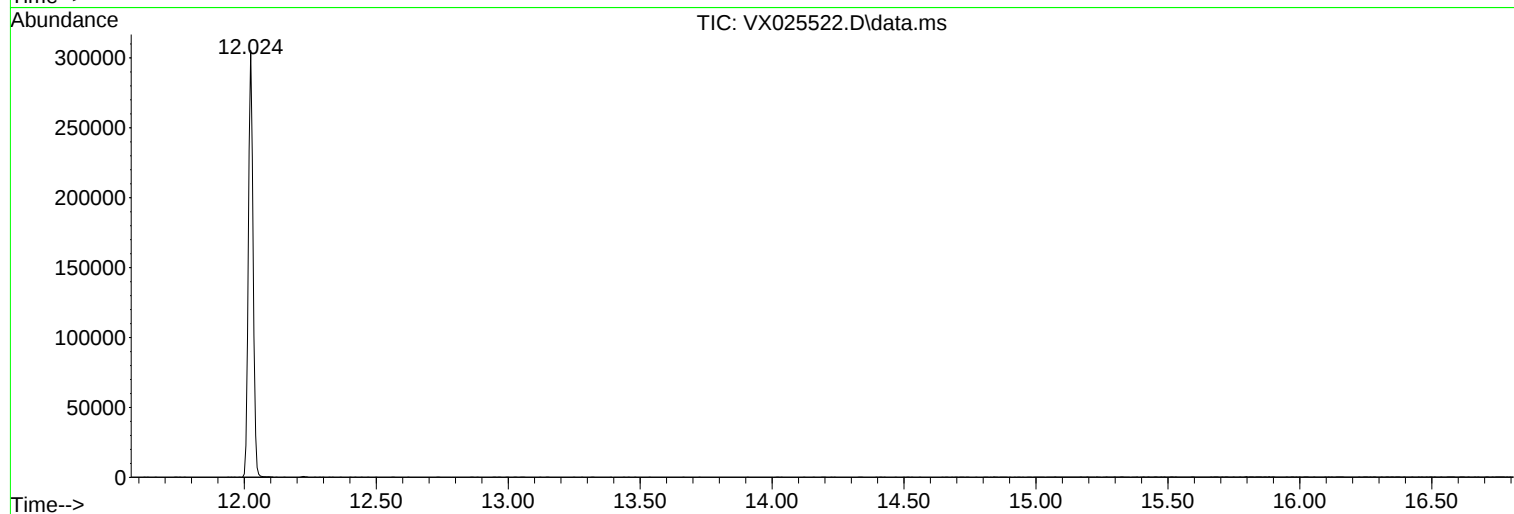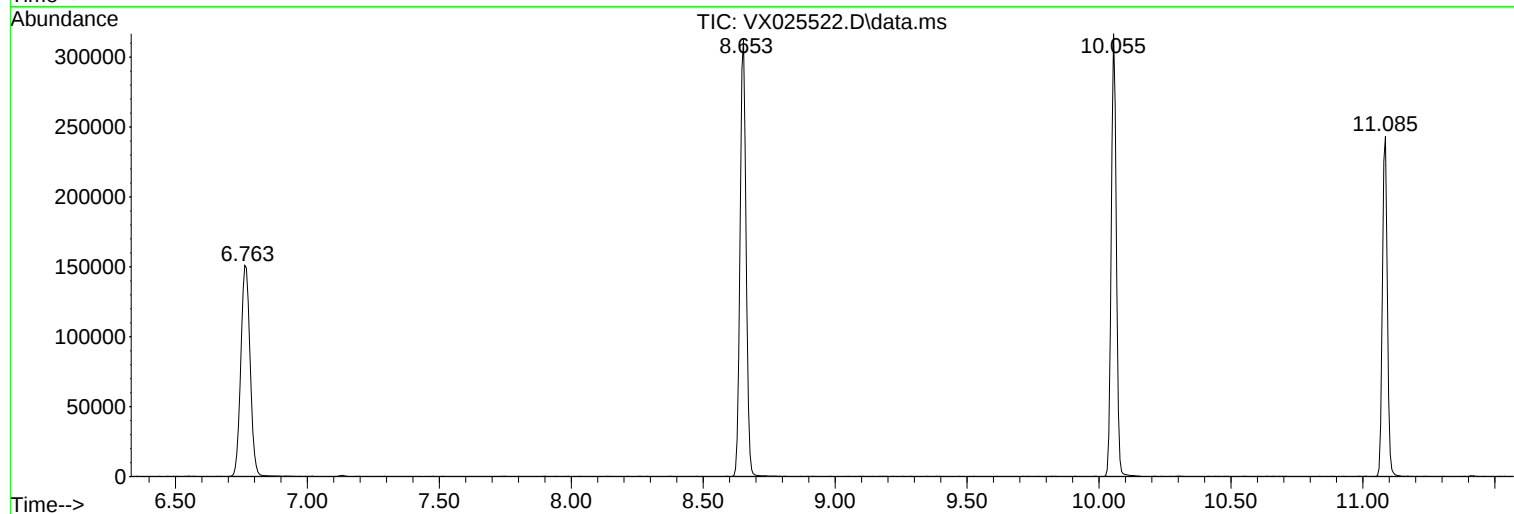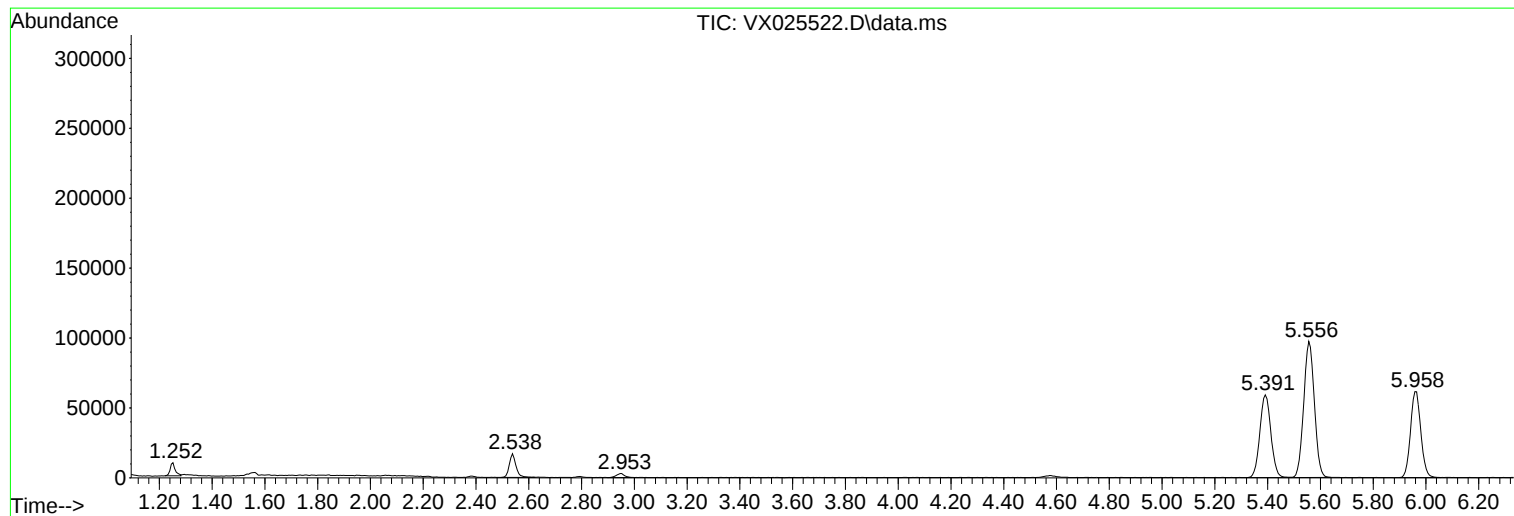

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
Data File : VX025522.D
Acq On : 04 Dec 2021 15:20
Operator : JC/MD
Sample : M4923-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB02-20211202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
Data File : VX025522.D
Acq On : 04 Dec 2021 15:20
Operator : JC/MD
Sample : M4923-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB02-20211202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc