

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
 Data File : VX025527.D
 Acq On : 04 Dec 2021 17:18
 Operator : JC/MD
 Sample : M4923-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TT180D1-20211201

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
 Title : SW846 8260

Signal : TIC: VX025527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	38	rBV	6729	13934	2.08%	0.416%
2	2.331	198	204	209	rBV4	5032	9551	1.42%	0.285%
3	5.391	695	706	719	rBV2	59968	171074	25.52%	5.104%
4	5.556	722	733	748	rVB2	97186	274177	40.90%	8.181%
5	5.958	789	799	816	rBV	62423	165820	24.73%	4.948%
6	6.763	922	931	944	rBV	156210	368950	55.03%	11.009%
7	7.129	982	991	1006	rBV	311759	670432	100.00%	20.004%
8	8.653	1234	1241	1253	rBV	318402	498722	74.39%	14.881%
9	10.055	1465	1471	1488	rBV	327180	437800	65.30%	13.063%
10	11.085	1634	1640	1650	rBV	254372	330932	49.36%	9.874%
11	12.024	1789	1794	1803	rBV	332869	410102	61.17%	12.236%




Sum of corrected areas: 3351494

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
Data File : VX025527.D
Acq On : 04 Dec 2021 17:18
Operator : JC/MD
Sample : M4923-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT180D1-20211201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

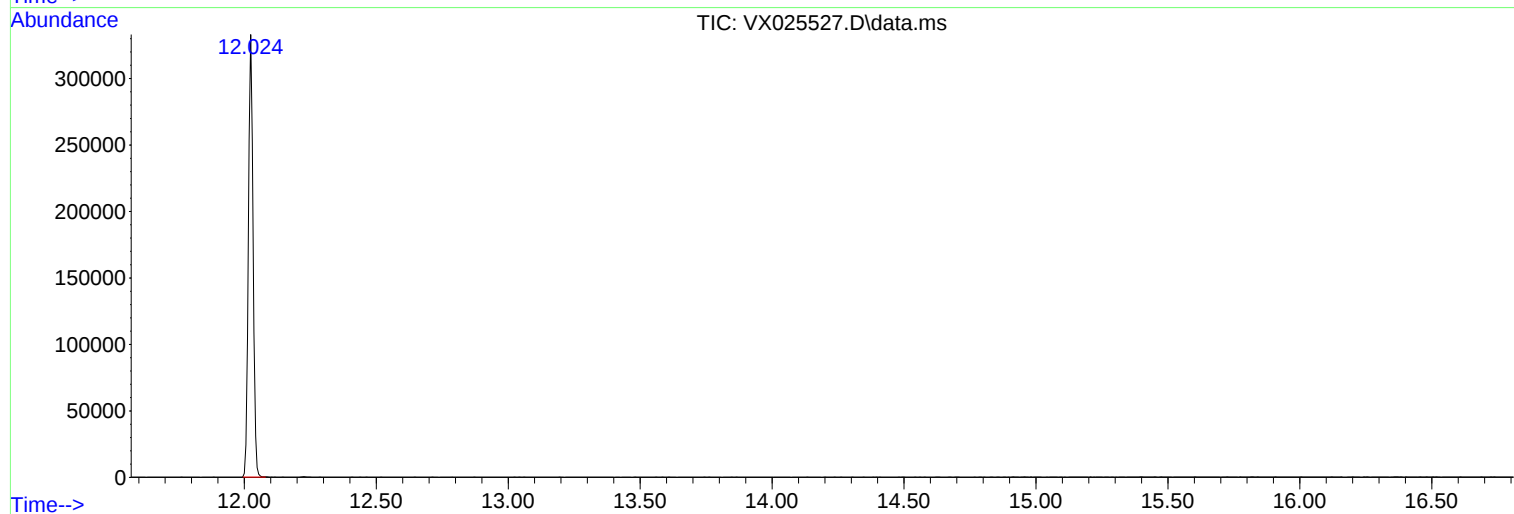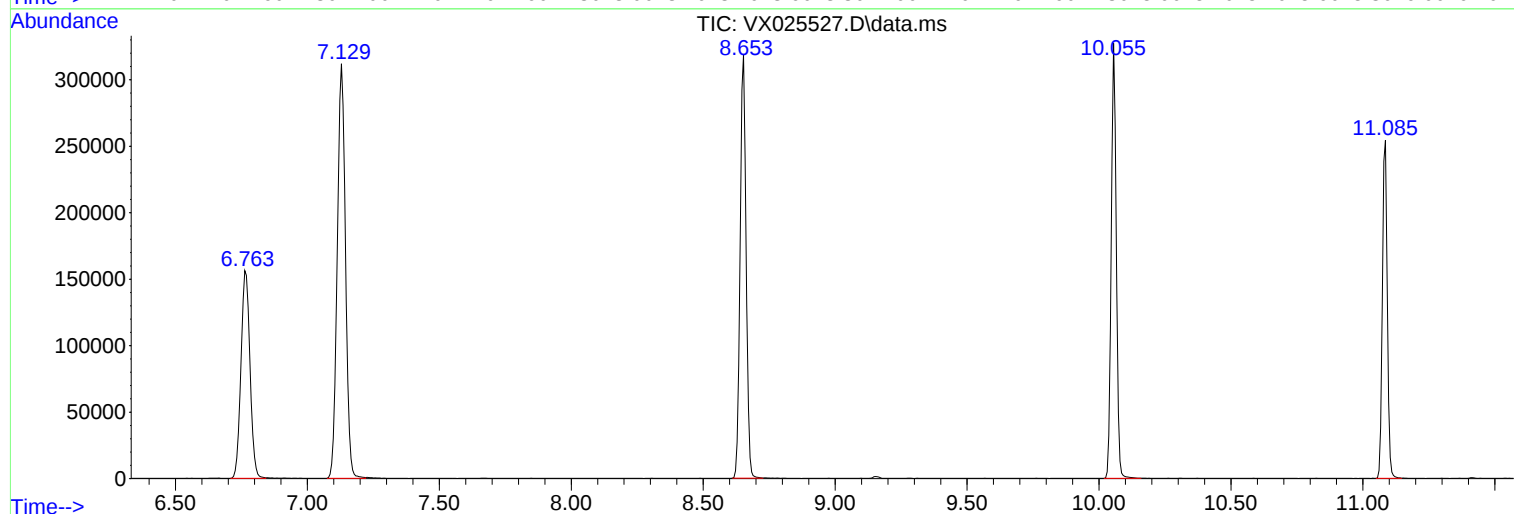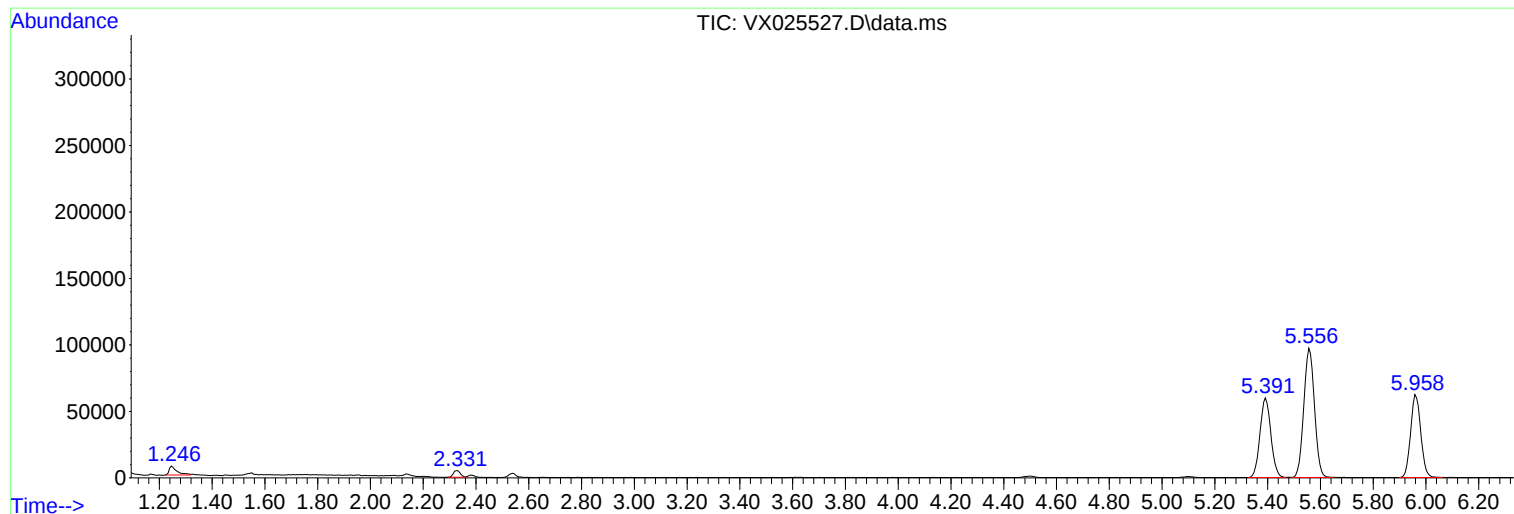

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
Data File : VX025527.D
Acq On : 04 Dec 2021 17:18
Operator : JC/MD
Sample : M4923-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT180D1-20211201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
Data File : VX025527.D
Acq On : 04 Dec 2021 17:18
Operator : JC/MD
Sample : M4923-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT180D1-20211201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------