

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
 Data File : VX025530.D
 Acq On : 04 Dec 2021 18:28
 Operator : JC/MD
 Sample : M4923-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BPOW1-8-20211201

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M

Title : SW846 8260

Signal : TIC: VX025530.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	20	26	36	rBV2	5347	11149	2.27%	0.421%
2	2.532	232	237	248	rVB	4005	7157	1.46%	0.270%
3	5.391	694	706	722	rBV2	58450	168416	34.31%	6.362%
4	5.556	722	733	750	rVB	97465	272084	55.43%	10.278%
5	5.958	789	799	814	rBV	62154	164355	33.48%	6.209%
6	6.763	922	931	949	rBV	148452	358159	72.97%	13.530%
7	7.129	984	991	999	rBV2	3901	8105	1.65%	0.306%
8	8.653	1234	1241	1249	rBV	311139	490851	100.00%	18.542%
9	10.055	1465	1471	1486	rBV	324126	431838	87.98%	16.313%
10	11.085	1634	1640	1649	rBV	252919	328645	66.95%	12.415%
11	12.024	1789	1794	1803	rBV	327227	406410	82.80%	15.353%




Sum of corrected areas: 2647169

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
Data File : VX025530.D
Acq On : 04 Dec 2021 18:28
Operator : JC/MD
Sample : M4923-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPOW1-8-20211201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

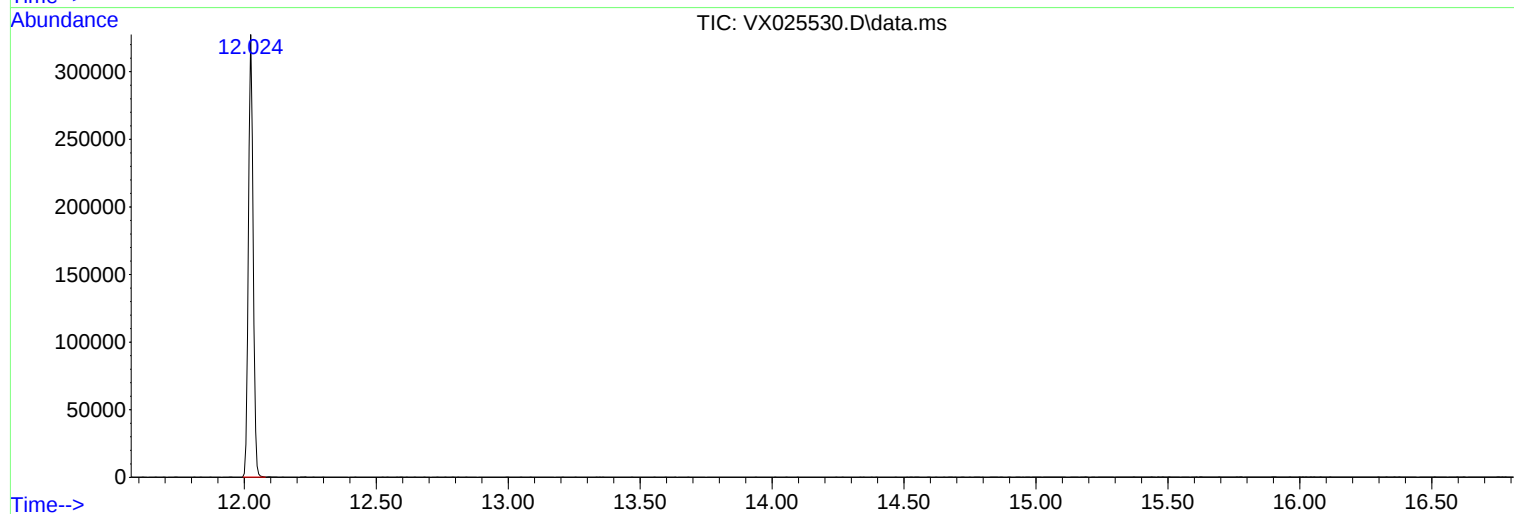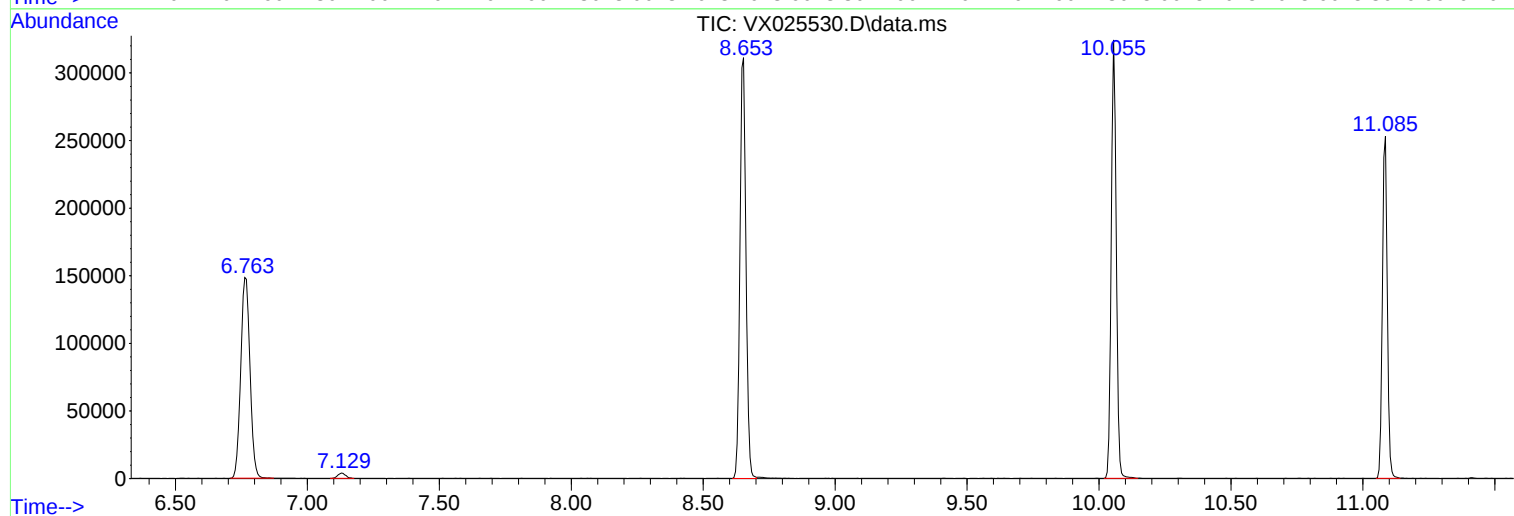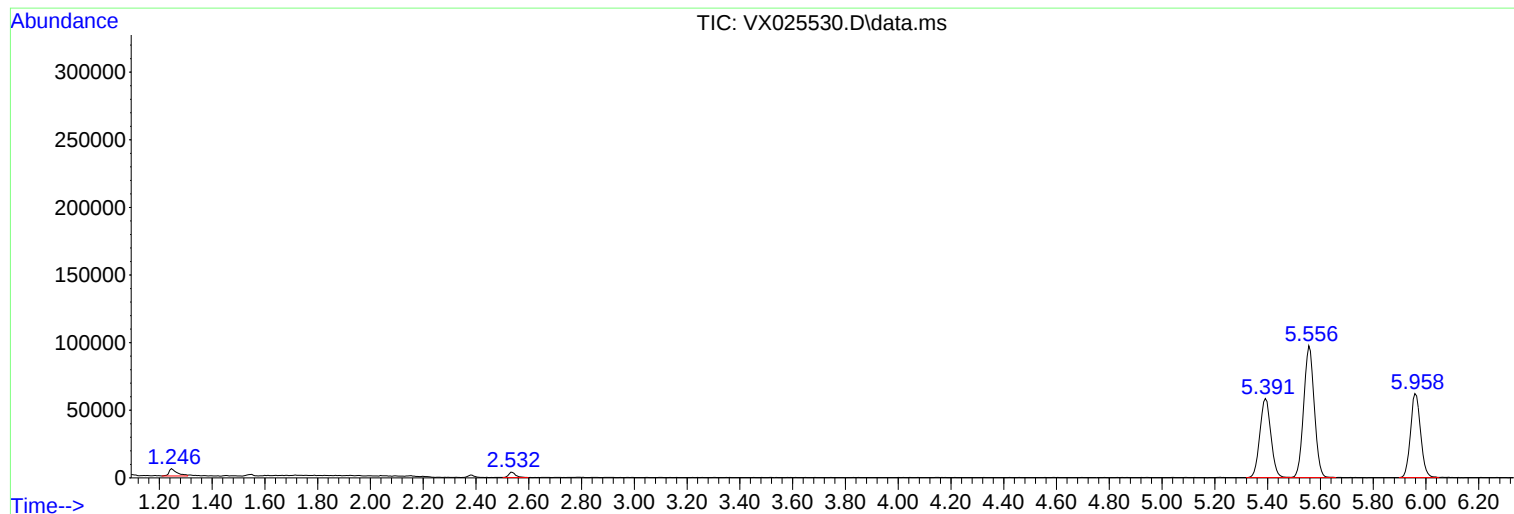

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
Data File : VX025530.D
Acq On : 04 Dec 2021 18:28
Operator : JC/MD
Sample : M4923-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPOW1-8-20211201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
Data File : VX025530.D
Acq On : 04 Dec 2021 18:28
Operator : JC/MD
Sample : M4923-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPOW1-8-20211201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc