

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
 Data File : VX025531.D
 Acq On : 04 Dec 2021 18:51
 Operator : JC/MD
 Sample : M4923-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BPOW1-7-20211201

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
 Title : SW846 8260

Signal : TIC: VX025531.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.245	22	26	32	rBV	5453	9931	2.06%	0.381%
2	2.532	232	237	246	rBV	4375	7700	1.60%	0.295%
3	5.391	694	706	721	rBV	56904	164588	34.12%	6.312%
4	5.556	722	733	751	rVB	94741	266603	55.27%	10.224%
5	5.958	789	799	812	rBV	60044	160924	33.36%	6.171%
6	6.763	916	931	950	rBV	151555	358894	74.40%	13.763%
7	7.129	986	991	998	rBV2	2693	5679	1.18%	0.218%
8	8.653	1234	1241	1255	rBV	309387	482353	100.00%	18.498%
9	10.055	1465	1471	1487	rBV	318207	425607	88.24%	16.322%
10	11.085	1634	1640	1655	rBV	249167	322757	66.91%	12.377%
11	12.024	1789	1794	1807	rBV	325323	402577	83.46%	15.439%




Sum of corrected areas: 2607613

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
Data File : VX025531.D
Acq On : 04 Dec 2021 18:51
Operator : JC/MD
Sample : M4923-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPOW1-7-20211201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

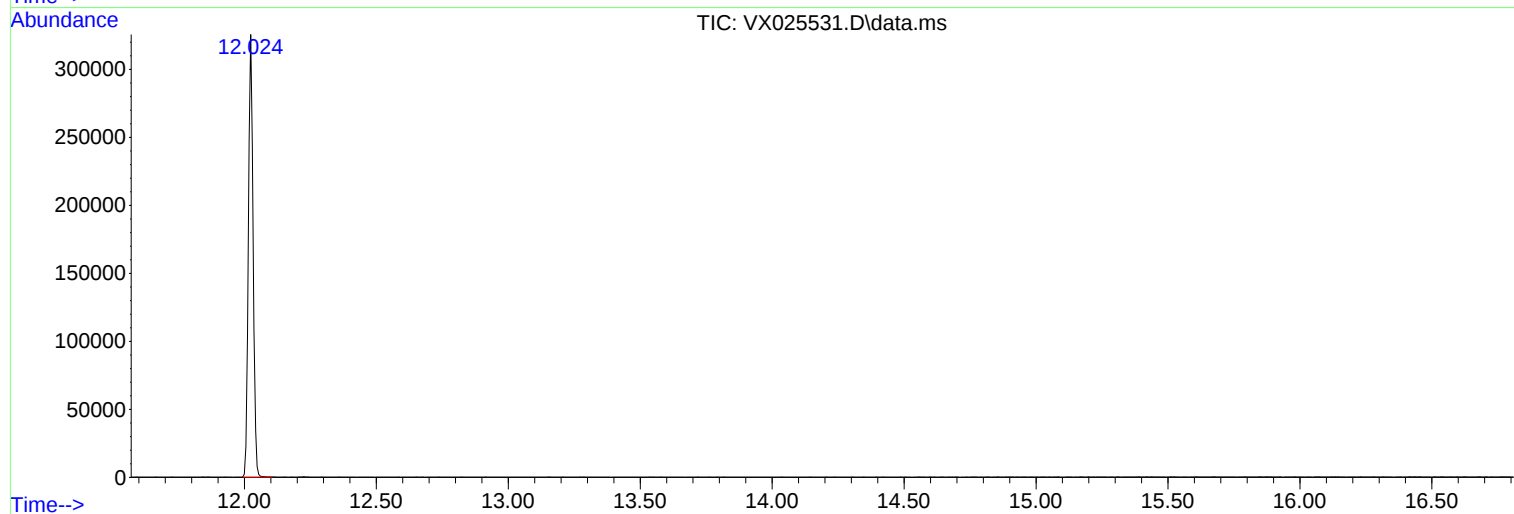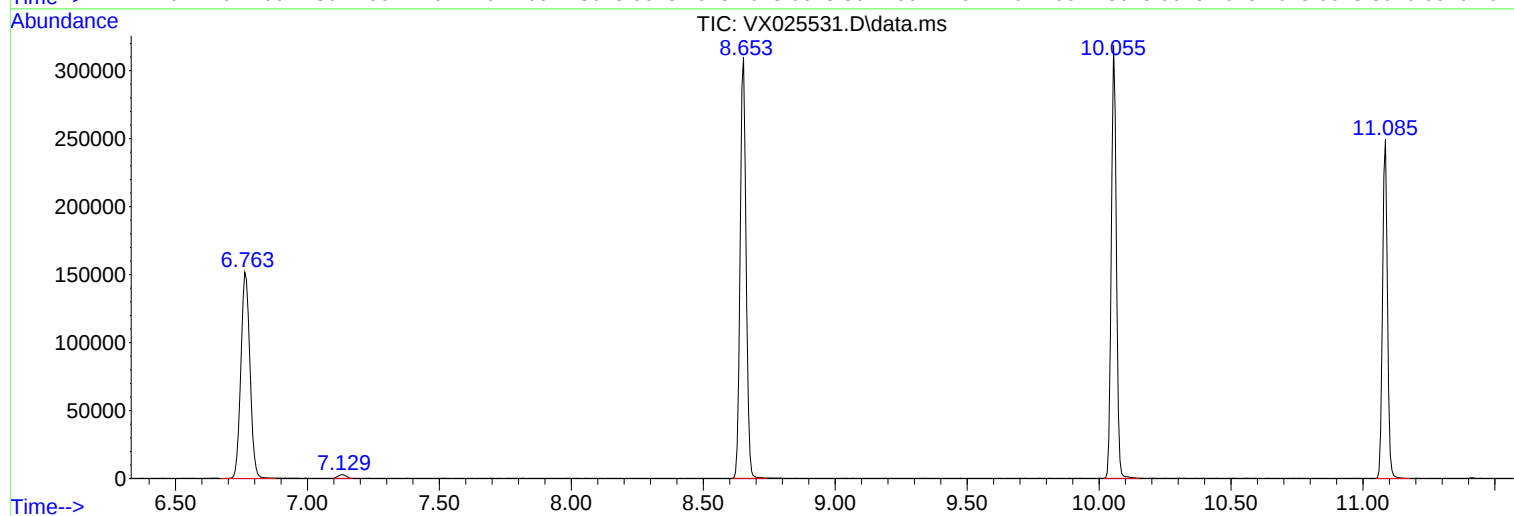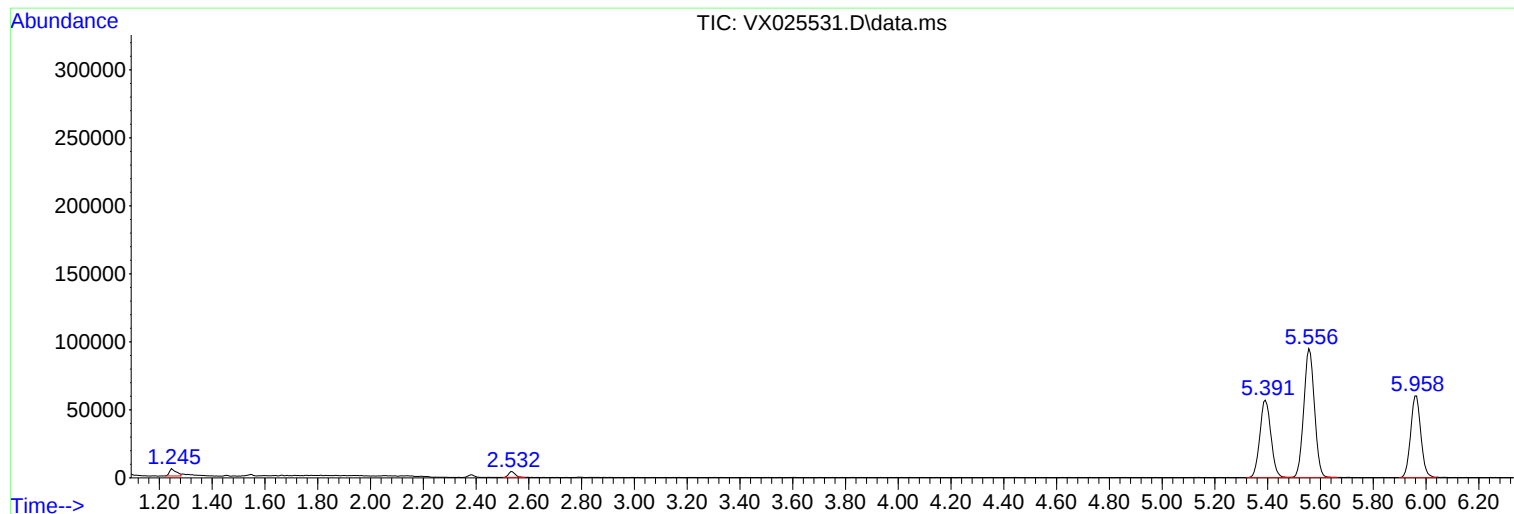

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
Data File : VX025531.D
Acq On : 04 Dec 2021 18:51
Operator : JC/MD
Sample : M4923-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPOW1-7-20211201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120421\
Data File : VX025531.D
Acq On : 04 Dec 2021 18:51
Operator : JC/MD
Sample : M4923-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPOW1-7-20211201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc