

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120424\
 Data File : VX044118.D
 Acq On : 04 Dec 2024 15:43
 Operator : JC/MD
 Sample : P5006-10DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 05 00:28:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 22 03:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	105677	50.000	ug/l	0.01
34) 1,4-Difluorobenzene	6.757	114	201675	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	175270	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	74917	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	94308	52.031	ug/l	0.01
Spiked Amount 50.000	Range 74 - 125		Recovery = 104.060%			
35) Dibromofluoromethane	5.379	113	66594	46.212	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 92.420%			
50) Toluene-d8	8.647	98	248998	50.125	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 100.260%			
62) 4-Bromofluorobenzene	11.079	95	86307	51.052	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 102.100%			
Target Compounds						Qvalue
5) Bromomethane	1.599	94	316	0.343	ug/l #	53
6) Chloroethane	1.636	64	411	0.450	ug/l #	42
16) Acetone	2.380	43	1308	1.571	ug/l	90
27) cis-1,2-Dichloroethene	4.483	96	1723	1.109	ug/l	93
31) Cyclohexane	5.532	56	1803	0.893	ug/l #	41
36) 1,1-Dichloropropene	5.550	75	9882	5.503	ug/l #	52
38) Carbon Tetrachloride	5.550	117	12665	6.277	ug/l #	17
40) Benzene	6.038	78	44054	7.876	ug/l	98
51) 4-Methyl-2-Pentanone	8.641	43	1326	0.613	ug/l #	1
52) Toluene	8.714	92	51529	15.391	ug/l	98
53) t-1,3-Dichloropropene	8.714	75	758	0.382	ug/l #	11
55) 1,1,2-Trichloroethane	9.025	97	661	0.478	ug/l #	15
58) 2-Chloroethyl Vinyl ether	8.086	63	25	Below Cal	#	46
67) Ethyl Benzene	10.189	91	185446	28.430	ug/l	99
68) m/p-Xylenes	10.299	106	26667	10.963	ug/l	98
69) o-Xylene	10.640	106	19428	8.180	ug/l	95
70) Styrene	10.640	104	1335	0.340	ug/l #	1
73) Isopropylbenzene	10.957	105	7004	1.216	ug/l	96
76) 1,2,3-Trichloropropane	11.079	75	48268	29.379	ug/l #	34
78) n-propylbenzene	11.311	91	2571	0.400	ug/l	89
79) 2-Chlorotoluene	11.378	91	4501	1.107	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.451	105	6984	1.474	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.079	75	48268	80.169	ug/l #	6
82) 4-Chlorotoluene	11.451	91	1006	0.219	ug/l #	46
83) tert-Butylbenzene	11.969	119	1757	0.374	ug/l	71
84) 1,2,4-Trimethylbenzene	11.750	105	23088	4.895	ug/l	99
85) sec-Butylbenzene	11.750	105	23088	4.013	ug/l #	57
86) p-Isopropyltoluene	12.006	119	1063	0.227	ug/l #	59
89) n-Butylbenzene	12.244	91	31485	7.641	ug/l #	45
90) Hexachloroethane	12.408	117	14286	17.976	ug/l #	18
92) 1,2-Dibromo-3-Chloropr...	12.969	75	100	0.253	ug/l #	4
95) Naphthalene	13.774	128	1843051	343.935	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120424\
Data File : VX044118.D
Acq On : 04 Dec 2024 15:43
Operator : JC/MD
Sample : P5006-10DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Dec 05 00:28:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 22 03:45:52 2024
Response via : Initial Calibration




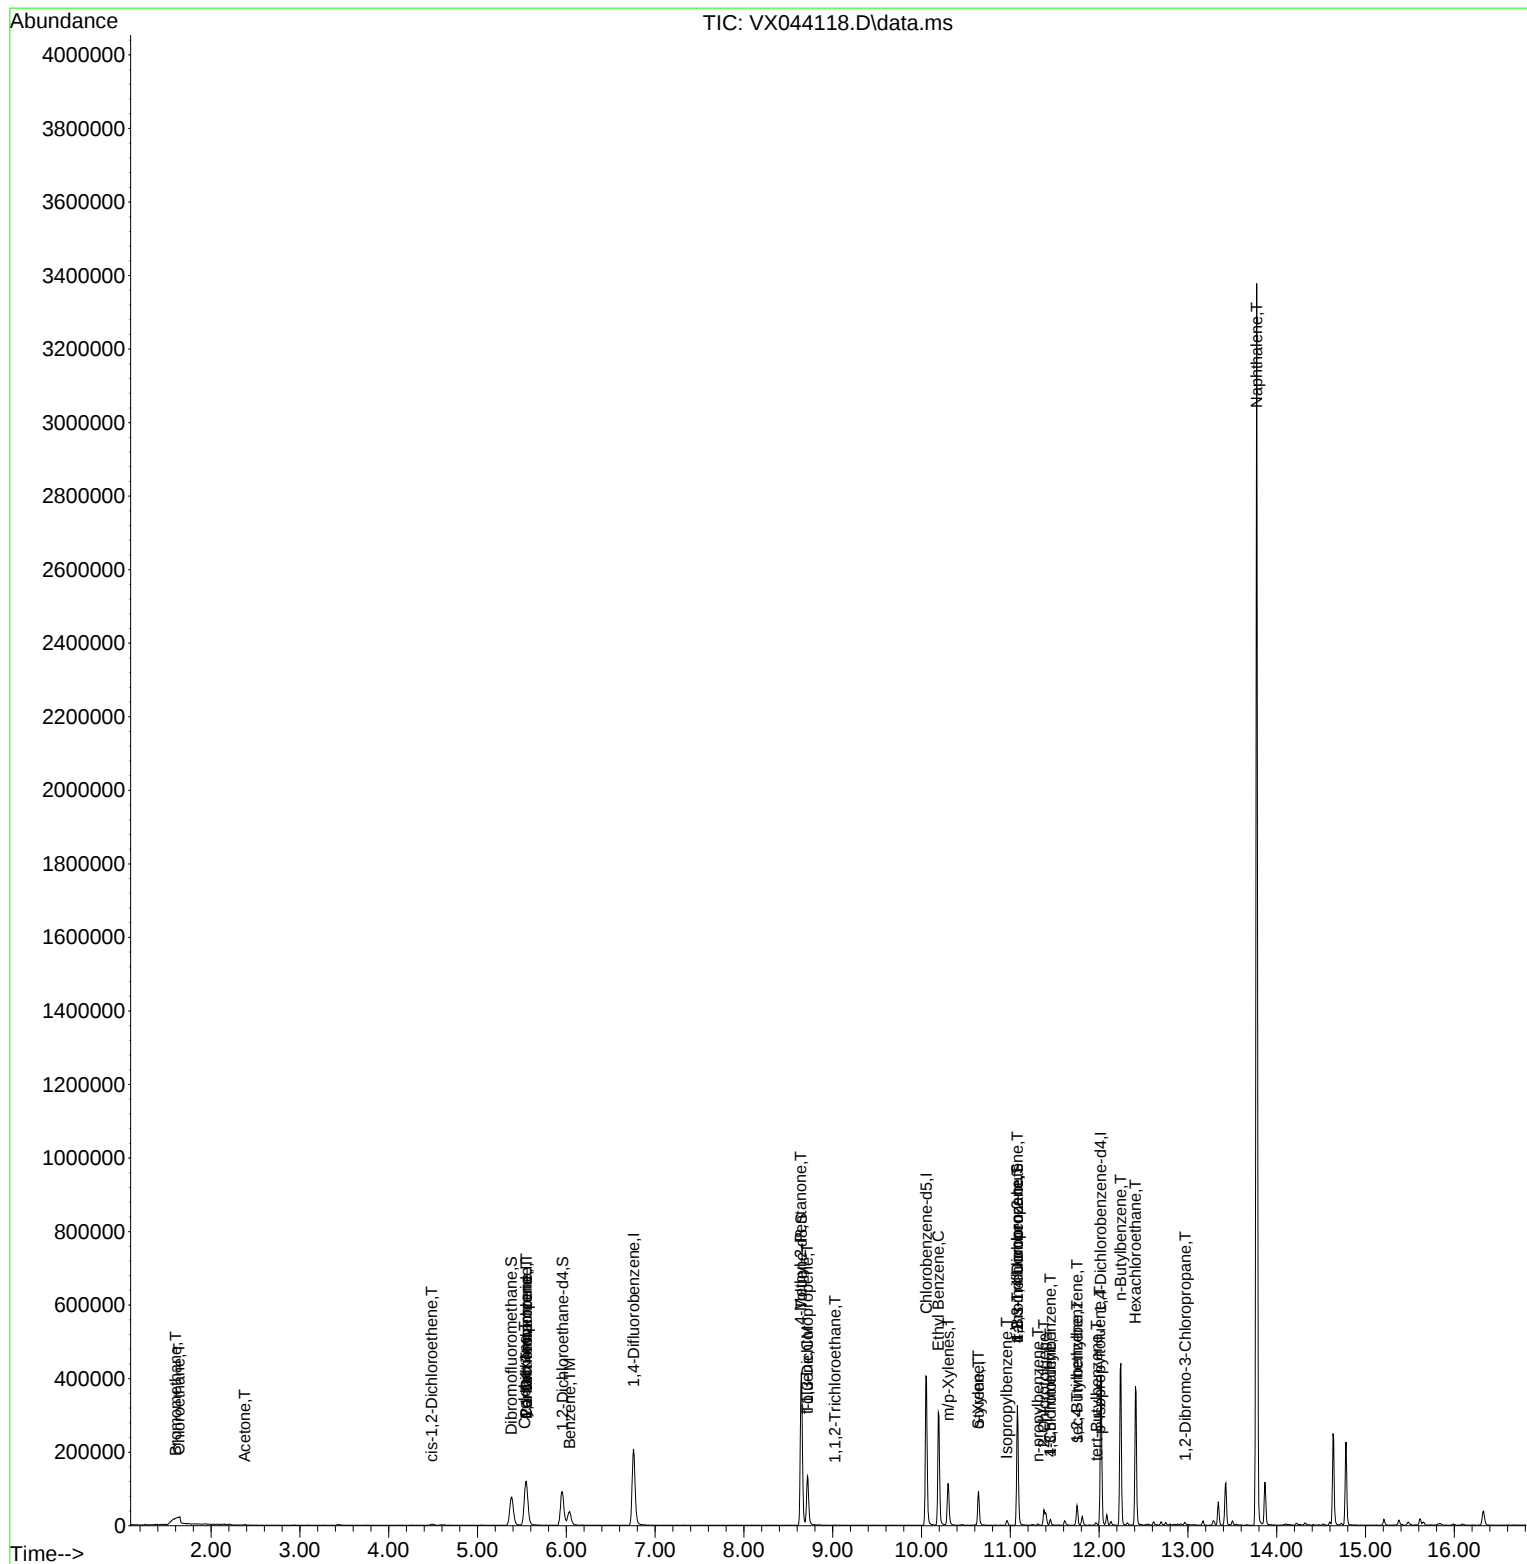




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.012 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 105677
Ion Ratio Lower Upper
168 100
99 69.2 51.8 77.8

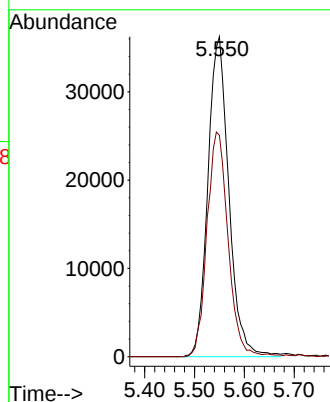

#5
Bromomethane
Concen: 0.343 ug/l
RT: 1.599 min Scan# 84
Delta R.T. 0.006 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43

Tgt Ion: 94 Resp: 316
Ion Ratio Lower Upper
94 100
96 47.7 73.9 110.9#


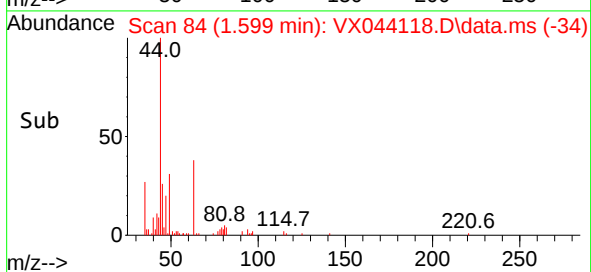
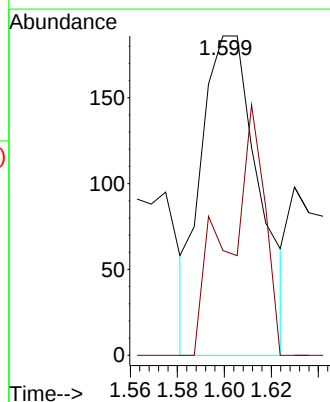
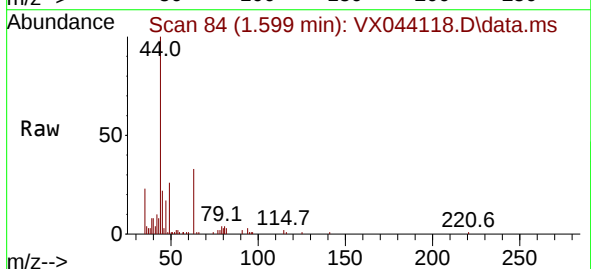


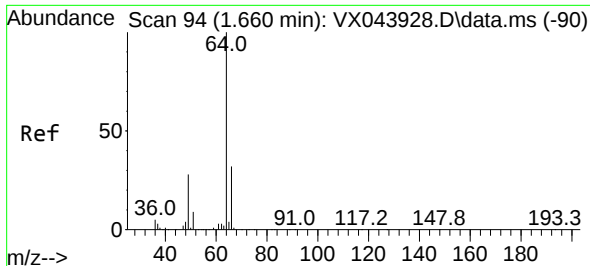

#6
Chloroethane
Concen: 0.450 ug/l
RT: 1.636 min Scan# 90
Delta R.T. -0.024 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 64 Resp: 411
Ion Ratio Lower Upper
64 100
66 0.0 25.9 38.9#

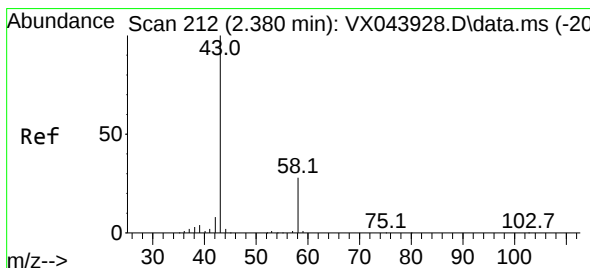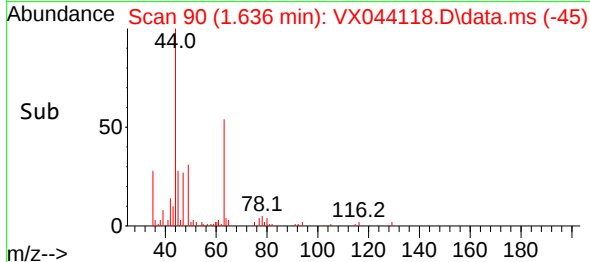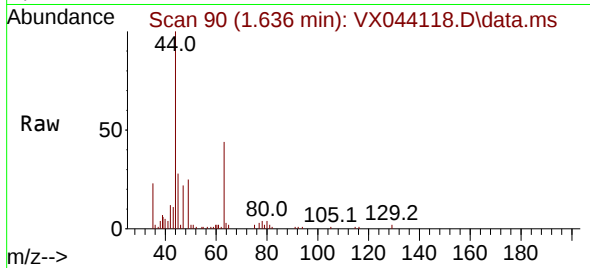

#16
Acetone
Concen: 1.571 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43

Tgt Ion: 43 Resp: 1308
Ion Ratio Lower Upper
43 100
58 33.6 22.7 34.1

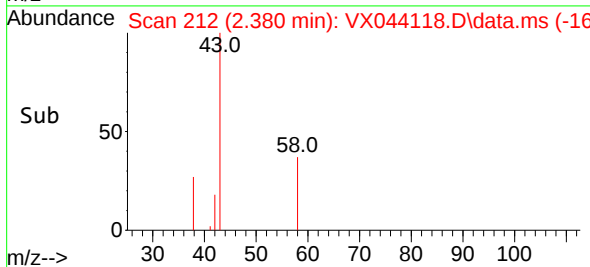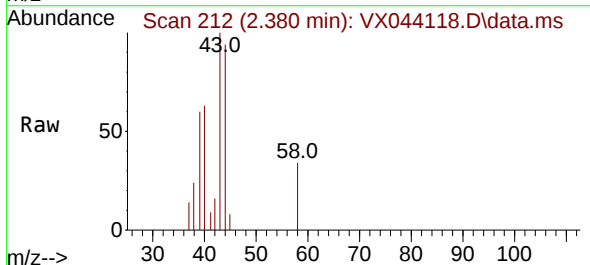



#27

cis-1,2-Dichloroethene

Concen: 1.109 ug/l

RT: 4.483 min Scan# 51

Delta R.T. 0.006 min


Lab File: VX044118.D

Acq: 04 Dec 2024 15:43

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion: 96 Resp: 1723

Ion Ratio Lower Upper

96 100

61 144.7 0.0 297.4

98 50.9 0.0 127.8

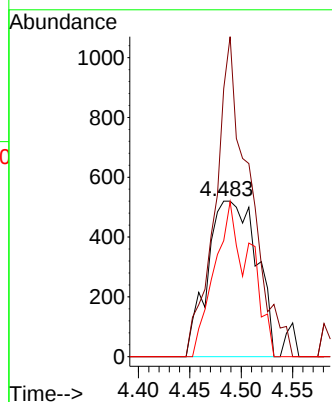

#31

Cyclohexane

Concen: 0.893 ug/l

RT: 5.532 min Scan# 729

Delta R.T. 0.073 min

Lab File: VX044118.D

Acq: 04 Dec 2024 15:43




Tgt Ion: 56 Resp: 1803


Ion Ratio Lower Upper

56 100

69 108.1 24.7 37.1#

84 58.1 68.7 103.1#


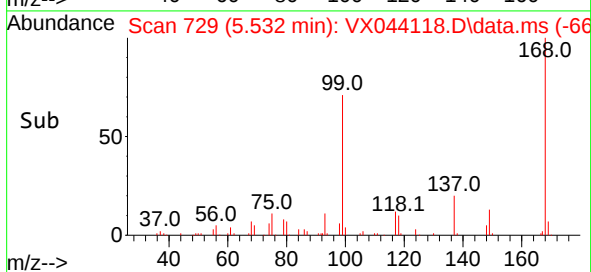

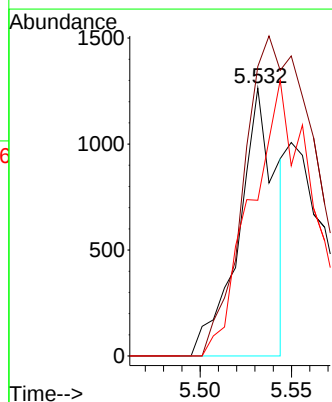




#33
 1,2-Dichloroethane-d4
 Concen: 52.031 ug/l
 RT: 5.958 min Scan# 797
 Delta R.T. 0.012 min
 Lab File: VX044118.D
 Acq: 04 Dec 2024 15:43




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 65 Resp: 94308
 Ion Ratio Lower Upper
 65 100
 67 48.6 0.0 100.8

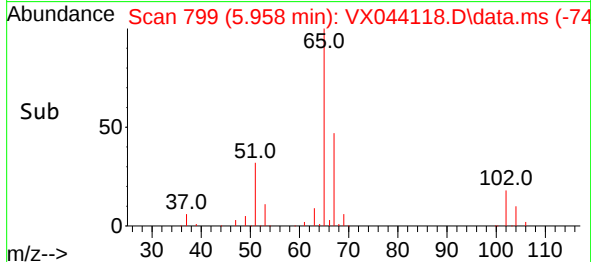

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.757 min Scan# 930
 Delta R.T. -0.000 min
 Lab File: VX044118.D
 Acq: 04 Dec 2024 15:43


Tgt Ion: 114 Resp: 201675
 Ion Ratio Lower Upper
 114 100
 63 22.0 0.0 44.0
 88 16.8 0.0 32.4

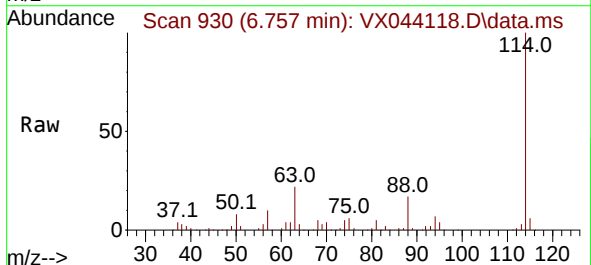






#35
Dibromofluoromethane
Concen: 46.212 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion:113 Resp: 66594
Ion Ratio Lower Upper
113 100
111 100.0 81.0 121.4
192 15.8 13.0 19.6




#36
1,1-Dichloropropene
Concen: 5.503 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.128 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43




Tgt Ion: 75 Resp: 9882
Ion Ratio Lower Upper
75 100
110 12.0 17.4 52.2#
77 0.0 25.8 38.8#

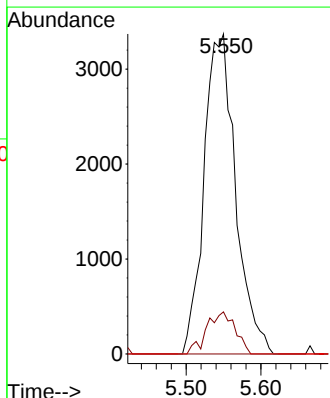






#38
Carbon Tetrachloride
Concen: 6.277 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.116 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 12665
Ion Ratio Lower Upper
117 100
119 5.3 75.2 112.8#
121 0.0 24.5 36.7#

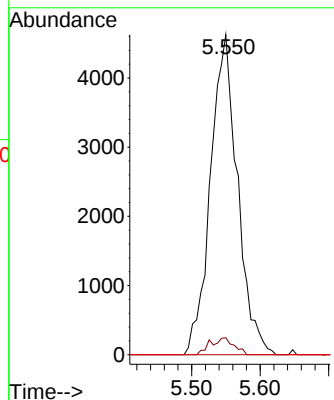

#40
Benzene
Concen: 7.876 ug/l
RT: 6.038 min Scan# 812
Delta R.T. 0.012 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43

Tgt Ion: 78 Resp: 44054
Ion Ratio Lower Upper
78 100
77 23.1 19.2 28.8

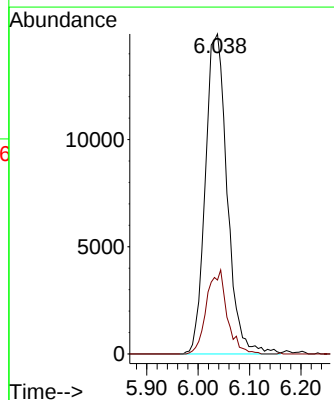



#50

Toluene-d8

Concen: 50.125 ug/l

RT: 8.647 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX044118.D

Acq: 04 Dec 2024 15:43

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 98 Resp: 248998

Ion Ratio Lower Upper

98 100

100 64.6 52.6 79.0

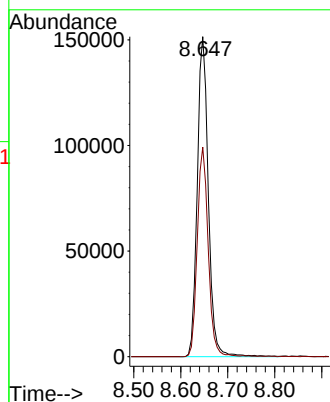

#51

4-Methyl-2-Pentanone

Concen: 0.613 ug/l

RT: 8.641 min Scan# 1239

Delta R.T. 0.067 min

Lab File: VX044118.D




Acq: 04 Dec 2024 15:43


Tgt Ion: 43 Resp: 1326

Ion Ratio Lower Upper

43 100

58 177.1 30.0 45.0#



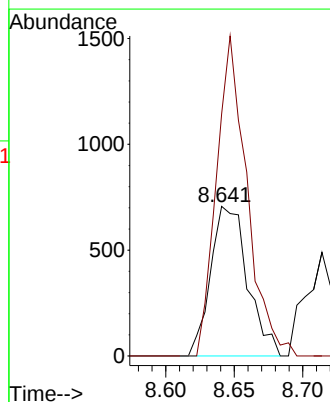





#52
Toluene
Concen: 15.391 ug/l
RT: 8.714 min Scan# 1251
Delta R.T. -0.000 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 92 Resp: 51529
Ion Ratio Lower Upper
92 100
91 172.3 139.7 209.5



#53
t-1,3-Dichloropropene
Concen: 0.382 ug/l
RT: 8.714 min Scan# 1251
Delta R.T. -0.262 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43


Tgt Ion: 75 Resp: 758
Ion Ratio Lower Upper
75 100
77 80.7 25.1 37.7#

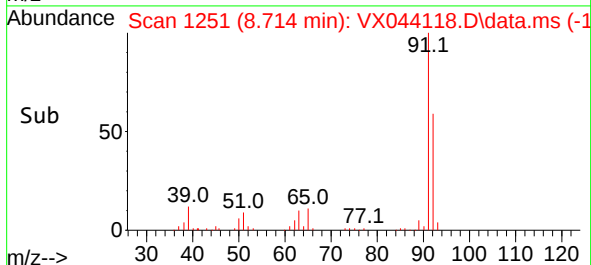






#55
 1,1,2-Trichloroethane
 Concen: 0.478 ug/l
 RT: 9.025 min Scan# 1148
 Delta R.T. -0.122 min
 Lab File: VX044118.D
 Acq: 04 Dec 2024 15:43

Instrument :
 MSVOA_X
 ClientSampleId :







Tgt Ion	Ratio	Lower	Upper
97	100		
83	0.0	69.4	104.0#
85	0.0	42.3	63.5#
99	0.0	49.6	74.4#



#58
 2-Chloroethyl Vinyl ether
 Concen: Below Cal
 RT: 8.086 min Scan# 1148
 Delta R.T. -0.152 min
 Lab File: VX044118.D
 Acq: 04 Dec 2024 15:43

Tgt Ion	Ratio	Lower	Upper
63	100		
106	0.0	23.0	34.6#









#62
4-Bromofluorobenzene
Concen: 51.052 ug/l
RT: 11.079 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 86307
Ion Ratio Lower Upper
95 100
174 69.2 0.0 150.4
176 67.0 0.0 146.0

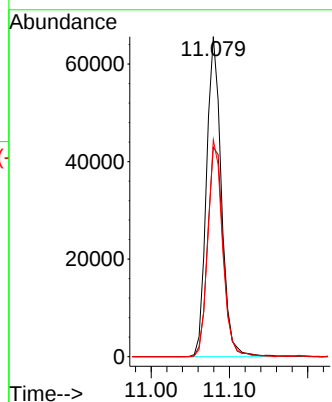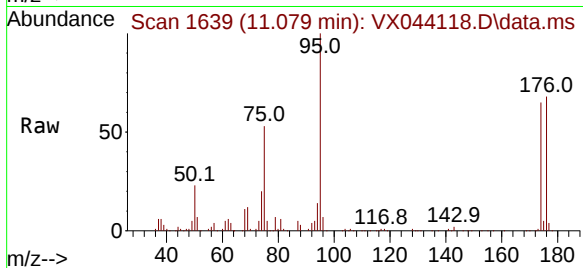

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.006 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43

Tgt Ion: 117 Resp: 175270
Ion Ratio Lower Upper
117 100
82 59.4 46.4 69.6
119 31.6 24.6 37.0



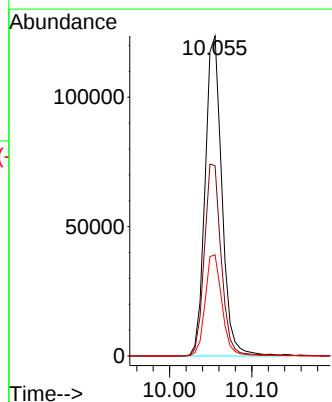
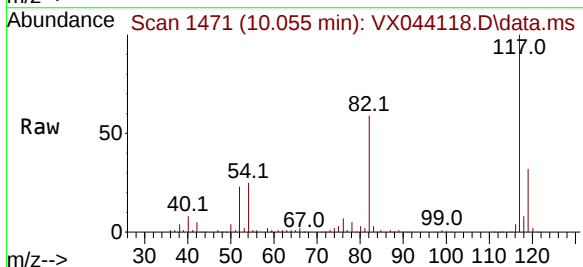




#67
Ethyl Benzene
Concen: 28.430 ug/l
RT: 10.189 min Scan# 1493
Delta R.T. -0.000 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 185446
Ion Ratio Lower Upper
91 100
106 28.7 23.6 35.4

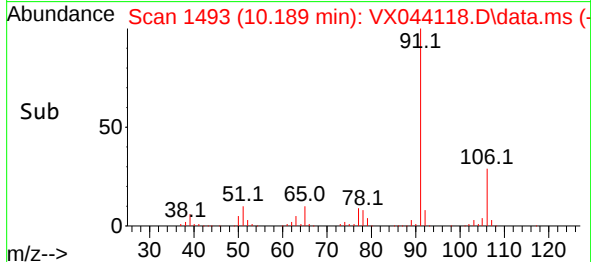

#68
m/p-Xylenes
Concen: 10.963 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43

Tgt Ion: 106 Resp: 26667
Ion Ratio Lower Upper
106 100
91 212.9 168.1 252.1


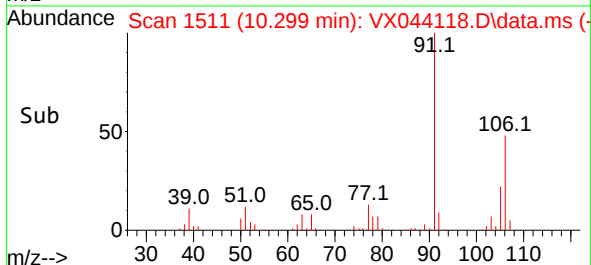
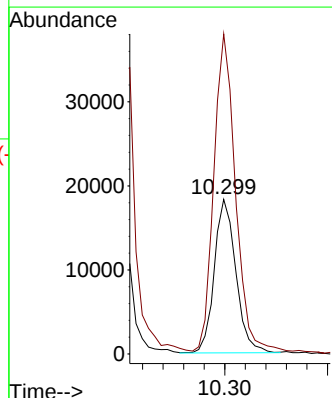
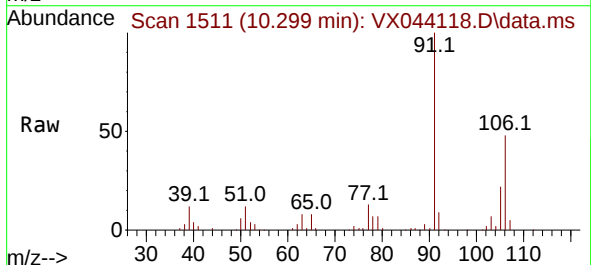




#69
o-Xylene
Concen: 8.180 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.000 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 19428
Ion Ratio Lower Upper
106 100
91 228.1 110.2 330.6



#70
Styrene
Concen: 0.340 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.012 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43

Tgt Ion:104 Resp: 1335
Ion Ratio Lower Upper
104 100
78 259.6 42.2 63.2#
103 212.5 44.7 67.1#









#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:152 Resp: 74917
Ion Ratio Lower Upper
152 100
115 65.2 45.4 136.2
150 161.7 0.0 353.0

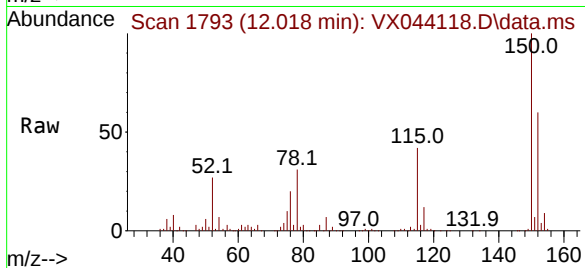

#73
Isopropylbenzene
Concen: 1.216 ug/l
RT: 10.957 min Scan# 1619
Delta R.T. -0.000 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43

Tgt Ion:105 Resp: 7004
Ion Ratio Lower Upper
105 100
120 27.9 13.0 38.9

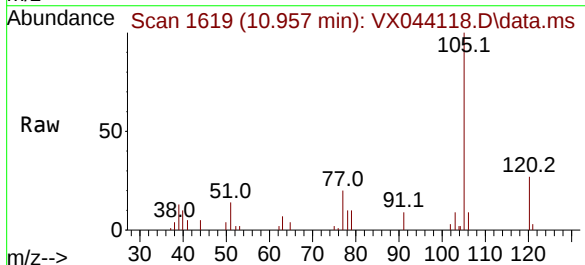



#76

1,2,3-Trichloropropane

Concen: 29.379 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX044118.D

Acq: 04 Dec 2024 15:43

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 48268

Ion Ratio Lower Upper

75 100

77 0.7 21.8 65.3#

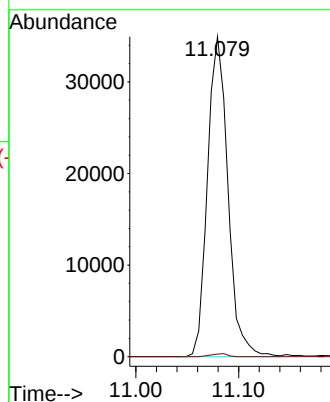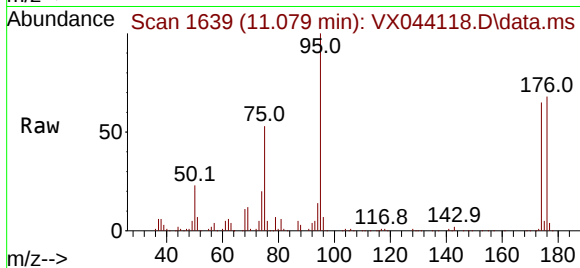

#78

n-propylbenzene

Concen: 0.400 ug/l

RT: 11.311 min Scan# 1677

Delta R.T. 0.012 min

Lab File: VX044118.D




Acq: 04 Dec 2024 15:43


Tgt Ion: 91 Resp: 2571

Ion Ratio Lower Upper

91 100

120 17.4 11.5 34.4

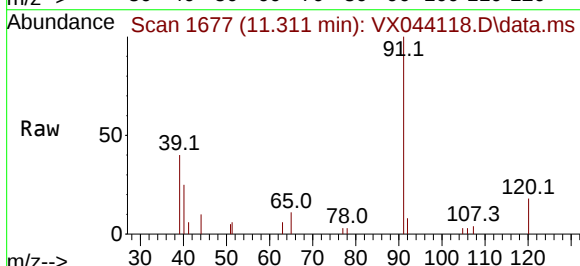



#79

2-Chlorotoluene

Concen: 1.107 ug/l

RT: 11.378 min Scan# 1

Delta R.T. 0.018 min

Lab File: VX044118.D

Acq: 04 Dec 2024 15:43

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 4501

Ion Ratio Lower Upper

91 100

126 0.0 16.6 49.8#

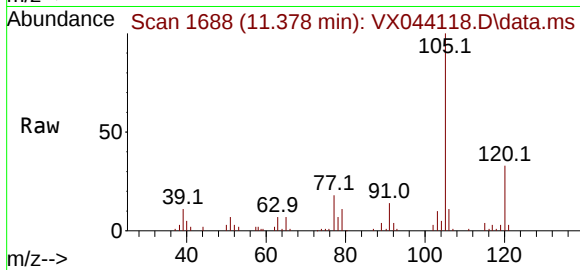

#80

1,3,5-Trimethylbenzene

Concen: 1.474 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. -0.000 min

Lab File: VX044118.D




Acq: 04 Dec 2024 15:43


Tgt Ion:105 Resp: 6984

Ion Ratio Lower Upper

105 100

120 46.2 23.3 69.8

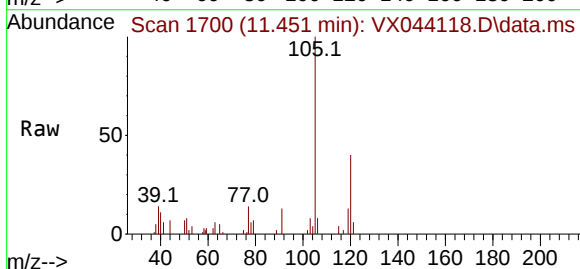



#81

trans-1,4-Dichloro-2-butene

Concen: 80.169 ug/l

RT: 11.079 min Scan# 1

Delta R.T. 0.061 min

Lab File: VX044118.D

Acq: 04 Dec 2024 15:43

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 75 Resp: 48268

Ion Ratio Lower Upper

75 100

53 0.0 86.7 130.1#

89 0.0 38.2 57.2#

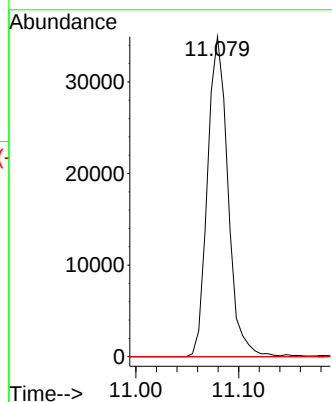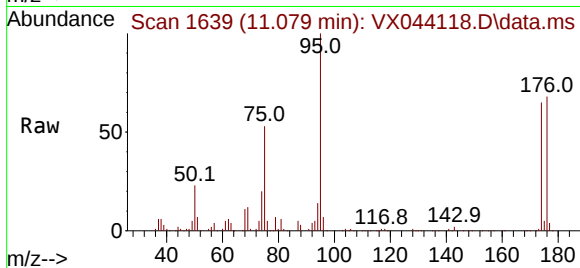

#82

4-Chlorotoluene

Concen: 0.219 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. -0.000 min

Lab File: VX044118.D




Acq: 04 Dec 2024 15:43


Tgt Ion: 91 Resp: 1006

Ion Ratio Lower Upper

91 100

126 0.0 14.3 42.9#

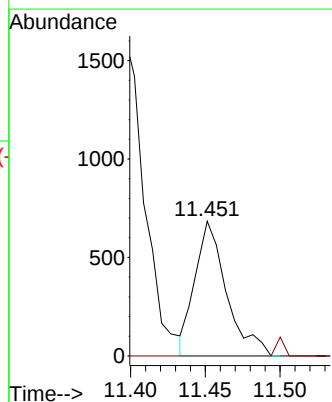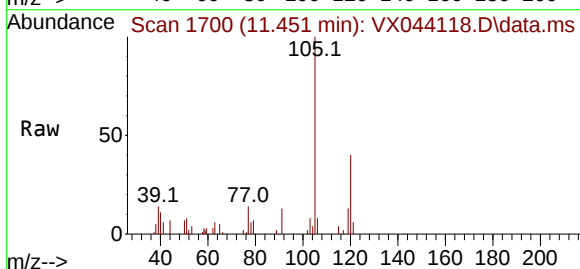



#83

tert-Butylbenzene

Concen: 0.374 ug/l

RT: 11.969 min Scan# 1785

Delta R.T. 0.256 min

Lab File: VX044118.D

Acq: 04 Dec 2024 15:43

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:119 Resp: 1757

Ion Ratio Lower Upper

119 100

91 36.0 31.0 93.0

134 30.9 11.6 34.8

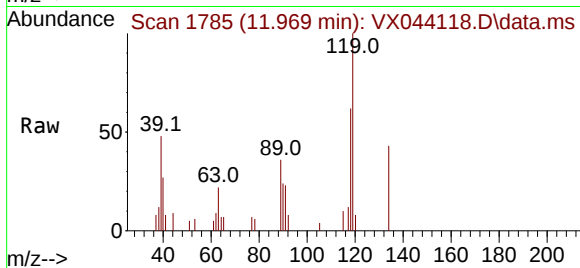

#84

1,2,4-Trimethylbenzene

Concen: 4.895 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX044118.D




Acq: 04 Dec 2024 15:43


Tgt Ion:105 Resp: 23088

Ion Ratio Lower Upper

105 100

120 43.0 21.9 65.7

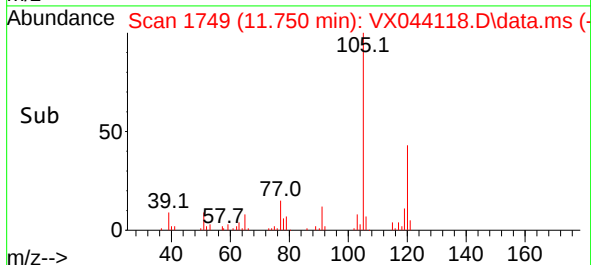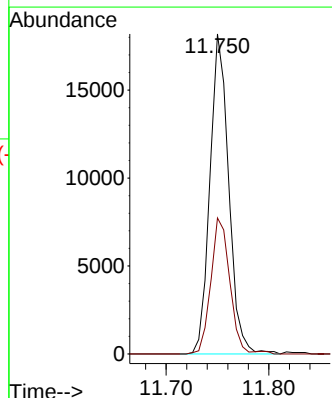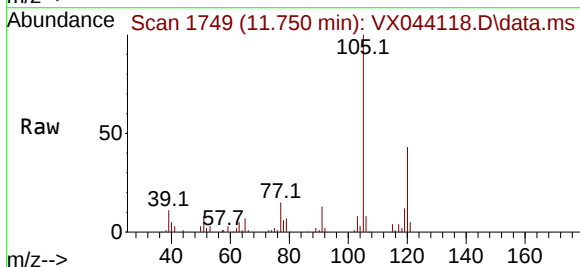



#85

sec-Butylbenzene

Concen: 4.013 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.140 min

Lab File: VX044118.D

Acq: 04 Dec 2024 15:43

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 23088

Ion Ratio Lower Upper

105 100

134 0.0 9.7 29.1#

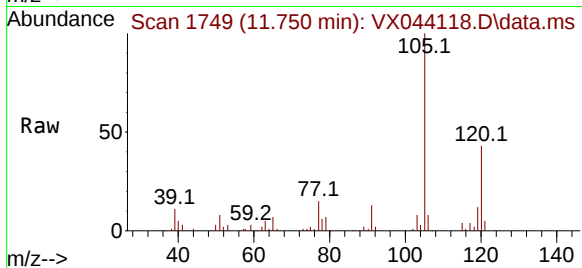

#86

p-Isopropyltoluene

Concen: 0.227 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. -0.000 min

Lab File: VX044118.D

Acq: 04 Dec 2024 15:43




Tgt Ion:119 Resp: 1063


Ion Ratio Lower Upper

119 100

134 41.9 13.0 38.9#

91 0.0 13.0 38.9#




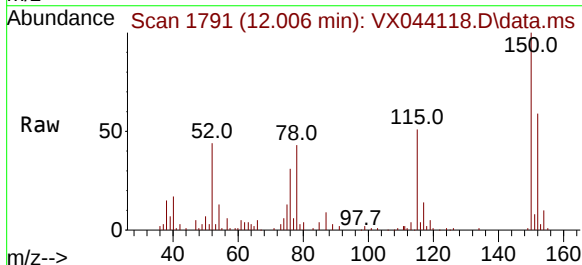




#89
n-Butylbenzene
Concen: 7.641 ug/l
RT: 12.244 min Scan# 1830
Delta R.T. -0.085 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 31485
Ion Ratio Lower Upper
91 100
92 11.0 26.6 79.8#
134 2.5 12.4 37.2#

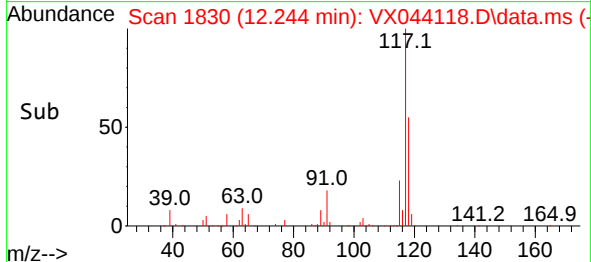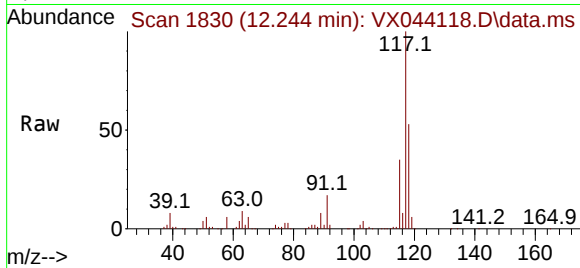

#90
Hexachloroethane
Concen: 17.976 ug/l
RT: 12.408 min Scan# 1857
Delta R.T. -0.128 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43


Tgt Ion: 117 Resp: 14286
Ion Ratio Lower Upper
117 100
201 0.0 32.4 97.0#

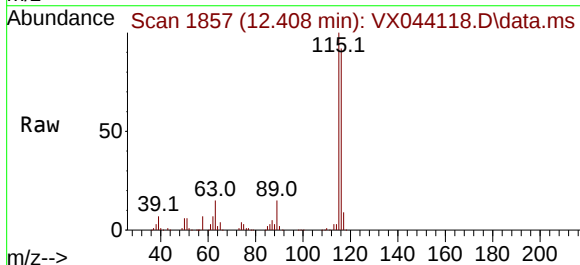






#92
1,2-Dibromo-3-Chloropropane
Concen: 0.253 ug/l
RT: 12.969 min Scan# 1944
Delta R.T. 0.030 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43

Instrument :
MSVOA_X
ClientSampleId :

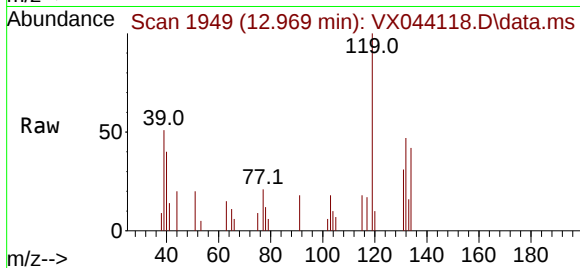

Tgt Ion: 75 Resp: 100
Ion Ratio Lower Upper
75 100
155 0.0 40.1 120.2#
157 0.0 49.6 149.0#

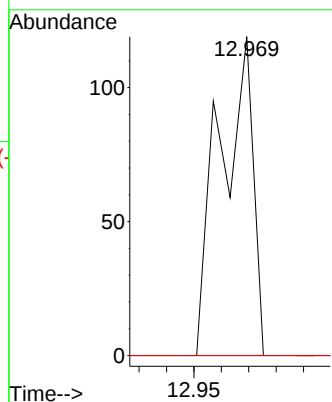

#95
Naphthalene
Concen: 343.935 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX044118.D
Acq: 04 Dec 2024 15:43

Tgt Ion:128 Resp: 1843051
Ion Ratio Lower Upper
128 100
127 13.2 10.2 15.2
129 11.0 8.6 12.8

