

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120424\
 Data File : VX044125.D
 Acq On : 04 Dec 2024 18:25
 Operator : JC/MD
 Sample : P5006-14RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 05 00:34:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 22 03:45:52 2024
 Response via : Initial Calibration


Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	108281	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	207723	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	187581	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	86376	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	95639	51.496	ug/l	0.00
Spiked Amount 50.000	Range 74	- 125	Recovery	=	103.000%	
35) Dibromofluoromethane	5.385	113	52533	35.393	ug/l	0.00
Spiked Amount 50.000	Range 75	- 124	Recovery	=	70.780%#	
50) Toluene-d8	8.647	98	257599	50.347	ug/l	0.00
Spiked Amount 50.000	Range 86	- 113	Recovery	=	100.700%	
62) 4-Bromofluorobenzene	11.079	95	93522	53.709	ug/l	0.00
Spiked Amount 50.000	Range 77	- 121	Recovery	=	107.420%	
Target Compounds						
					Qvalue	
6) Chloroethane	1.636	64	257	0.275	ug/l #	42
16) Acetone	2.386	43	14942	17.517	ug/l	98
18) Methyl Acetate	2.709	43	468	0.236	ug/l #	52
20) Methylene Chloride	2.794	84	911	0.629	ug/l #	77
25) 2-Butanone	4.593	43	2217	2.014	ug/l #	84
27) cis-1,2-Dichloroethene	4.495	96	831	0.522	ug/l	91
29) Tetrahydrofuran	5.038	42	727	1.077	ug/l #	40
31) Cyclohexane	5.544	56	3234	1.562	ug/l #	38
36) 1,1-Dichloropropene	5.550	75	10818	5.849	ug/l #	50
38) Carbon Tetrachloride	5.550	117	13127	6.316	ug/l #	15
40) Benzene	6.038	78	14482	2.514	ug/l	93
44) Trichloroethene	7.117	130	415	0.254	ug/l	48
51) 4-Methyl-2-Pentanone	8.580	43	1192	0.535	ug/l	98
52) Toluene	8.720	92	8428	2.444	ug/l	99
67) Ethyl Benzene	10.189	91	312956	44.830	ug/l	99
68) m/p-Xylenes	10.299	106	23284	8.944	ug/l	98
69) o-Xylene	10.640	106	26756	10.526	ug/l	98
70) Styrene	10.646	104	1754	0.417	ug/l #	1
73) Isopropylbenzene	10.964	105	28446	4.284	ug/l	98
76) 1,2,3-Trichloropropane	11.079	75	53022	27.992	ug/l #	34
78) n-propylbenzene	11.305	91	14431	1.946	ug/l	98
79) 2-Chlorotoluene	11.396	91	7419	1.582	ug/l #	44
80) 1,3,5-Trimethylbenzene	11.451	105	25543	4.676	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.079	75	53022	76.382	ug/l #	6
82) 4-Chlorotoluene	11.451	91	3181	0.601	ug/l #	46
83) tert-Butylbenzene	11.969	119	6939	1.282	ug/l	69
84) 1,2,4-Trimethylbenzene	11.750	105	95911	17.636	ug/l	98
85) sec-Butylbenzene	11.750	105	95911	14.458	ug/l #	57
86) p-Isopropyltoluene	12.012	119	4521	0.839	ug/l #	72
89) n-Butylbenzene	12.317	91	5444	1.146	ug/l #	4
90) Hexachloroethane	12.695	117	46465	50.711	ug/l #	18
92) 1,2-Dibromo-3-Chloropr...	12.963	75	324	0.711	ug/l #	4
95) Naphthalene	13.774	128	4687643	758.719	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Dec 05 00:34:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 22 03:45:52 2024
Response via : Initial Calibration

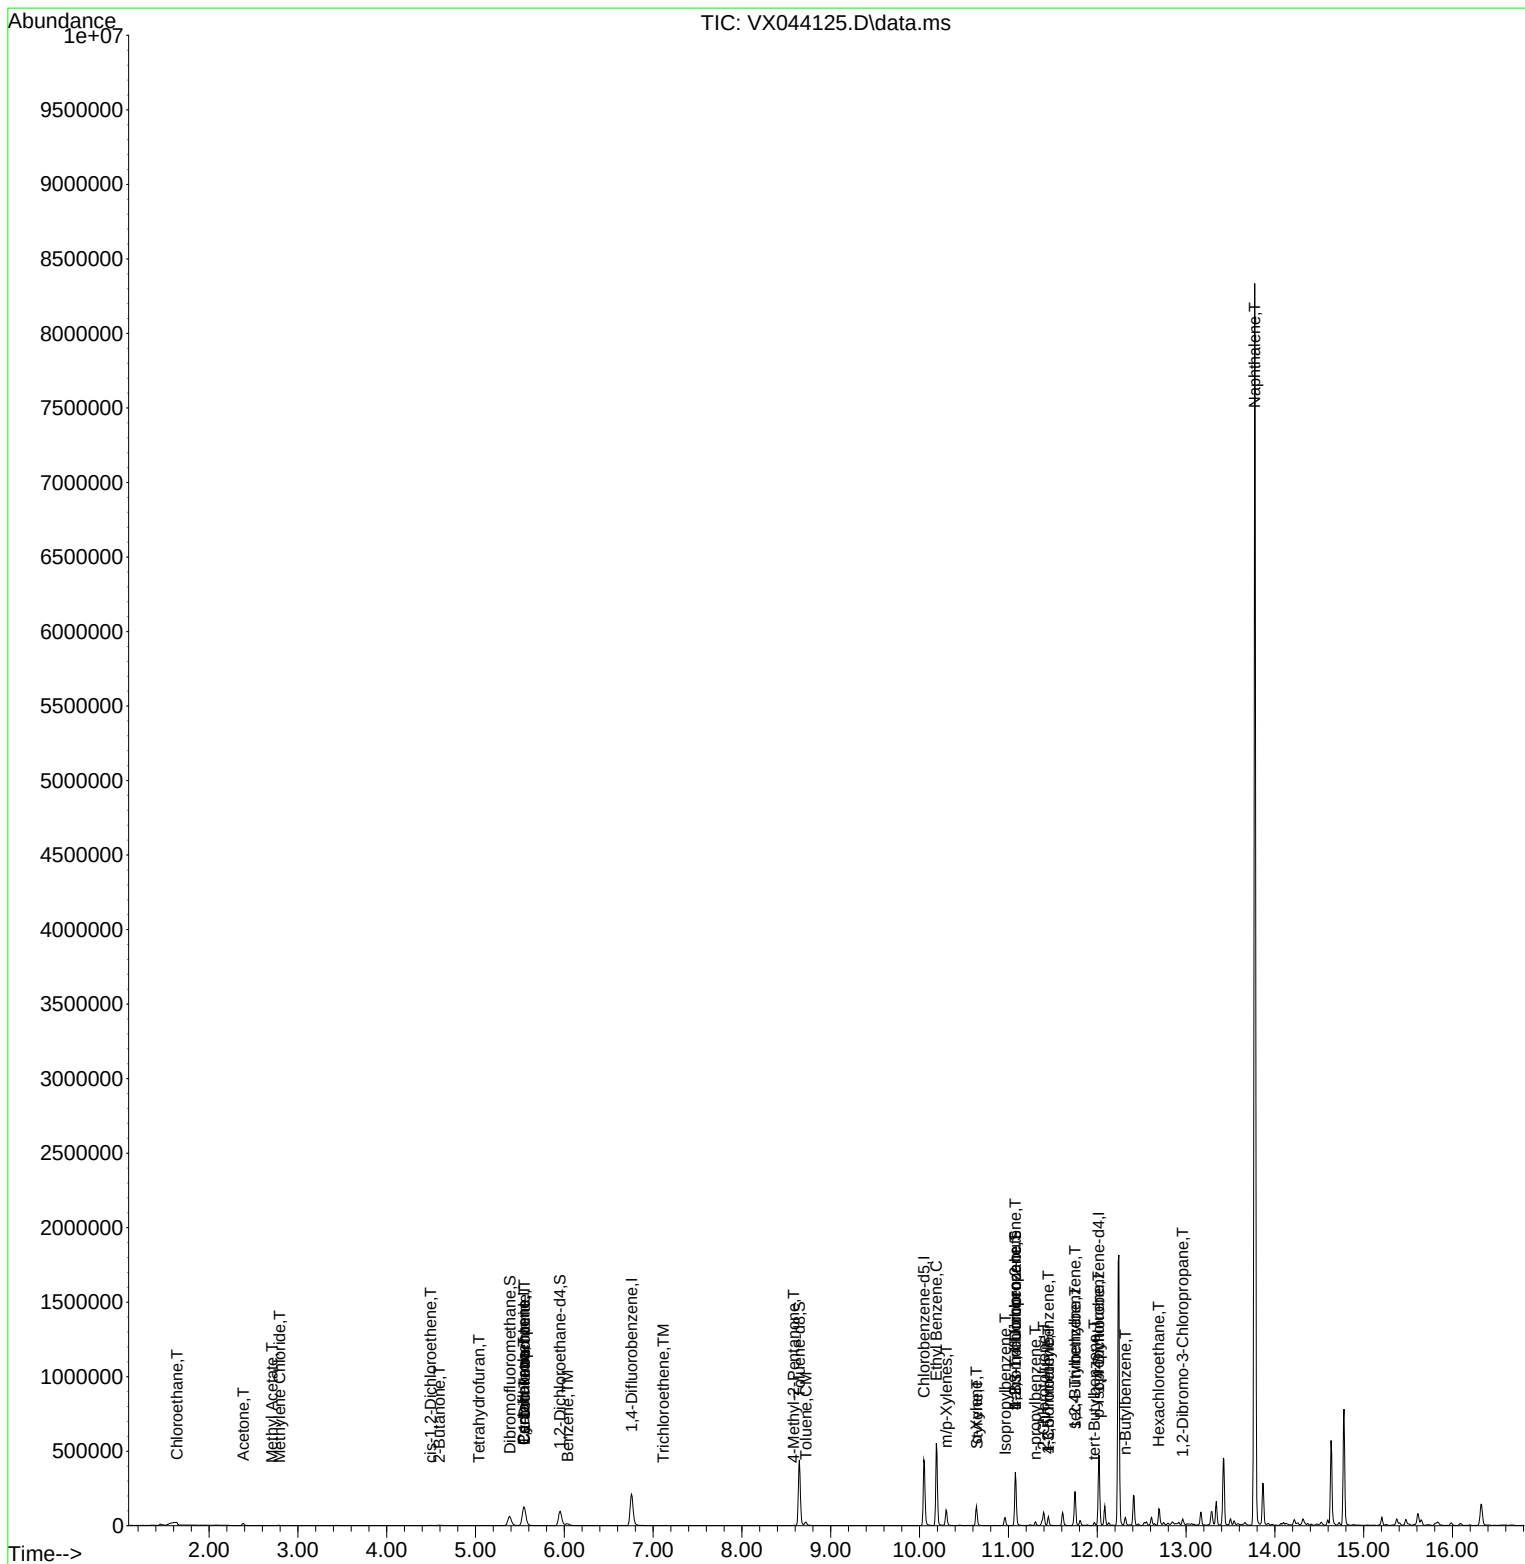




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25




Instrument :

MSVOA_X

ClientSampleId :







Tgt Ion:168 Resp: 108281
Ion Ratio Lower Upper
168 100
99 70.0 51.8 77.8

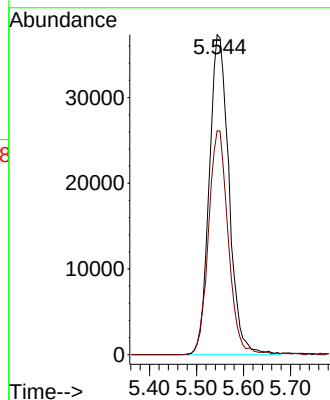

#6
Chloroethane
Concen: 0.275 ug/l
RT: 1.636 min Scan# 90
Delta R.T. -0.024 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25

Tgt Ion: 64 Resp: 257
Ion Ratio Lower Upper
64 100
66 0.0 25.9 38.9#



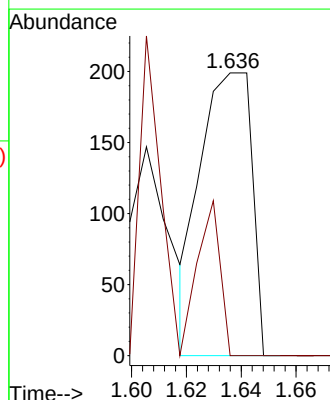
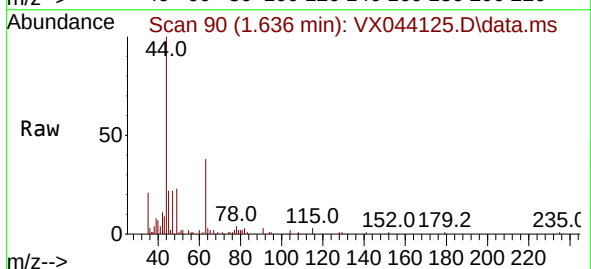




#16
Acetone
Concen: 17.517 ug/l
RT: 2.386 min Scan# 212
Delta R.T. 0.006 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 14942
Ion Ratio Lower Upper
43 100
58 29.3 22.7 34.1

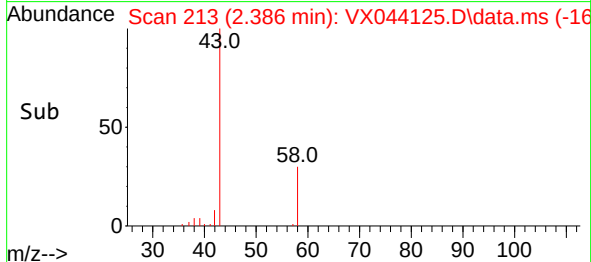

#18
Methyl Acetate
Concen: 0.236 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.006 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25


Tgt Ion: 43 Resp: 468
Ion Ratio Lower Upper
43 100
74 0.0 18.9 28.3#

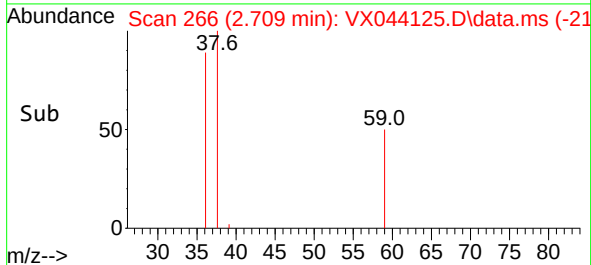






#20
Methylene Chloride
Concen: 0.629 ug/l
RT: 2.794 min Scan# 21
Delta R.T. 0.012 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 84 Resp: 911
Ion Ratio Lower Upper
84 100
49 98.9 102.7 154.1#
51 36.6 31.7 47.5
86 44.6 53.9 80.9#



#25
2-Butanone
Concen: 2.014 ug/l
RT: 4.593 min Scan# 575
Delta R.T. 0.037 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25

Tgt Ion: 43 Resp: 2217
Ion Ratio Lower Upper
43 100
72 17.3 20.2 30.2#









#27
 cis-1,2-Dichloroethene
 Concen: 0.522 ug/l
 RT: 4.495 min Scan# 51
 Delta R.T. 0.018 min
 Lab File: VX044125.D
 Acq: 04 Dec 2024 18:25

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 96 Resp: 831




Ion	Ratio	Lower	Upper
96	100		
61	135.3	0.0	297.4
98	59.2	0.0	127.8

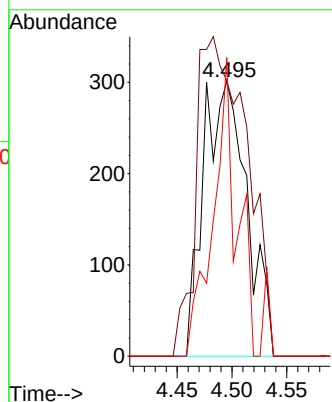


#29
 Tetrahydrofuran
 Concen: 1.077 ug/l
 RT: 5.038 min Scan# 648
 Delta R.T. 0.037 min
 Lab File: VX044125.D
 Acq: 04 Dec 2024 18:25

Tgt Ion: 42 Resp: 727


Ion	Ratio	Lower	Upper
42	100		
72	9.8	36.4	54.6#
71	0.0	33.4	50.0#

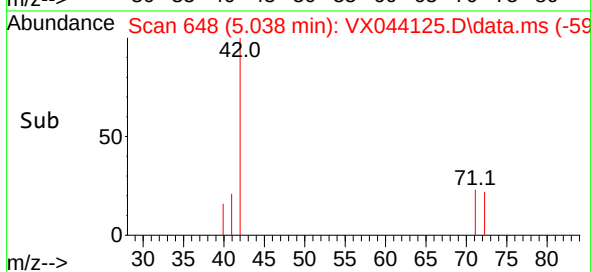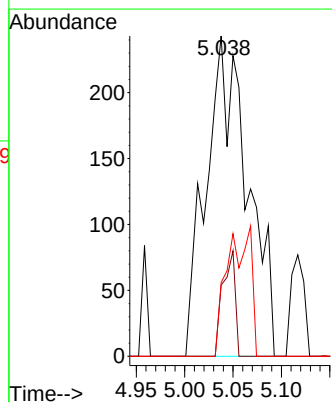






#31
Cyclohexane
Concen: 1.562 ug/l
RT: 5.544 min Scan# 717
Delta R.T. 0.085 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 56 Resp: 3234
Ion Ratio Lower Upper
56 100
69 134.3 24.7 37.1#
84 70.5 68.7 103.1



#33
1,2-Dichloroethane-d4
Concen: 51.496 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.006 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25


Tgt Ion: 65 Resp: 95639
Ion Ratio Lower Upper
65 100
67 48.4 0.0 100.8

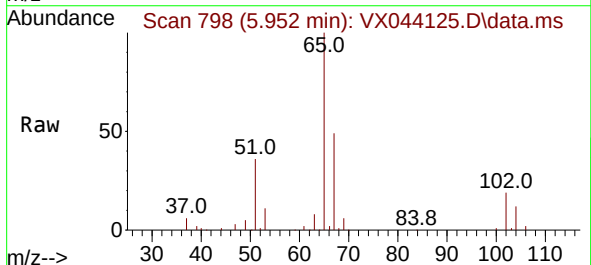






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:114 Resp: 207723
Ion Ratio Lower Upper
114 100
63 22.9 0.0 44.0
88 16.3 0.0 32.4



#35
Dibromofluoromethane
Concen: 35.393 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25


Tgt Ion:113 Resp: 52533
Ion Ratio Lower Upper
113 100
111 103.1 81.0 121.4
192 16.4 13.0 19.6

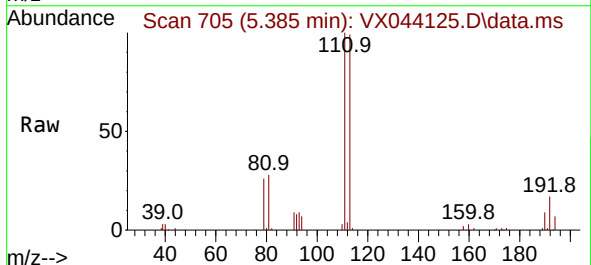






#36
1,1-Dichloropropene
Concen: 5.849 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.128 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 75 Resp: 10818
Ion Ratio Lower Upper
75 100
110 9.9 17.4 52.2#
77 0.0 25.8 38.8#

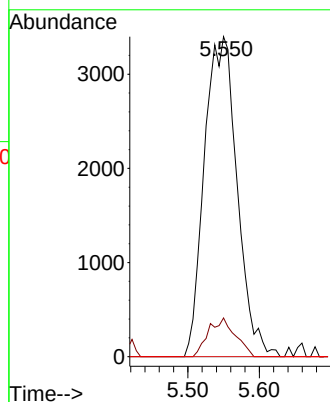

#38
Carbon Tetrachloride
Concen: 6.316 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.116 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25

Tgt Ion: 117 Resp: 13127
Ion Ratio Lower Upper
117 100
119 3.3 75.2 112.8#
121 0.0 24.5 36.7#

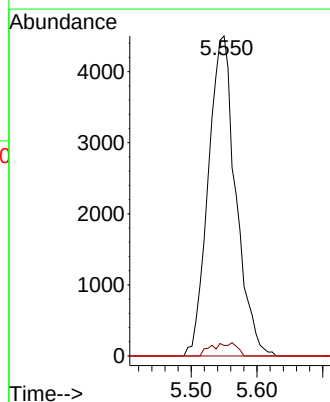

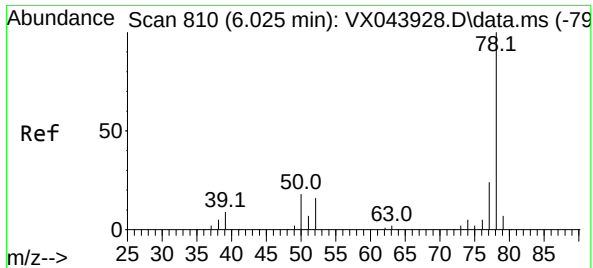

#40

Benzene

Concen: 2.514 ug/l

RT: 6.038 min Scan# 810

Delta R.T. 0.012 min

Lab File: VX044125.D

Acq: 04 Dec 2024 18:25

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 78 Resp: 14482

Ion Ratio Lower Upper

78 100

77 20.4 19.2 28.8

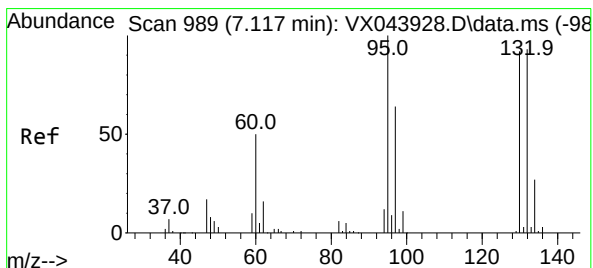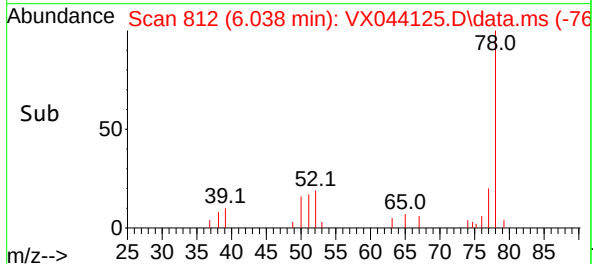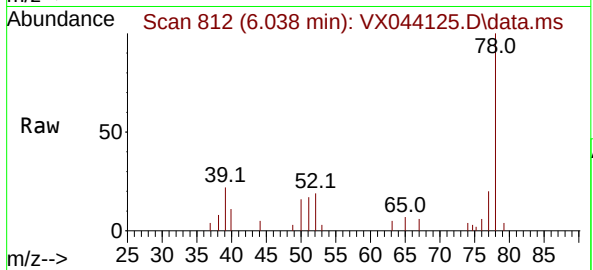

#44

Trichloroethene

Concen: 0.254 ug/l

RT: 7.117 min Scan# 989

Delta R.T. -0.000 min

Lab File: VX044125.D




Acq: 04 Dec 2024 18:25


Tgt Ion:130 Resp: 415

Ion Ratio Lower Upper

130 100

95 54.0 0.0 217.8


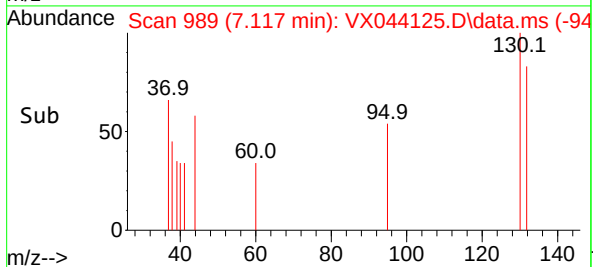

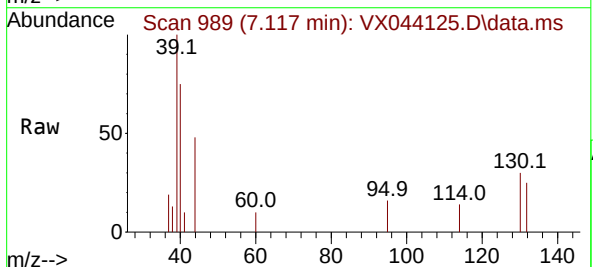




#50
Toluene-d8
Concen: 50.347 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 98 Resp: 257599
Ion Ratio Lower Upper
98 100
100 64.8 52.6 79.0

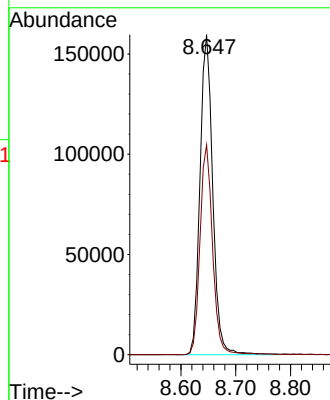

#51
4-Methyl-2-Pentanone
Concen: 0.535 ug/l
RT: 8.580 min Scan# 1229
Delta R.T. 0.006 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25

Tgt Ion: 43 Resp: 1192
Ion Ratio Lower Upper
43 100
58 38.6 30.0 45.0

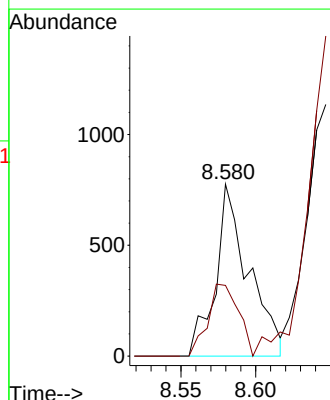



#52

Toluene

Concen: 2.444 ug/l

RT: 8.720 min Scan# 1251

Delta R.T. 0.006 min

Lab File: VX044125.D

Acq: 04 Dec 2024 18:25

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 92 Resp: 8428

Ion Ratio Lower Upper

92 100

91 172.6 139.7 209.5

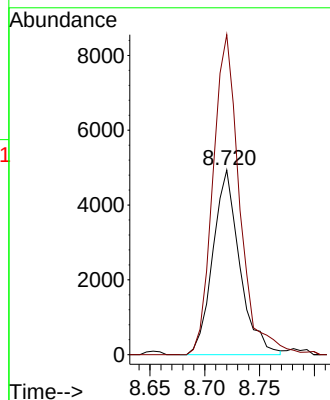

#62

4-Bromofluorobenzene

Concen: 53.709 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.000 min

Lab File: VX044125.D

Acq: 04 Dec 2024 18:25




Tgt Ion: 95 Resp: 93522


Ion Ratio Lower Upper

95 100

174 70.2 0.0 150.4

176 66.9 0.0 146.0



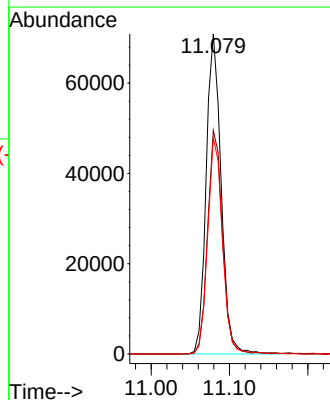





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. -0.000 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 187581
Ion Ratio Lower Upper
117 100
82 61.2 46.4 69.6
119 31.7 24.6 37.0

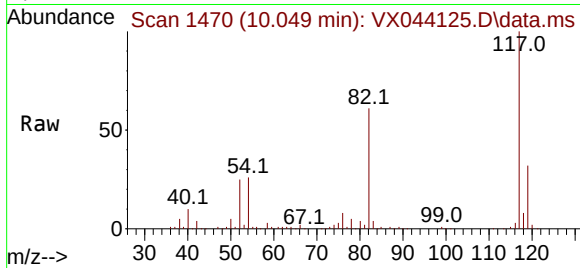

#67
Ethyl Benzene
Concen: 44.830 ug/l
RT: 10.189 min Scan# 1493
Delta R.T. -0.000 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25

Tgt Ion: 91 Resp: 312956
Ion Ratio Lower Upper
91 100
106 29.1 23.6 35.4




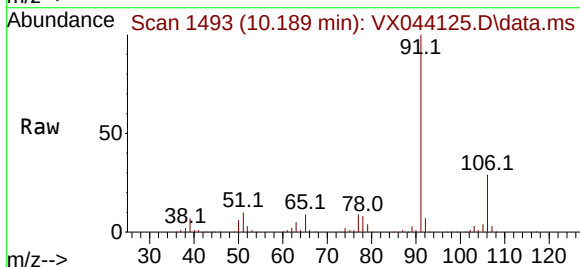




#68
m/p-Xylenes
Concen: 8.944 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 23284
Ion Ratio Lower Upper
106 100
91 206.3 168.1 252.1



#69
o-Xylene
Concen: 10.526 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.000 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25

Tgt Ion:106 Resp: 26756
Ion Ratio Lower Upper
106 100
91 224.2 110.2 330.6





#70

Styrene

Concen: 0.417 ug/l

RT: 10.646 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX044125.D





Acq: 04 Dec 2024 18:25

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion:104	Resp:	1754
Ion Ratio	Lower	Upper
104	100	
78	269.0	42.2 63.2#
103	209.2	44.7 67.1#

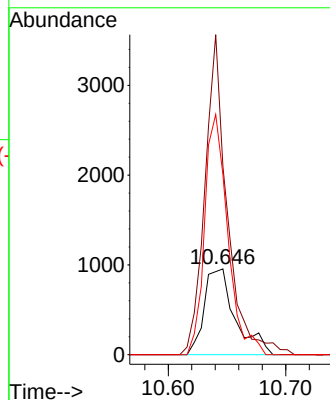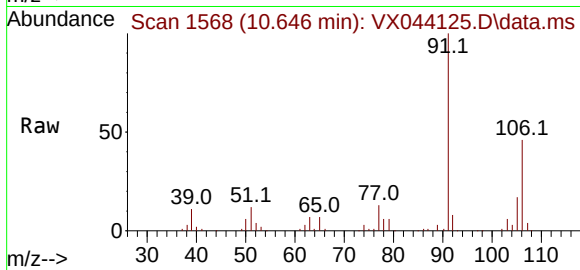

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l




RT: 12.018 min Scan# 1793


Delta R.T. -0.006 min

Lab File: VX044125.D

Acq: 04 Dec 2024 18:25

Tgt Ion:152	Resp:	86376
Ion Ratio	Lower	Upper
152	100	
115	64.5	45.4 136.2
150	158.3	0.0 353.0

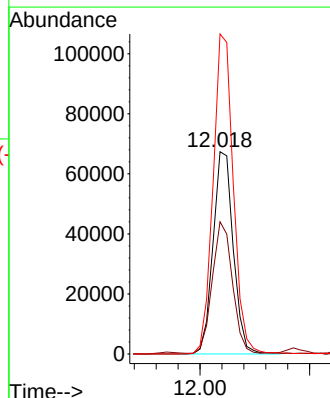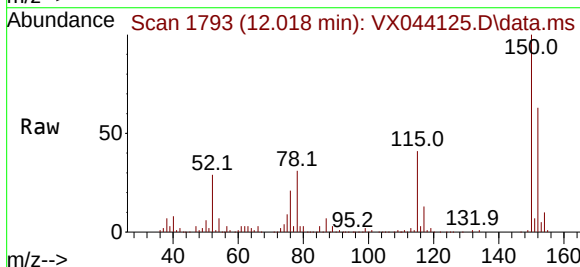



#73

Isopropylbenzene

Concen: 4.284 ug/l

RT: 10.964 min Scan# 1620

Delta R.T. 0.006 min

Lab File: VX044125.D

Acq: 04 Dec 2024 18:25

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 28446

Ion Ratio Lower Upper

105 100

120 24.9 13.0 38.9

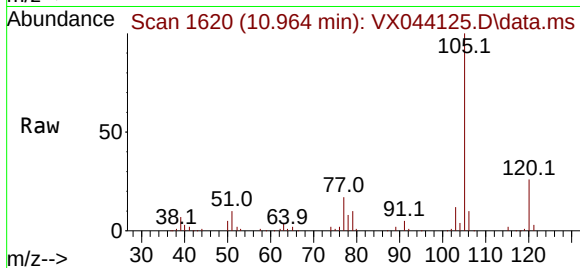

#76

1,2,3-Trichloropropane

Concen: 27.992 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX044125.D




Acq: 04 Dec 2024 18:25


Tgt Ion: 75 Resp: 53022

Ion Ratio Lower Upper

75 100

77 1.2 21.8 65.3#

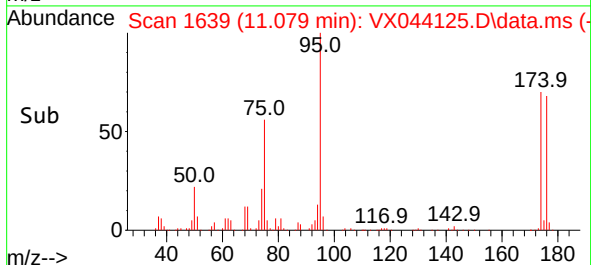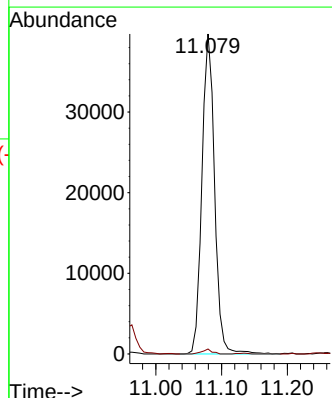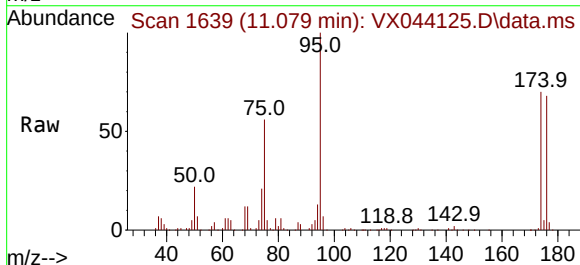



#78

n-propylbenzene

Concen: 1.946 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.006 min

Lab File: VX044125.D

Acq: 04 Dec 2024 18:25

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 14431

Ion Ratio Lower Upper

91 100

120 23.7 11.5 34.4

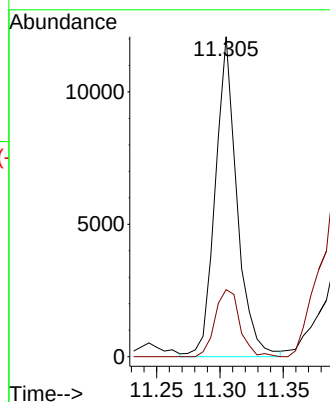

#79

2-Chlorotoluene

Concen: 1.582 ug/l

RT: 11.396 min Scan# 1691

Delta R.T. 0.037 min

Lab File: VX044125.D




Acq: 04 Dec 2024 18:25


Tgt Ion: 91 Resp: 7419

Ion Ratio Lower Upper

91 100

126 1.3 16.6 49.8#

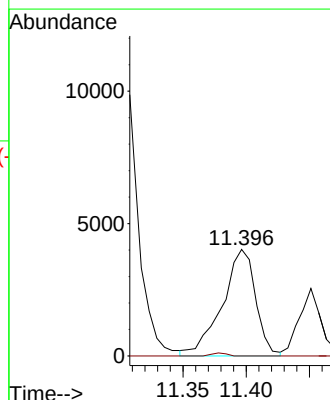



#80

1,3,5-Trimethylbenzene

Concen: 4.676 ug/l

RT: 11.451 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX044125.D

Acq: 04 Dec 2024 18:25

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 25543

Ion Ratio Lower Upper

105 100

120 47.0 23.3 69.8

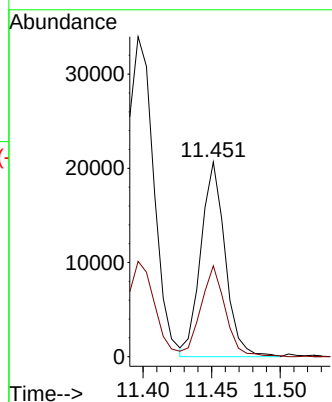

#81

trans-1,4-Dichloro-2-butene

Concen: 76.382 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX044125.D

Acq: 04 Dec 2024 18:25




Tgt Ion: 75 Resp: 53022


Ion Ratio Lower Upper

75 100

53 0.0 86.7 130.1#

89 0.0 38.2 57.2#




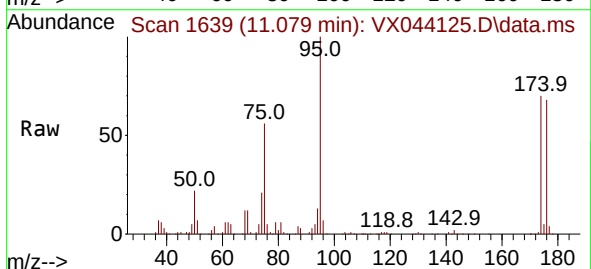




#82
4-Chlorotoluene
Concen: 0.601 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 3181
Ion Ratio Lower Upper
91 100
126 0.0 14.3 42.9#

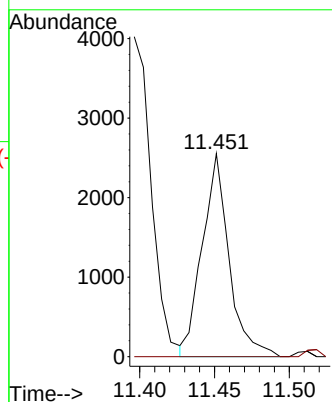

#83
tert-Butylbenzene
Concen: 1.282 ug/l
RT: 11.969 min Scan# 1785
Delta R.T. 0.256 min
Lab File: VX044125.D
Acq: 04 Dec 2024 18:25

Tgt Ion: 119 Resp: 6939
Ion Ratio Lower Upper
119 100
91 31.2 31.0 93.0
134 25.6 11.6 34.8

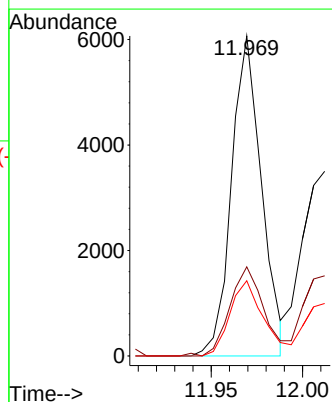



#84

1,2,4-Trimethylbenzene

Concen: 17.636 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX044125.D

Acq: 04 Dec 2024 18:25

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 95911

Ion Ratio Lower Upper

105 100

120 42.6 21.9 65.7

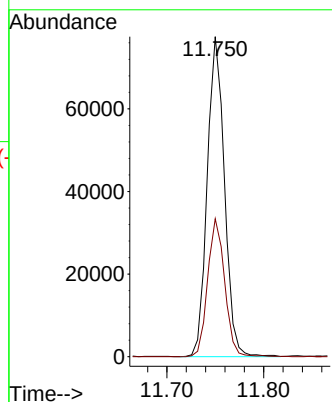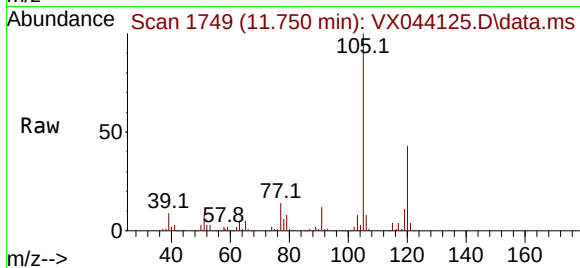

#85

sec-Butylbenzene

Concen: 14.458 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.140 min

Lab File: VX044125.D




Acq: 04 Dec 2024 18:25


Tgt Ion:105 Resp: 95911

Ion Ratio Lower Upper

105 100

134 0.0 9.7 29.1#

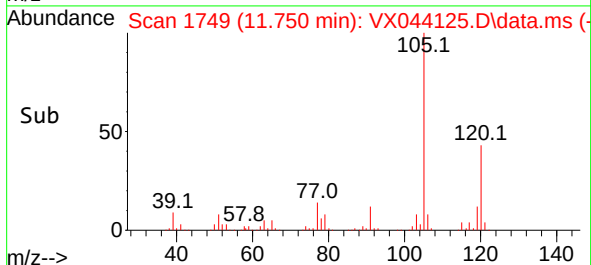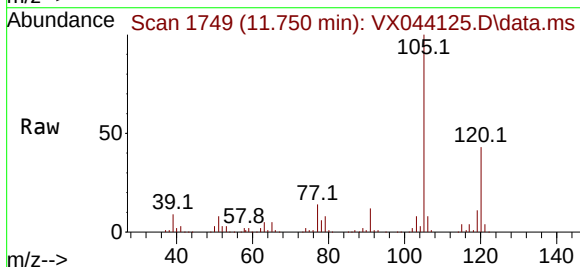



#86

p-Isopropyltoluene

Concen: 0.839 ug/l

RT: 12.012 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX044125.D

Acq: 04 Dec 2024 18:25

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:119 Resp: 4521

Ion Ratio Lower Upper

119 100

134 29.0 13.0 38.9

91 0.0 13.0 38.9#

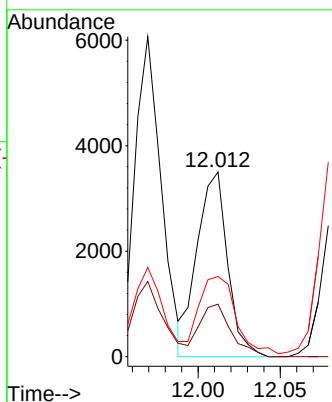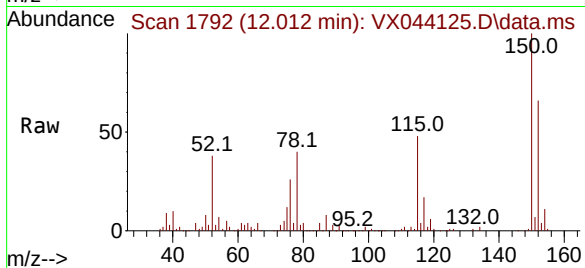

#89

n-Butylbenzene

Concen: 1.146 ug/l

RT: 12.317 min Scan# 1842

Delta R.T. -0.012 min

Lab File: VX044125.D

Acq: 04 Dec 2024 18:25




Tgt Ion: 91 Resp: 5444


Ion Ratio Lower Upper

91 100

92 20.9 26.6 79.8#

134 127.8 12.4 37.2#

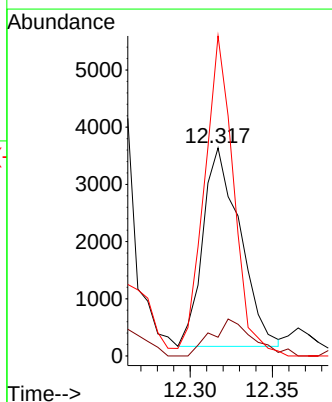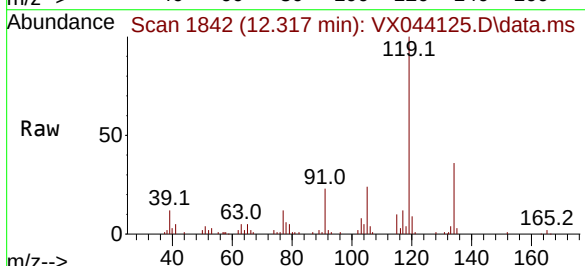



#90

Hexachloroethane

Concen: 50.711 ug/l

RT: 12.695 min Scan# 1904

Delta R.T. 0.158 min

Lab File: VX044125.D

Acq: 04 Dec 2024 18:25

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:117 Resp: 46465

Ion Ratio Lower Upper

117 100

201 0.0 32.4 97.0#

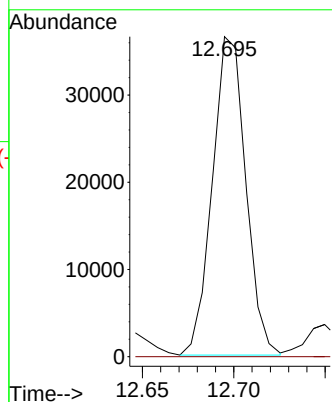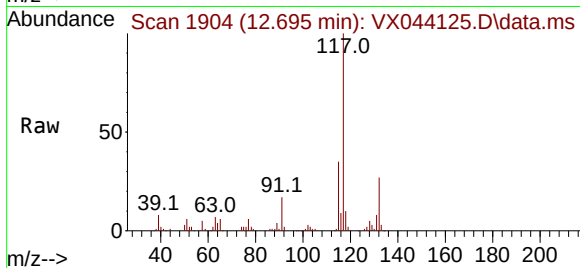

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.711 ug/l

RT: 12.963 min Scan# 1948

Delta R.T. 0.024 min

Lab File: VX044125.D

Acq: 04 Dec 2024 18:25




Tgt Ion: 75 Resp: 324


Ion Ratio Lower Upper

75 100

155 0.0 40.1 120.2#

157 0.0 49.6 149.0#

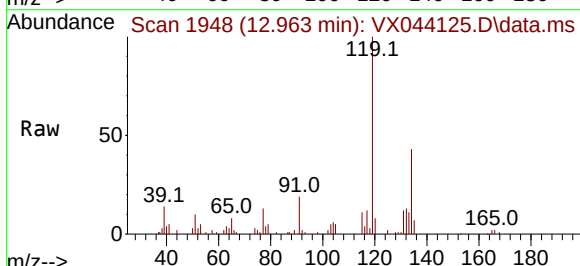



#95

Naphthalene

Concen: 758.719 ug/l

RT: 13.774 min Scan# 20

Delta R.T. -0.000 min


Lab File: VX044125.D

Acq: 04 Dec 2024 18:25

Instrument :

MSVOA_X

ClientSampleId :

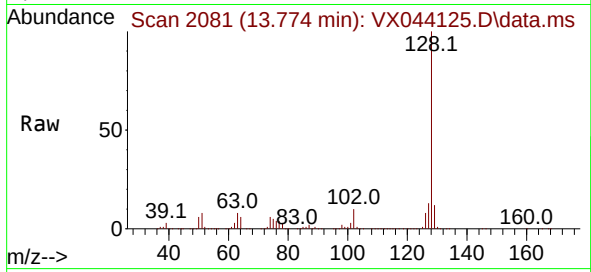

Tgt Ion:128 Resp: 4687643

Ion	Ratio	Lower	Upper
128	100		
127	13.3	10.2	15.2
129	11.4	8.6	12.8

