

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120424\
 Data File : VX044129.D
 Acq On : 04 Dec 2024 19:57
 Operator : JC/MD
 Sample : P5006-04RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 05 00:37:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 22 03:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	101936	50.000	ug/l	0.01
34) 1,4-Difluorobenzene	6.757	114	199845	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	169469	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	68386	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	91520	52.346	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 104.700%	
35) Dibromofluoromethane	5.385	113	49951	34.980	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 69.960%#	
50) Toluene-d8	8.647	98	245054	49.783	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 99.560%	
62) 4-Bromofluorobenzene	11.079	95	80566	48.092	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 96.180%	


Target Compounds					Qvalue	
4) Vinyl Chloride	1.368	62	497	0.344	ug/l #	40
11) Tert butyl alcohol	2.983	59	436	1.554	ug/l #	73
14) Allyl chloride	2.642	41	487	0.254	ug/l #	21
15) Acrylonitrile	3.075	53	207	0.303	ug/l #	47
16) Acetone	2.380	43	24857	30.955	ug/l	93
20) Methylene Chloride	2.788	84	939	0.689	ug/l #	70
25) 2-Butanone	4.593	43	4336	4.185	ug/l	98
27) cis-1,2-Dichloroethene	4.489	96	7330	4.890	ug/l	89
29) Tetrahydrofuran	5.026	42	338	0.532	ug/l #	86
31) Cyclohexane	5.544	56	3048	1.564	ug/l #	51
36) 1,1-Dichloropropene	5.544	75	10595	5.954	ug/l #	50
38) Carbon Tetrachloride	5.550	117	12283	6.143	ug/l #	16
40) Benzene	6.037	78	14623	2.638	ug/l	97
51) 4-Methyl-2-Pentanone	8.580	43	1103	0.514	ug/l #	79
52) Toluene	8.726	92	3847	1.160	ug/l	91
67) Ethyl Benzene	10.195	91	86422	13.703	ug/l	98
68) m/p-Xylenes	10.299	106	11205	4.764	ug/l	99
69) o-Xylene	10.640	106	8554	3.725	ug/l	99
73) Isopropylbenzene	10.963	105	8899	1.693	ug/l	96
76) 1,2,3-Trichloropropane	11.079	75	47552	31.708	ug/l #	34
78) n-propylbenzene	11.305	91	2805	0.478	ug/l	100
79) 2-Chlorotoluene	11.402	91	2336	0.629	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.451	105	7833	1.811	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.079	75	47552	86.523	ug/l #	6
82) 4-Chlorotoluene	11.451	91	1090	0.260	ug/l #	46
83) tert-Butylbenzene	11.750	119	3225	0.752	ug/l #	38
84) 1,2,4-Trimethylbenzene	11.750	105	30130	6.998	ug/l	94
85) sec-Butylbenzene	11.750	105	30130	5.737	ug/l #	57
86) p-Isopropyltoluene	12.012	119	1222	0.286	ug/l #	68
89) n-Butylbenzene	12.317	91	2135	0.568	ug/l #	12
90) Hexachloroethane	12.695	117	12273	16.918	ug/l #	18
95) Naphthalene	13.774	128	1759335	359.667	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120424\
Data File : VX044129.D
Acq On : 04 Dec 2024 19:57
Operator : JC/MD
Sample : P5006-04RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Dec 05 00:37:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 22 03:45:52 2024
Response via : Initial Calibration

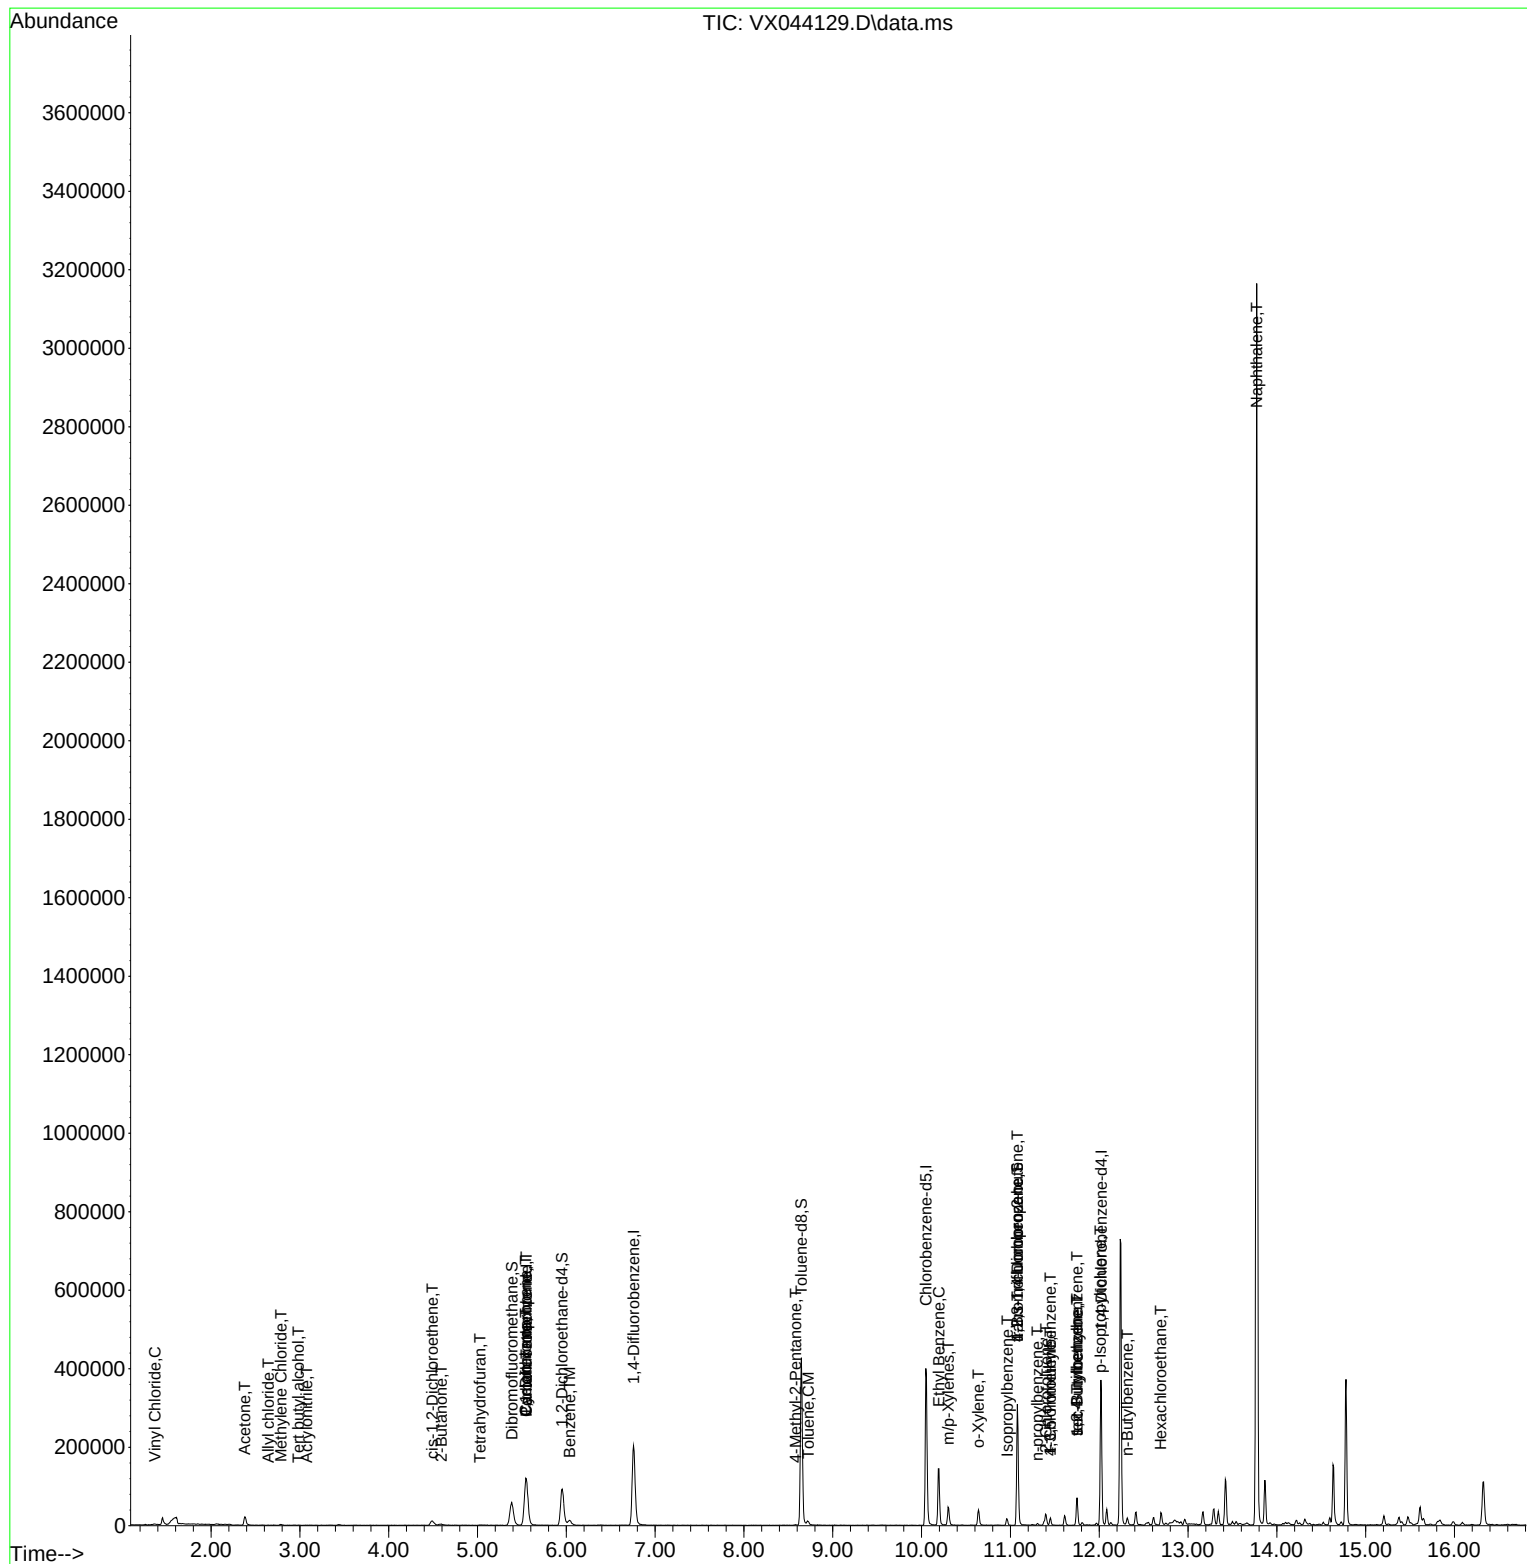



#1
Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.550 min Scan# 71

Delta R.T. 0.012 min


Lab File: VX044129.D

Acq: 04 Dec 2024 19:57

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion:168 Resp: 101936

Ion Ratio Lower Upper

168 100

99 68.1 51.8 77.8

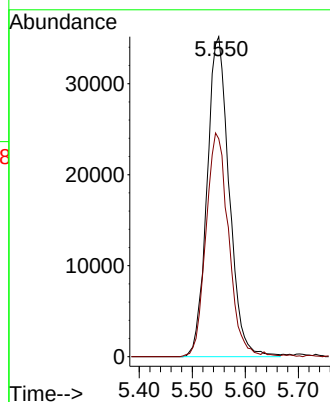

#4

Vinyl Chloride

Concen: 0.344 ug/l

RT: 1.368 min Scan# 46

Delta R.T. -0.006 min

Lab File: VX044129.D




Acq: 04 Dec 2024 19:57


Tgt Ion: 62 Resp: 497

Ion Ratio Lower Upper

62 100

64 66.8 26.2 39.4#


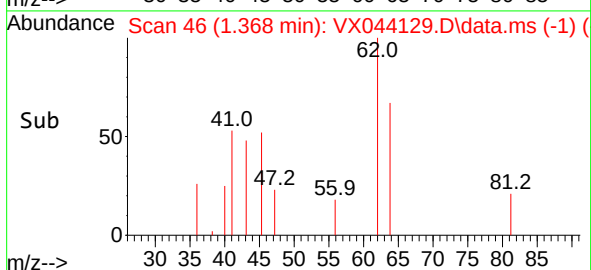
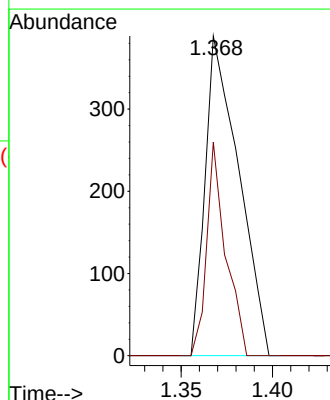



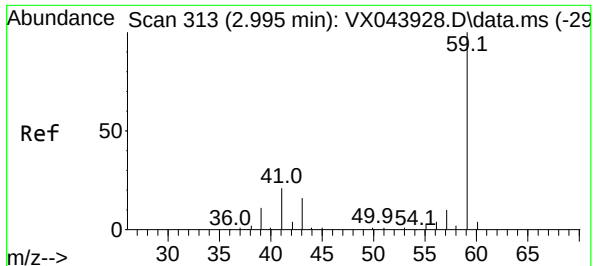

#11
Tert butyl alcohol
Concen: 1.554 ug/l
RT: 2.983 min Scan# 311
Delta R.T. -0.012 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 59 Resp: 436
Ion Ratio Lower Upper
59 100
57 0.0 7.9 11.9#

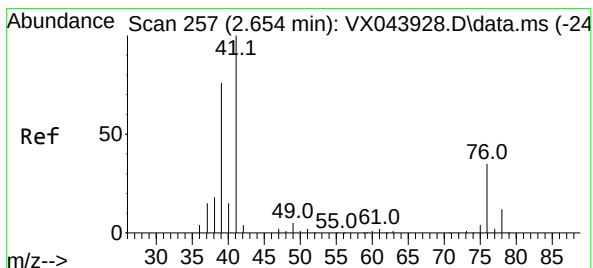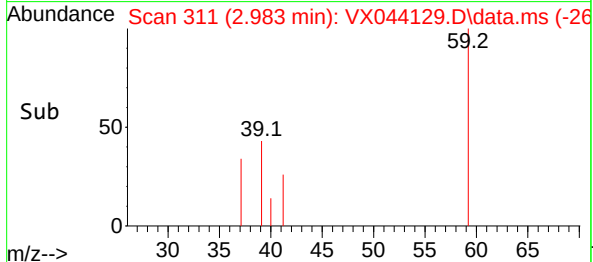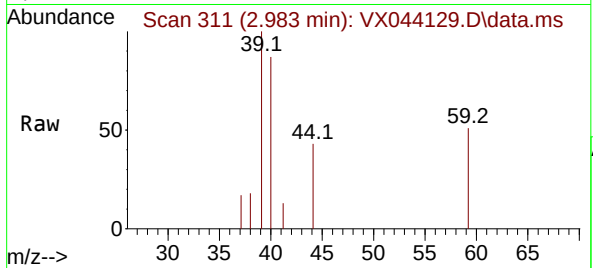

#14
Allyl chloride
Concen: 0.254 ug/l
RT: 2.642 min Scan# 255
Delta R.T. -0.012 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57

Tgt Ion: 41 Resp: 487
Ion Ratio Lower Upper
41 100
39 0.0 59.5 89.3#
76 0.0 27.4 41.2#

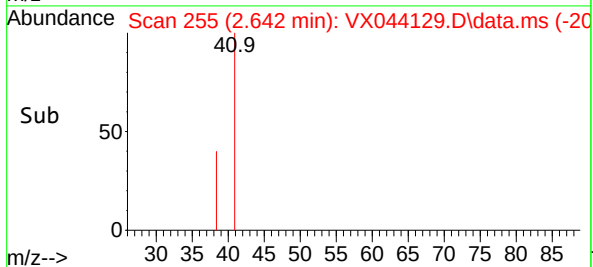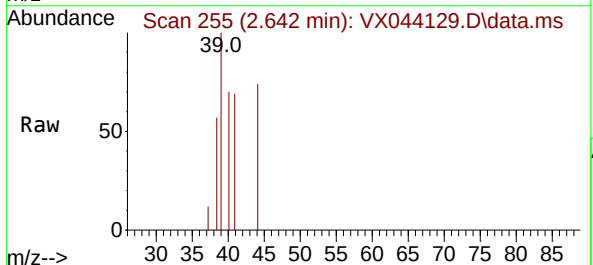



#15

Acrylonitrile

Concen: 0.303 ug/l

RT: 3.075 min Scan# 31

Delta R.T. 0.012 min


Lab File: VX044129.D

Acq: 04 Dec 2024 19:57




Instrument :

MSVOA_X

ClientSampleId :



Tgt Ion: 53	Resp: 207
Ion Ratio	Lower Upper
53 100	
52 30.0	66.5 99.7#
51 13.0	30.2 45.4#

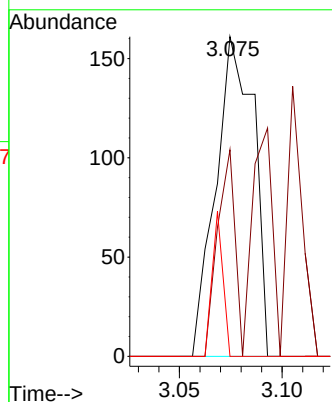

#16

Acetone

Concen: 30.955 ug/l




RT: 2.380 min Scan# 212


Delta R.T. -0.000 min

Lab File: VX044129.D

Acq: 04 Dec 2024 19:57


Tgt Ion: 43	Resp: 24857
Ion Ratio	Lower Upper
43 100	
58 24.8	22.7 34.1

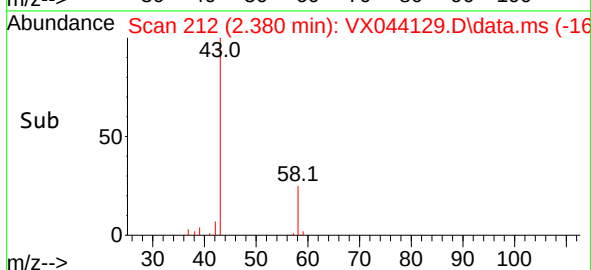






#20
Methylene Chloride
Concen: 0.689 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57

Instrument :
MSVOA_X
ClientSampleId :



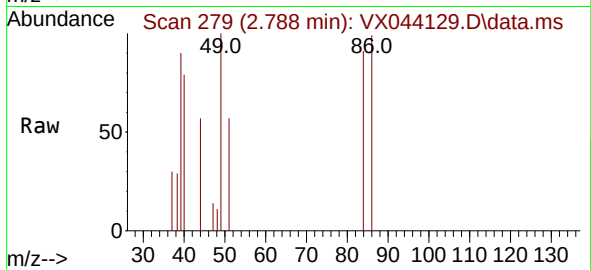



Tgt Ion:	84	Resp:	939
Ion	Ratio	Lower	Upper
84	100		
49	109.5	102.7	154.1
51	62.9	31.7	47.5#
86	108.2	53.9	80.9#

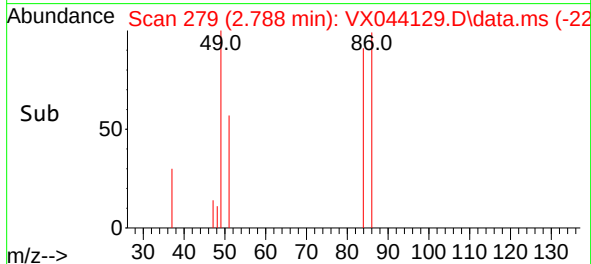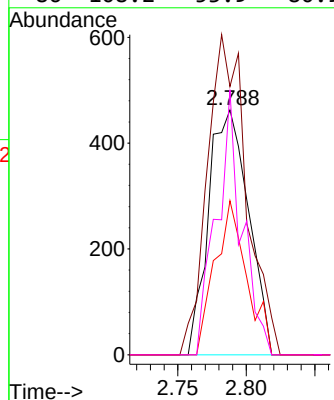

#25
2-Butanone
Concen: 4.185 ug/l
RT: 4.593 min Scan# 575
Delta R.T. 0.036 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57

Tgt Ion:	43	Resp:	4336
Ion	Ratio	Lower	Upper
43	100		
72	24.0	20.2	30.2

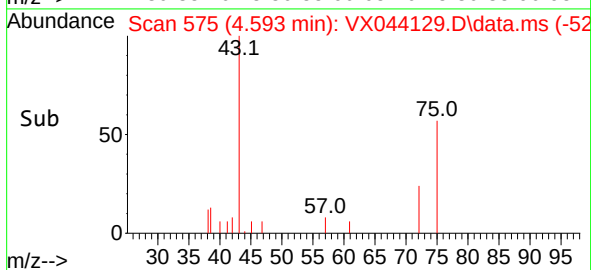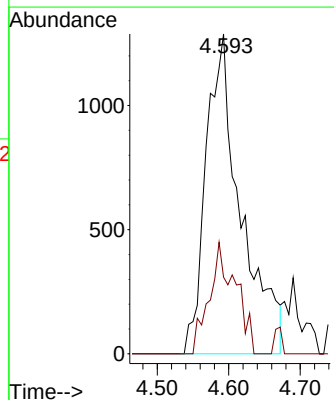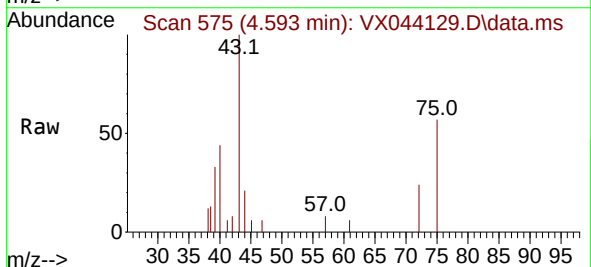



#27

cis-1,2-Dichloroethene

Concen: 4.890 ug/l

RT: 4.489 min Scan# 51

Delta R.T. 0.012 min


Lab File: VX044129.D

Acq: 04 Dec 2024 19:57

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion: 96 Resp: 7330

Ion Ratio Lower Upper

96 100

61 130.1 0.0 297.4

98 61.0 0.0 127.8

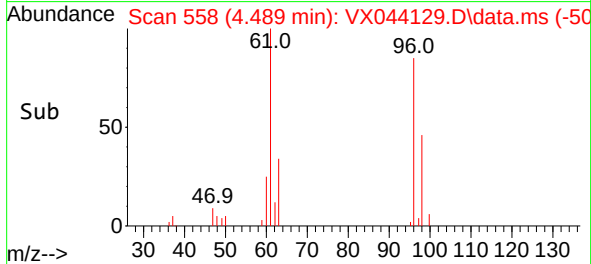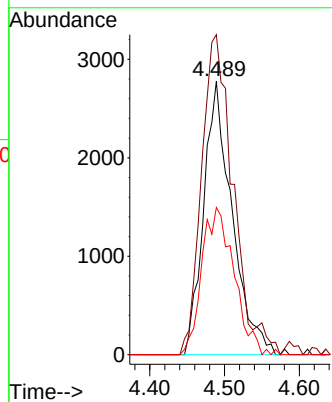

#29

Tetrahydrofuran

Concen: 0.532 ug/l

RT: 5.026 min Scan# 646

Delta R.T. 0.024 min

Lab File: VX044129.D

Acq: 04 Dec 2024 19:57




Tgt Ion: 42 Resp: 338


Ion Ratio Lower Upper

42 100

72 40.5 36.4 54.6


71 27.8 33.4 50.0#

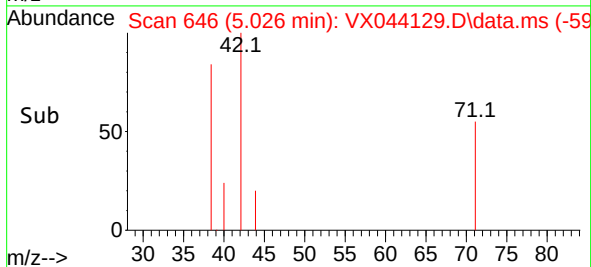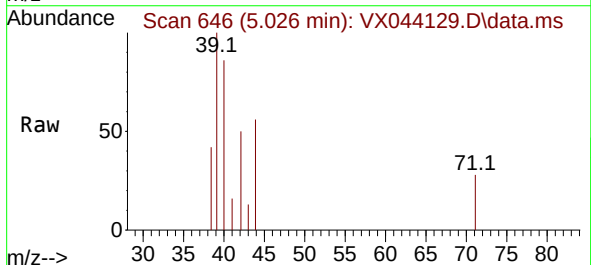






#31
Cyclohexane
Concen: 1.564 ug/l
RT: 5.544 min Scan# 717
Delta R.T. 0.085 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 56 Resp: 3048
Ion Ratio Lower Upper
56 100
69 106.5 24.7 37.1#
84 101.2 68.7 103.1

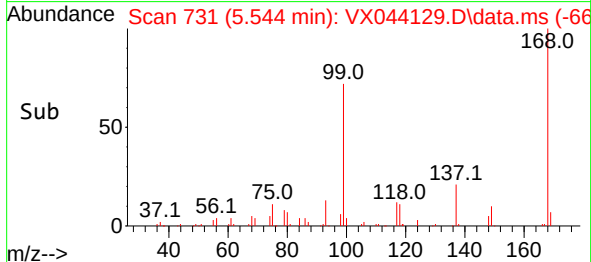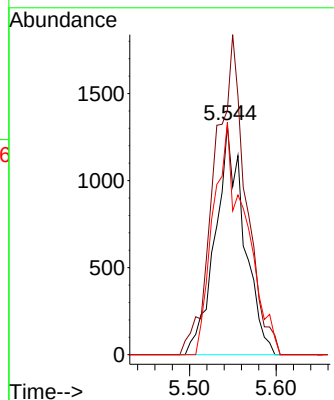

#33
1,2-Dichloroethane-d4
Concen: 52.346 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.006 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57


Tgt Ion: 65 Resp: 91520
Ion Ratio Lower Upper
65 100
67 49.8 0.0 100.8

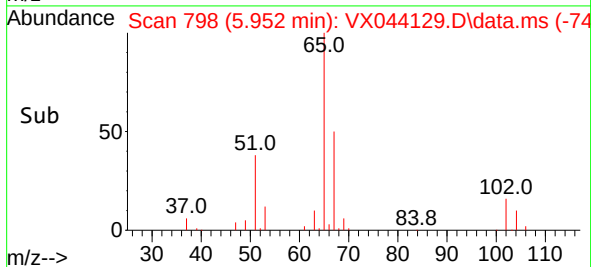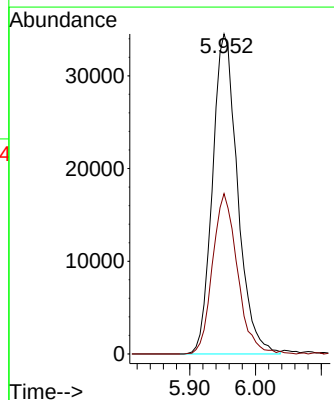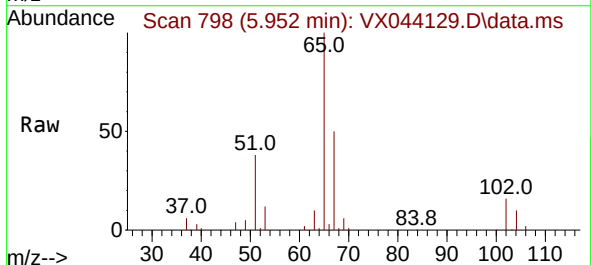






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion:114 Resp: 199845
Ion Ratio Lower Upper
114 100
63 21.1 0.0 44.0
88 16.1 0.0 32.4

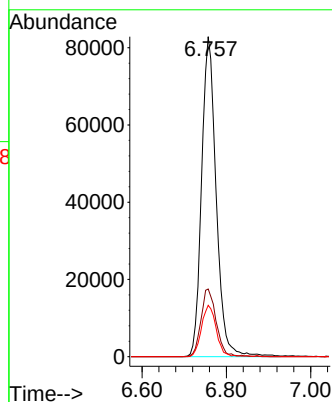


#35
Dibromofluoromethane
Concen: 34.980 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57



Tgt Ion:113 Resp: 49951
Ion Ratio Lower Upper
113 100
111 100.6 81.0 121.4
192 15.8 13.0 19.6

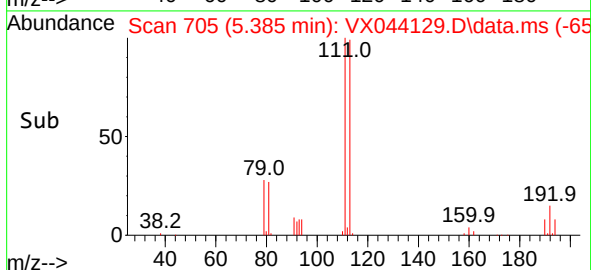



#36

1,1-Dichloropropene

Concen: 5.954 ug/l

RT: 5.544 min Scan# 71

Delta R.T. -0.134 min


Lab File: VX044129.D

Acq: 04 Dec 2024 19:57

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion: 75 Resp: 10595

Ion Ratio Lower Upper

75 100

110 10.2 17.4 52.2#

77 0.0 25.8 38.8#

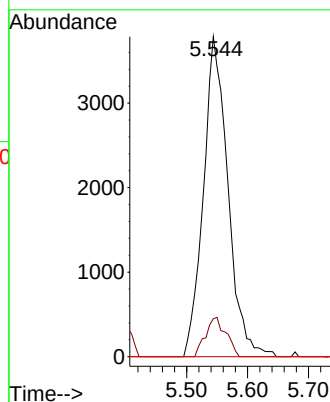

#38

Carbon Tetrachloride

Concen: 6.143 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.116 min

Lab File: VX044129.D

Acq: 04 Dec 2024 19:57




Tgt Ion: 117 Resp: 12283


Ion Ratio Lower Upper

117 100

119 4.3 75.2 112.8#

121 0.0 24.5 36.7#


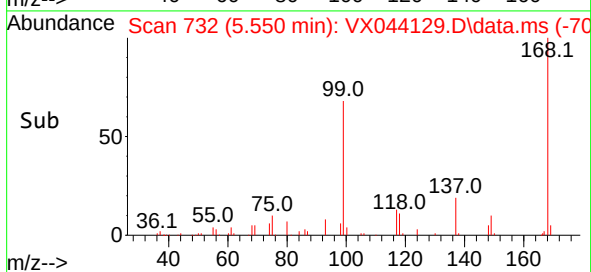
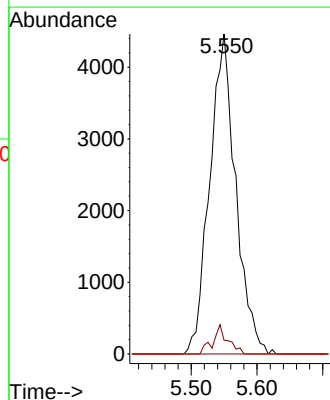



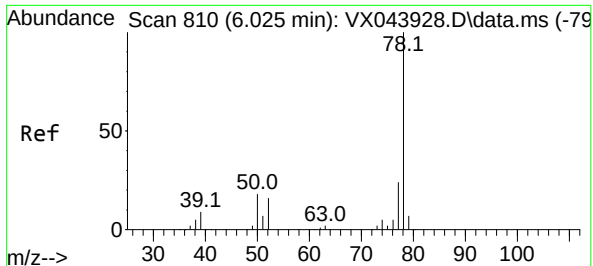

#40
Benzene
Concen: 2.638 ug/l
RT: 6.037 min Scan# 81
Delta R.T. 0.012 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 78 Resp: 14623
Ion Ratio Lower Upper
78 100
77 22.5 19.2 28.8

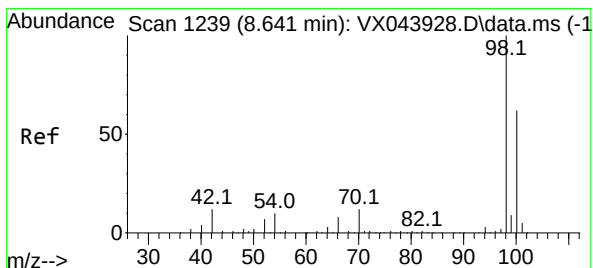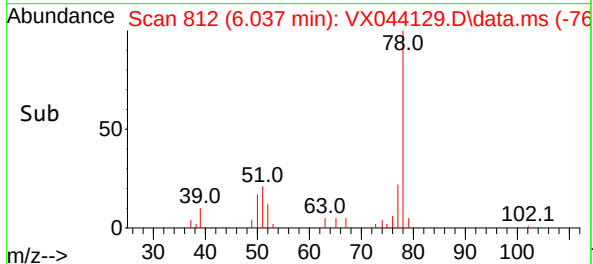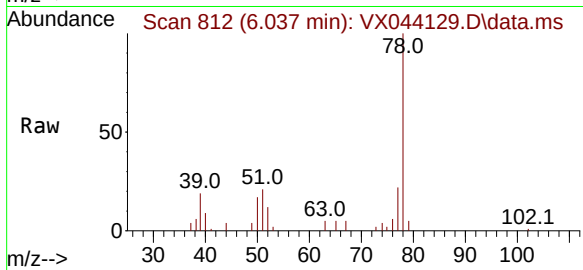

#50
Toluene-d8
Concen: 49.783 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.006 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57

Tgt Ion: 98 Resp: 245054
Ion Ratio Lower Upper
98 100
100 63.9 52.6 79.0


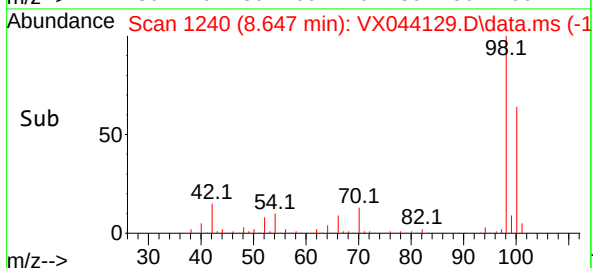

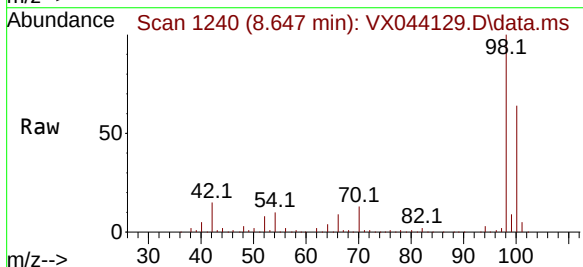




#51
4-Methyl-2-Pentanone
Concen: 0.514 ug/l
RT: 8.580 min Scan# 1103
Delta R.T. 0.006 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 1103
Ion Ratio Lower Upper
43 100
58 25.0 30.0 45.0#

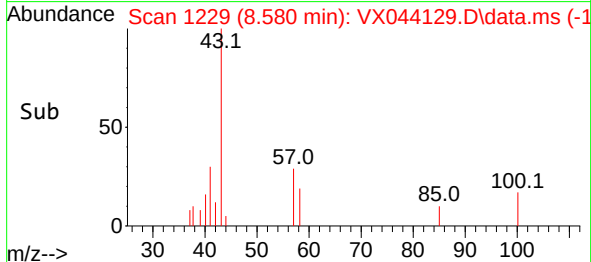

#52
Toluene
Concen: 1.160 ug/l
RT: 8.726 min Scan# 1253
Delta R.T. 0.012 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57

Tgt Ion: 92 Resp: 3847
Ion Ratio Lower Upper
92 100
91 161.8 139.7 209.5


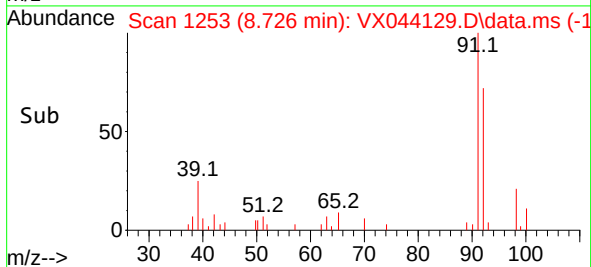

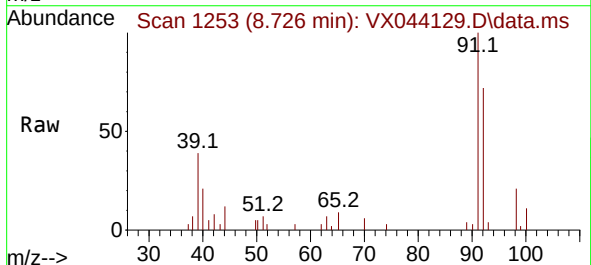




#62
4-Bromofluorobenzene
Concen: 48.092 ug/l
RT: 11.079 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 80566
Ion Ratio Lower Upper
95 100
174 68.4 0.0 150.4
176 66.4 0.0 146.0

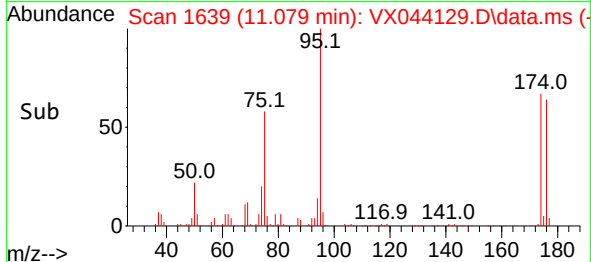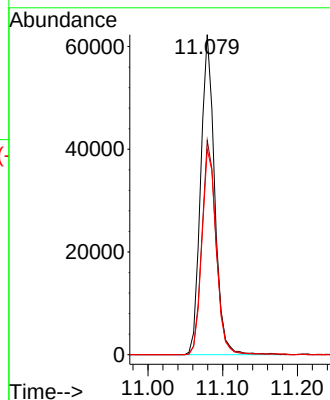

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. -0.000 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57

Tgt Ion: 117 Resp: 169469
Ion Ratio Lower Upper
117 100
82 62.0 46.4 69.6
119 32.6 24.6 37.0

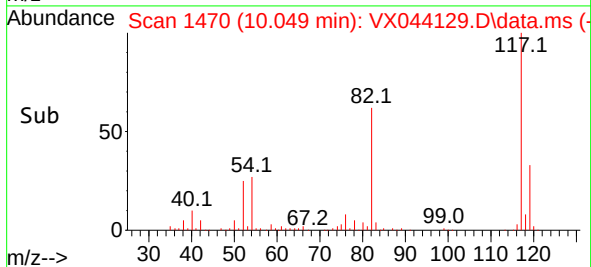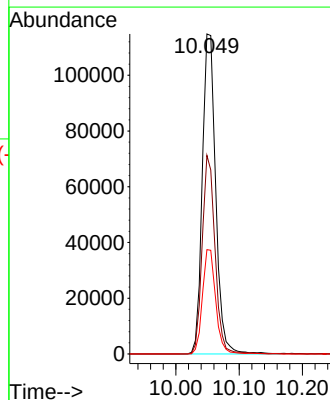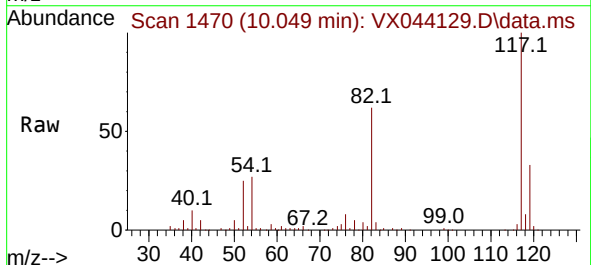



#67

Ethyl Benzene

Concen: 13.703 ug/l

RT: 10.195 min Scan# 1493

Delta R.T. 0.006 min

Lab File: VX044129.D

Acq: 04 Dec 2024 19:57

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 86422

Ion Ratio Lower Upper

91 100

106 28.4 23.6 35.4

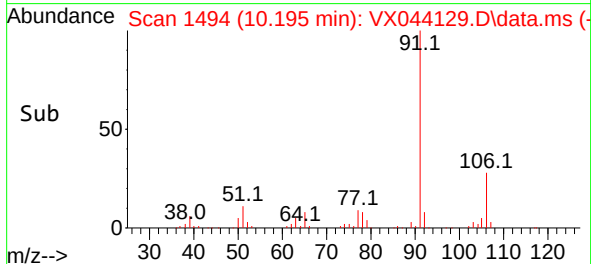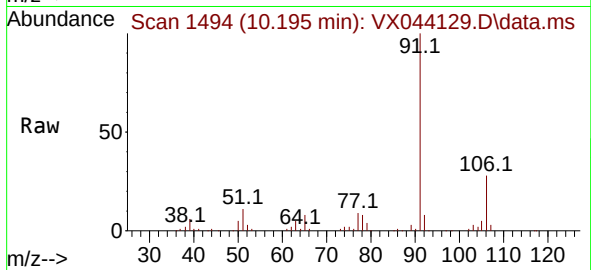

#68

m/p-Xylenes

Concen: 4.764 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. -0.000 min

Lab File: VX044129.D




Acq: 04 Dec 2024 19:57


Tgt Ion:106 Resp: 11205

Ion Ratio Lower Upper

106 100

91 211.5 168.1 252.1


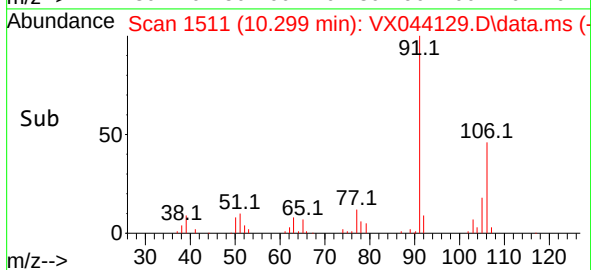

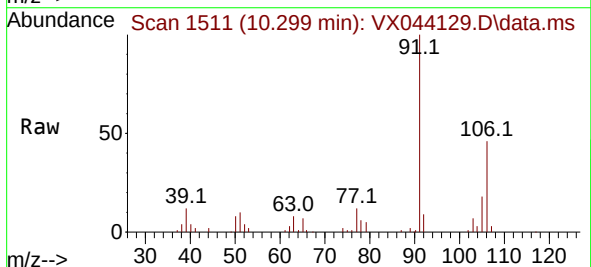




#69
o-Xylene
Concen: 3.725 ug/l
RT: 10.640 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 8554
Ion Ratio Lower Upper
106 100
91 222.6 110.2 330.6

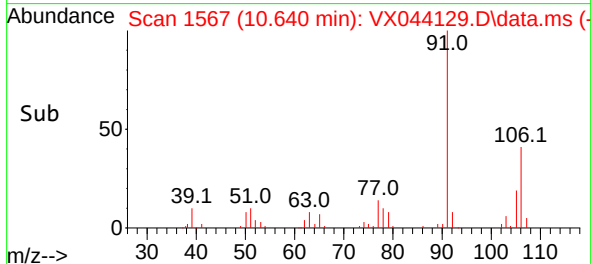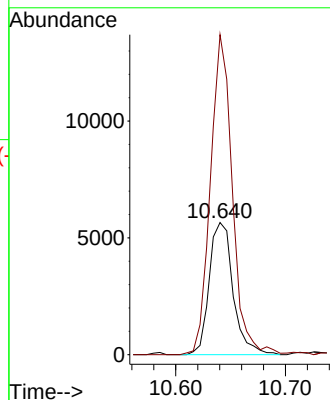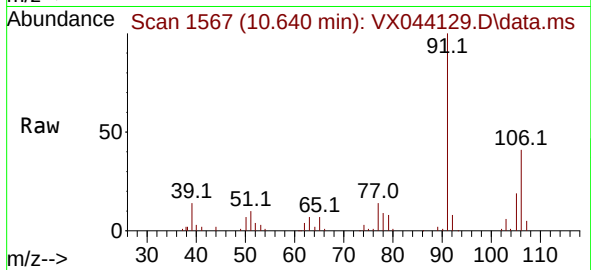

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57

Tgt Ion:152 Resp: 68386
Ion Ratio Lower Upper
152 100
115 65.6 45.4 136.2
150 160.9 0.0 353.0



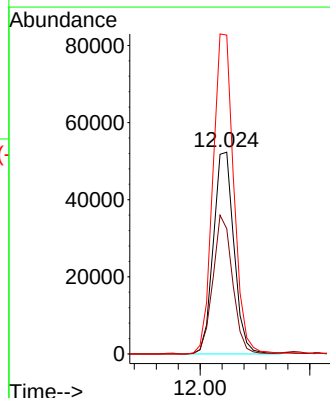
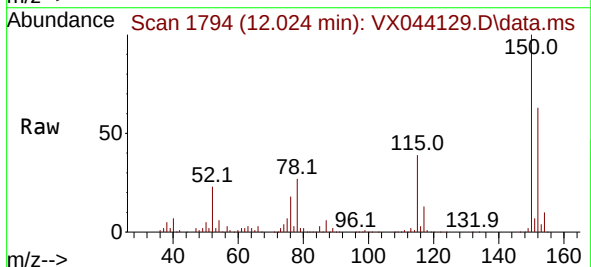




#73
Isopropylbenzene
Concen: 1.693 ug/l
RT: 10.963 min Scan# 1619
Delta R.T. 0.006 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 8899
Ion Ratio Lower Upper
105 100
120 23.7 13.0 38.9

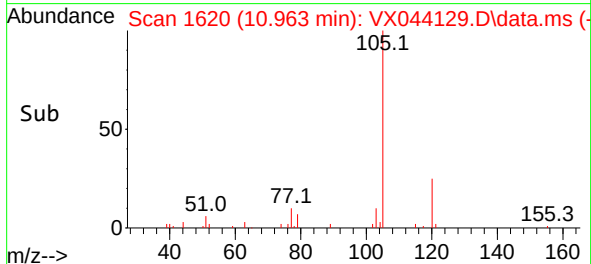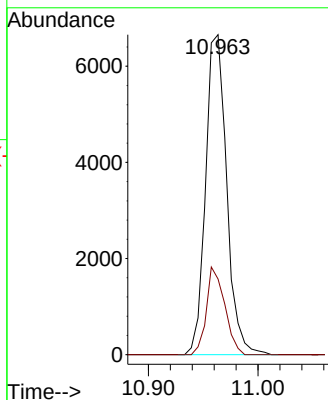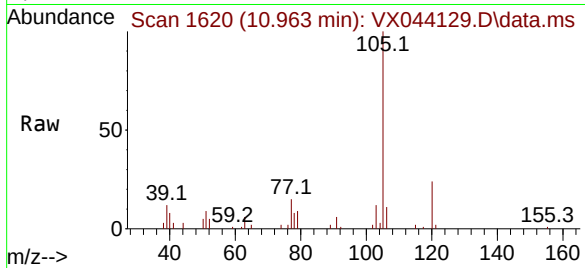

#76
1,2,3-Trichloropropane
Concen: 31.708 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57

Tgt Ion: 75 Resp: 47552
Ion Ratio Lower Upper
75 100
77 0.9 21.8 65.3#

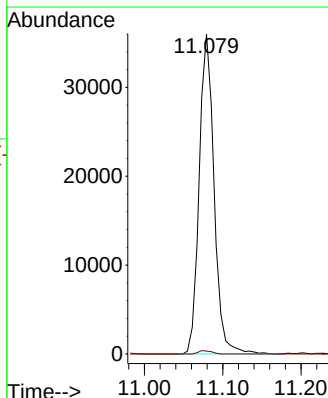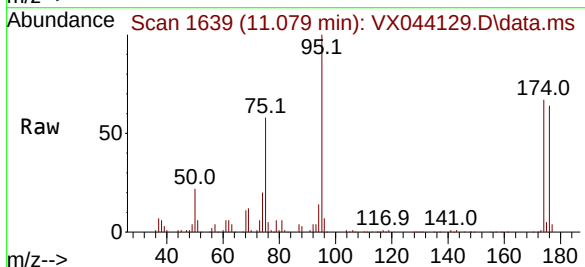



#78

n-propylbenzene

Concen: 0.478 ug/l

RT: 11.305 min Scan# 1675

Delta R.T. 0.006 min

Lab File: VX044129.D

Acq: 04 Dec 2024 19:57

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 2805

Ion Ratio Lower Upper

91 100

120 22.7 11.5 34.4

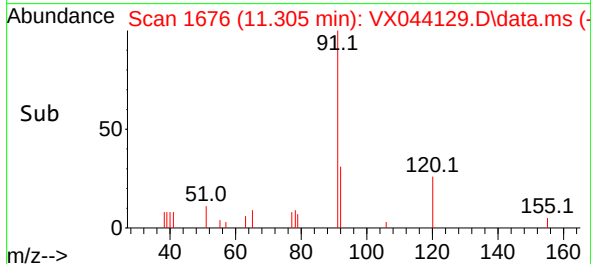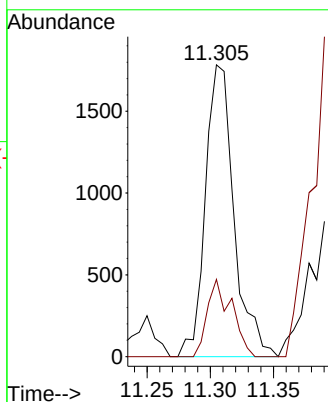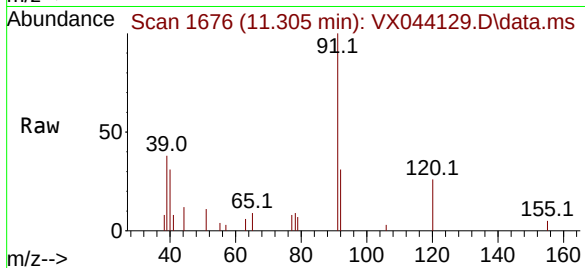

#79

2-Chlorotoluene

Concen: 0.629 ug/l

RT: 11.402 min Scan# 1692

Delta R.T. 0.043 min

Lab File: VX044129.D




Acq: 04 Dec 2024 19:57


Tgt Ion: 91 Resp: 2336

Ion Ratio Lower Upper

91 100

126 0.0 16.6 49.8#



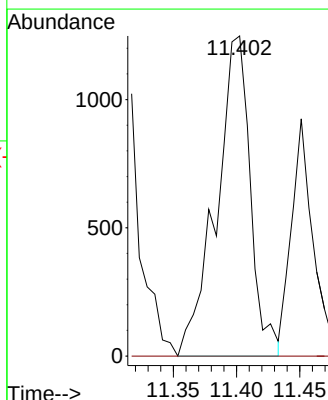
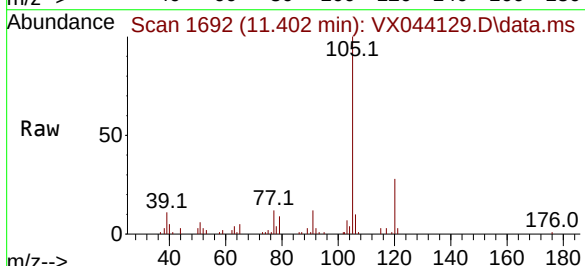




#80
1,3,5-Trimethylbenzene
Concen: 1.811 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 7833
Ion Ratio Lower Upper
105 100
120 45.8 23.3 69.8

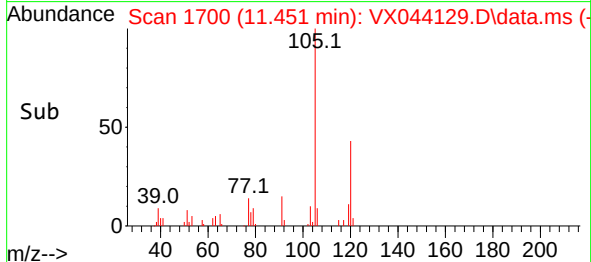

#81
trans-1,4-Dichloro-2-butene
Concen: 86.523 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57

Tgt Ion: 75 Resp: 47552
Ion Ratio Lower Upper
75 100
53 0.0 86.7 130.1#
89 0.0 38.2 57.2#


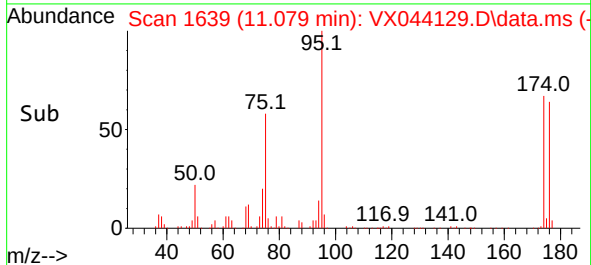

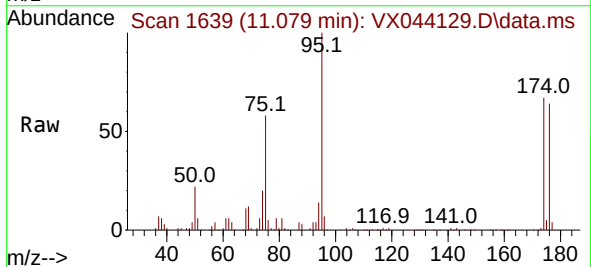




#82
4-Chlorotoluene
Concen: 0.260 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 1090
Ion Ratio Lower Upper
91 100
126 0.0 14.3 42.9#

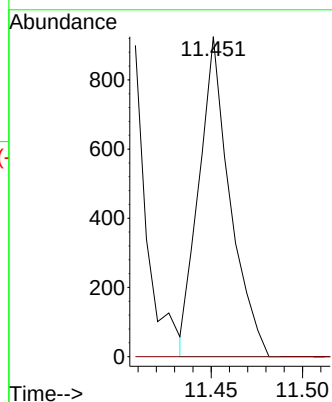

#83
tert-Butylbenzene
Concen: 0.752 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. 0.036 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57

Tgt Ion: 119 Resp: 3225
Ion Ratio Lower Upper
119 100
91 114.1 31.0 93.0#
134 0.0 11.6 34.8#

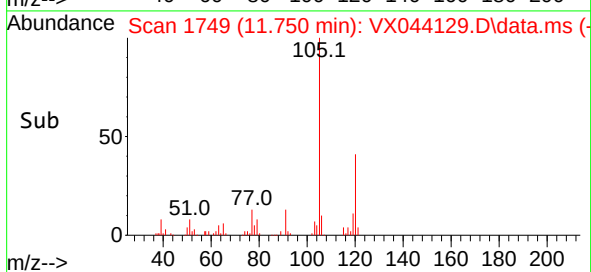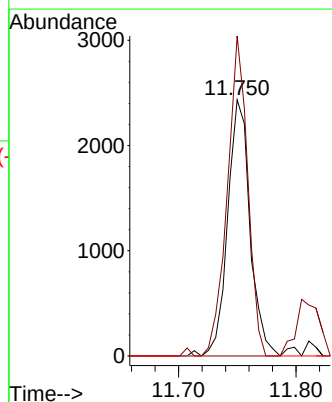



#84

1,2,4-Trimethylbenzene

Concen: 6.998 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX044129.D

Acq: 04 Dec 2024 19:57

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 30130

Ion Ratio Lower Upper

105 100

120 40.1 21.9 65.7

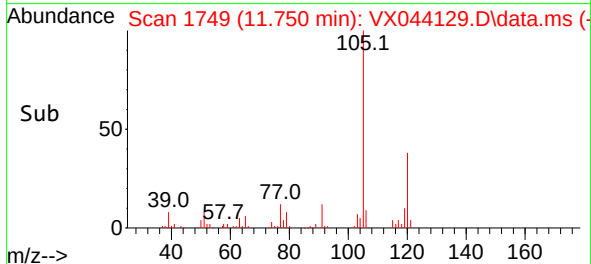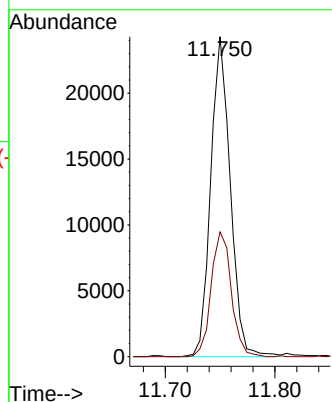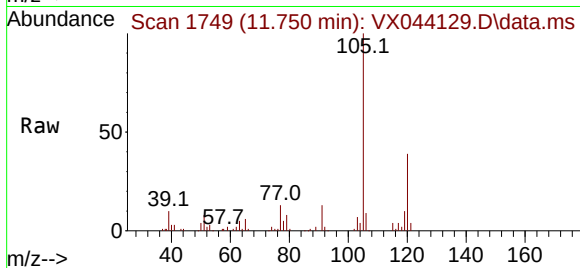

#85

sec-Butylbenzene

Concen: 5.737 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.140 min

Lab File: VX044129.D




Acq: 04 Dec 2024 19:57


Tgt Ion:105 Resp: 30130

Ion Ratio Lower Upper

105 100

134 0.0 9.7 29.1#




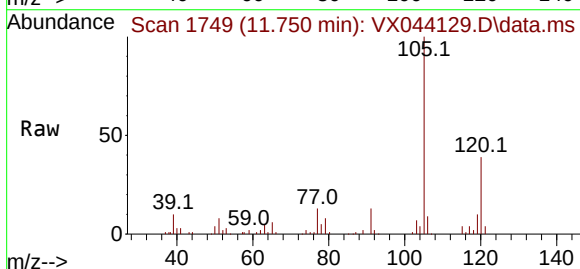




#86
p-Isopropyltoluene
Concen: 0.286 ug/l
RT: 12.012 min Scan# 1791
Delta R.T. 0.006 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:119 Resp: 1222
Ion Ratio Lower Upper
119 100
134 32.9 13.0 38.9
91 0.0 13.0 38.9#

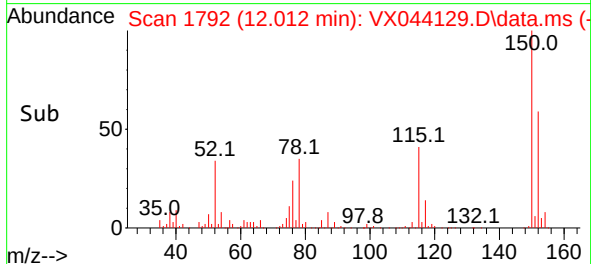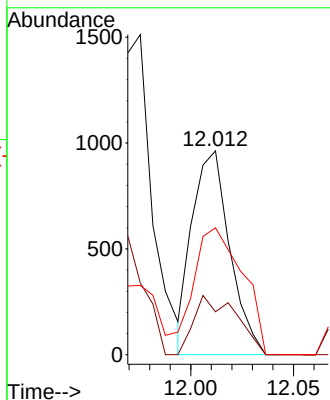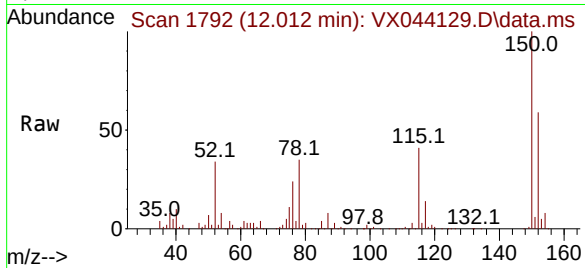

#89
n-Butylbenzene
Concen: 0.568 ug/l
RT: 12.317 min Scan# 1842
Delta R.T. -0.012 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57

Tgt Ion: 91 Resp: 2135
Ion Ratio Lower Upper
91 100
92 19.3 26.6 79.8#
134 111.6 12.4 37.2#


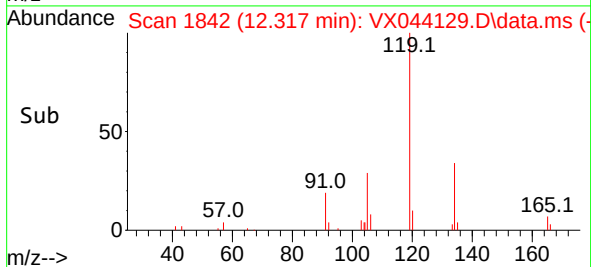
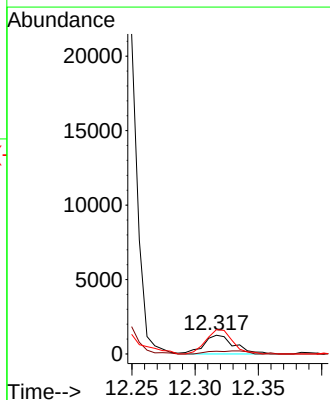
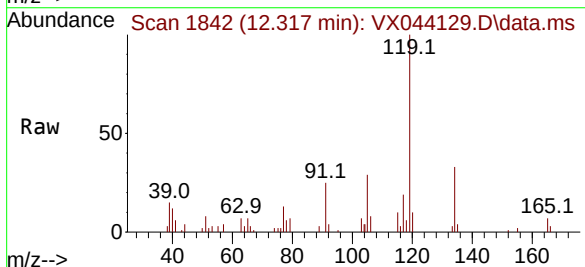




#90
Hexachloroethane
Concen: 16.918 ug/l
RT: 12.695 min Scan# 1904
Delta R.T. 0.158 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion:117 Resp: 12273
Ion Ratio Lower Upper
117 100
201 0.0 32.4 97.0#

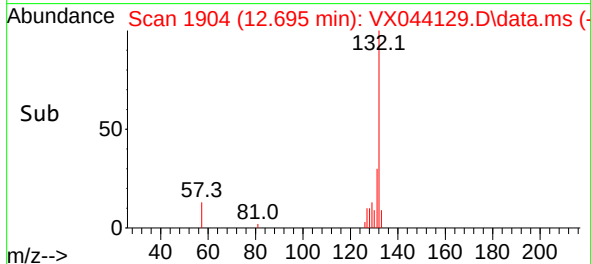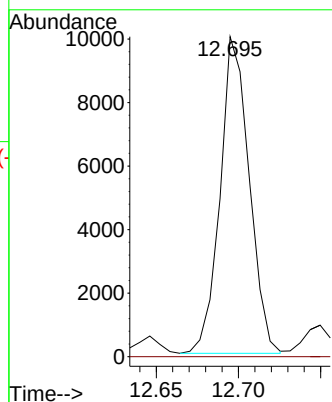

#95
Naphthalene
Concen: 359.667 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX044129.D
Acq: 04 Dec 2024 19:57

Tgt Ion:128 Resp: 1759335
Ion Ratio Lower Upper
128 100
127 13.1 10.2 15.2
129 11.0 8.6 12.8

