


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX120518\
 Data File : VX006289.D
 Acq On : 05 Dec 2018 09:48
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
 Title : SW846 8260
 Last Update : Fri Nov 30 03:55:33 2018

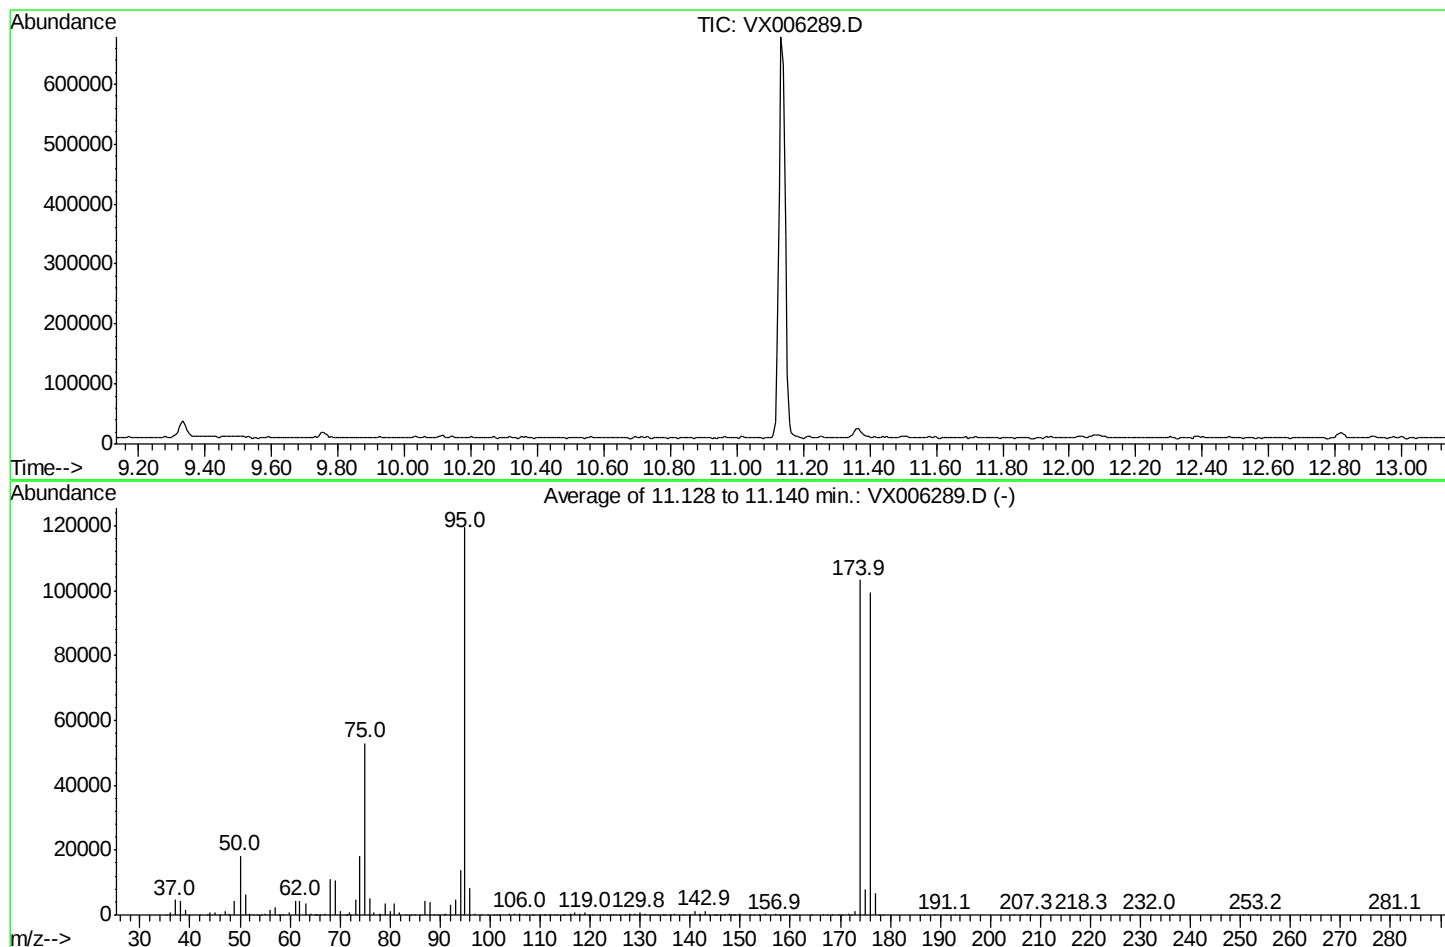

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	18273	PASS
75	95	30	60	44.4	53016	PASS
95	95	100	100	100.0	119498	PASS
96	95	5	9	7.0	8362	PASS
173	174	0.00	2	1.1	1131	PASS
174	95	50	100	86.5	103333	PASS
175	174	5	9	7.7	7911	PASS
176	174	95	101	96.1	99325	PASS
177	176	5	9	6.8	6740	PASS