

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX120519\
 Data File : VX013767.D
 Acq On : 05 Dec 2019 11:10
 Operator : JC/SP
 Sample : VX1205WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1205WBL01

Quant Time: Dec 06 02:40:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\624X111119W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Tue Nov 12 01:16:13 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.00	128	111777	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	6.85	114	631890	30.00	ug/l	0.00
57) Chlorobenzene-d5	10.10	117	536206	30.00	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	6.05	65	242370	29.36	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	97.87%
60) 4-Bromofluorobenzene	11.13	95	239280	27.76	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	92.53%
63) Toluene-d8	8.71	98	730198	30.11	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	100.37%


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX120519\
Data File : VX013767.D
Acq On : 05 Dec 2019 11:10
Operator : JC/SP
Sample : VX1205WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1205WBL01

Quant Time: Dec 06 02:40:28 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X111119W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Tue Nov 12 01:16:13 2019
Response via : Initial Calibration

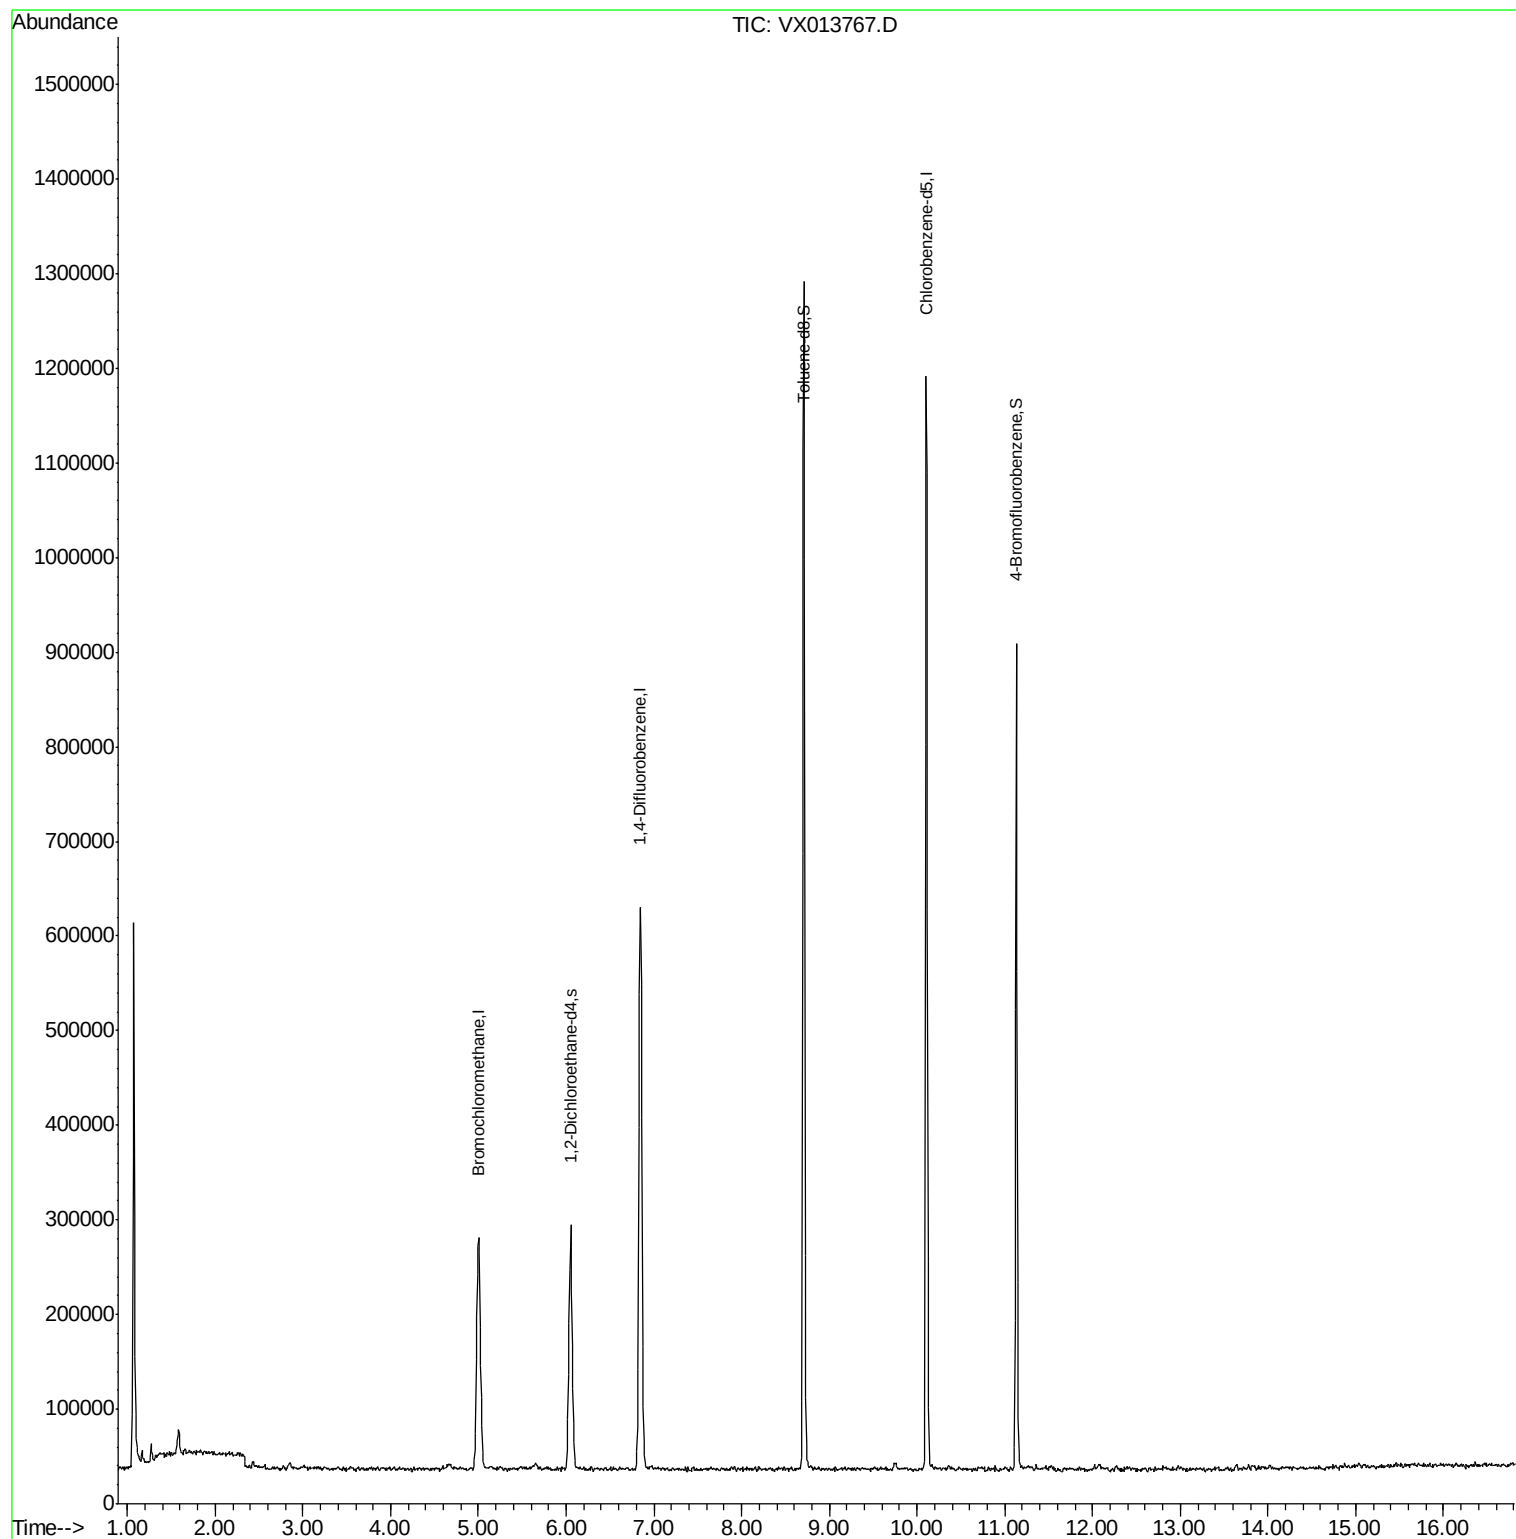

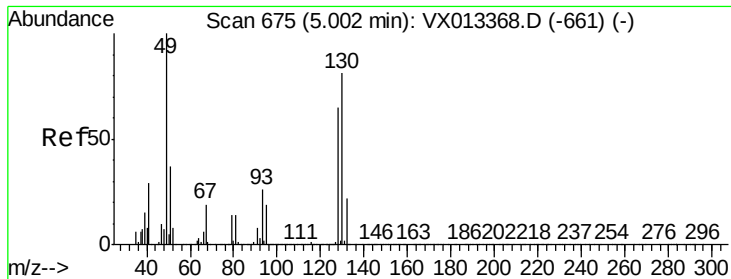

#1

Bromochloromethane

Concen: 30.000 ug/l

RT: 5.00 min Scan# 674

Delta R.T. -0.01 min

Lab File: VX013767.D

Acq: 05 Dec 2019 11:10

Instrument :

MSVOA_X

ClientSampleId :

VX1205WBL01


Tot Ion:128 Resp: 111777

Ion Ratio Lower Upper

128 100

49 156.0 0.0 388.3




130 129.6 0.0 318.5

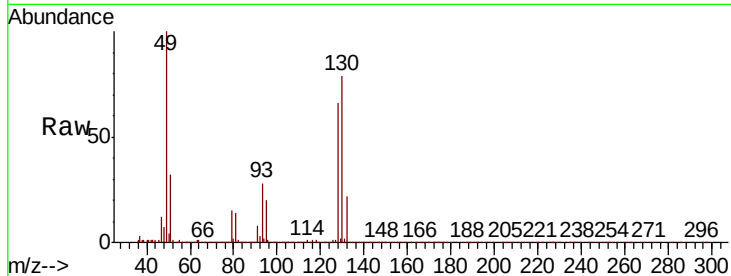

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VX0

Ion 130.00 (129.70 to 130.70): V

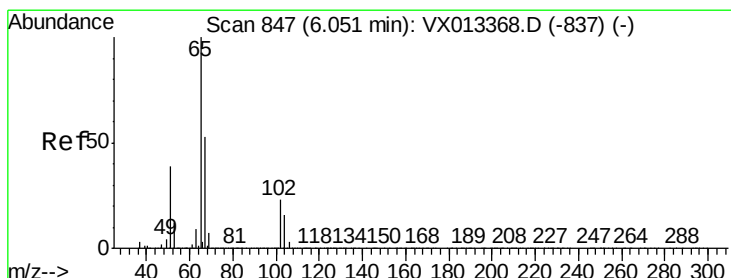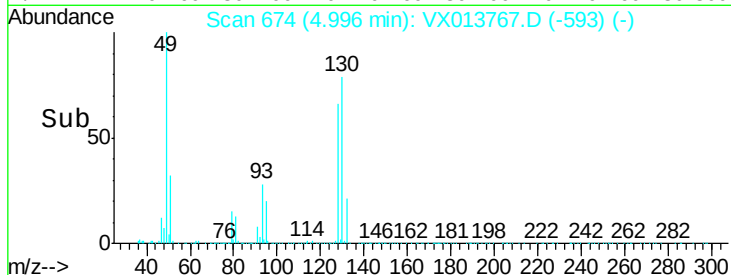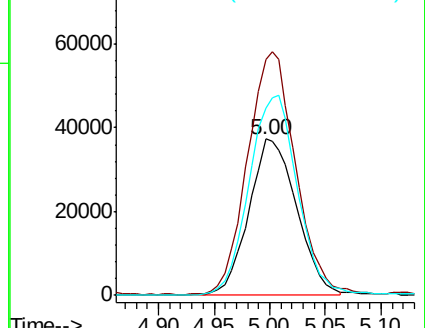

#27

1,2-Dichloroethane-d4

Concen: 29.365 ug/l

RT: 6.05 min Scan# 847

Delta R.T. 0.00 min

Lab File: VX013767.D


Acq: 05 Dec 2019 11:10

Tgt Ion: 65 Resp: 242370

Ion Ratio Lower Upper



65 100


67 51.4 41.0 61.6

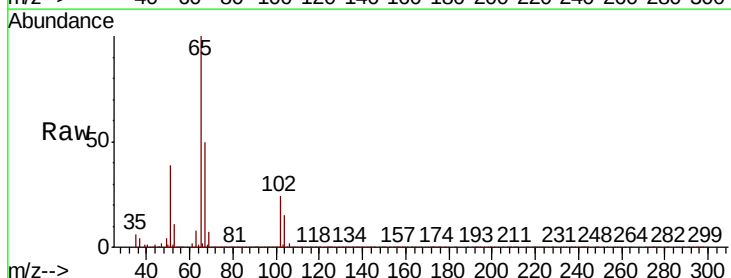

Abundance Ion 65.00 (64.70 to 65.70): VX0

Ion 67.00 (66.70 to 67.70): VX0



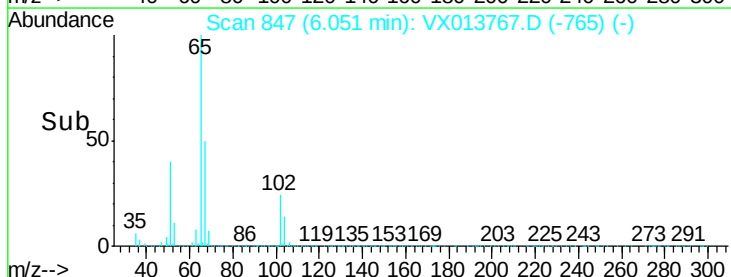
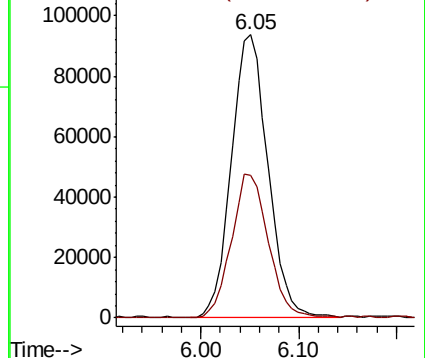


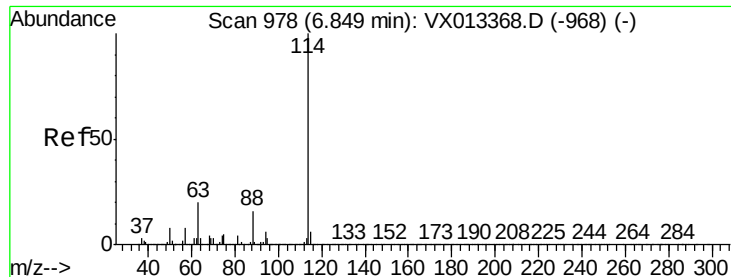

#28
 1,4-Difluorobenzene
 Concen: 30.000 ug/l
 RT: 6.85 min Scan# 978
 Delta R.T. 0.00 min
 Lab File: VX013767.D
 Acq: 05 Dec 2019 11:10




Instrument :
 MSVOA_X
 ClientSampleId :
 VX1205WBL01


Tot Ion:	114	Resp:	631890
Ion	Ratio	Lower	Upper
114	100		
63	20.2	16.1	24.1
88	15.5	12.3	18.5

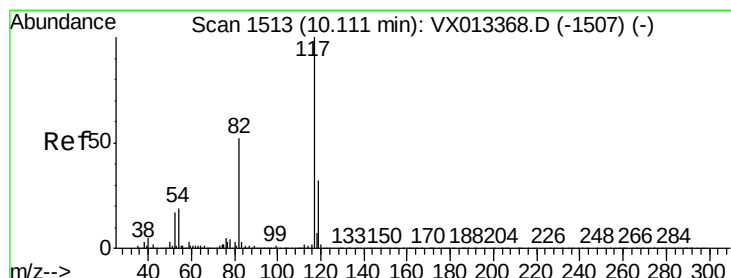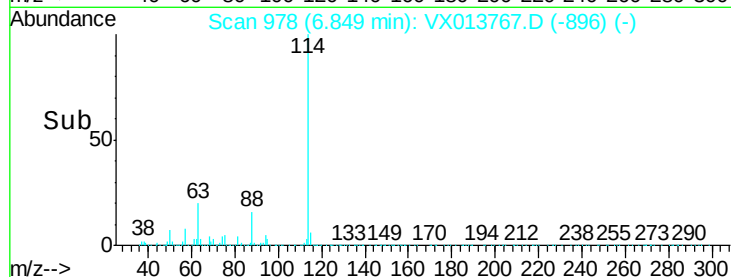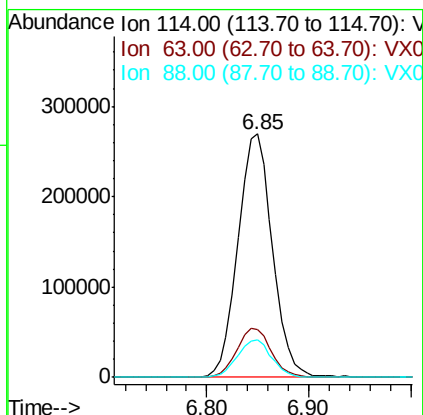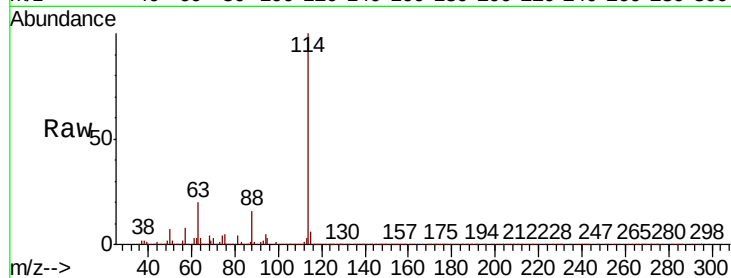

#57
 Chlorobenzene-d5
 Concen: 30.000 ug/l
 RT: 10.10 min Scan# 1512
 Delta R.T. -0.01 min
 Lab File: VX013767.D
 Acq: 05 Dec 2019 11:10

Tgt Ion:	117	Resp:	536206
Ion	Ratio	Lower	Upper
117	100		
82	54.2	43.7	65.5
119	32.2	25.5	38.3

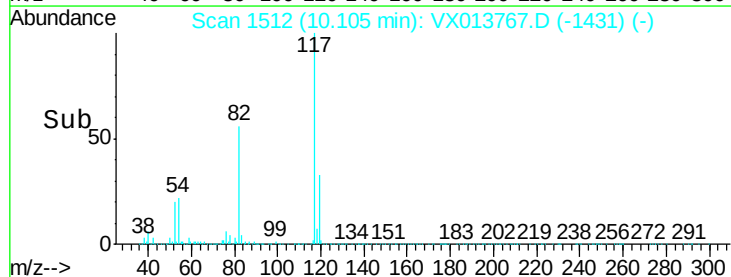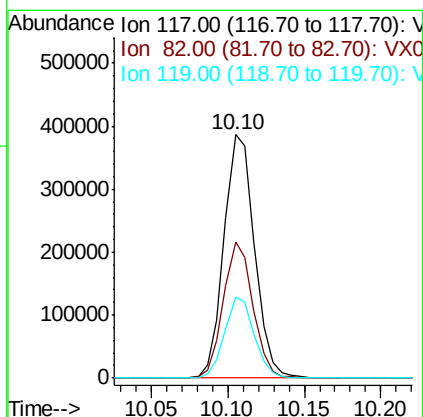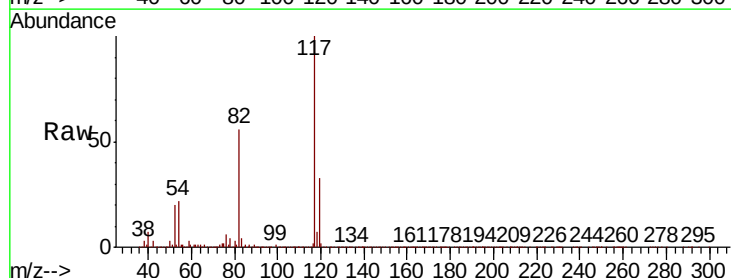

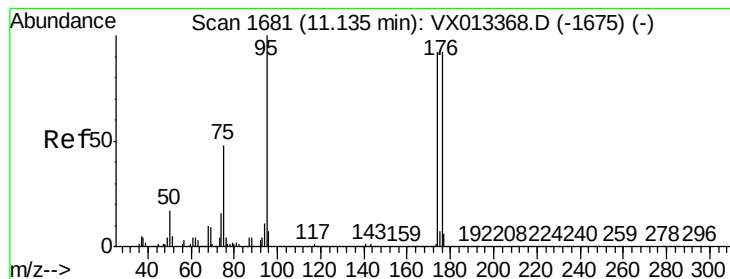

#60

4-Bromofluorobenzene

Concen: 27.764 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. -0.01 min

Lab File: VX013767.D

Acq: 05 Dec 2019 11:10

Instrument :

MSVOA_X

ClientSampleId :

VX1205WBL01





Tot Ion: 95 Resp: 239280

Ion Ratio Lower Upper

95 100

174 90.1 70.2 105.2

176 86.7 68.3 102.5

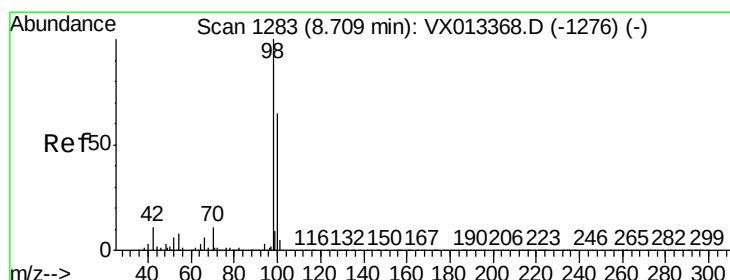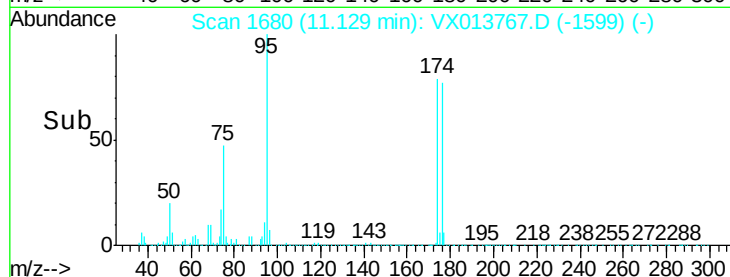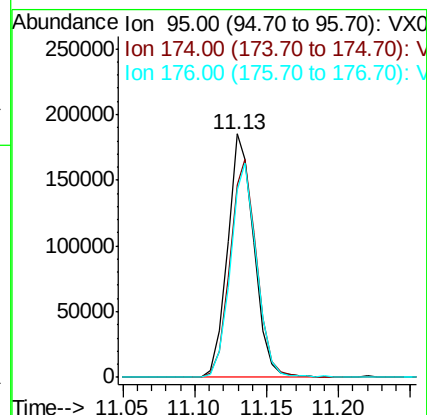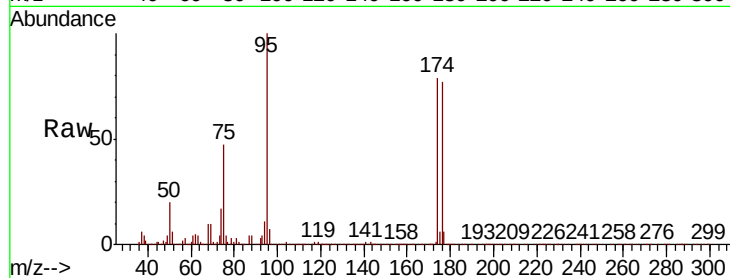

#63

Toluene-d8

Concen: 30.115 ug/l

RT: 8.71 min Scan# 1283

Delta R.T. -0.00 min

Lab File: VX013767.D

Acq: 05 Dec 2019 11:10

Tgt Ion: 98 Resp: 730198

Ion Ratio Lower Upper

98 100

100 66.3 52.5 78.7

