
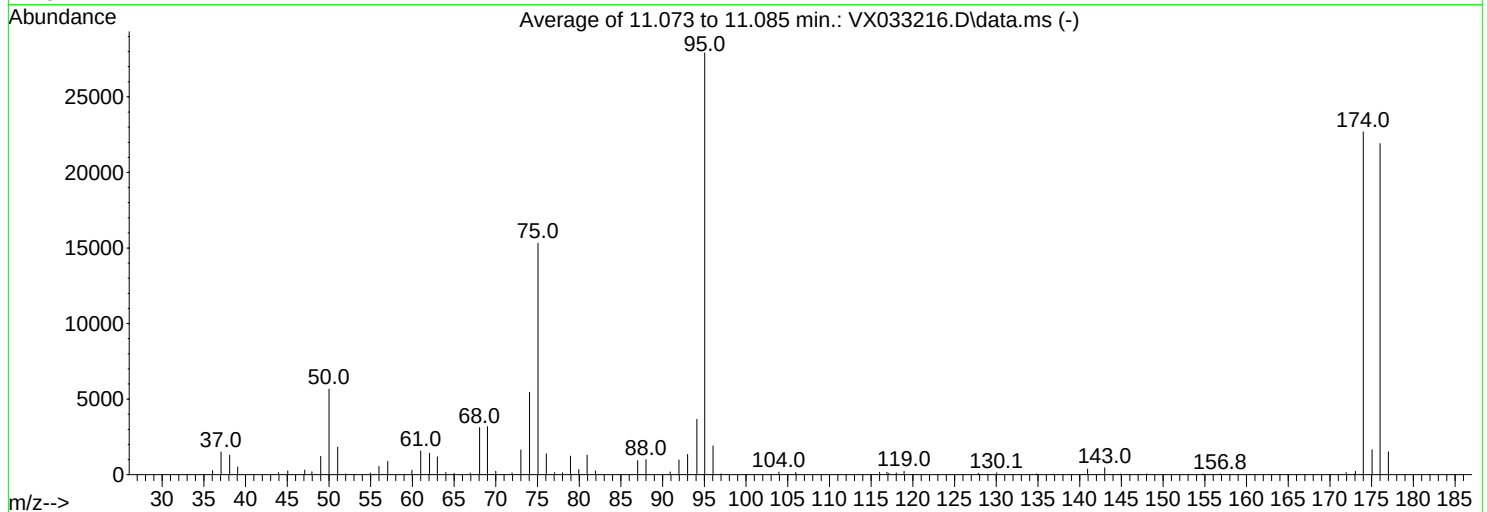


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120522\
 Data File : VX033216.D
 Acq On : 05 Dec 2022 10:09
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X111022W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Nov 11 05:24:06 2022

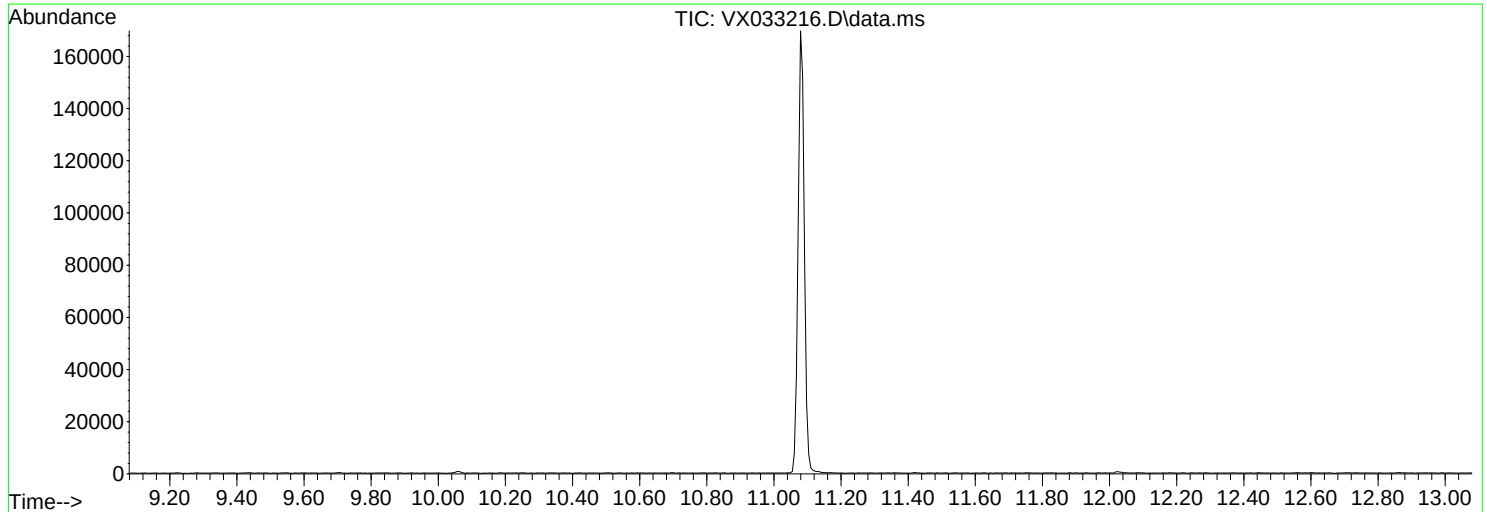

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	5668	PASS
75	95	30	60	54.9	15317	PASS
95	95	100	100	100.0	27917	PASS
96	95	5	9	6.8	1902	PASS
173	174	0.00	2	1.0	224	PASS
174	95	50	100	81.3	22686	PASS
175	174	5	9	7.3	1649	PASS
176	174	95	101	96.6	21913	PASS
177	176	5	9	6.9	1513	PASS