
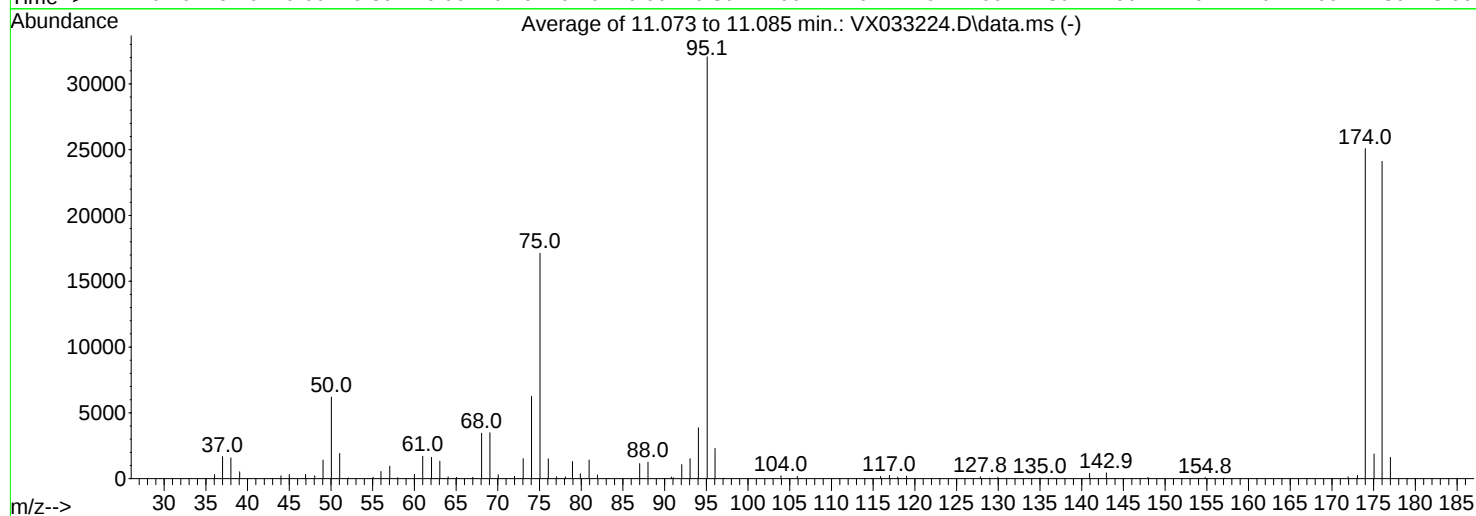


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120522\
 Data File : VX033224.D
 Acq On : 05 Dec 2022 14:21
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
 Title : SW846 8260
 Last Update : Tue Nov 22 13:58:46 2022

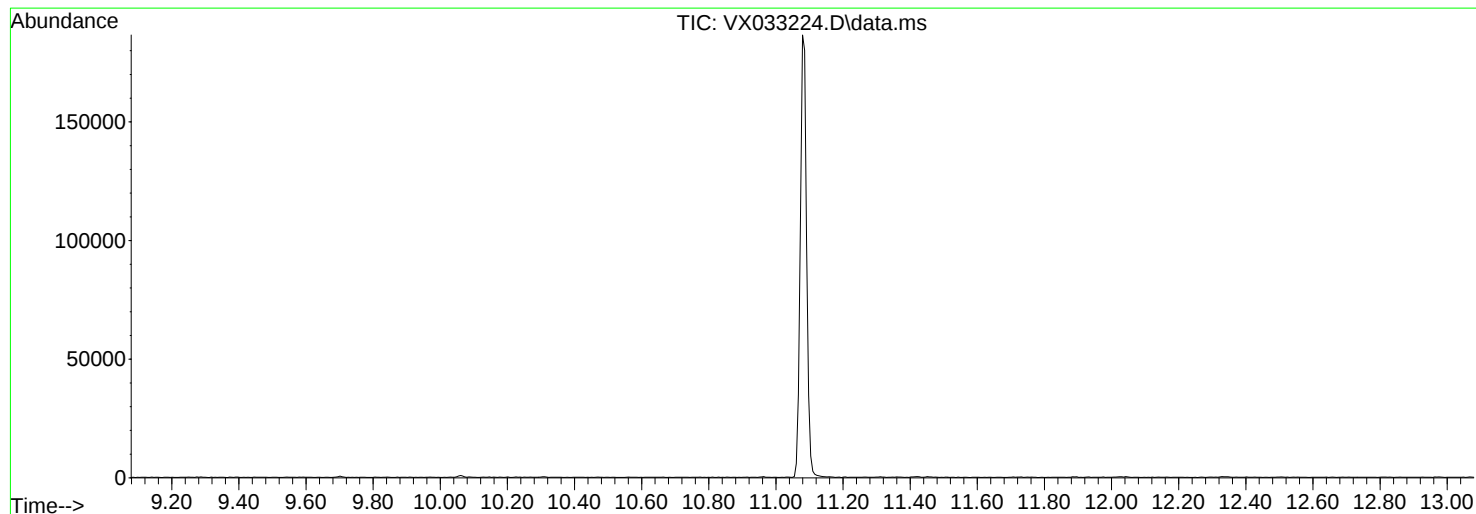

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	6203	PASS
75	95	30	60	53.5	17136	PASS
95	95	100	100	100.0	32056	PASS
96	95	5	9	7.2	2302	PASS
173	174	0.00	2	1.0	259	PASS
174	95	50	100	78.2	25080	PASS
175	174	5	9	7.5	1876	PASS
176	174	95	101	96.2	24118	PASS
177	176	5	9	6.7	1620	PASS