

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120523\
 Data File : VX039079.D
 Acq On : 05 Dec 2023 13:05
 Operator : JC/MD
 Sample : VX1205MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK639

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039079.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rBV	165312	168527	14.96%	1.883%
2	1.551	74	76	78	rBV2	3367	2809	0.25%	0.031%
3	1.587	78	82	85	rVV2	2789	6176	0.55%	0.069%
4	1.673	91	96	108	rVB	97894	148513	13.18%	1.660%
5	1.892	129	132	135	rVV3	1932	2671	0.24%	0.030%
6	1.941	138	140	142	rVB	1886	1287	0.11%	0.014%
7	2.081	161	163	165	rVB3	1388	996	0.09%	0.011%
8	2.111	165	168	171	rBV	2340	2761	0.25%	0.031%
9	2.215	183	185	186	rBV2	1831	1133	0.10%	0.013%
10	2.307	194	200	210	rBV	257588	401152	35.61%	4.483%
11	2.416	216	218	222	rBV	1378	1243	0.11%	0.014%
12	2.508	231	233	237	rVB2	3375	3786	0.34%	0.042%
13	2.703	261	265	267	rBV	2190	2957	0.26%	0.033%
14	2.861	289	291	293	rBV	1499	931	0.08%	0.010%
15	3.605	411	413	415	rBV	1368	1035	0.09%	0.012%
16	3.666	421	423	424	rVB	2746	1669	0.15%	0.019%
17	3.684	424	426	427	rBV	2264	1896	0.17%	0.021%
18	3.788	440	443	446	rBV	2290	3345	0.30%	0.037%
19	3.849	451	453	456	rVB	1393	1552	0.14%	0.017%
20	3.879	456	458	459	rBV	1415	1122	0.10%	0.013%
21	4.014	478	480	482	rBV2	1255	1139	0.10%	0.013%
22	4.117	495	497	500	rVB	1853	1743	0.15%	0.019%
23	4.300	524	527	528	rBV	1655	1587	0.14%	0.018%
24	4.446	542	551	565	rBV	105804	311277	27.63%	3.479%
25	4.757	600	602	603	rVB	1496	860	0.08%	0.010%
26	4.776	603	605	608	rBV2	1018	1055	0.09%	0.012%
27	4.812	610	611	613	rBV	1572	1463	0.13%	0.016%
28	4.983	637	639	640	rVV	1697	1798	0.16%	0.020%
29	5.050	640	650	665	rVB	140057	447155	39.70%	4.997%
30	5.276	685	687	688	rBV	1515	1151	0.10%	0.013%
31	5.385	702	705	710	rBV	2110	4024	0.36%	0.045%
32	5.519	725	727	730	rVB	2166	2395	0.21%	0.027%
33	5.556	730	733	734	rBV	1170	1602	0.14%	0.018%
34	5.794	771	772	774	rBV	1660	1149	0.10%	0.013%
35	5.964	789	800	814	rBV2	375944	1126451	100.00%	12.589%
36	6.318	857	858	859	rBV	2021	1043	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120523\
 Data File : VX039079.D
 Acq On : 05 Dec 2023 13:05
 Operator : JC/MD
 Sample : VX1205MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK639

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	6.391	868	870	871	rVB	1711	926	0.08%	0.010%
38	6.507	888	889	891	rBV	1622	1354	0.12%	0.015%
39	6.672	915	916	918	rBV2	919	977	0.09%	0.011%
40	6.757	920	930	944	rVV	263249	637298	56.58%	7.122%
41	6.928	957	958	960	rBV	1748	963	0.09%	0.011%
42	6.995	967	969	971	rVB	1614	1414	0.13%	0.016%
43	7.111	984	988	994	rBV6	3260	6606	0.59%	0.074%
44	7.306	1010	1020	1031	rBV	225795	514965	45.72%	5.755%
45	7.428	1038	1040	1043	rBV	1623	1400	0.12%	0.016%
46	7.574	1062	1064	1066	rBV	1577	1362	0.12%	0.015%
47	7.818	1101	1104	1109	rBV2	1912	3670	0.33%	0.041%
48	7.946	1123	1125	1127	rVV	1341	1528	0.14%	0.017%
49	7.995	1131	1133	1135	rBV	2909	1992	0.18%	0.022%
50	8.092	1145	1149	1150	rBV	1380	1727	0.15%	0.019%
51	8.165	1160	1161	1164	rBV	2089	1505	0.13%	0.017%
52	8.324	1180	1187	1194	rBV	176266	291364	25.87%	3.256%
53	8.647	1234	1240	1250	rBV	574858	910635	80.84%	10.177%
54	8.946	1285	1289	1298	rBV	128925	189214	16.80%	2.115%
55	9.098	1312	1314	1315	rBV	1541	1289	0.11%	0.014%
56	9.269	1340	1342	1343	rBV	2582	1700	0.15%	0.019%
57	9.378	1355	1360	1374	rBV	498094	721142	64.02%	8.059%
58	10.049	1465	1470	1480	rBV	552875	773603	68.68%	8.645%
59	10.189	1490	1493	1494	rBV	3253	2774	0.25%	0.031%
60	10.305	1509	1512	1516	rBV2	3130	3700	0.33%	0.041%
61	10.415	1529	1530	1531	rBV	1864	907	0.08%	0.010%
62	10.647	1562	1568	1570	rBV2	3803	6541	0.58%	0.073%
63	10.738	1581	1583	1585	rBV	2346	2123	0.19%	0.024%
64	10.762	1585	1587	1588	rVB	2138	1451	0.13%	0.016%
65	10.829	1597	1598	1603	rBV	1797	2450	0.22%	0.027%
66	10.866	1603	1604	1605	rBV	2315	1106	0.10%	0.012%
67	11.037	1630	1632	1634	rBV	1150	1152	0.10%	0.013%
68	11.189	1652	1657	1669	rVB	436141	559062	49.63%	6.248%
69	11.335	1679	1681	1682	rVB	1764	1041	0.09%	0.012%
70	11.354	1682	1684	1686	rBV	1214	1002	0.09%	0.011%
71	11.427	1694	1696	1697	rBV	1626	1004	0.09%	0.011%
72	11.445	1697	1699	1704	rVB2	2783	3860	0.34%	0.043%
73	11.579	1717	1721	1722	rBV	1776	2139	0.19%	0.024%
74	11.665	1733	1735	1737	rBV	1459	1211	0.11%	0.014%
75	11.829	1760	1762	1765	rVB	1619	1451	0.13%	0.016%
76	11.969	1784	1785	1788	rVB	2898	1855	0.16%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120523\
 Data File : VX039079.D
 Acq On : 05 Dec 2023 13:05
 Operator : JC/MD
 Sample : VX1205MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK639

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.018	1788	1793	1802	rBV	608051	782187	69.44%	8.741%
78	12.317	1837	1842	1850	rBV	626534	785583	69.74%	8.779%
79	12.689	1901	1903	1905	rBV2	1460	1474	0.13%	0.016%
80	12.799	1920	1921	1923	rBV	1431	1108	0.10%	0.012%
81	12.933	1941	1943	1945	rBV	2844	2543	0.23%	0.028%
82	13.012	1954	1956	1957	rBV	1724	1031	0.09%	0.012%
83	13.109	1969	1972	1975	rBV2	4366	5873	0.52%	0.066%
84	13.262	1995	1997	1999	rBV	1418	1240	0.11%	0.014%
85	13.329	2004	2008	2013	rBV	2301	4624	0.41%	0.052%
86	13.445	2025	2027	2028	rBV	1842	1564	0.14%	0.017%
87	13.591	2047	2051	2056	rVV3	5179	7562	0.67%	0.085%
88	13.774	2078	2081	2086	rVB3	7468	10356	0.92%	0.116%
89	13.963	2108	2112	2115	rBV2	4435	6547	0.58%	0.073%
90	14.274	2161	2163	2164	rBV	1693	1141	0.10%	0.013%
91	14.603	2215	2217	2219	rVB	1738	1003	0.09%	0.011%
92	14.871	2260	2261	2263	rBV	2227	1628	0.14%	0.018%
93	14.926	2268	2270	2271	rVV	2035	888	0.08%	0.010%
94	15.219	2317	2318	2321	rVB	2646	1544	0.14%	0.017%
95	15.603	2379	2381	2383	rBV2	1696	1514	0.13%	0.017%
96	15.902	2428	2430	2432	rVB	2049	1468	0.13%	0.016%
97	16.054	2453	2455	2457	rVB	2189	1488	0.13%	0.017%
98	16.341	2500	2502	2503	rBV	1747	1181	0.10%	0.013%
99	16.383	2507	2509	2510	rBV	1544	863	0.08%	0.010%
100	16.402	2510	2512	2513	rBV	1339	886	0.08%	0.010%




Sum of corrected areas: 8948212

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120523\
Data File : VX039079.D
Acq On : 05 Dec 2023 13:05
Operator : JC/MD
Sample : VX1205MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK639

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

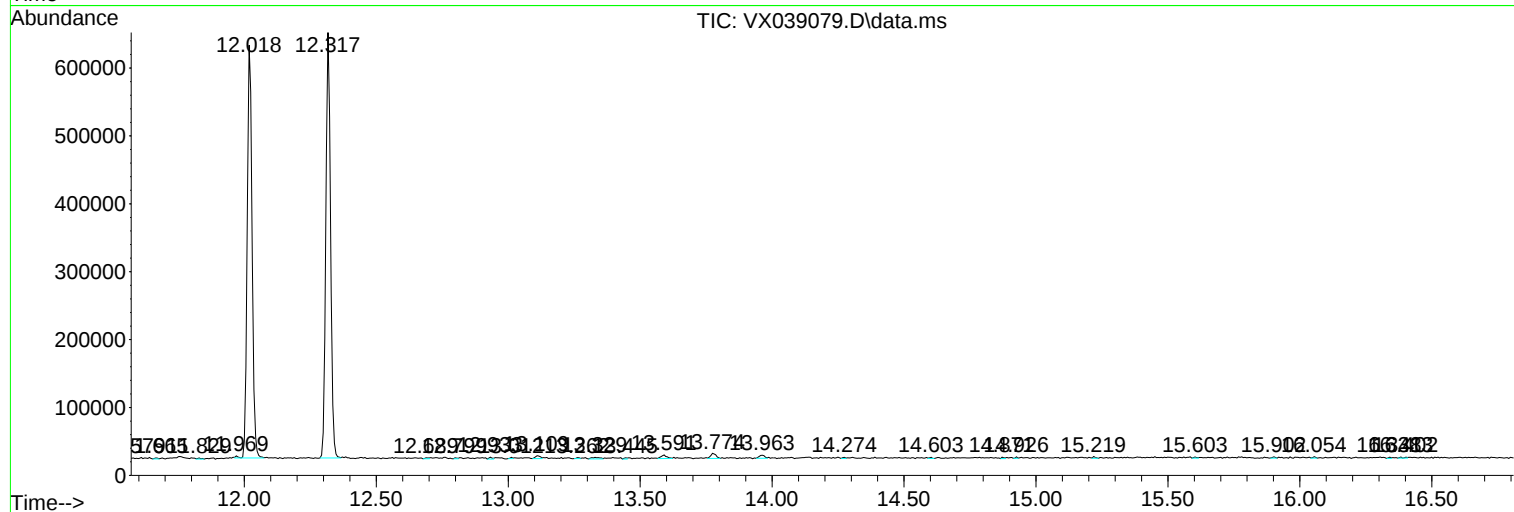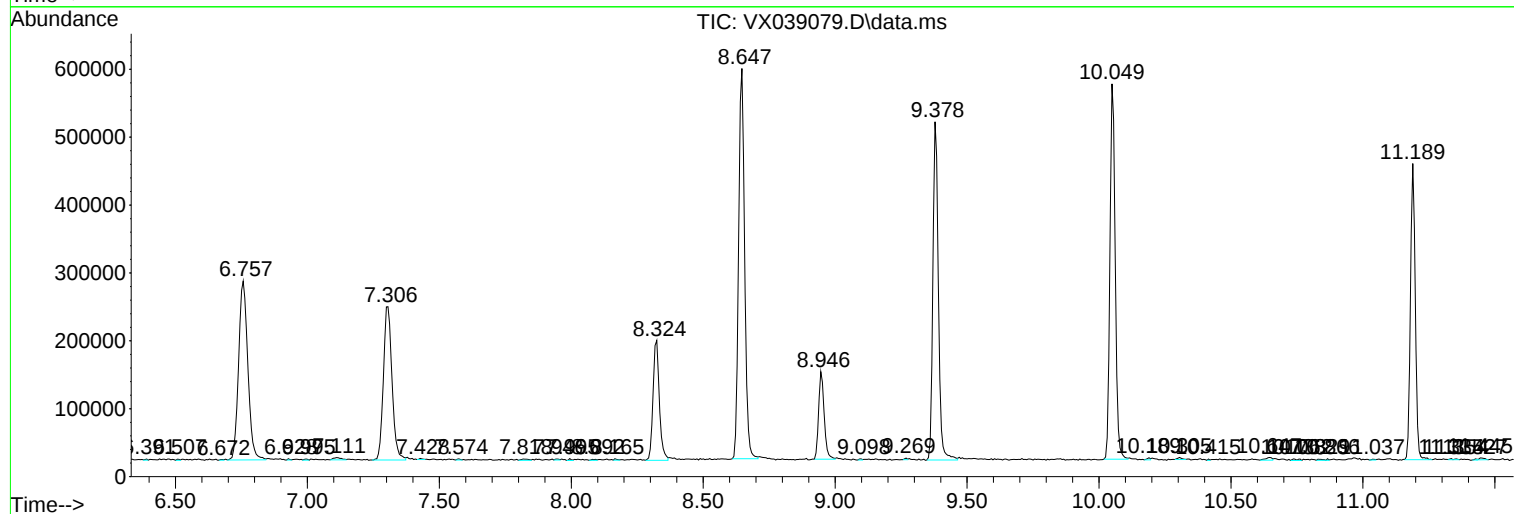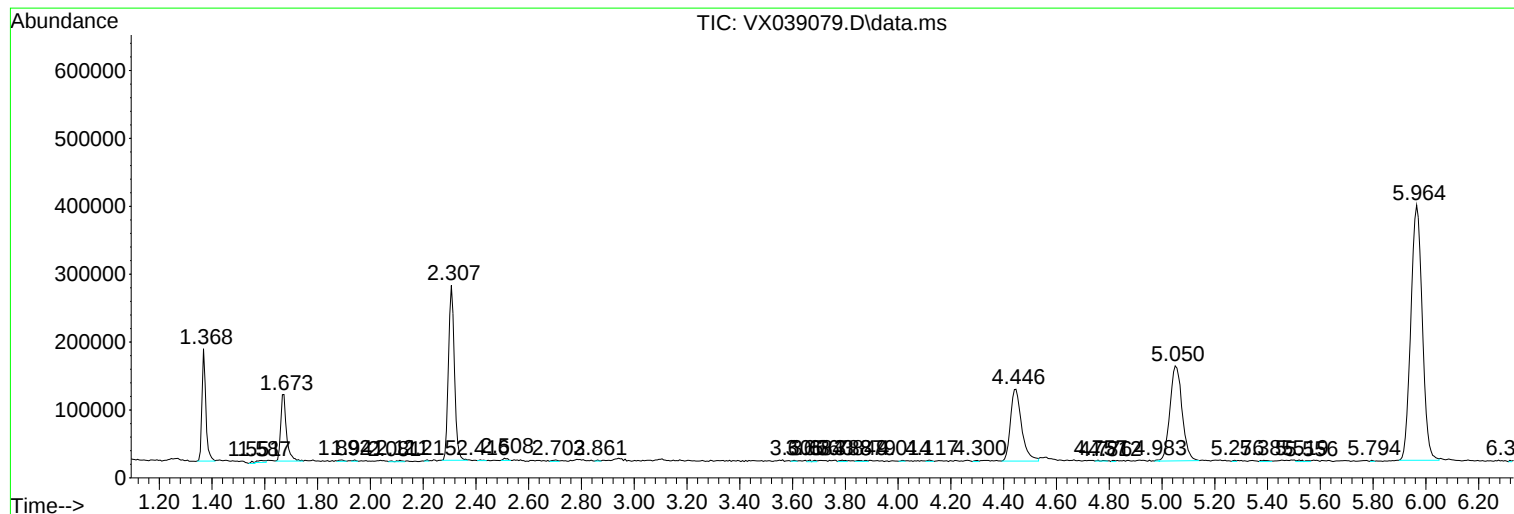

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120523\
Data File : VX039079.D
Acq On : 05 Dec 2023 13:05
Operator : JC/MD
Sample : VX1205MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK639

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120523\
Data File : VX039079.D
Acq On : 05 Dec 2023 13:05
Operator : JC/MD
Sample : VX1205MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK639

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------