

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120523\
 Data File : VX039080.D
 Acq On : 05 Dec 2023 13:31
 Operator : JC/MD
 Sample : VX1205WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK640

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039080.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.227	21	23	24	rBV	2188	1158	0.10%	0.013%
2	1.252	24	27	28	rVV2	2624	2590	0.23%	0.030%
3	1.368	43	46	55	rBV	152962	164116	14.57%	1.872%
4	1.551	74	76	78	rBV2	2314	1998	0.18%	0.023%
5	1.569	78	79	80	rBV	3569	2529	0.22%	0.029%
6	1.666	91	95	106	rVB	97257	139983	12.43%	1.597%
7	1.886	129	131	137	rVV4	1718	2011	0.18%	0.023%
8	1.959	139	143	145	rVB	2486	2670	0.24%	0.030%
9	2.081	160	163	164	rBV2	2501	2148	0.19%	0.025%
10	2.160	174	176	177	rBV2	1239	1011	0.09%	0.012%
11	2.307	194	200	209	rBV	245169	386081	34.28%	4.405%
12	2.514	229	234	237	rBV2	3776	6756	0.60%	0.077%
13	2.715	265	267	268	rVB	2164	1487	0.13%	0.017%
14	2.739	268	271	272	rBV	1424	1489	0.13%	0.017%
15	2.788	275	279	284	rVV3	3217	6775	0.60%	0.077%
16	2.928	299	302	304	rBV2	4140	5342	0.47%	0.061%
17	3.191	344	345	346	rBV	2008	928	0.08%	0.011%
18	3.215	347	349	353	rVB	2012	1885	0.17%	0.022%
19	3.428	383	384	386	rBV	1530	1467	0.13%	0.017%
20	3.593	410	411	412	rBV	2035	1078	0.10%	0.012%
21	3.697	425	428	429	rVB	1639	1487	0.13%	0.017%
22	3.721	429	432	433	rBV	1667	1475	0.13%	0.017%
23	3.806	444	446	448	rBV	1979	1372	0.12%	0.016%
24	3.977	472	474	476	rBV2	1357	1307	0.12%	0.015%
25	4.117	496	497	500	rBV	1635	2016	0.18%	0.023%
26	4.276	522	523	524	rBV	1527	1039	0.09%	0.012%
27	4.446	543	551	564	rBV	107287	307062	27.26%	3.503%
28	4.763	602	603	606	rBV	1338	1241	0.11%	0.014%
29	4.849	615	617	620	rVB	2145	1670	0.15%	0.019%
30	4.922	627	629	631	rVB	1998	1862	0.17%	0.021%
31	4.946	631	633	634	rBV	1963	1377	0.12%	0.016%
32	5.056	639	651	664	rVV	137113	432798	38.43%	4.938%
33	5.330	694	696	697	rBV	1175	985	0.09%	0.011%
34	5.379	700	704	707	rBV	2137	4509	0.40%	0.051%
35	5.739	761	763	764	rBV	1706	1366	0.12%	0.016%
36	5.964	789	800	814	rBV2	370893	1126254	100.00%	12.850%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120523\
 Data File : VX039080.D
 Acq On : 05 Dec 2023 13:31
 Operator : JC/MD
 Sample : VX1205WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK640

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	6.288	851	853	855	rBV	1403	966	0.09%	0.011%
38	6.348	862	863	864	rBV	1951	1048	0.09%	0.012%
39	6.403	871	872	874	rBV	1177	824	0.07%	0.009%
40	6.422	874	875	876	rBV	2621	1231	0.11%	0.014%
41	6.458	879	881	884	rVV	1368	1702	0.15%	0.019%
42	6.519	889	891	892	rBV	1676	835	0.07%	0.010%
43	6.666	913	915	917	rBV	1191	1286	0.11%	0.015%
44	6.757	921	930	942	rBV	257967	610328	54.19%	6.964%
45	6.922	955	957	960	rBV2	1300	1302	0.12%	0.015%
46	7.306	1012	1020	1037	rBV	225779	504263	44.77%	5.753%
47	7.482	1047	1049	1052	rBV	1815	1945	0.17%	0.022%
48	7.580	1063	1065	1070	rVB	1196	1731	0.15%	0.020%
49	7.952	1124	1126	1128	rVB	1547	1001	0.09%	0.011%
50	8.043	1139	1141	1145	rVB	1577	1912	0.17%	0.022%
51	8.098	1145	1150	1151	rBV	1550	1871	0.17%	0.021%
52	8.324	1181	1187	1199	rBV	167333	285563	25.36%	3.258%
53	8.433	1204	1205	1207	rBV	1319	935	0.08%	0.011%
54	8.647	1233	1240	1249	rBV	558652	894730	79.44%	10.209%
55	8.897	1279	1281	1284	rVB	1705	1115	0.10%	0.013%
56	8.946	1284	1289	1298	rBV	126553	194654	17.28%	2.221%
57	9.189	1327	1329	1332	rBV	2322	1866	0.17%	0.021%
58	9.250	1337	1339	1340	rBV	1499	1130	0.10%	0.013%
59	9.281	1340	1344	1346	rBV2	2310	2918	0.26%	0.033%
60	9.378	1355	1360	1368	rBV	499511	721776	64.09%	8.235%
61	9.610	1396	1398	1400	rBV	1215	857	0.08%	0.010%
62	9.689	1409	1411	1415	rVV3	1736	1917	0.17%	0.022%
63	9.830	1432	1434	1435	rBV	1413	1034	0.09%	0.012%
64	9.976	1456	1458	1459	rBV	1355	1352	0.12%	0.015%
65	10.049	1465	1470	1484	rVB	526902	753750	66.93%	8.600%
66	10.384	1524	1525	1530	rBV	1532	1709	0.15%	0.019%
67	10.647	1565	1568	1572	rBV5	3003	5896	0.52%	0.067%
68	11.146	1648	1650	1651	rBV	1803	1298	0.12%	0.015%
69	11.189	1652	1657	1669	rVB	439118	556817	49.44%	6.353%
70	11.457	1697	1701	1702	rBV2	3113	3717	0.33%	0.042%
71	11.756	1746	1750	1754	rBV2	3474	5149	0.46%	0.059%
72	11.976	1784	1786	1788	rBV	2224	1581	0.14%	0.018%
73	12.018	1788	1793	1801	rVB	605600	758109	67.31%	8.650%
74	12.225	1825	1827	1828	rVB	1821	1159	0.10%	0.013%
75	12.317	1837	1842	1850	rBV	591554	760739	67.55%	8.680%
76	12.378	1850	1852	1857	rVB	2541	2634	0.23%	0.030%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120523\
 Data File : VX039080.D
 Acq On : 05 Dec 2023 13:31
 Operator : JC/MD
 Sample : VX1205WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK640

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.756	1913	1914	1918	rBV	1516	2425	0.22%	0.028%
78	12.811	1921	1923	1927	rVB	1758	1993	0.18%	0.023%
79	12.860	1929	1931	1934	rBV	1869	1845	0.16%	0.021%
80	12.945	1943	1945	1947	rBV	1364	1455	0.13%	0.017%
81	13.116	1971	1973	1977	rVB2	3138	2659	0.24%	0.030%
82	13.262	1995	1997	1999	rBV	1661	1100	0.10%	0.013%
83	13.591	2047	2051	2056	rVB3	3945	6286	0.56%	0.072%
84	13.640	2057	2059	2060	rBV2	1454	869	0.08%	0.010%
85	13.774	2078	2081	2085	rVV2	3927	5016	0.45%	0.057%
86	13.963	2109	2112	2116	rBV3	2698	3765	0.33%	0.043%
87	14.176	2145	2147	2148	rBV2	1281	1258	0.11%	0.014%
88	14.384	2180	2181	2183	rBV	2220	1171	0.10%	0.013%
89	14.408	2183	2185	2186	rVV	1525	1180	0.10%	0.013%
90	14.445	2190	2191	2194	rVB	1761	1027	0.09%	0.012%
91	14.542	2205	2207	2210	rVB	2190	2588	0.23%	0.030%
92	14.579	2211	2213	2215	rBV	2010	1642	0.15%	0.019%
93	14.646	2222	2224	2225	rBV	1585	1213	0.11%	0.014%
94	15.030	2284	2287	2289	rBV	1943	2415	0.21%	0.028%
95	15.103	2297	2299	2301	rBV	1489	1268	0.11%	0.014%
96	15.127	2301	2303	2305	rVV	1564	1419	0.13%	0.016%
97	15.603	2379	2381	2385	rVB	2064	1992	0.18%	0.023%
98	15.835	2417	2419	2420	rBV	1480	1470	0.13%	0.017%
99	16.237	2484	2485	2488	rBV	1774	862	0.08%	0.010%
100	16.755	2568	2570	2571	rBV	2151	1652	0.15%	0.019%




Sum of corrected areas: 8764542

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120523\
Data File : VX039080.D
Acq On : 05 Dec 2023 13:31
Operator : JC/MD
Sample : VX1205WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK640

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

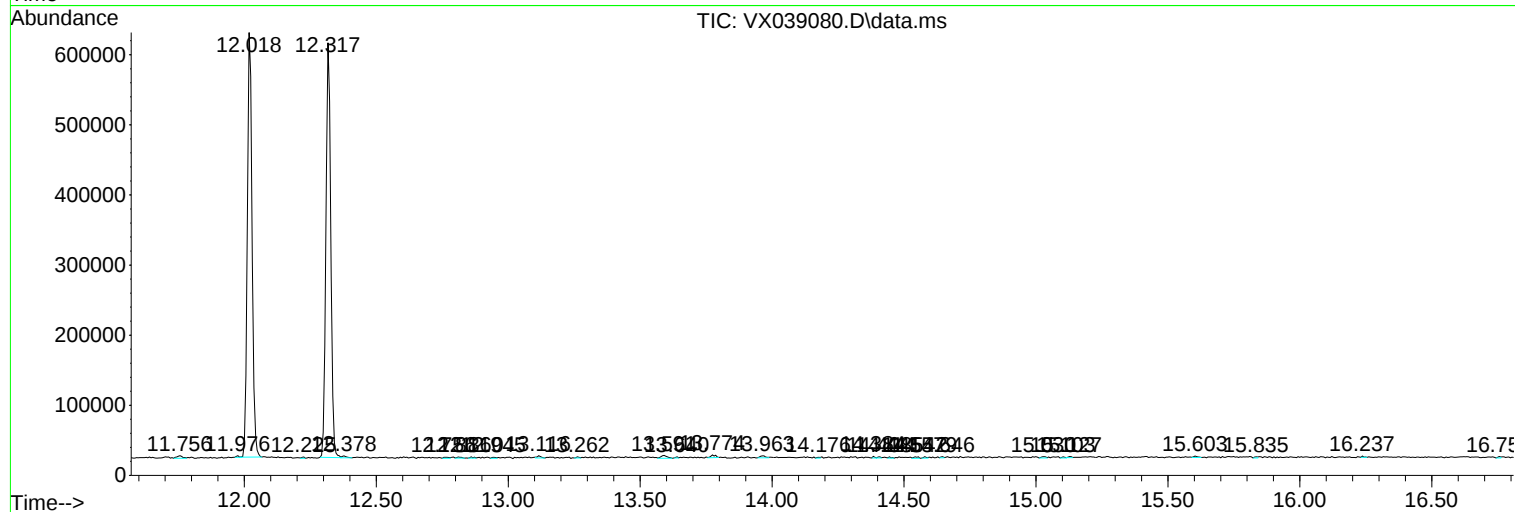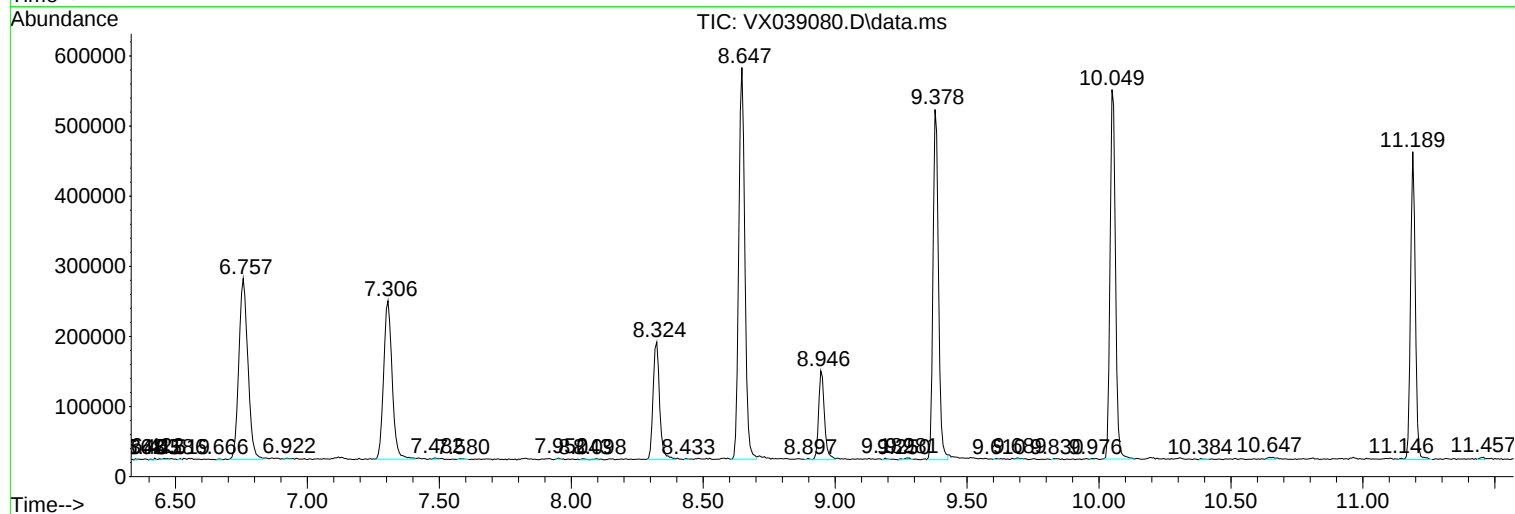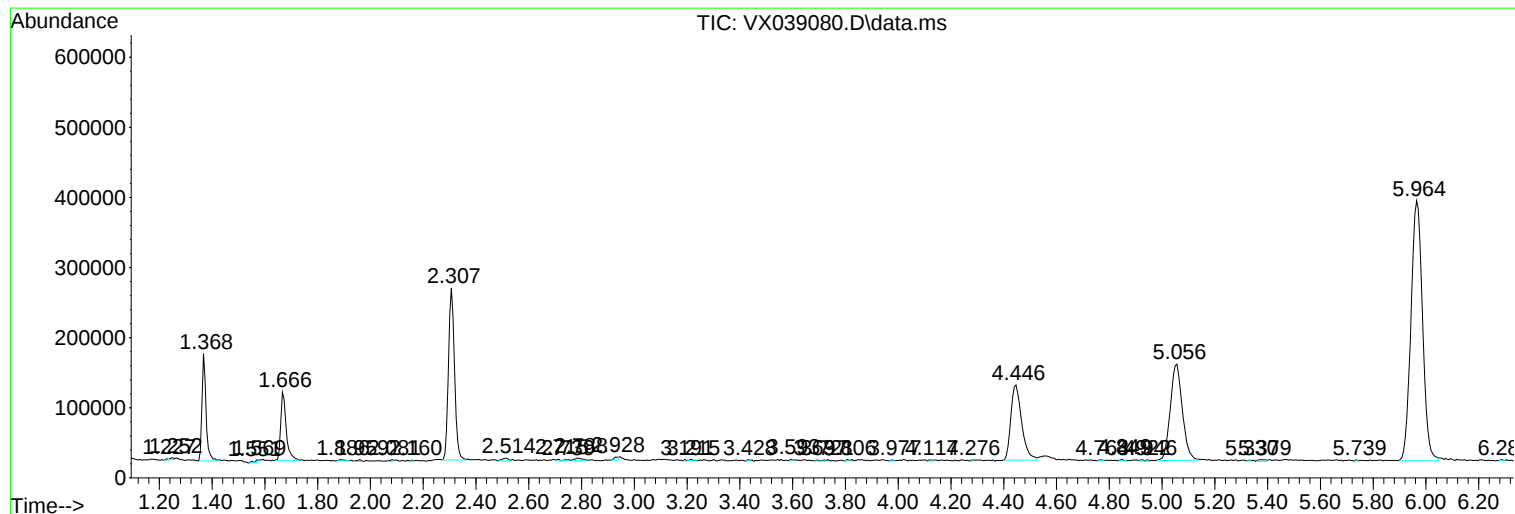

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120523\
Data File : VX039080.D
Acq On : 05 Dec 2023 13:31
Operator : JC/MD
Sample : VX1205WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK640

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120523\
Data File : VX039080.D
Acq On : 05 Dec 2023 13:31
Operator : JC/MD
Sample : VX1205WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK640

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc