
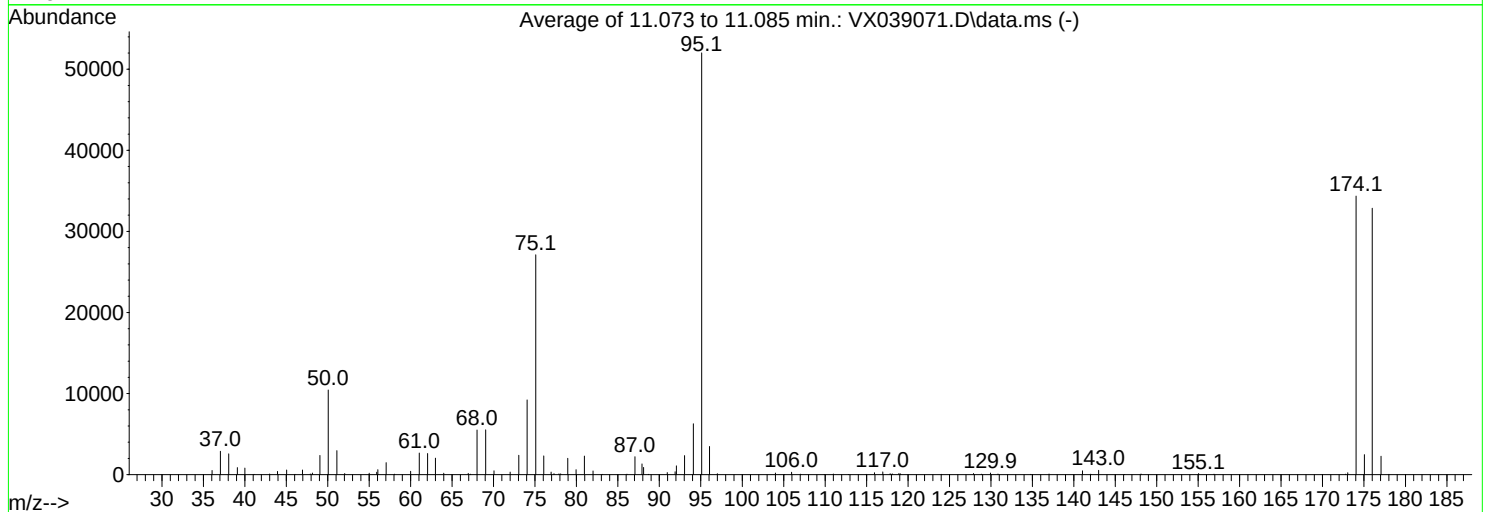


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120523\
Data File : VX039071.D
Acq On : 05 Dec 2023 09:48
Operator : JC/MD
Sample : BFB652
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB652

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Title : VOC Analysis
Last Update : Wed Dec 06 02:19:46 2023

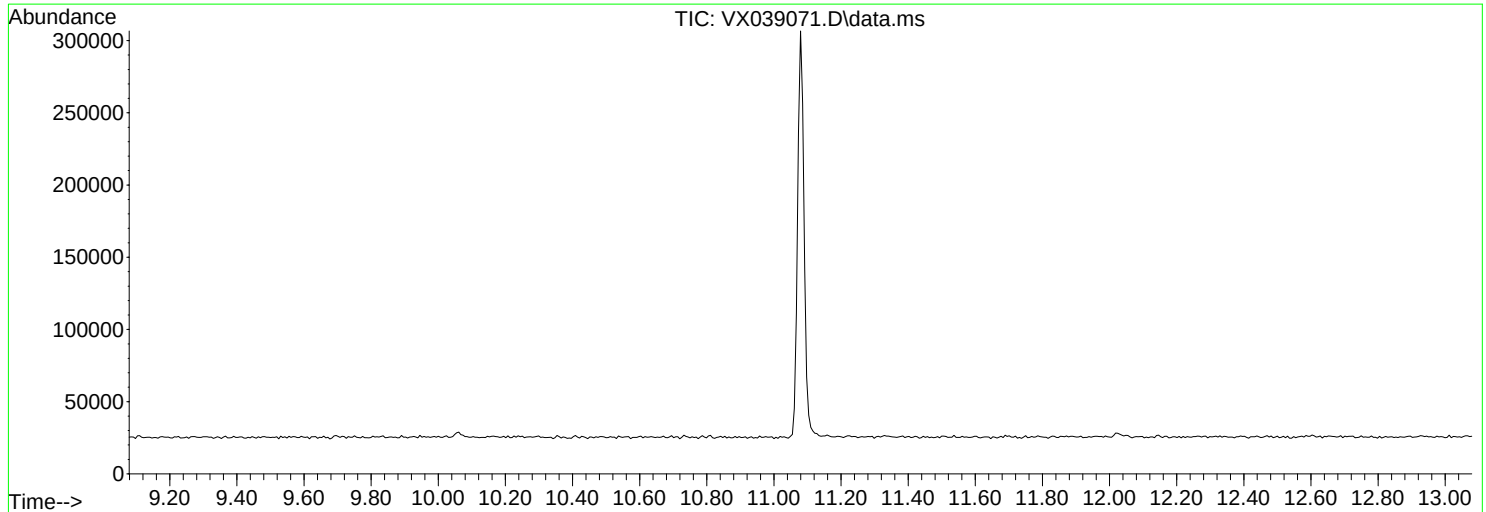

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	10443	PASS
75	95	30	80	52.1	27117	PASS
95	95	100	100	100.0	52024	PASS
96	95	5	9	6.7	3476	PASS
173	174	0.00	2	0.7	228	PASS
174	95	50	120	66.0	34357	PASS
175	174	5	9	7.2	2458	PASS
176	174	95	101	95.7	32864	PASS
177	176	5	9	6.9	2267	PASS

m/z	Abundance
36.10	130.0
39.10	107.0
40.00	24280.0
44.00	185.0

Instrument :
MSVOA_X
ClientSampleId :
BFB652

m/z	Abundance
36.00	472.0
37.10	2773.0
38.10	2317.0
39.10	1064.0
40.00	25600.0
41.10	106.0
44.00	696.0
45.00	567.0
47.00	515.0
48.10	217.0
49.00	2307.0
50.10	10046.0
51.10	2809.0
52.00	122.0
55.00	191.0
55.90	869.0
57.10	1601.0
58.10	66.0
60.00	396.0
61.00	2283.0
62.10	2537.0
63.00	2040.0
64.00	166.0
67.00	143.0
68.00	5324.0
69.00	4897.0
70.00	432.0
72.00	272.0
73.00	2499.0
74.00	8287.0
75.10	25056.0
76.10	2000.0
77.00	313.0
78.00	146.0
79.00	1827.0
79.90	480.0
80.90	2222.0
82.00	436.0
87.10	1982.0
87.90	2091.0
88.70	146.0
91.00	281.0
91.90	1094.0
93.00	2073.0
94.10	5471.0
95.10	46768.0
96.10	3257.0
97.00	139.0
103.90	197.0
106.10	212.0
107.00	54.0
109.90	84.0
111.00	87.0
115.90	154.0
117.00	288.0
117.90	143.0
119.00	255.0
127.90	131.0
128.80	77.0
130.00	154.0
130.90	76.0
134.80	68.0
137.10	109.0
141.00	356.0
142.00	54.0
143.00	446.0
148.20	56.0
155.00	101.0
172.80	184.0
174.00	26272.0
175.00	2035.0
176.00	25584.0
177.00	1812.0

Instrument :
MSVOA_X
ClientSampleId :
BFB652

m/z	Abundance
36.10	954.0
37.10	3455.0
38.10	3261.0
39.10	1109.0
40.00	24840.0
43.00	141.0
43.90	603.0
45.00	634.0
46.00	76.0
46.80	698.0
48.20	402.0
49.10	2875.0
50.00	11939.0
51.10	3616.0
52.00	132.0
55.00	197.0
56.10	1020.0
57.00	1618.0
58.10	71.0
60.10	354.0
61.10	3199.0
62.10	2982.0
63.00	2268.0
64.10	213.0
66.80	173.0
67.20	166.0
68.00	6483.0
69.10	6268.0
70.00	565.0
71.90	435.0
73.10	2731.0
74.10	11128.0
75.10	31744.0
76.10	2824.0
76.90	318.0
77.30	343.0
77.80	149.0
78.90	2487.0
80.00	704.0
81.00	2681.0
82.00	527.0
83.10	65.0
86.10	107.0
87.00	2462.0
88.10	2686.0
90.90	244.0
92.10	1995.0
93.10	2810.0
94.10	7587.0
95.10	60296.0
96.10	4022.0
97.00	96.0
104.00	237.0
105.90	361.0
107.10	102.0
111.00	80.0
115.00	62.0
116.00	327.0
116.90	318.0
118.10	285.0
118.80	238.0
124.00	62.0
127.90	145.0
128.90	116.0
130.00	225.0
130.70	82.0
134.80	60.0
136.90	90.0
141.10	478.0
142.10	97.0
143.00	558.0
148.10	108.0
155.10	162.0
156.90	107.0
173.00	348.0
174.00	39976.0
175.10	2859.0
176.00	37768.0
177.00	2521.0
178.00	108.0

Instrument :
MSVOA_X
ClientSampleId :
BFB652

m/z	Abundance
36.10	529.0
37.00	2406.0
38.00	2129.0
39.10	781.0
40.00	24840.0
43.00	79.0
44.00	466.0
45.10	504.0
46.10	60.0
47.00	505.0
47.90	251.0
49.00	1956.0
50.10	9345.0
51.10	2472.0
52.10	135.0
55.00	126.0
56.00	810.0
57.00	1197.0
58.00	71.0
59.90	472.0
61.00	2493.0
62.00	2320.0
63.00	1797.0
63.90	181.0
67.00	182.0
68.00	4730.0
69.10	5437.0
70.10	448.0
72.10	252.0
73.10	1936.0
74.00	8237.0
75.10	24552.0
76.00	2108.0
77.00	346.0
78.10	282.0
78.90	1740.0
79.90	632.0
80.90	1943.0
82.00	407.0
83.10	83.0
86.10	85.0
87.00	2164.0
87.90	1869.0
90.90	266.0
92.00	1268.0
93.00	2160.0
94.10	5758.0
95.10	49008.0
96.00	3148.0
97.00	110.0
104.10	167.0
105.10	75.0
105.90	320.0
111.00	59.0
112.80	52.0
114.90	58.0
116.00	260.0
117.00	396.0
117.80	209.0
119.10	285.0
124.10	86.0
127.90	172.0
129.90	194.0
130.90	85.0
136.90	58.0
141.00	596.0
143.00	605.0
146.10	52.0
148.00	98.0
155.00	145.0
156.90	59.0
173.10	337.0
174.10	36824.0
175.10	2481.0
176.00	35240.0
177.10	2467.0

Instrument :
MSVOA_X
ClientSampleId :
BFB652