

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120524\
 Data File : VX044148.D
 Acq On : 05 Dec 2024 15:30
 Operator : JC/MD
 Sample : P5066-03 100X
 Misc : 6.19g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 06 04:09:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 06 03:51:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	234807	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	205739	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	85505	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	87799	40.860	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	81.720%		
7) Chloroethane-d5	1.642	69	64035	38.471	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	76.940%		
11) 1,1-Dichloroethene-d2	2.294	65	36433	39.646	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	79.300%		
21) 2-Butanone-d5	4.465	46	115892	88.092	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	88.090%		
24) Chloroform-d	5.056	84	165887	40.660	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.320%		
26) 1,2-Dichloroethane-d4	5.952	65	119257	41.334	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.660%		
32) Benzene-d6	5.970	84	308669	43.420	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.840%		
36) 1,2-Dichloropropane-d6	7.306	67	96856	43.878	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	87.760%		
41) Toluene-d8	8.647	98	274788	41.805	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.620%		
43) trans-1,3-Dichloroprop...	8.952	79	41469	39.093	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.180%		
47) 2-Hexanone-d5	9.384	63	78806	91.563	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	91.560%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	127818	43.184	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	86.360%		
66) 1,2-Dichlorobenzene-d4	12.317	152	88364	44.354	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.700%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	8.324	75	3850	1.465	ug/L	# 71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120524\
Data File : VX044148.D
Acq On : 05 Dec 2024 15:30
Operator : JC/MD
Sample : P5066-03 100X
Misc : 6.19g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Dec 06 04:09:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 06 03:51:43 2024
Response via : Initial Calibration

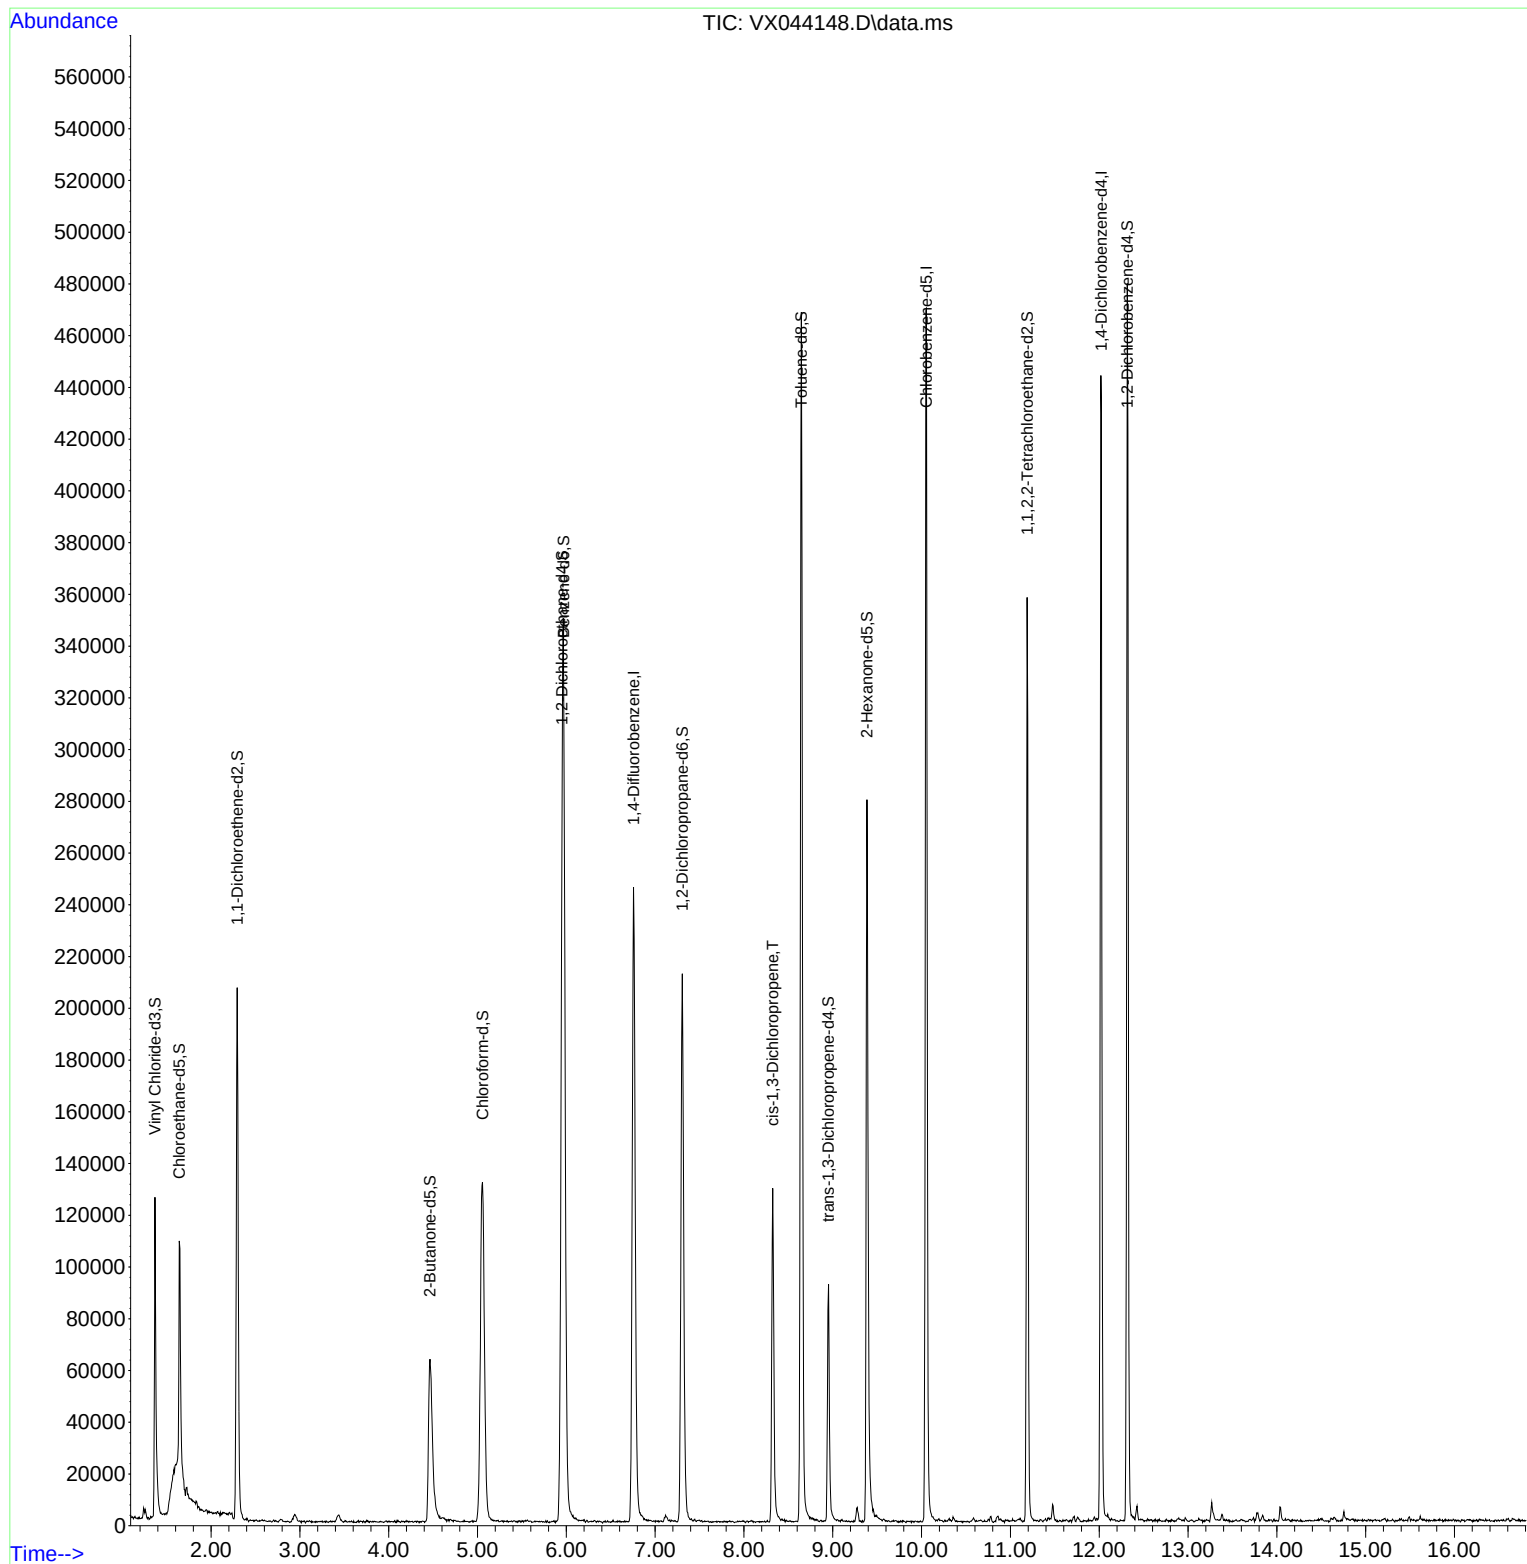

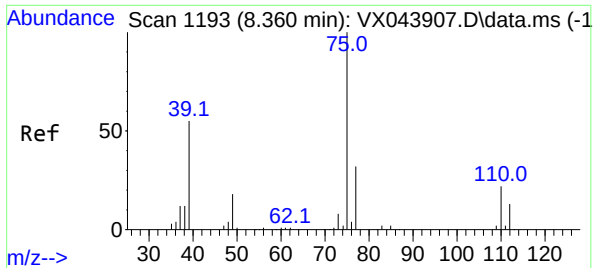

#39
cis-1,3-Dichloropropene
Concen: 1.465 ug/L
RT: 8.324 min Scan# 11
Delta R.T. -0.043 min
Lab File: VX044148.D
Acq: 05 Dec 2024 15:30

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 75 Resp: 3850
Ion Ratio Lower Upper
75 100
77 46.5 21.6 40.0#

