

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120524\
 Data File : VX044154.D
 Acq On : 05 Dec 2024 17:49
 Operator : JC/MD
 Sample : P5066-11ME
 Misc : 4.48g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 16 11:23:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 07 03:56:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	239877	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	211675	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	89325	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	88658	40.388	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	80.780%		
7) Chloroethane-d5	1.642	69	66717	39.235	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	78.460%		
11) 1,1-Dichloroethene-d2	2.294	65	36448	38.824	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	77.640%		
21) 2-Butanone-d5	4.465	46	121977	90.758	ug/L	0.01
Spiked Amount 100.000	Range 40 - 130		Recovery =	90.760%		
24) Chloroform-d	5.050	84	170987	41.025	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.040%		
26) 1,2-Dichloroethane-d4	5.952	65	127556	43.276	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.560%		
32) Benzene-d6	5.964	84	320169	43.775	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.540%		
36) 1,2-Dichloropropane-d6	7.306	67	101869	44.855	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	89.720%		
41) Toluene-d8	8.647	98	287260	42.477	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	84.960%		
43) trans-1,3-Dichloroprop...	8.952	79	43869	40.196	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.400%		
47) 2-Hexanone-d5	9.384	63	83119	93.866	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	93.870%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	136646	44.872	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	89.740%		
66) 1,2-Dichlorobenzene-d4	12.317	152	95386	45.831	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.660%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	8.318	75	3667	1.356	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120524\
Data File : VX044154.D
Acq On : 05 Dec 2024 17:49
Operator : JC/MD
Sample : P5066-11ME
Misc : 4.48g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Dec 16 11:23:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 03:56:15 2024
Response via : Initial Calibration

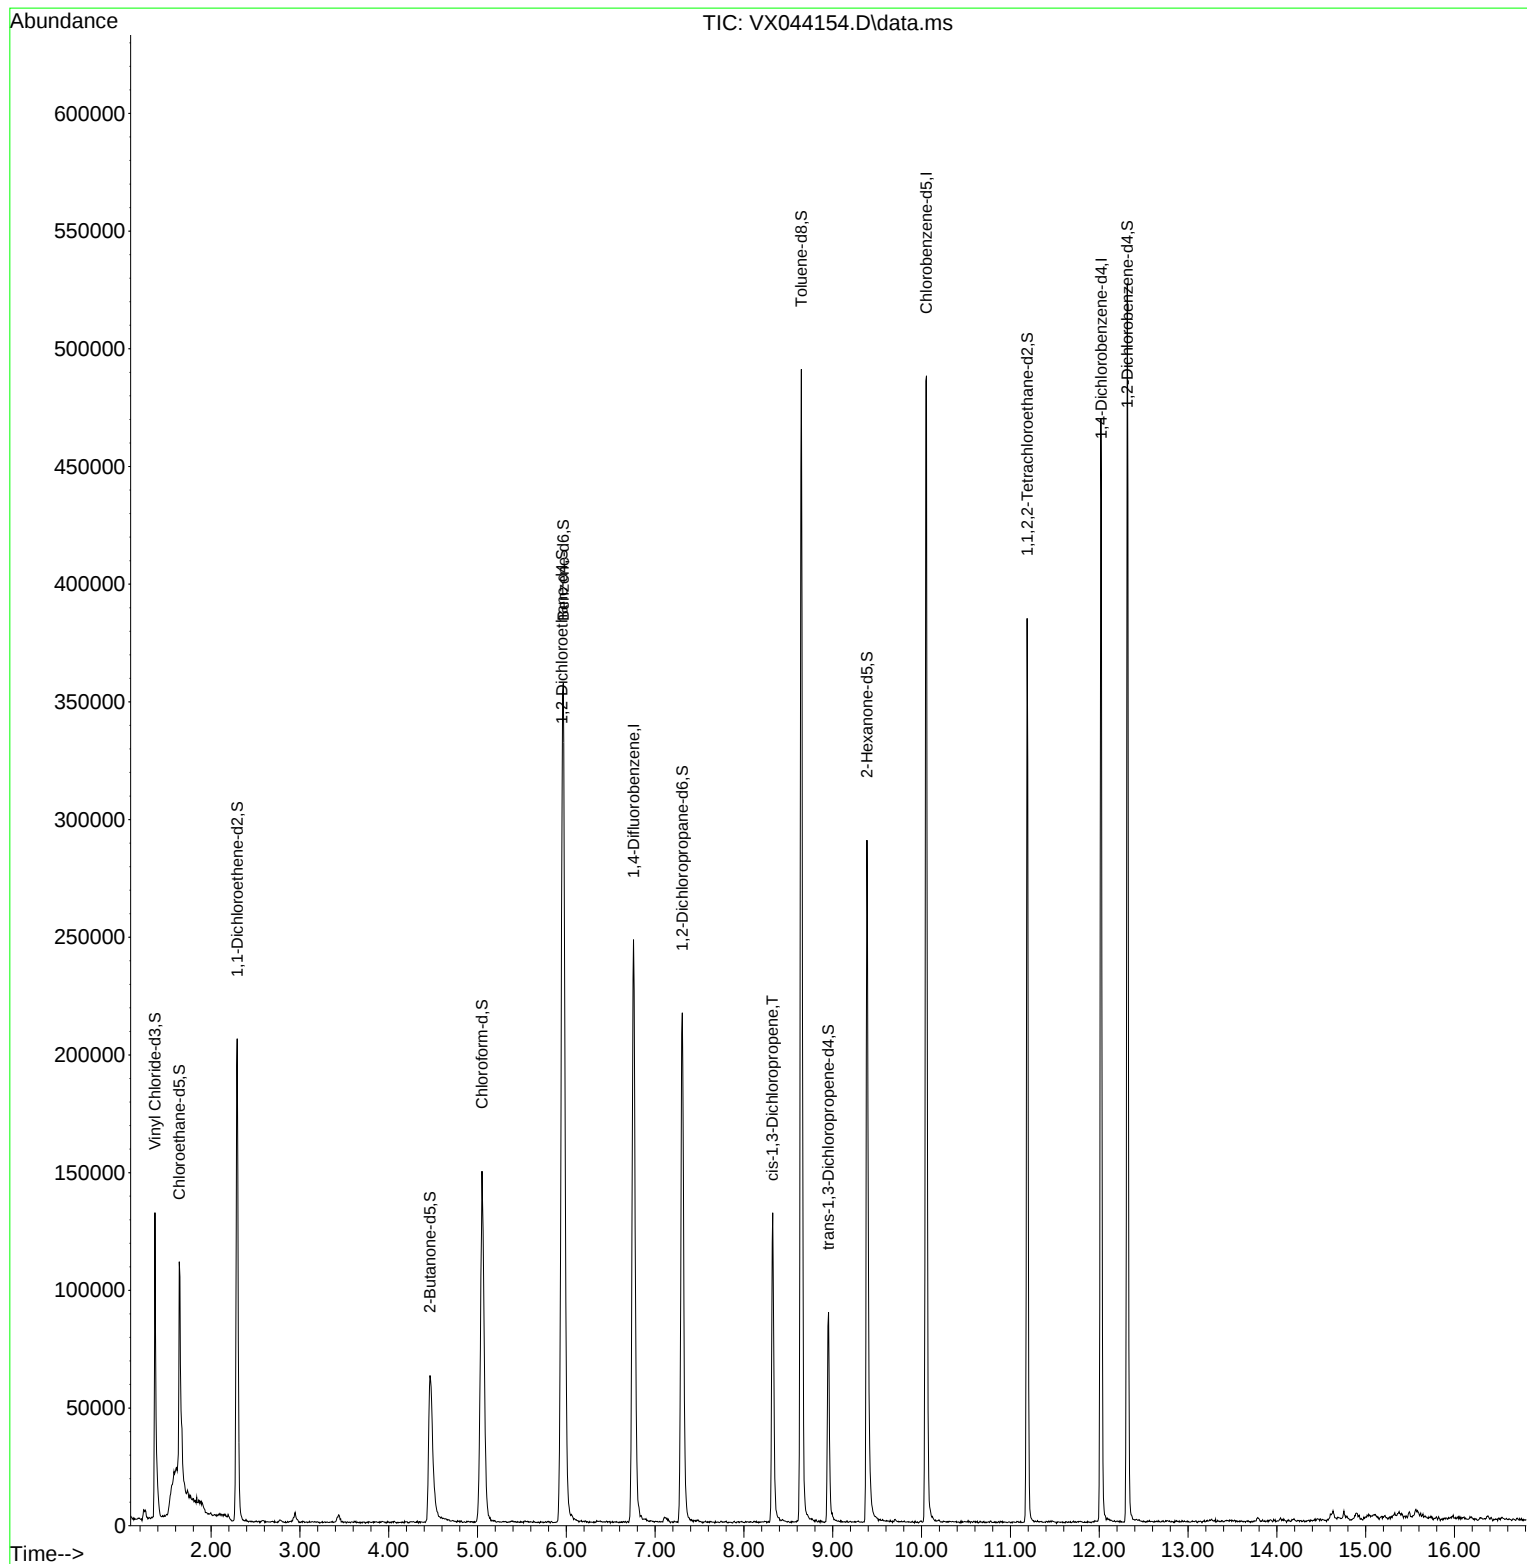

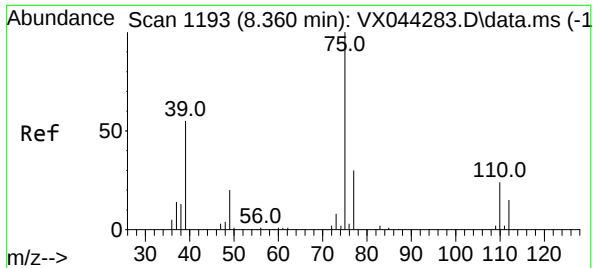

#39
 cis-1,3-Dichloropropene
 Concen: 1.356 ug/L
 RT: 8.318 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VX044154.D
 Acq: 05 Dec 2024 17:49

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 75 Resp: 3667
 Ion Ratio Lower Upper
 75 100
 77 34.0 21.6 40.0

