

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120524\
 Data File : VX044156.D
 Acq On : 05 Dec 2024 18:36
 Operator : JC/MD
 Sample : P5066-13 20X
 Misc : 5.74g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 06 04:10:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 06 03:51:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	228375	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	202223	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	82582	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	84283	40.329	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	80.660%		
7) Chloroethane-d5	1.642	69	60251	37.217	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	74.440%		
11) 1,1-Dichloroethene-d2	2.288	65	35573	39.800	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	79.600%		
21) 2-Butanone-d5	4.465	46	109735	85.761	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	85.760%		
24) Chloroform-d	5.056	84	161424	40.681	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.360%		
26) 1,2-Dichloroethane-d4	5.952	65	116185	41.404	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.800%		
32) Benzene-d6	5.964	84	297108	42.520	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.040%		
36) 1,2-Dichloropropane-d6	7.306	67	92915	42.825	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	85.640%		
41) Toluene-d8	8.647	98	269613	41.731	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.460%		
43) trans-1,3-Dichloroprop...	8.952	79	39518	37.902	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	75.800%		
47) 2-Hexanone-d5	9.385	63	77025	91.050	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	91.050%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	127295	43.755	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.520%		
66) 1,2-Dichlorobenzene-d4	12.317	152	86410	44.909	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.820%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	8.318	75	3679	1.424	ug/L #	76
61) 1,2,3-Trichloropropane	12.018	75	12449	6.509	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120524\
Data File : VX044156.D
Acq On : 05 Dec 2024 18:36
Operator : JC/MD
Sample : P5066-13 20X
Misc : 5.74g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Dec 06 04:10:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 06 03:51:43 2024
Response via : Initial Calibration




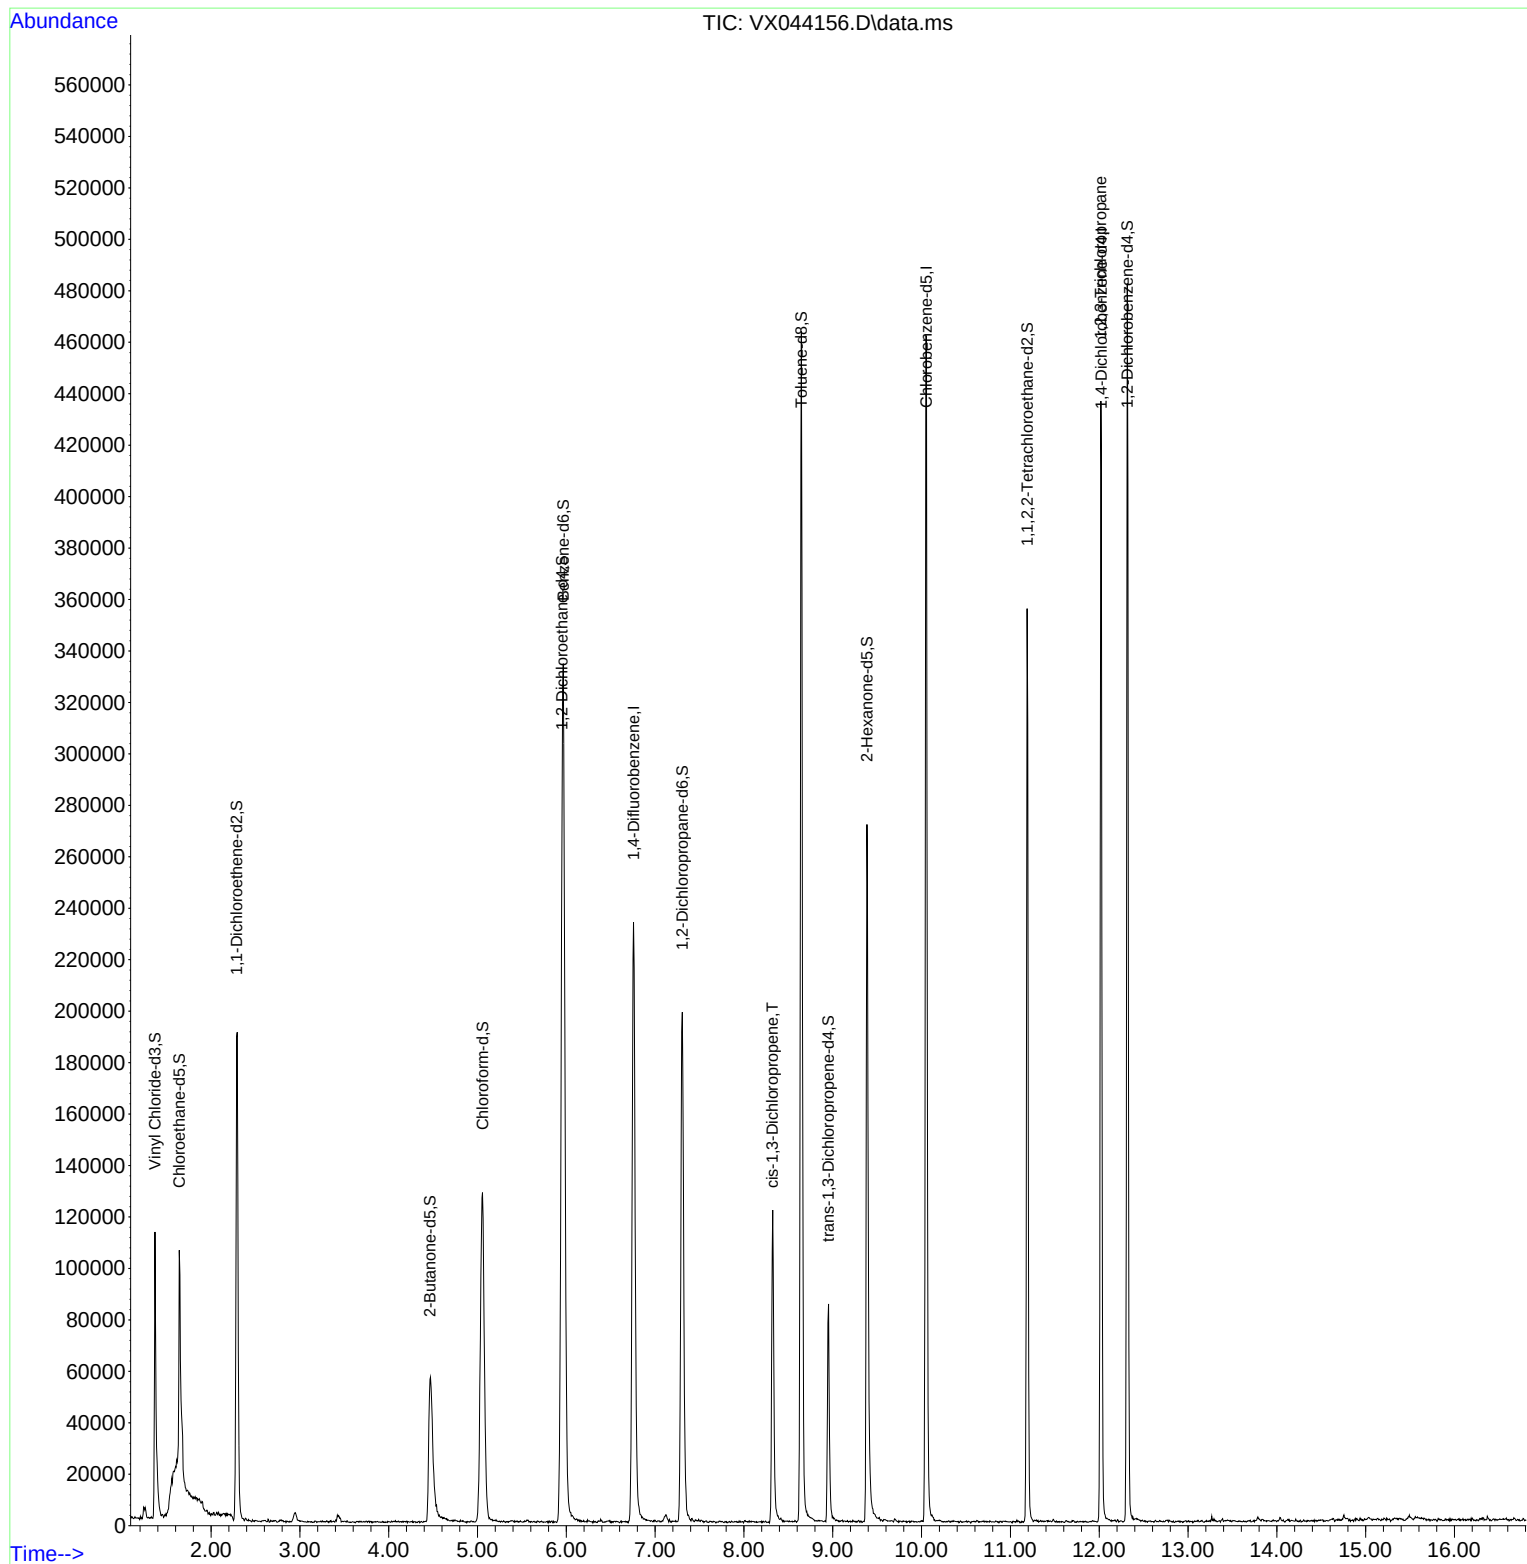


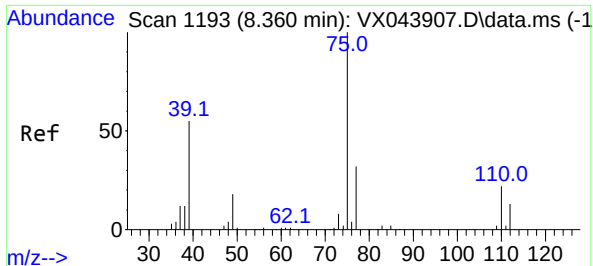

#39
cis-1,3-Dichloropropene
Concen: 1.424 ug/L
RT: 8.318 min Scan# 1193
Delta R.T. -0.049 min
Lab File: VX044156.D
Acq: 05 Dec 2024 18:36

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 75 Resp: 3679
Ion Ratio Lower Upper
75 100
77 44.2 21.6 40.0#

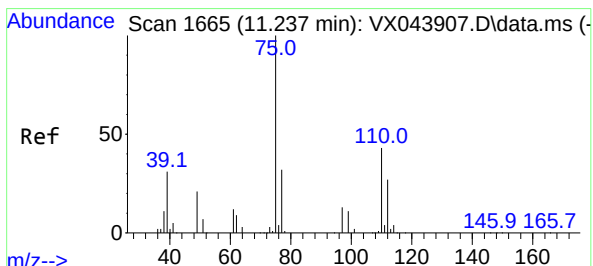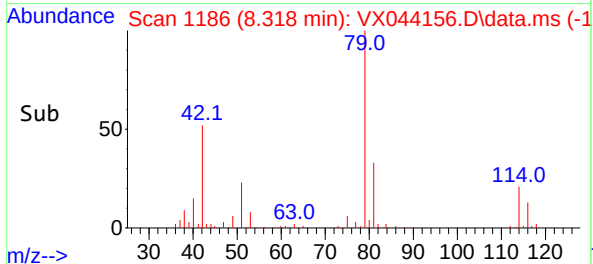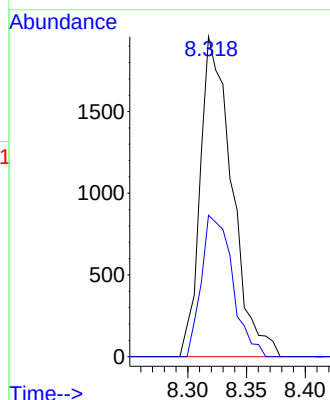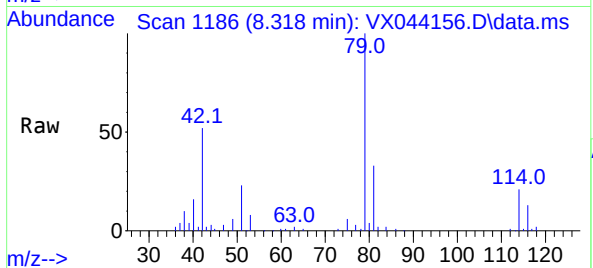

#61
1,2,3-Trichloropropane
Concen: 6.509 ug/L
RT: 12.018 min Scan# 1793
Delta R.T. 0.780 min
Lab File: VX044156.D
Acq: 05 Dec 2024 18:36

Tgt Ion: 75 Resp: 12449
Ion Ratio Lower Upper
75 100
77 33.9 25.8 38.6
110 3.5 33.3 49.9#

