

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120524\
 Data File : VX044158.D
 Acq On : 05 Dec 2024 19:22
 Operator : JC/MD
 Sample : P5066-15 20X
 Misc : 6.65g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 06 04:10:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 06 03:51:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	221113	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	193866	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	78958	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	79885	39.480	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	78.960%		
7) Chloroethane-d5	1.642	69	59753	38.121	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	76.240%		
11) 1,1-Dichloroethene-d2	2.294	65	34046	39.343	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.680%		
21) 2-Butanone-d5	4.465	46	106403	85.888	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	85.890%		
24) Chloroform-d	5.056	84	154531	40.223	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.440%		
26) 1,2-Dichloroethane-d4	5.952	65	111280	40.958	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.920%		
32) Benzene-d6	5.964	84	286482	42.767	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.540%		
36) 1,2-Dichloropropane-d6	7.306	67	89730	43.140	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	86.280%		
41) Toluene-d8	8.647	98	246413	39.784	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	79.560#		
43) trans-1,3-Dichloroprop...	8.952	79	36523	36.539	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	73.080%		
47) 2-Hexanone-d5	9.384	63	71767	88.491	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	88.490%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	120380	43.162	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	86.320%		
66) 1,2-Dichlorobenzene-d4	12.317	152	76662	41.671	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.340%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	8.324	75	3146	1.271	ug/L #	66
61) 1,2,3-Trichloropropane	12.018	75	10643	5.820	ug/L #	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120524\
Data File : VX044158.D
Acq On : 05 Dec 2024 19:22
Operator : JC/MD
Sample : P5066-15 20X
Misc : 6.65g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Dec 06 04:10:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 06 03:51:43 2024
Response via : Initial Calibration

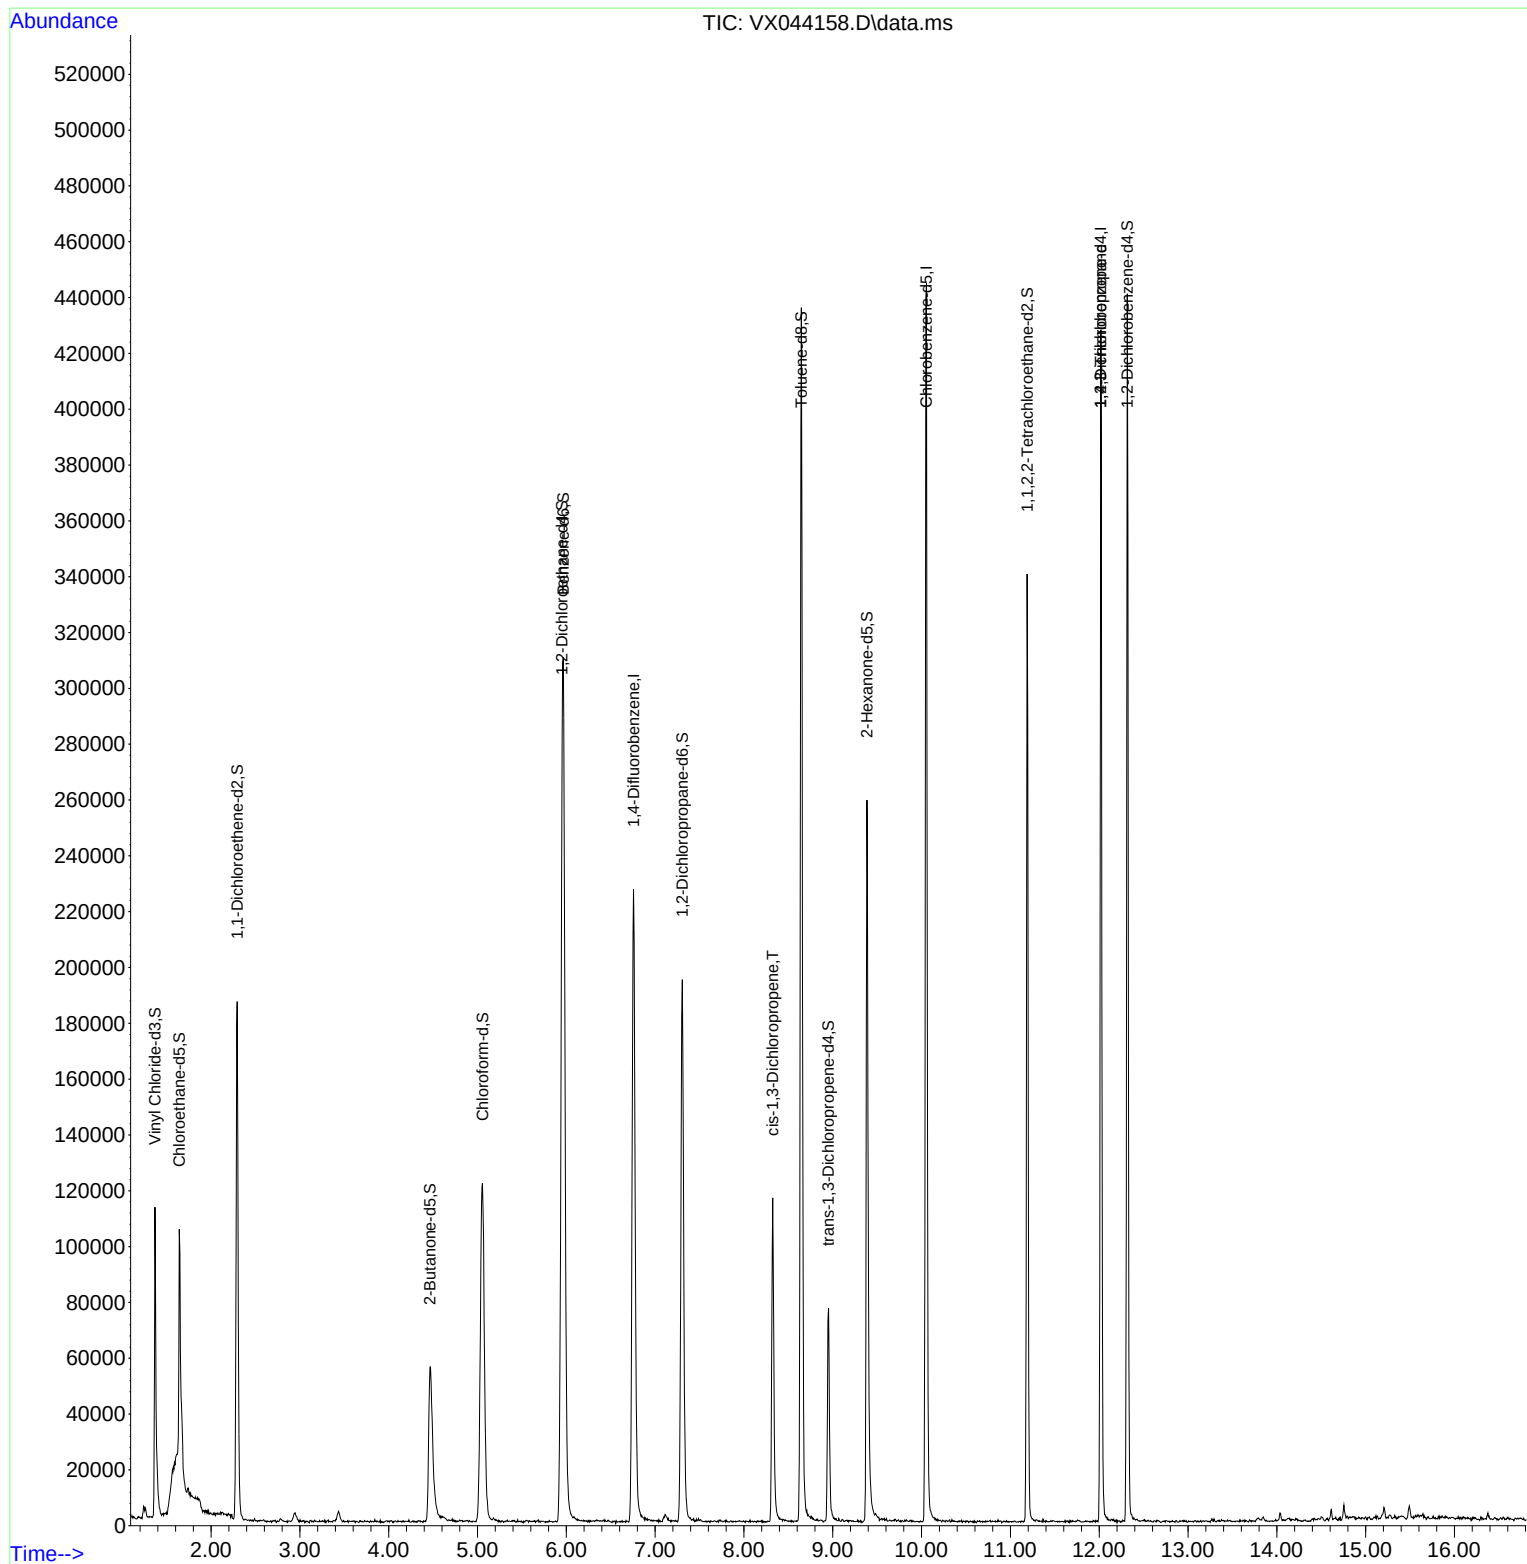

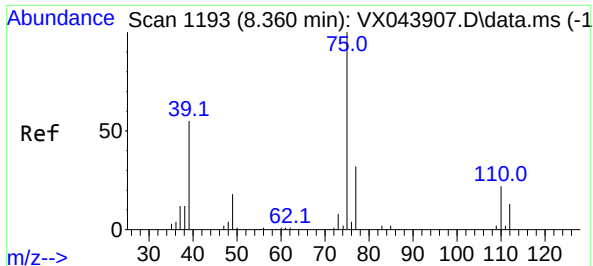

#39

cis-1,3-Dichloropropene

Concen: 1.271 ug/L

RT: 8.324 min Scan# 1193

Delta R.T. -0.043 min

Lab File: VX044158.D

Acq: 05 Dec 2024 19:22

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 3146

Ion Ratio Lower Upper

75 100

77 49.6 21.6 40.0#

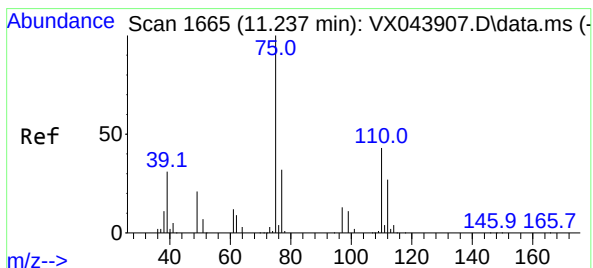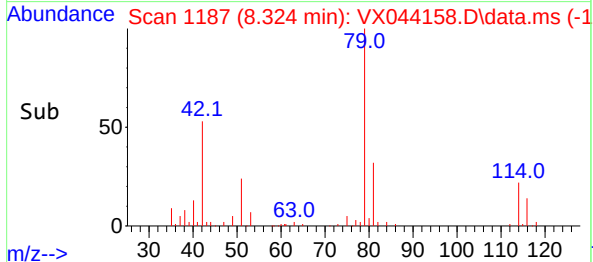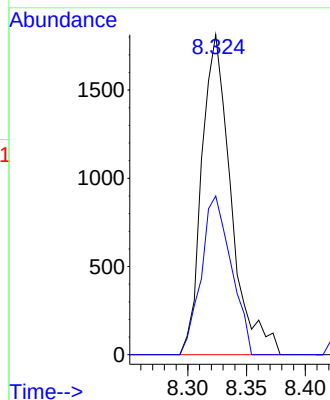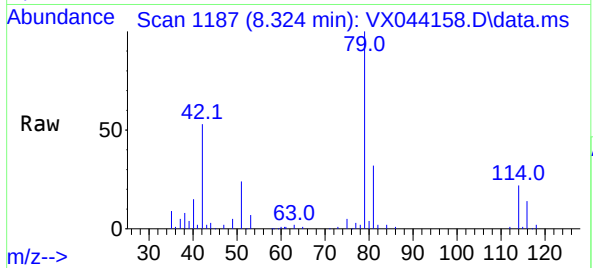

#61

1,2,3-Trichloropropane

Concen: 5.820 ug/L

RT: 12.018 min Scan# 1793

Delta R.T. 0.780 min

Lab File: VX044158.D

Acq: 05 Dec 2024 19:22

Tgt Ion: 75 Resp: 10643

Ion Ratio Lower Upper

75 100

77 37.0 25.8 38.6

110 3.5 33.3 49.9#

