

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120524\
 Data File : VX044142.D
 Acq On : 05 Dec 2024 12:10
 Operator : JC/MD
 Sample : VIBLK683
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK683

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044142.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	23	25	26	rBV	4030	2633	0.23%	0.032%
2	1.367	42	46	57	rBV	141800	167984	14.70%	2.042%
3	1.648	88	92	101	rVB	109199	162655	14.23%	1.977%
4	2.294	192	198	211	rVB	256181	387217	33.87%	4.707%
5	2.501	228	232	237	rVB	4648	6989	0.61%	0.085%
6	2.593	245	247	248	rBV2	614	529	0.05%	0.006%
7	2.782	271	278	284	rBV7	2413	5386	0.47%	0.065%
8	2.940	299	304	306	rBV5	1639	2898	0.25%	0.035%
9	3.087	322	328	336	rBV4	4827	10572	0.92%	0.129%
10	3.148	336	338	342	rVV2	924	792	0.07%	0.010%
11	3.428	380	384	392	rVB4	2782	6133	0.54%	0.075%
12	3.623	414	416	418	rVB2	1289	908	0.08%	0.011%
13	3.647	418	420	422	rBV2	511	544	0.05%	0.007%
14	3.708	429	430	432	rBV	621	618	0.05%	0.008%
15	4.007	477	479	483	rVV3	734	1013	0.09%	0.012%
16	4.227	512	515	517	rBV	535	630	0.06%	0.008%
17	4.294	523	526	529	rBV4	542	643	0.06%	0.008%
18	4.458	546	553	569	rBV2	72596	227011	19.86%	2.760%
19	4.720	594	596	597	rBV2	695	614	0.05%	0.007%
20	4.891	622	624	626	rBV2	1056	1327	0.12%	0.016%
21	4.964	632	636	639	rVB5	712	943	0.08%	0.011%
22	5.056	639	651	671	rBV	151429	482582	42.22%	5.866%
23	5.373	701	703	706	rBV4	978	863	0.08%	0.010%
24	5.537	729	730	732	rBV2	593	561	0.05%	0.007%
25	5.653	747	749	750	rBV2	1037	867	0.08%	0.011%
26	5.964	788	800	817	rBV3	378100	1143095	100.00%	13.896%
27	6.421	874	875	878	rBV4	619	589	0.05%	0.007%
28	6.488	884	886	889	rBV4	646	722	0.06%	0.009%
29	6.757	922	930	946	rBV	236725	567313	49.63%	6.896%
30	7.019	971	973	977	rVB2	765	764	0.07%	0.009%
31	7.122	984	990	997	rVV7	5309	14018	1.23%	0.170%
32	7.208	1002	1004	1006	rBV3	538	518	0.05%	0.006%
33	7.305	1012	1020	1030	rBV	230380	516301	45.17%	6.276%
34	7.616	1069	1071	1075	rBV3	740	967	0.08%	0.012%
35	7.677	1079	1081	1083	rBV2	611	591	0.05%	0.007%
36	7.824	1103	1105	1108	rBV3	813	933	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120524\
 Data File : VX044142.D
 Acq On : 05 Dec 2024 12:10
 Operator : JC/MD
 Sample : VIBLK683
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK683

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

37	8.013	1134	1136	1139	rVB3	829	762	0.07%	0.009%
38	8.043	1139	1141	1143	rBV2	676	649	0.06%	0.008%
39	8.323	1181	1187	1202	rBV	150741	262814	22.99%	3.195%
40	8.579	1227	1229	1233	rBV3	1139	1291	0.11%	0.016%
41	8.647	1234	1240	1249	rBV	538148	858600	75.11%	10.437%
42	8.866	1272	1276	1279	rBV5	817	1387	0.12%	0.017%
43	8.945	1284	1289	1300	rBV	107459	173970	15.22%	2.115%
44	9.165	1319	1325	1331	rBV6	1633	3220	0.28%	0.039%
45	9.274	1338	1343	1351	rBV4	6569	11359	0.99%	0.138%
46	9.384	1356	1361	1378	rBV	326117	500484	43.78%	6.084%
47	9.610	1394	1398	1406	rVB4	1595	3334	0.29%	0.041%
48	9.695	1411	1412	1414	rBV2	1053	753	0.07%	0.009%
49	9.787	1426	1427	1430	rBV2	652	685	0.06%	0.008%
50	9.854	1436	1438	1443	rVB2	919	958	0.08%	0.012%
51	9.902	1443	1446	1449	rBV2	448	639	0.06%	0.008%
52	10.049	1465	1470	1487	rVV	464275	688978	60.27%	8.375%
53	10.195	1490	1494	1503	rVV2	6971	11671	1.02%	0.142%
54	10.262	1503	1505	1508	rVV3	683	731	0.06%	0.009%
55	10.305	1508	1512	1519	rVB2	6773	10933	0.96%	0.133%
56	10.463	1536	1538	1540	rBV2	848	721	0.06%	0.009%
57	10.597	1556	1560	1562	rBV3	622	845	0.07%	0.010%
58	10.658	1562	1570	1578	rBV4	6986	18223	1.59%	0.222%
59	10.963	1615	1620	1625	rBV2	6964	9533	0.83%	0.116%
60	11.006	1625	1627	1631	rVB4	557	762	0.07%	0.009%
61	11.103	1639	1643	1646	rBV5	653	1028	0.09%	0.012%
62	11.189	1652	1657	1665	rBV	395623	522126	45.68%	6.347%
63	11.311	1675	1677	1679	rBV2	1023	825	0.07%	0.010%
64	11.451	1696	1700	1705	rVB	8238	9861	0.86%	0.120%
65	11.579	1719	1721	1724	rBV2	519	630	0.06%	0.008%
66	11.756	1745	1750	1753	rVV2	7845	10633	0.93%	0.129%
67	11.859	1764	1767	1768	rBV3	696	635	0.06%	0.008%
68	11.969	1782	1785	1789	rBV	11355	15476	1.35%	0.188%
69	12.018	1789	1793	1804	rVB	435860	578191	50.58%	7.029%
70	12.213	1821	1825	1827	rVB3	512	588	0.05%	0.007%
71	12.243	1827	1830	1833	rBV2	1373	1316	0.12%	0.016%
72	12.274	1833	1835	1837	rBV3	682	777	0.07%	0.009%
73	12.317	1837	1842	1852	rBV	534283	701840	61.40%	8.532%
74	12.432	1859	1861	1863	rVB3	809	593	0.05%	0.007%
75	12.506	1871	1873	1875	rVB3	683	518	0.05%	0.006%
76	12.762	1912	1915	1920	rBV4	1152	1330	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120524\
 Data File : VX044142.D
 Acq On : 05 Dec 2024 12:10
 Operator : JC/MD
 Sample : VIBLK683
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK683

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	12.841	1926	1928	1932	rBV3	644	608	0.05%	0.007%
78	12.945	1943	1945	1952	rVB4	1138	1781	0.16%	0.022%
79	12.993	1952	1953	1956	rBV3	576	571	0.05%	0.007%
80	13.115	1968	1973	1978	rBV4	9159	13108	1.15%	0.159%
81	13.316	2005	2006	2009	rBV2	709	727	0.06%	0.009%
82	13.390	2015	2018	2020	rBV2	795	1177	0.10%	0.014%
83	13.444	2026	2027	2030	rBV3	613	523	0.05%	0.006%
84	13.591	2047	2051	2057	rVV2	10479	15395	1.35%	0.187%
85	13.780	2077	2082	2092	rVV	23555	32852	2.87%	0.399%
86	13.877	2096	2098	2100	rBV2	766	642	0.06%	0.008%
87	13.963	2107	2112	2120	rBV3	12184	18936	1.66%	0.230%
88	14.127	2136	2139	2143	rBV3	2041	2688	0.24%	0.033%
89	14.487	2196	2198	2201	rVB3	585	600	0.05%	0.007%
90	14.554	2206	2209	2212	rVV3	678	687	0.06%	0.008%
91	14.639	2220	2223	2224	rBV	546	674	0.06%	0.008%
92	14.682	2227	2230	2232	rVB4	548	642	0.06%	0.008%
93	14.822	2252	2253	2259	rVB3	814	1036	0.09%	0.013%
94	14.877	2259	2262	2264	rBV2	597	667	0.06%	0.008%
95	14.902	2264	2266	2268	rVB2	900	655	0.06%	0.008%
96	14.938	2268	2272	2273	rBV3	507	595	0.05%	0.007%
97	15.182	2309	2312	2313	rBV3	593	535	0.05%	0.007%
98	15.865	2422	2424	2426	rBV3	800	682	0.06%	0.008%
99	15.895	2426	2429	2432	rBV4	899	1196	0.10%	0.015%
100	16.499	2526	2528	2531	rVB3	865	743	0.06%	0.009%


Sum of corrected areas: 8226112

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120524\
Data File : VX044142.D
Acq On : 05 Dec 2024 12:10
Operator : JC/MD
Sample : VIBLK683
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK683

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

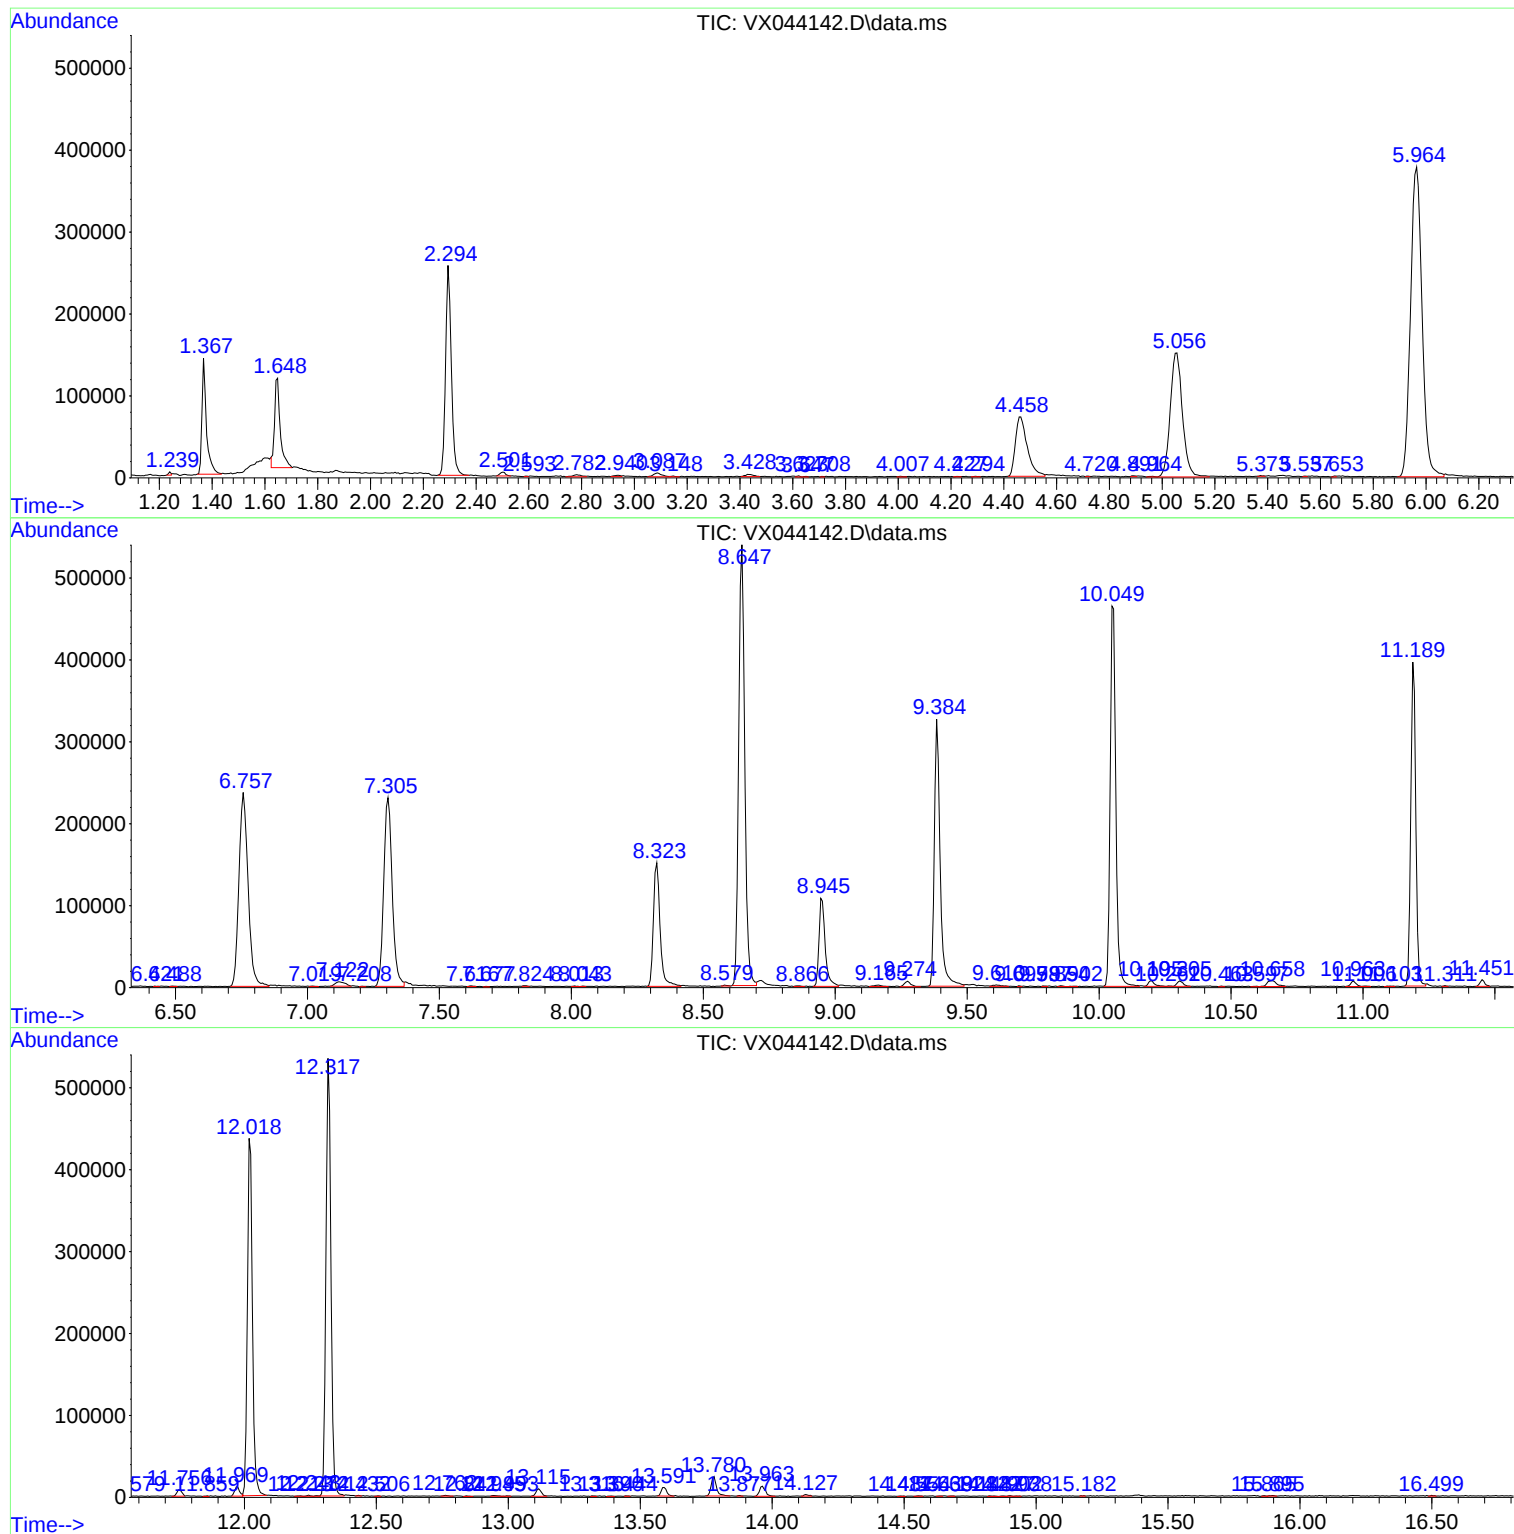

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120524\
Data File : VX044142.D
Acq On : 05 Dec 2024 12:10
Operator : JC/MD
Sample : VIBLK683
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK683

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120524\
Data File : VX044142.D
Acq On : 05 Dec 2024 12:10
Operator : JC/MD
Sample : VIBLK683
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK683

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc