
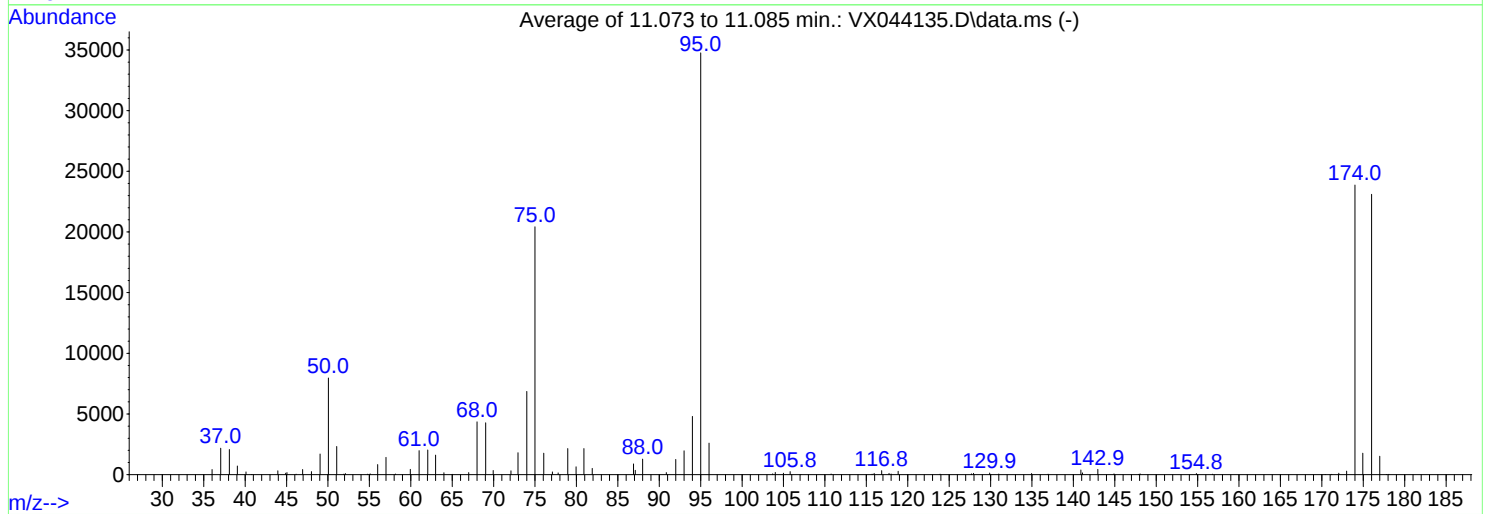


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120524\
Data File : VX044135.D
Acq On : 05 Dec 2024 08:43
Operator : JC/MD
Sample : BFB703
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB703

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Title : VOC Analysis
Last Update : Sat Dec 07 03:56:15 2024

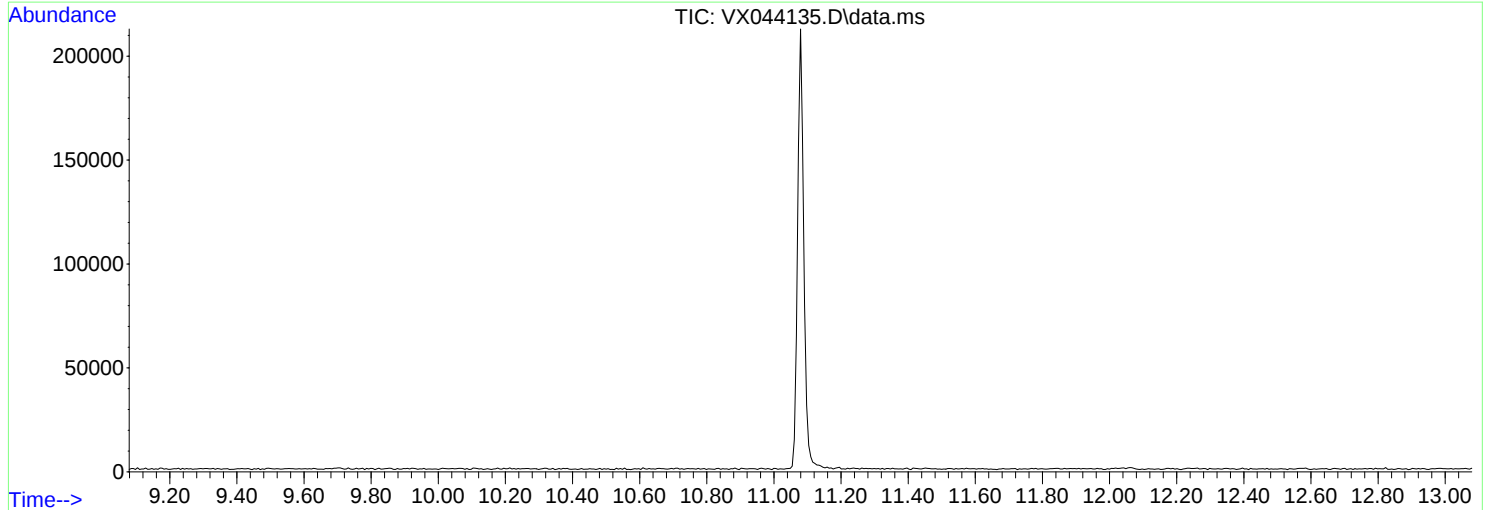

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.9	7960	PASS
75	95	30	80	58.7	20421	PASS
95	95	100	100	100.0	34763	PASS
96	95	5	9	7.5	2592	PASS
173	174	0.00	2	1.2	297	PASS
174	95	50	120	68.7	23872	PASS
175	174	5	9	7.4	1771	PASS
176	174	95	101	96.8	23104	PASS
177	176	5	9	6.6	1516	PASS

m/z	Abundance
38.50	203.0
39.10	511.0
39.90	517.0
41.10	113.0
43.90	163.0

Instrument :
MSVOA_X
ClientSampleId :
BFB703

m/z	Abundance
36.00	361.0
37.10	2114.0
38.10	2187.0
39.00	1433.0
39.90	450.0
40.80	54.0
44.00	463.0
44.90	351.0
46.20	68.0
46.90	305.0
48.00	163.0
49.00	1545.0
50.00	7296.0
51.00	2277.0
51.90	113.0
55.10	136.0
56.10	662.0
57.00	1499.0
58.10	60.0
59.90	466.0
61.00	1827.0
62.00	1962.0
63.00	1309.0
63.90	117.0
67.00	120.0
68.00	4146.0
69.00	4186.0
69.90	207.0
72.10	335.0
73.00	1865.0
74.00	6490.0
75.00	18424.0
76.00	1946.0
77.10	233.0
77.80	181.0
78.90	2007.0
79.90	553.0
80.90	2057.0
81.90	527.0
86.90	1293.0
87.90	1241.0
90.90	246.0
92.00	1467.0
93.00	1476.0
94.00	4358.0
95.00	32368.0
96.00	2292.0
103.70	202.0
105.00	85.0
105.80	320.0
110.80	103.0
115.70	125.0
116.90	210.0
117.80	153.0
118.80	230.0
123.90	66.0
127.70	201.0
130.00	90.0
131.00	89.0
134.90	89.0
137.00	79.0
140.90	520.0
143.00	253.0
144.90	96.0
147.90	65.0
154.90	108.0
156.80	82.0
172.10	87.0
173.00	283.0
174.00	18736.0
174.90	1429.0
176.00	16816.0
177.00	1108.0
178.10	66.0

Instrument :
MSVOA_X
ClientSampleId :
BFB703

m/z	Abundance
35.90	614.0
37.00	2689.0
38.10	2547.0
39.00	1178.0
40.10	658.0
44.00	658.0
45.10	324.0
47.00	612.0
47.90	258.0
49.10	2209.0
50.10	10007.0
51.10	2797.0
52.10	112.0
54.80	112.0
56.00	1045.0
57.00	1687.0
58.20	90.0
60.00	536.0
61.00	2317.0
62.00	2470.0
63.00	1948.0
64.00	198.0
67.10	189.0
68.00	5149.0
69.00	4782.0
70.00	513.0
72.10	398.0
73.00	2114.0
74.00	8019.0
75.00	24952.0
76.10	1997.0
77.20	297.0
77.80	185.0
78.90	2619.0
80.00	815.0
80.90	2460.0
81.90	520.0
86.90	1366.0
88.00	1610.0
90.80	153.0
92.00	1063.0
93.00	2678.0
94.00	5300.0
95.00	40280.0
96.00	3382.0
104.00	302.0
105.00	164.0
105.90	216.0
107.10	52.0
110.70	56.0
116.00	185.0
116.90	469.0
117.70	178.0
118.90	346.0
123.90	62.0
127.90	185.0
129.80	125.0
131.00	85.0
134.90	113.0
136.90	56.0
140.90	627.0
142.90	589.0
144.90	85.0
148.10	113.0
154.80	118.0
156.80	55.0
170.40	61.0
171.20	78.0
172.00	136.0
173.00	423.0
174.00	29448.0
175.00	2204.0
176.00	28648.0
177.00	1975.0

Instrument :
MSVOA_X
ClientSampleId :
BFB703

m/z	Abundance
36.10	281.0
37.10	1712.0
38.10	1472.0
39.10	1067.0
39.90	421.0
44.00	336.0
45.00	205.0
46.10	54.0
47.00	352.0
48.10	330.0
49.00	1344.0
50.00	6578.0
51.00	1881.0
52.10	156.0
55.10	84.0
55.90	780.0
57.00	1105.0
59.90	302.0
61.00	1812.0
62.10	1669.0
63.00	1566.0
64.10	156.0
65.00	65.0
66.90	194.0
68.00	3754.0
69.10	3855.0
69.90	304.0
72.10	224.0
72.90	1433.0
74.00	6067.0
75.00	17888.0
76.00	1354.0
77.00	140.0
77.80	83.0
79.00	1829.0
80.00	558.0
80.90	1942.0
81.90	483.0
87.10	1056.0
88.10	995.0
90.80	110.0
92.00	1241.0
93.00	1732.0
94.00	4760.0
95.00	31640.0
96.00	2103.0
104.00	243.0
105.00	100.0
105.70	202.0
115.90	136.0
116.80	320.0
118.00	170.0
118.80	252.0
128.00	132.0
129.90	169.0
135.00	79.0
141.10	438.0
142.90	448.0
148.00	101.0
154.90	69.0
172.00	133.0
172.90	185.0
174.00	23432.0
174.90	1681.0
176.00	23848.0
177.00	1466.0
177.80	57.0

Instrument :
MSVOA_X
ClientSampleId :
BFB703