

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120525\
 Data File : VX048738.D
 Acq On : 05 Dec 2025 15:55
 Operator : JC/MD
 Sample : Q3789-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Quant Time: Dec 05 22:06:52 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120425W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 05 03:27:34 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	140193	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.745	114	290551	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	224650	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	129713	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.940	65	128233	68.149	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	136.300%#
35) Dibromofluoromethane	5.373	113	87231	43.603	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	87.200%
50) Toluene-d8	8.635	98	293644	41.874	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	83.740%#
62) 4-Bromofluorobenzene	11.061	95	104604	43.258	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	86.520%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120525\
Data File : VX048738.D
Acq On : 05 Dec 2025 15:55
Operator : JC/MD
Sample : Q3789-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Time: Dec 05 22:06:52 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120425W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 05 03:27:34 2025
Response via : Initial Calibration




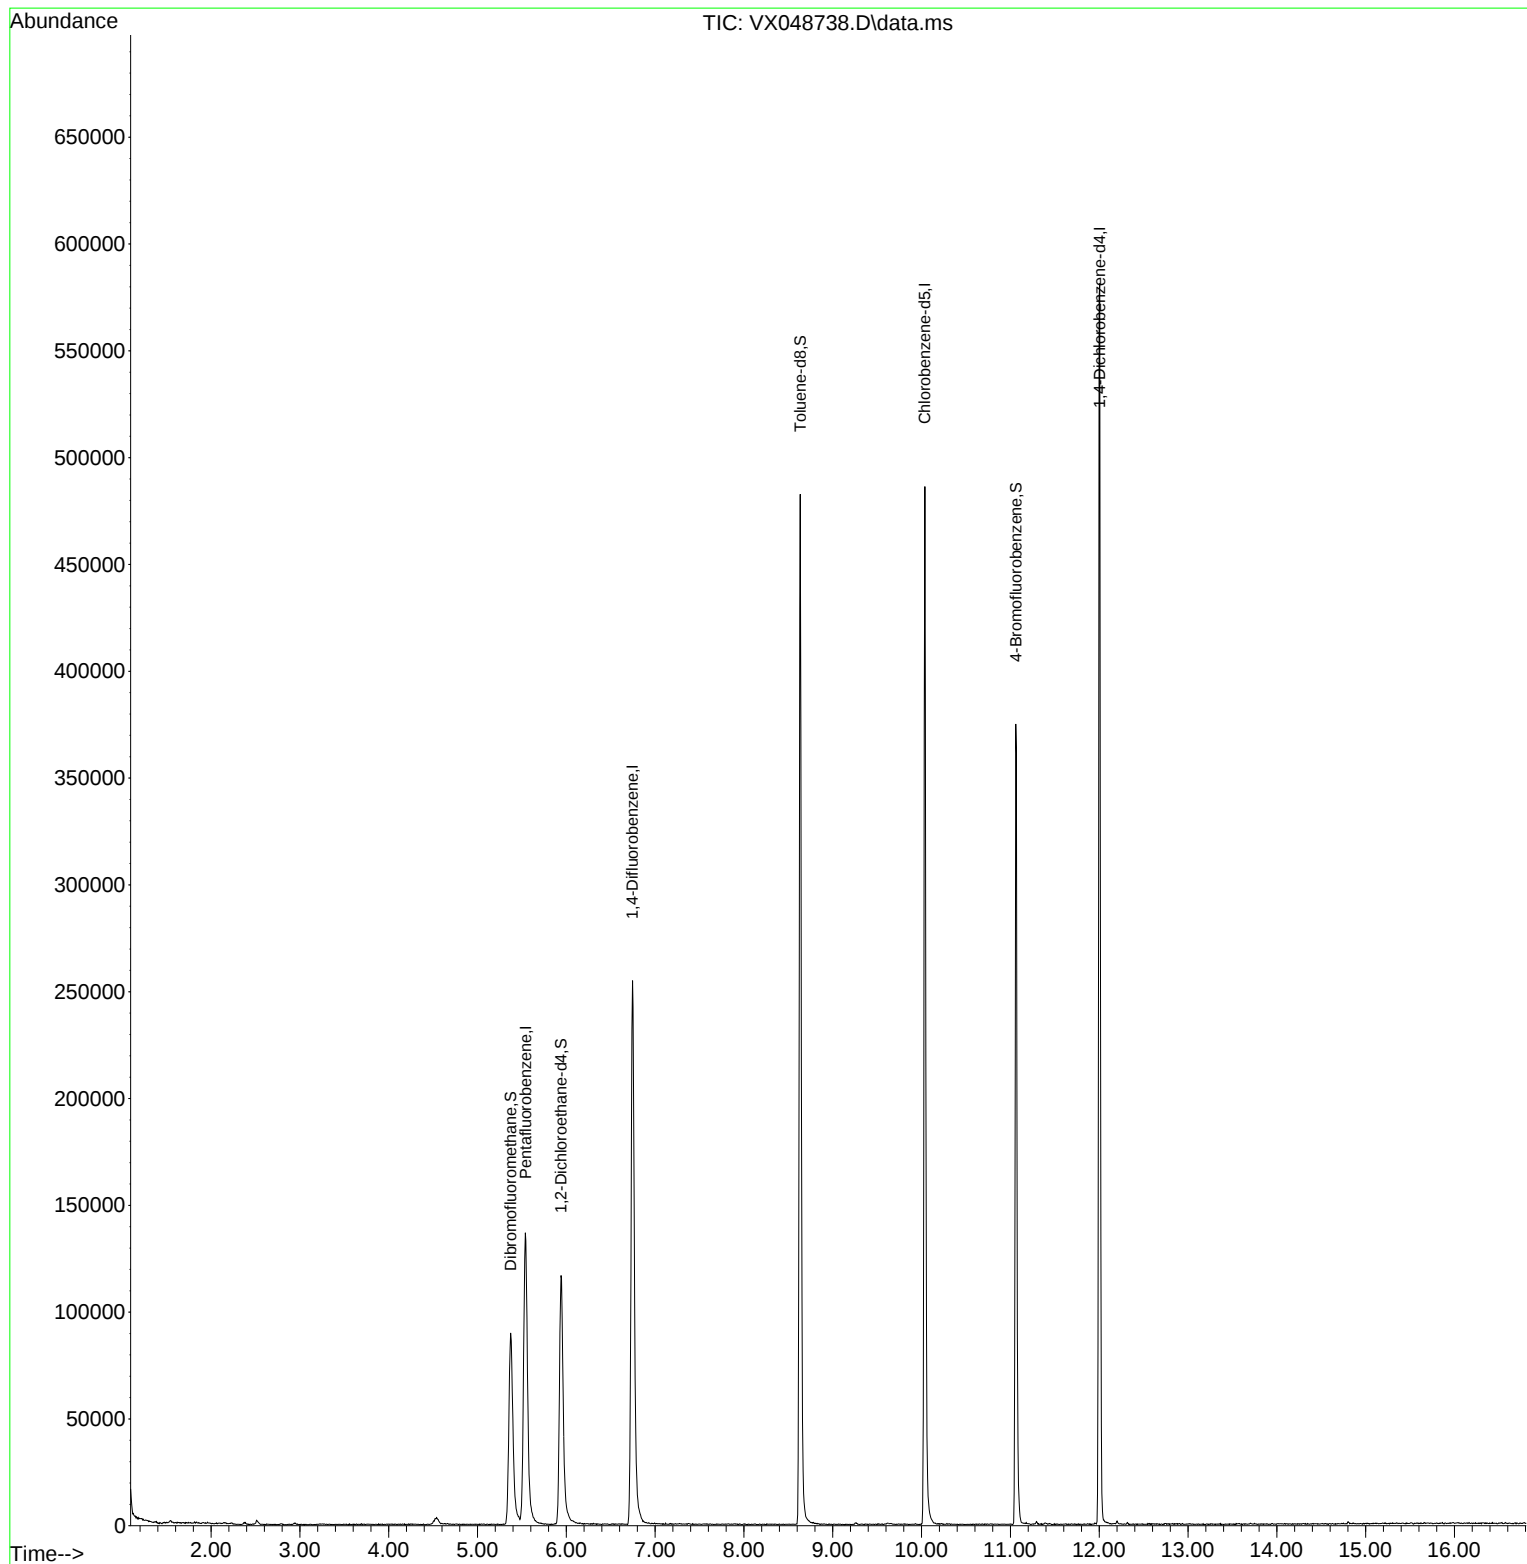


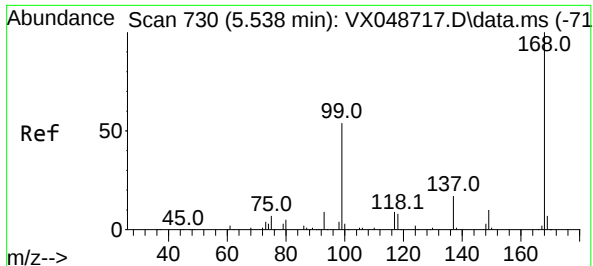

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 731
Delta R.T. 0.006 min
Lab File: VX048738.D
Acq: 05 Dec 2025 15:55




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:168 Resp: 140193
Ion Ratio Lower Upper
168 100
99 57.3 44.2 66.4

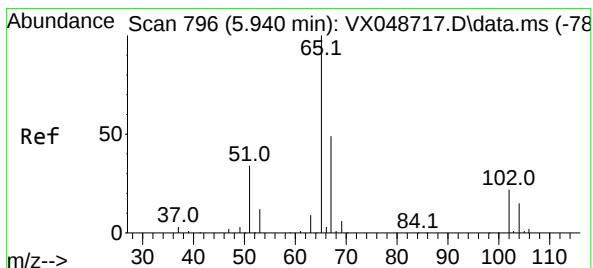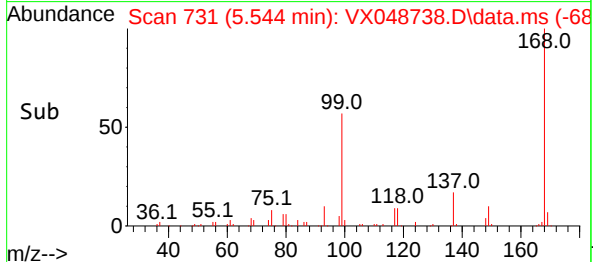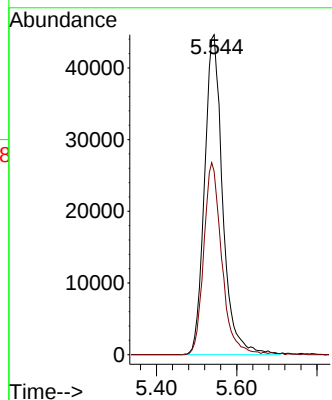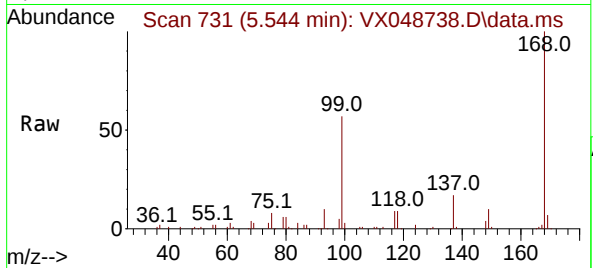

#33
1,2-Dichloroethane-d4
Concen: 68.149 ug/l
RT: 5.940 min Scan# 796
Delta R.T. -0.000 min
Lab File: VX048738.D
Acq: 05 Dec 2025 15:55

Tgt Ion: 65 Resp: 128233
Ion Ratio Lower Upper
65 100
67 52.9 0.0 107.4


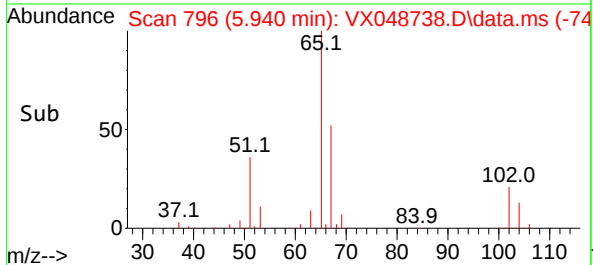
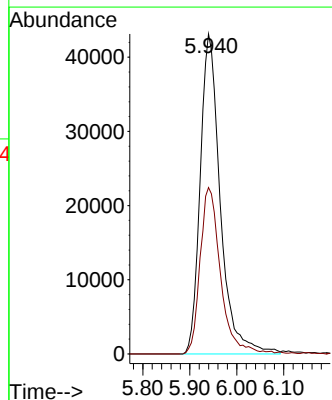
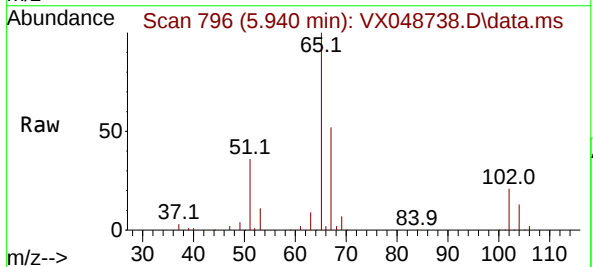


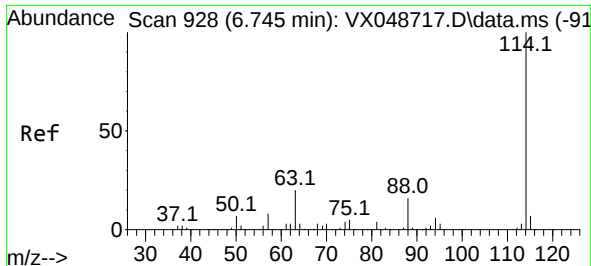

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.745 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX048738.D
Acq: 05 Dec 2025 15:55




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:114 Resp: 290551
Ion Ratio Lower Upper
114 100
63 20.6 0.0 39.0
88 15.0 0.0 31.8

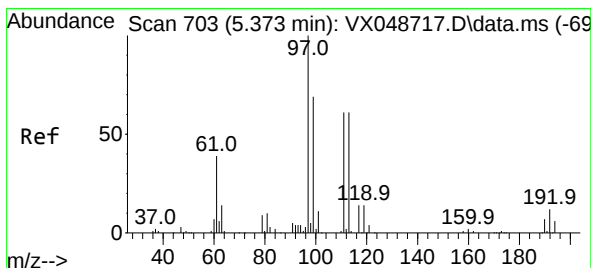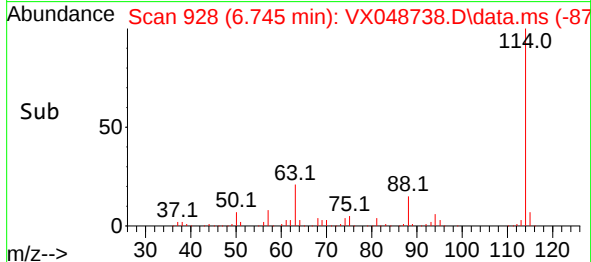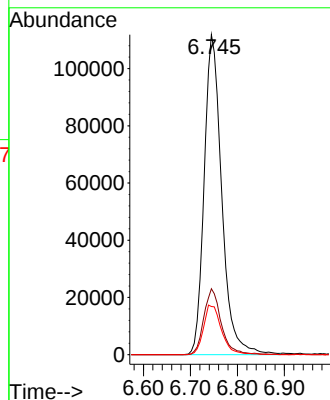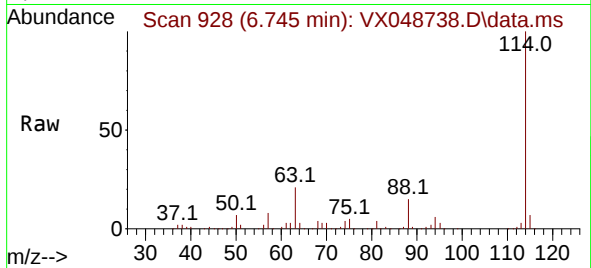

#35
Dibromofluoromethane
Concen: 43.603 ug/l
RT: 5.373 min Scan# 703
Delta R.T. -0.000 min
Lab File: VX048738.D
Acq: 05 Dec 2025 15:55

Tgt Ion:113 Resp: 87231
Ion Ratio Lower Upper
113 100
111 103.4 79.5 119.3
192 19.1 16.1 24.1


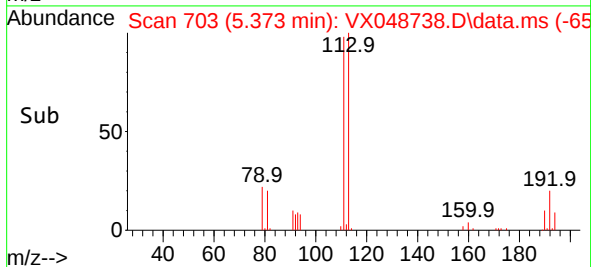
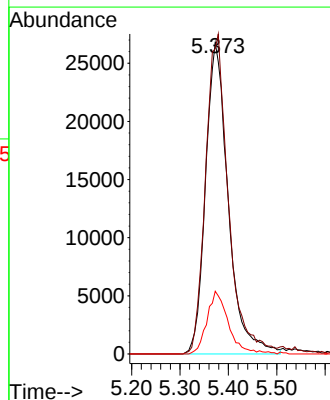
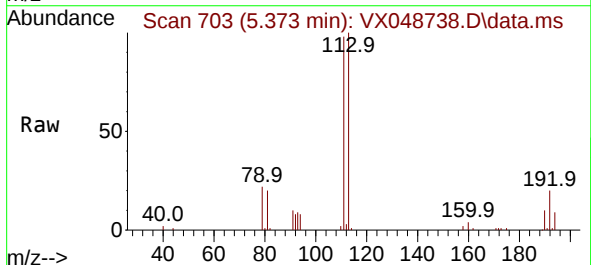


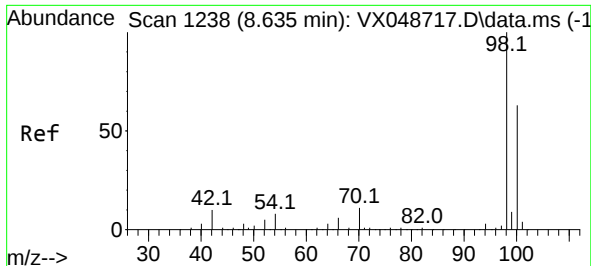

#50
Toluene-d8
Concen: 41.874 ug/l
RT: 8.635 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX048738.D
Acq: 05 Dec 2025 15:55




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion: 98 Resp: 293644
Ion Ratio Lower Upper
98 100
100 65.1 53.4 80.0

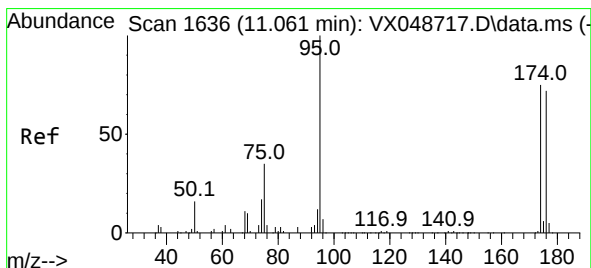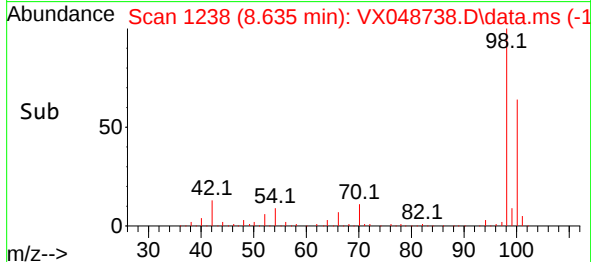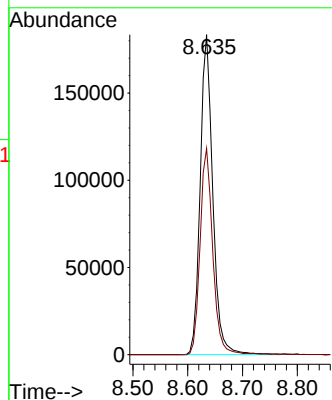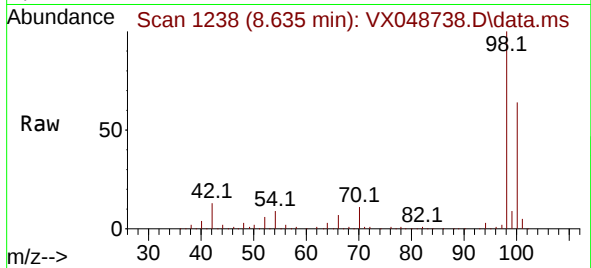

#62
4-Bromofluorobenzene
Concen: 43.258 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.000 min
Lab File: VX048738.D
Acq: 05 Dec 2025 15:55

Tgt Ion: 95 Resp: 104604
Ion Ratio Lower Upper
95 100
174 80.5 0.0 157.8
176 76.8 0.0 154.0


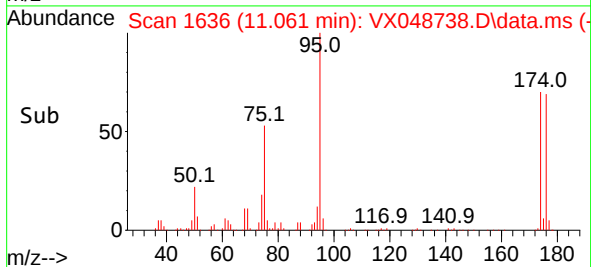
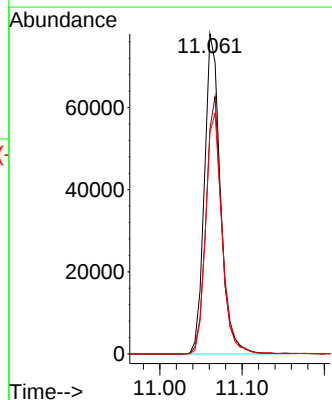
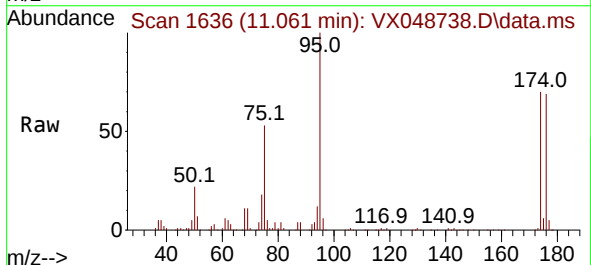


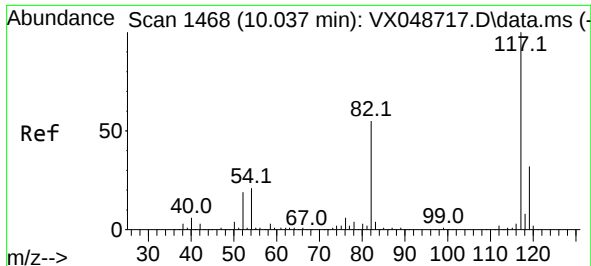

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. -0.000 min
Lab File: VX048738.D
Acq: 05 Dec 2025 15:55

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Tgt Ion:117 Resp: 224650
Ion Ratio Lower Upper
117 100
82 55.9 44.1 66.1
119 31.6 25.2 37.8

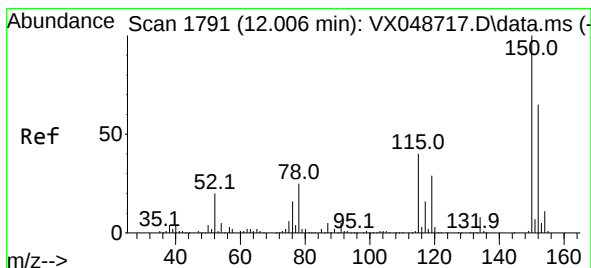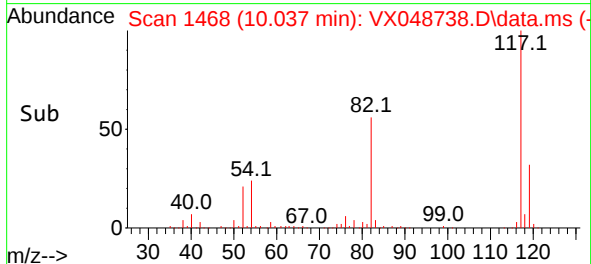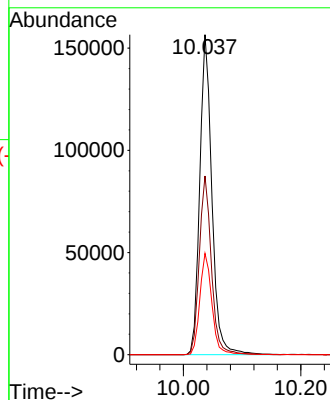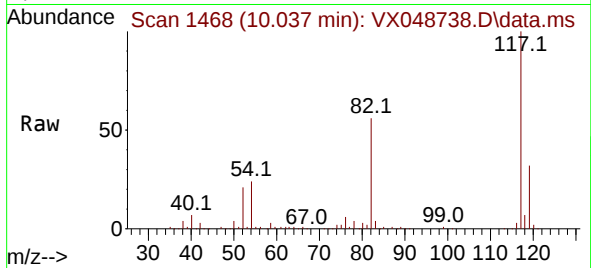

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.000 min
Lab File: VX048738.D
Acq: 05 Dec 2025 15:55

Tgt Ion:152 Resp: 129713
Ion Ratio Lower Upper
152 100
115 59.2 42.1 126.4
150 155.7 0.0 347.8

