


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX120618\
Data File : VX006307.D
Acq On : 06 Dec 2018 10:03
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
Title : SW846 8260
Last Update : Fri Nov 30 03:55:33 2018

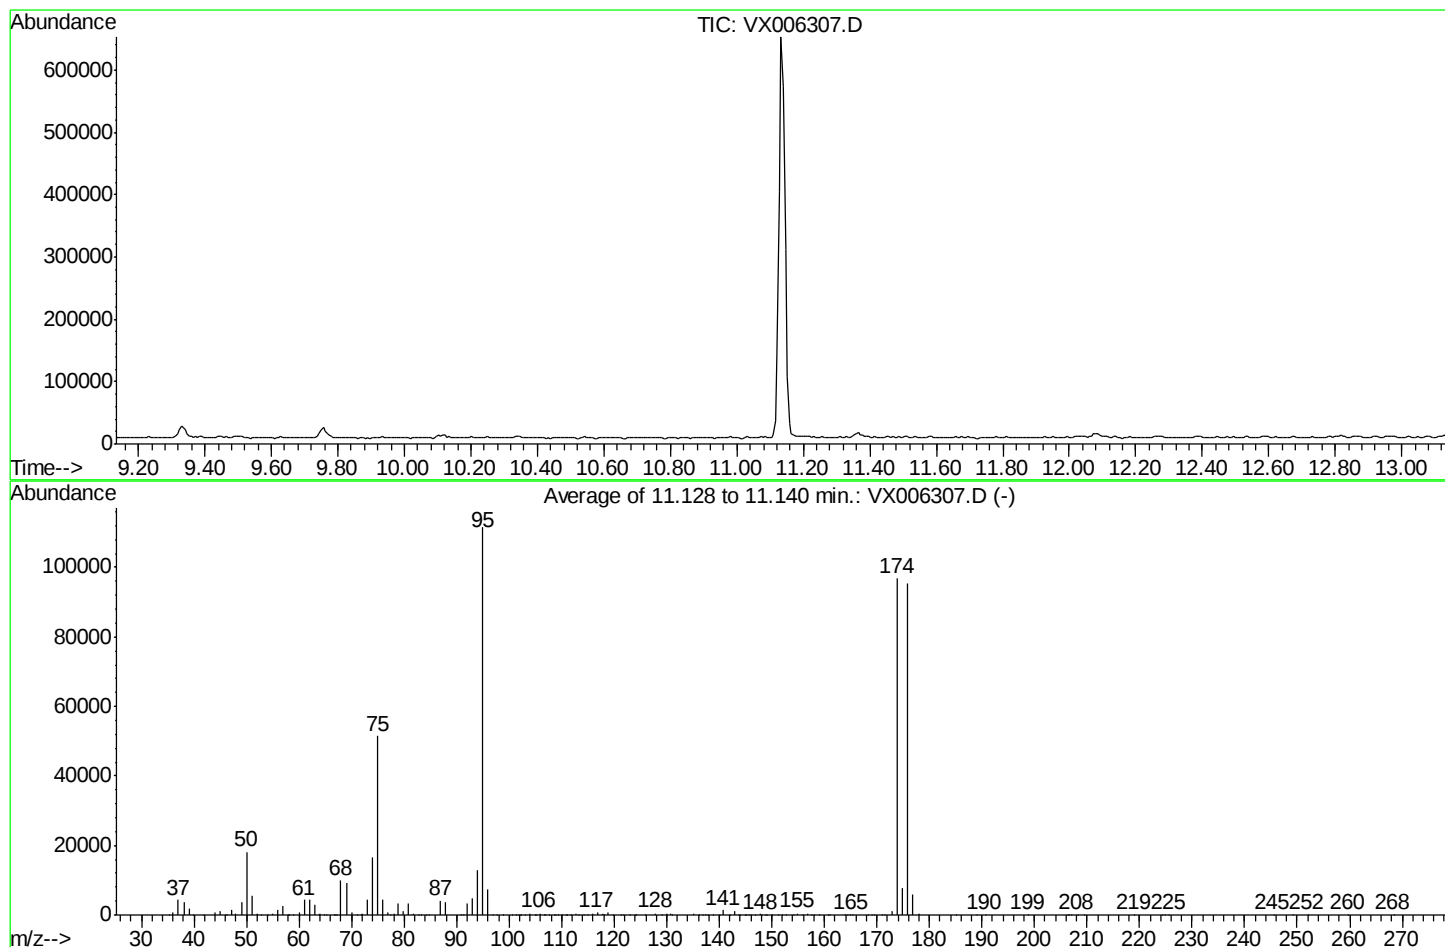

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	18237	PASS
75	95	30	60	46.1	51457	PASS
95	95	100	100	100.0	111530	PASS
96	95	5	9	6.7	7492	PASS
173	174	0.00	2	1.2	1191	PASS
174	95	50	100	86.7	96750	PASS
175	174	5	9	8.0	7699	PASS
176	174	95	101	98.7	95514	PASS
177	176	5	9	6.3	5980	PASS