


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX120619\  
Data File : VX013811.D  
Acq On : 06 Dec 2019 20:08  
Operator : JC/SP  
Sample : BFB  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 28 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X112619W.M  
Title : SW846 8260  
Last Update : Tue Nov 26 15:53:00 2019

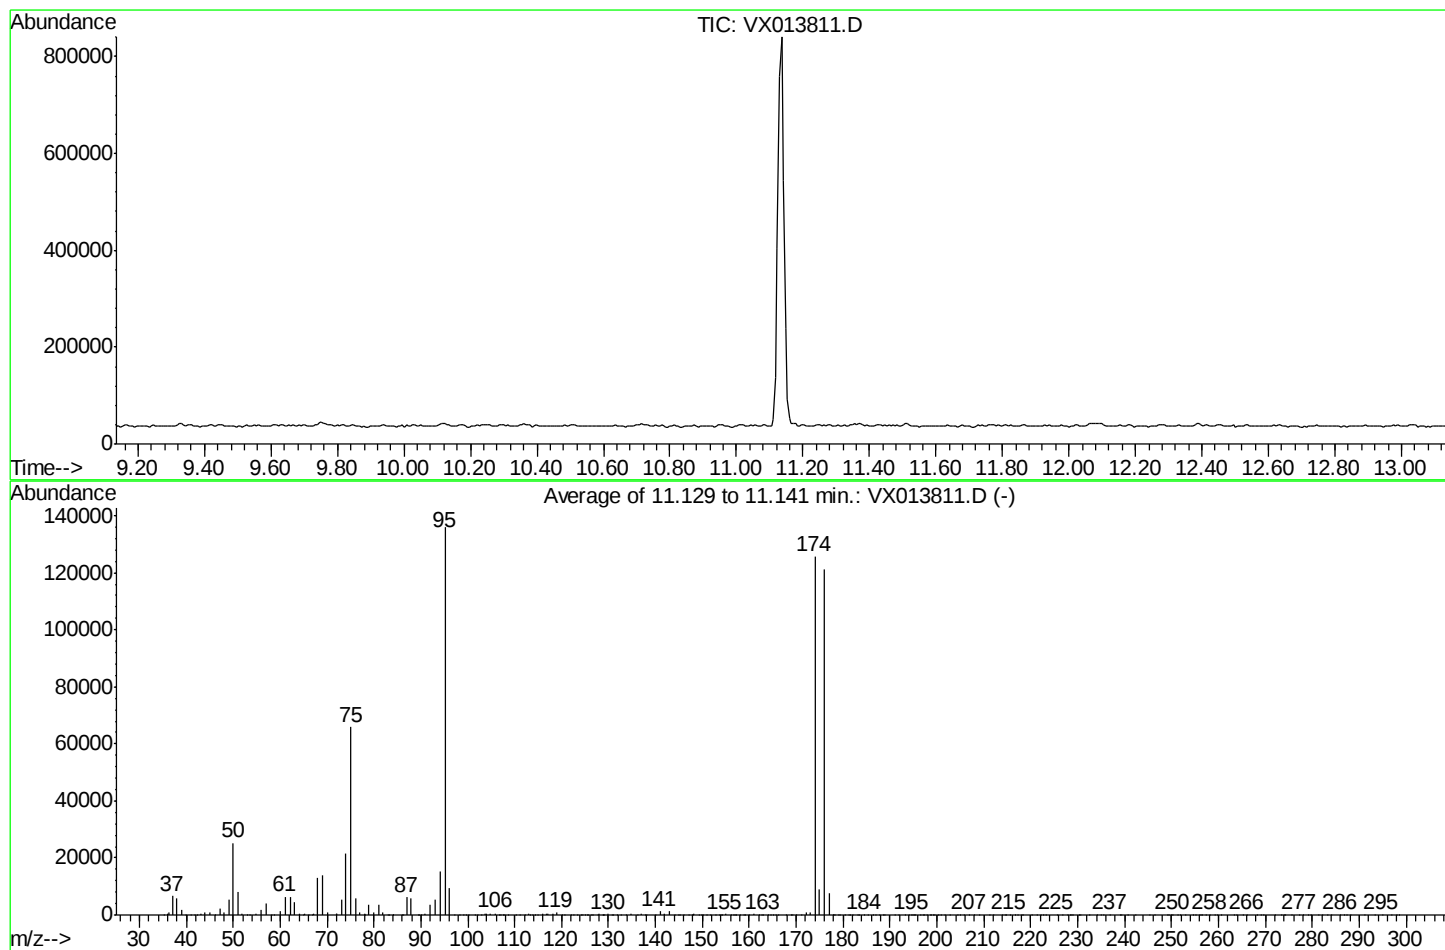

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1670

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 18.6      | 25213   | PASS             |
| 75          | 95           | 30           | 60           | 48.5      | 65939   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 135917  | PASS             |
| 96          | 95           | 5            | 9            | 6.9       | 9370    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.7       | 927     | PASS             |
| 174         | 95           | 50           | 100          | 92.4      | 125600  | PASS             |
| 175         | 174          | 5            | 9            | 7.3       | 9168    | PASS             |
| 176         | 174          | 95           | 101          | 96.6      | 121309  | PASS             |
| 177         | 176          | 5            | 9            | 6.3       | 7629    | PASS             |