

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120621\
 Data File : VX025546.D
 Acq On : 06 Dec 2021 14:08
 Operator : JC/MD
 Sample : M4923-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE105D1-20211202

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
 Title : SW846 8260

Signal : TIC: VX025546.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	33	rBV	3726	6733	1.32%	0.213%
2	2.331	198	204	210	rBV3	8858	16273	3.20%	0.514%
3	5.391	694	706	720	rBV2	59698	173006	34.04%	5.462%
4	5.556	722	733	746	rVV	101219	283677	55.82%	8.955%
5	5.958	790	799	813	rBV	61938	165398	32.54%	5.221%
6	6.769	922	932	946	rBV	154891	369095	72.62%	11.652%
7	7.129	982	991	1012	rBV	239196	508224	100.00%	16.044%
8	8.653	1234	1241	1253	rBV	321072	500055	98.39%	15.786%
9	10.055	1465	1471	1489	rBV	324317	432783	85.16%	13.662%
10	11.085	1634	1640	1652	rBV	248338	323054	63.57%	10.198%
11	12.024	1789	1794	1805	rBV	308893	389431	76.63%	12.294%




Sum of corrected areas: 3167729

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120621\
Data File : VX025546.D
Acq On : 06 Dec 2021 14:08
Operator : JC/MD
Sample : M4923-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE105D1-20211202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

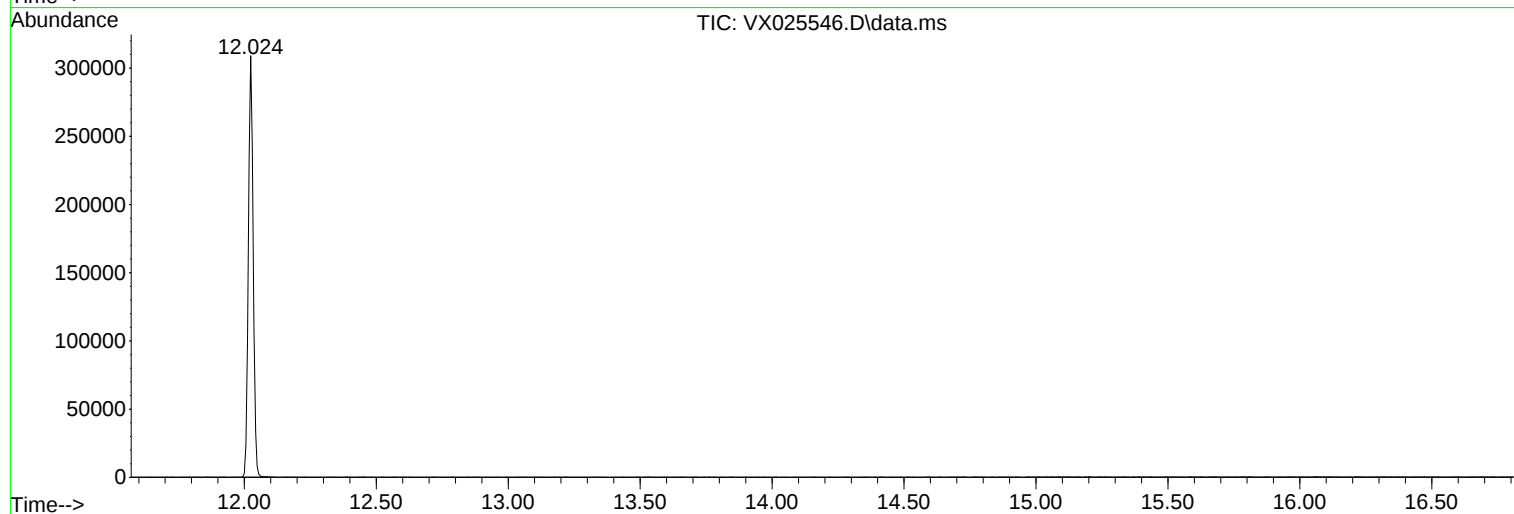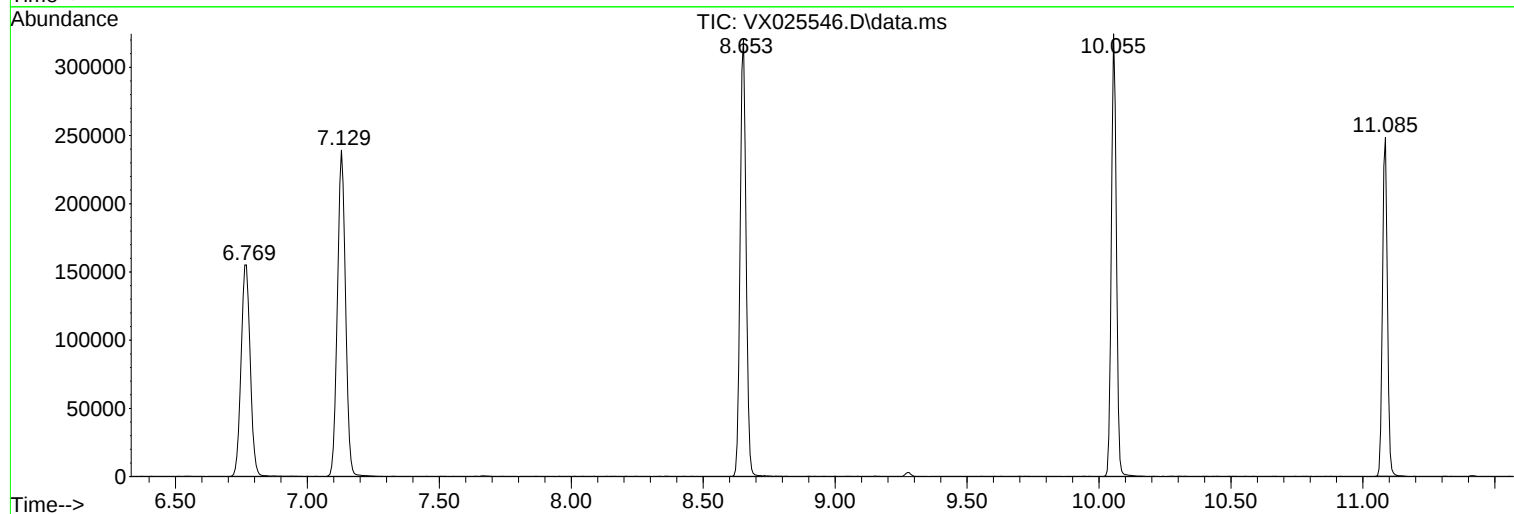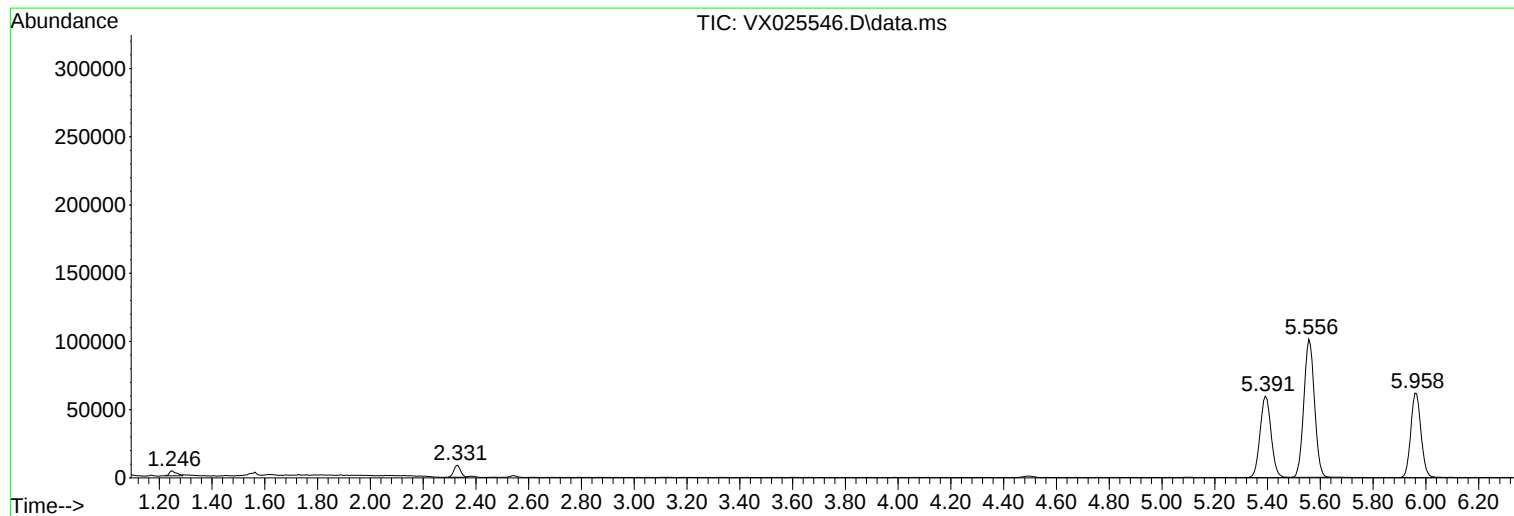

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120621\
Data File : VX025546.D
Acq On : 06 Dec 2021 14:08
Operator : JC/MD
Sample : M4923-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE105D1-20211202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120621\
Data File : VX025546.D
Acq On : 06 Dec 2021 14:08
Operator : JC/MD
Sample : M4923-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE105D1-20211202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc