
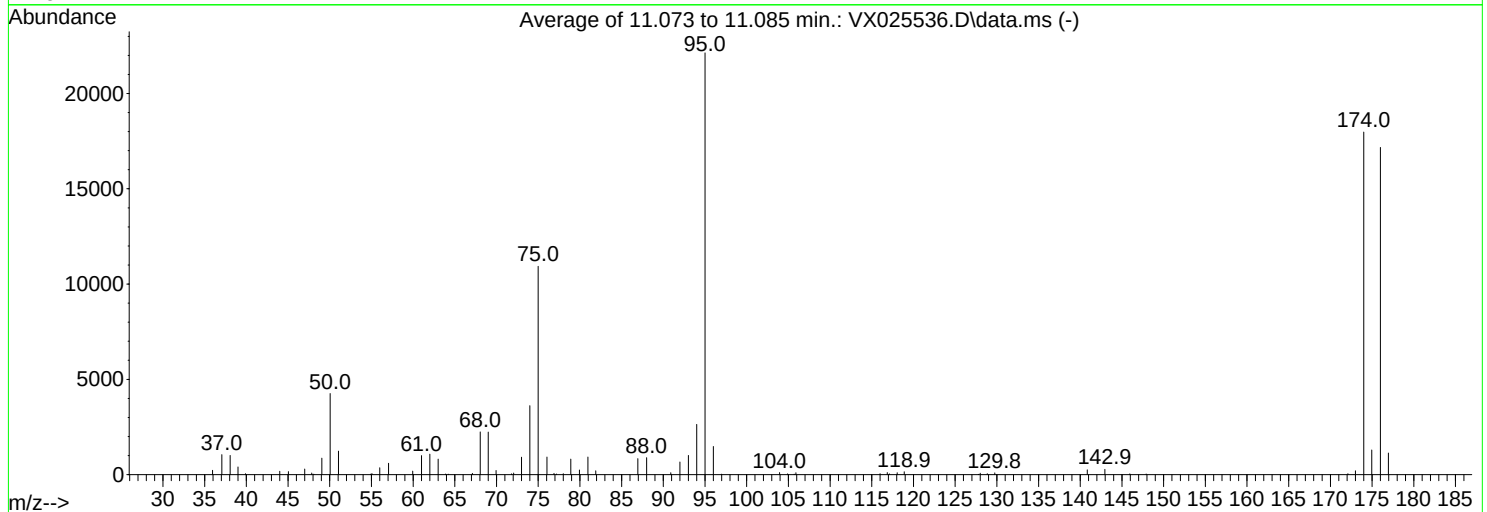


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120621\
 Data File : VX025536.D
 Acq On : 06 Dec 2021 09:43
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
 Title : SW846 8260
 Last Update : Wed Nov 17 15:36:16 2021

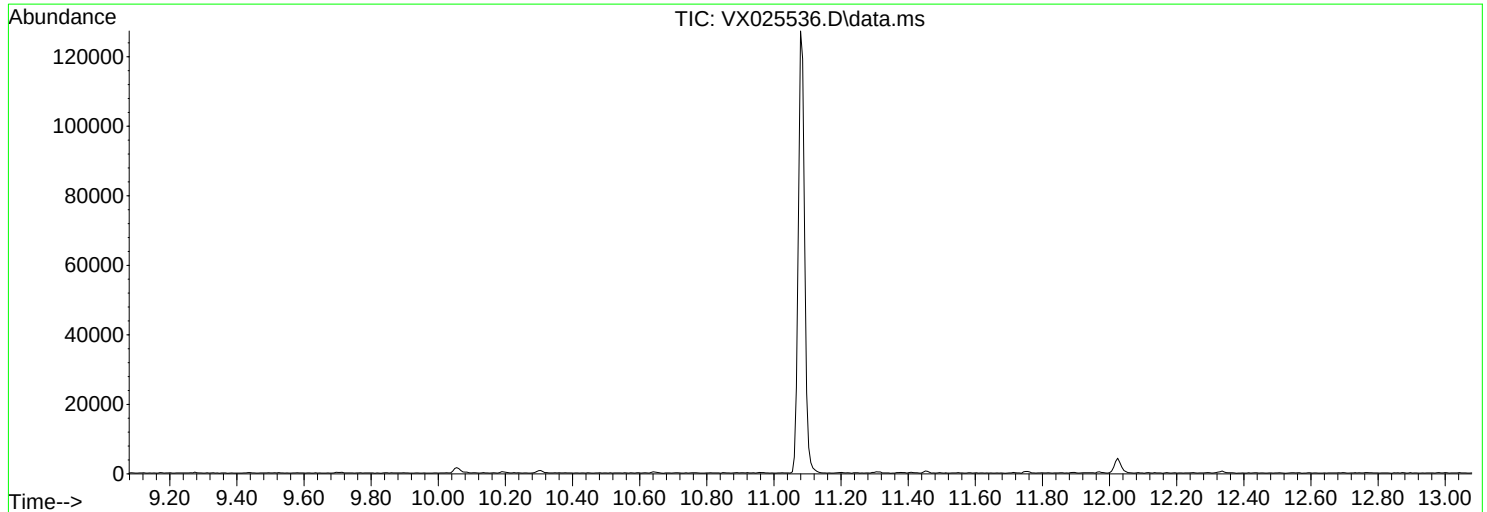

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	4254	PASS
75	95	30	60	49.4	10933	PASS
95	95	100	100	100.0	22133	PASS
96	95	5	9	6.7	1477	PASS
173	174	0.00	2	1.1	198	PASS
174	95	50	100	81.2	17980	PASS
175	174	5	9	7.2	1294	PASS
176	174	95	101	95.5	17168	PASS
177	176	5	9	6.6	1133	PASS