

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120622\
 Data File : VX033266.D
 Acq On : 06 Dec 2022 18:08
 Operator : JC/MD
 Sample : N5875-08DL 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-42DL

Quant Time: Dec 07 01:34:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 22 13:58:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	106075	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	163262	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	164660	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	97982	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	98567	98.109	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 196.220%#			
35) Dibromofluoromethane	5.391	113	76874	83.521	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 167.040%#			
50) Toluene-d8	8.647	98	269078	99.290	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 198.580%#			
62) 4-Bromofluorobenzene	11.079	95	92148	76.215	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 152.420%#			
Target Compounds					Qvalue	
11) Tert butyl alcohol	3.002	59	21696	132.493	ug/l #	88
13) Acrolein	2.343	56	1237	6.576	ug/l #	82
14) Allyl chloride	2.782	41	11340	7.588	ug/l #	59
15) Acrylonitrile	3.105	53	2180	4.707	ug/l #	31
16) Acetone	2.343	43	3718	7.707	ug/l #	54
18) Methyl Acetate	2.782	43	25672	19.223	ug/l #	51
19) Methyl tert-butyl Ether	3.111	73	126695	39.465	ug/l #	82
20) Methylene Chloride	2.788	84	924	Below Cal	#	51
22) Diisopropyl ether	3.764	45	2344	0.720	ug/l #	80
23) Vinyl Acetate	3.770	43	1211	0.475	ug/l #	72
25) 2-Butanone	4.581	43	137	0.206	ug/l #	47
36) 1,1-Dichloropropene	5.556	75	8054	5.473	ug/l #	50
38) Carbon Tetrachloride	5.550	117	10870	6.658	ug/l #	15
39) Methylcyclohexane	7.361	83	974	0.580	ug/l #	12
40) Benzene	6.044	78	134888	32.690	ug/l	98
41) Methacrylonitrile	5.135	41	356	0.493	ug/l #	31
42) 1,2-Dichloroethane	6.038	62	1524	0.917	ug/l #	77
43) Isopropyl Acetate	6.349	43	443	0.209	ug/l #	61
48) Methyl methacrylate	7.775	41	518	0.474	ug/l #	83
51) 4-Methyl-2-Pentanone	8.507	43	1160	0.885	ug/l #	56
55) 1,1,2-Trichloroethane	9.104	97	1368	1.238	ug/l #	19
56) Ethyl methacrylate	9.104	69	318	0.209	ug/l #	13
59) 2-Hexanone	9.580	43	563	0.582	ug/l	72
76) 1,2,3-Trichloropropane	11.079	75	48806	26.302	ug/l #	37
80) 1,3,5-Trimethylbenzene	11.616	105	1449	0.246	ug/l	77
81) trans-1,4-Dichloro-2-b...	11.079	75	48806	85.493	ug/l #	6
85) sec-Butylbenzene	11.890	105	2192	0.313	ug/l #	69
89) n-Butylbenzene	12.317	91	1490	0.291	ug/l #	1
90) Hexachloroethane	12.701	117	44152	45.283	ug/l #	12

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120622\
Data File : VX033266.D
Acq On : 06 Dec 2022 18:08
Operator : JC/MD
Sample : N5875-08DL 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-42DL

Quant Time: Dec 07 01:34:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112222W.M
Quant Title : SW846 8260
QLast Update : Tue Nov 22 13:58:46 2022
Response via : Initial Calibration




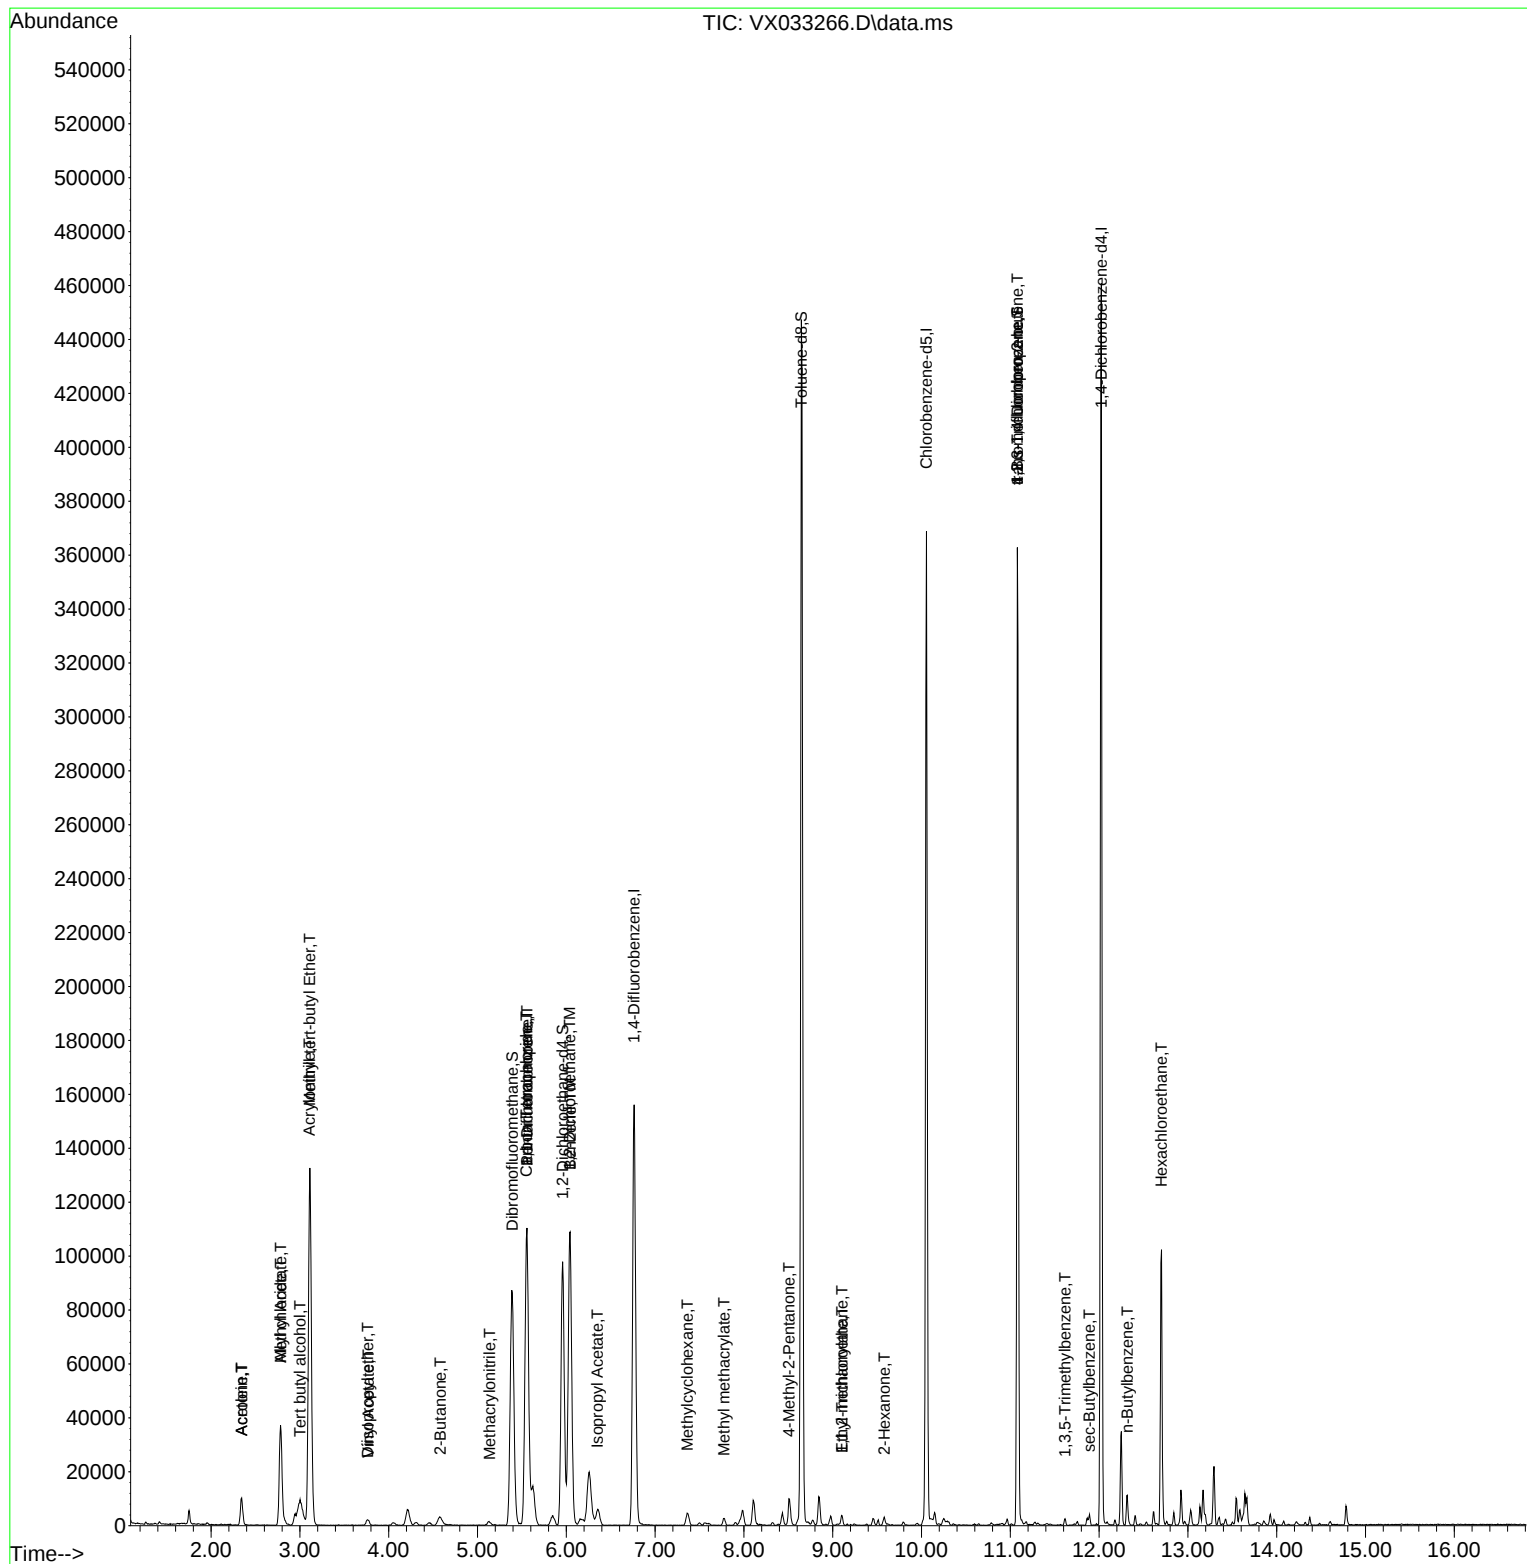




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX033266.D
Acq: 06 Dec 2022 18:08




Instrument :
MSVOA_X
ClientSampleId :
MW-42DL


Tgt Ion:168 Resp: 106075
Ion Ratio Lower Upper
168 100
99 57.5 46.1 69.1

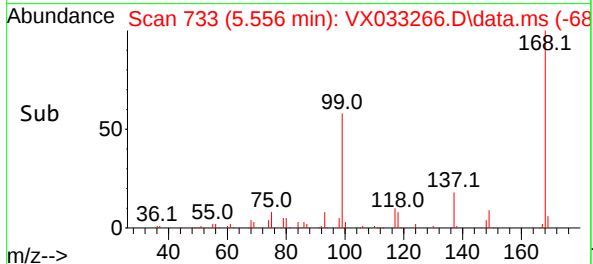

#11
Tert butyl alcohol
Concen: 132.493 ug/l
RT: 3.002 min Scan# 314
Delta R.T. 0.037 min
Lab File: VX033266.D
Acq: 06 Dec 2022 18:08

Tgt Ion: 59 Resp: 21696
Ion Ratio Lower Upper
59 100
57 5.8 8.2 12.4#

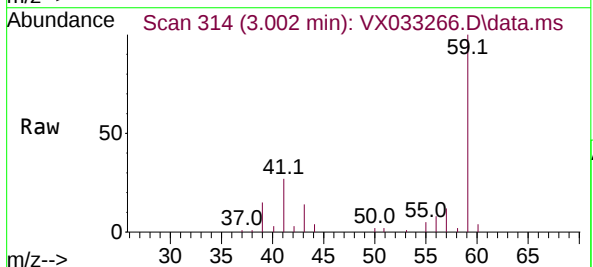



#13

Acrolein

Concen: 6.576 ug/l

RT: 2.343 min Scan# 206

Delta R.T. 0.110 min

Lab File: VX033266.D

Acq: 06 Dec 2022 18:08

Instrument :

MSVOA_X

ClientSampleId :





MW-42DL

Tgt Ion: 56 Resp: 1237

Ion Ratio Lower Upper

56 100

55 56.5 56.9 85.3#

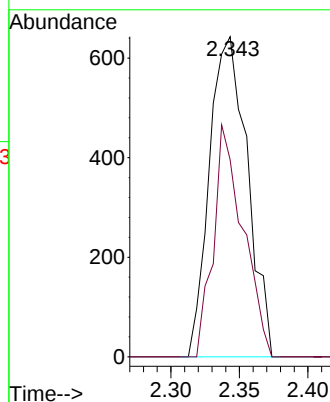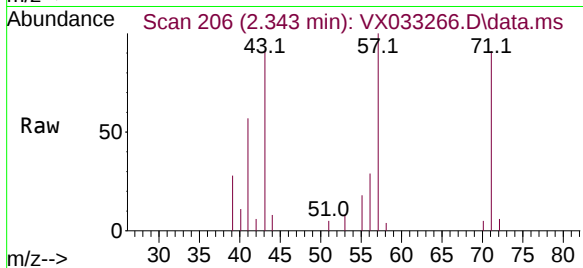

#14

Allyl chloride

Concen: 7.588 ug/l

RT: 2.782 min Scan# 278

Delta R.T. 0.116 min

Lab File: VX033266.D

Acq: 06 Dec 2022 18:08




Tgt Ion: 41 Resp: 11340


Ion Ratio Lower Upper

41 100

39 49.4 61.4 92.2#

76 0.0 29.2 43.8#

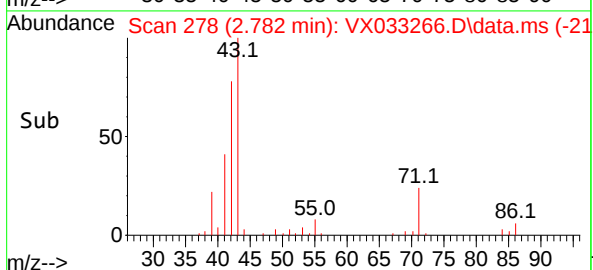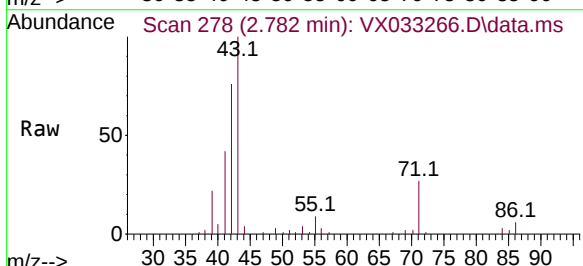

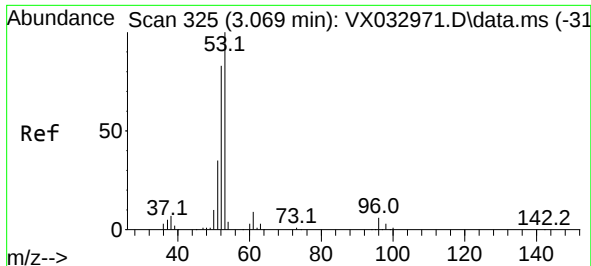

#15

Acrylonitrile

Concen: 4.707 ug/l

RT: 3.105 min Scan# 31

Delta R.T. 0.043 min

Lab File: VX033266.D

Acq: 06 Dec 2022 18:08

Instrument :

MSVOA_X

ClientSampleId :

MW-42DL





Tgt Ion: 53 Resp: 2180

Ion Ratio Lower Upper

53 100

52 17.5 67.4 101.0#

51 74.0 30.3 45.5#

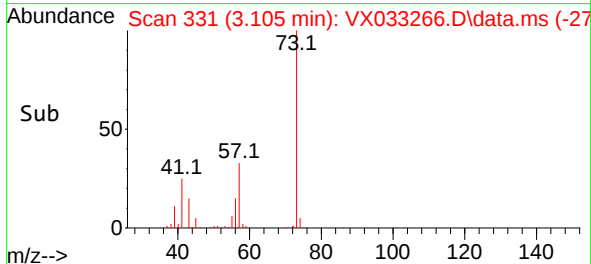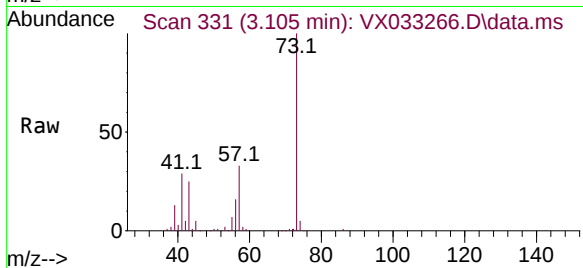

#16

Acetone

Concen: 7.707 ug/l

RT: 2.343 min Scan# 206

Delta R.T. -0.037 min

Lab File: VX033266.D




Acq: 06 Dec 2022 18:08


Tgt Ion: 43 Resp: 3718

Ion Ratio Lower Upper

43 100

58 4.8 23.8 35.8#


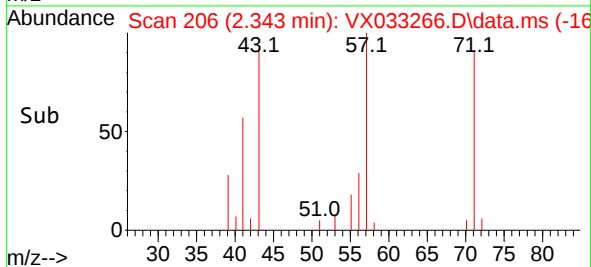

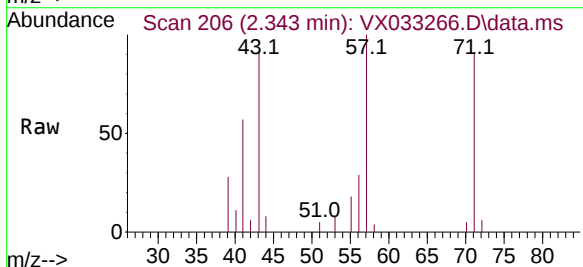




#18
Methyl Acetate
Concen: 19.223 ug/l
RT: 2.782 min Scan# 21
Delta R.T. 0.079 min
Lab File: VX033266.D
Acq: 06 Dec 2022 18:08




Instrument :
MSVOA_X
ClientSampleId :
MW-42DL


Tgt Ion: 43 Resp: 25672
Ion Ratio Lower Upper
43 100
74 0.0 19.4 29.0#

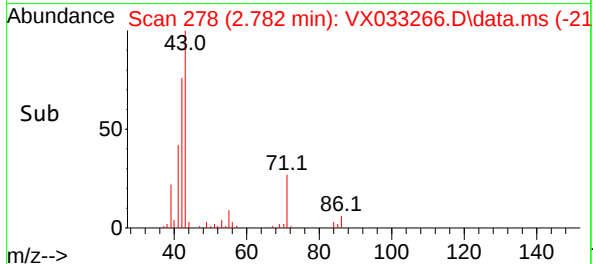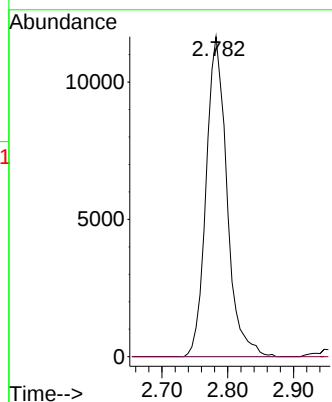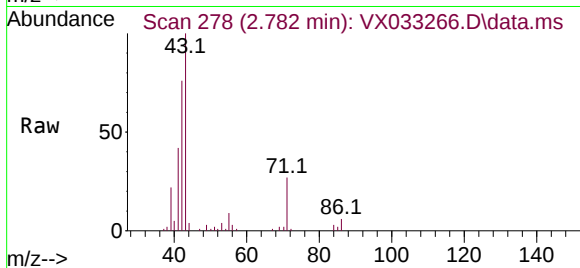

#19
Methyl tert-butyl Ether
Concen: 39.465 ug/l
RT: 3.111 min Scan# 332
Delta R.T. 0.000 min
Lab File: VX033266.D
Acq: 06 Dec 2022 18:08

Tgt Ion: 73 Resp: 126695
Ion Ratio Lower Upper
73 100
57 29.4 16.6 25.0#


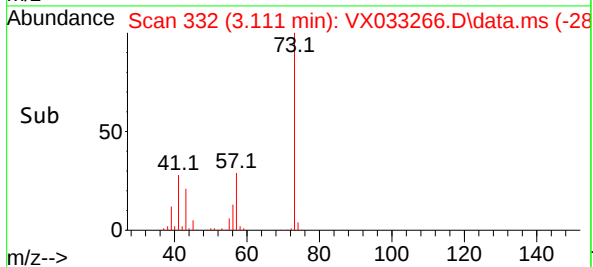
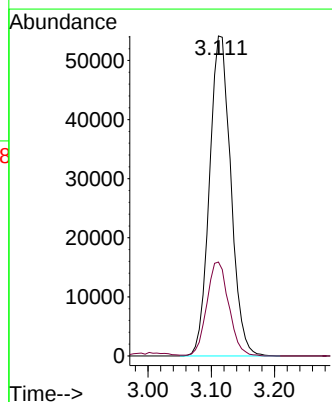
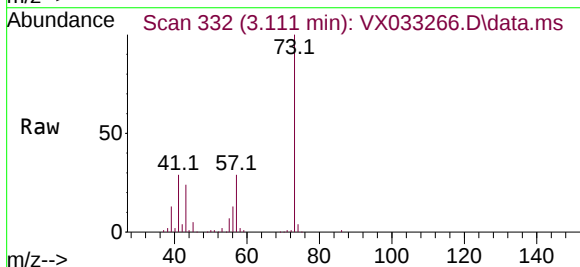


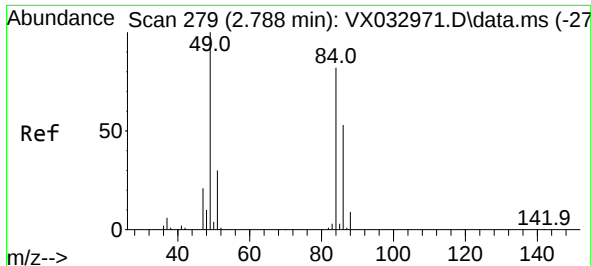

#20
Methylene Chloride
Concen: Below Cal
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX033266.D
Acq: 06 Dec 2022 18:08




Instrument :
MSVOA_X
ClientSampleId :
MW-42DL


Tgt Ion:	84	Resp:	924
Ion	Ratio	Lower	Upper
84	100		
49	122.0	101.0	151.6
51	89.2	31.1	46.7#
86	157.3	52.3	78.5#

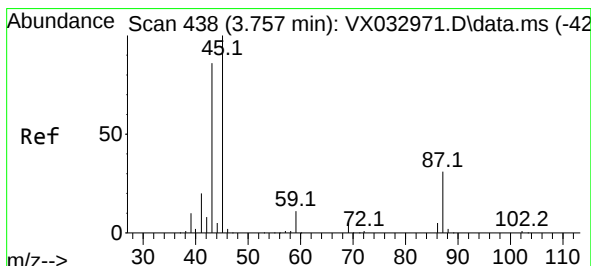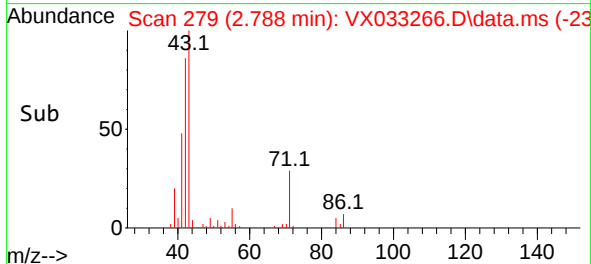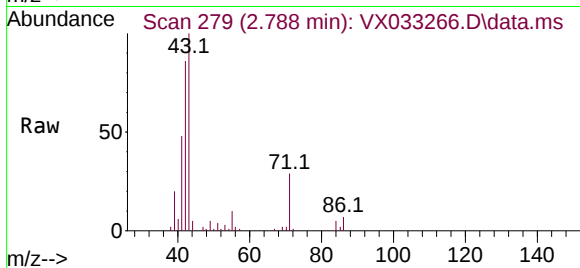

#22
Diisopropyl ether
Concen: 0.720 ug/l
RT: 3.764 min Scan# 439
Delta R.T. 0.001 min
Lab File: VX033266.D
Acq: 06 Dec 2022 18:08

Tgt Ion:	45	Resp:	2344
Ion	Ratio	Lower	Upper
45	100		
43	45.9	56.4	84.6#
87	29.7	24.4	36.6
59	15.1	9.5	14.3#

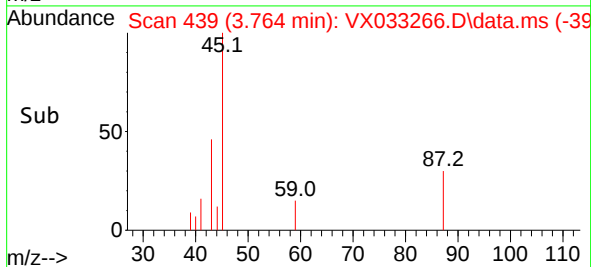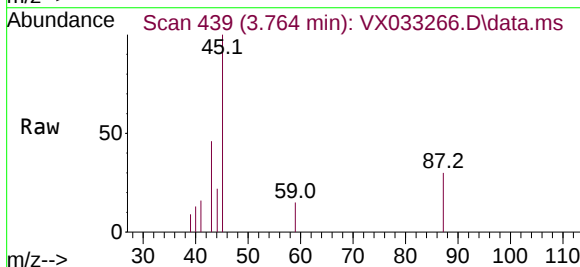



#23

Vinyl Acetate

Concen: 0.475 ug/l

RT: 3.770 min Scan# 44

Delta R.T. 0.049 min

Lab File: VX033266.D

Acq: 06 Dec 2022 18:08

Instrument :

MSVOA_X

ClientSampleId :





MW-42DL

Tgt Ion: 43 Resp: 1211

Ion Ratio Lower Upper

43 100

86 0.0 8.6 12.8#

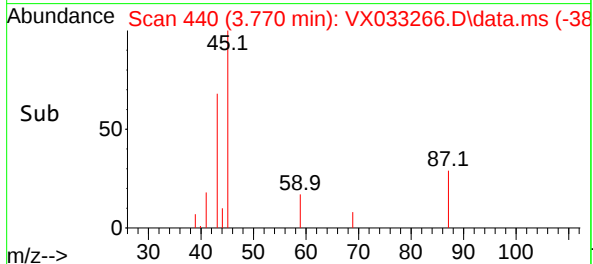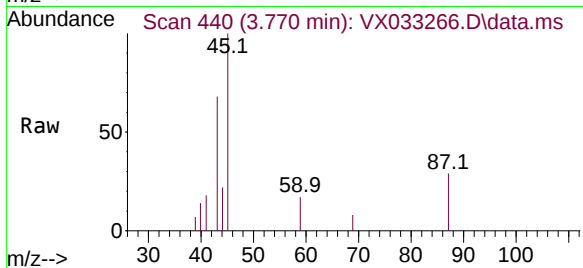

#25

2-Butanone

Concen: 0.206 ug/l

RT: 4.581 min Scan# 573

Delta R.T. 0.025 min

Lab File: VX033266.D




Acq: 06 Dec 2022 18:08


Tgt Ion: 43 Resp: 137

Ion Ratio Lower Upper

43 100

72 0.0 22.2 33.2#

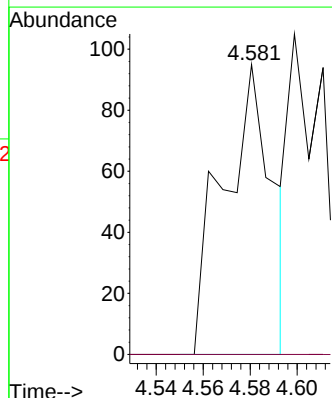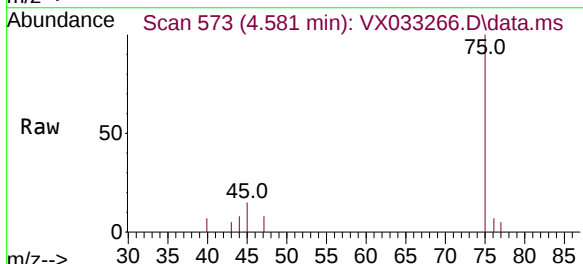



#33

1,2-Dichloroethane-d4

Concen: 98.109 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX033266.D

Acq: 06 Dec 2022 18:08

Instrument :

MSVOA_X

ClientSampleId :





MW-42DL

Tgt Ion: 65 Resp: 98567

Ion Ratio Lower Upper

65 100

67 50.1 0.0 101.8

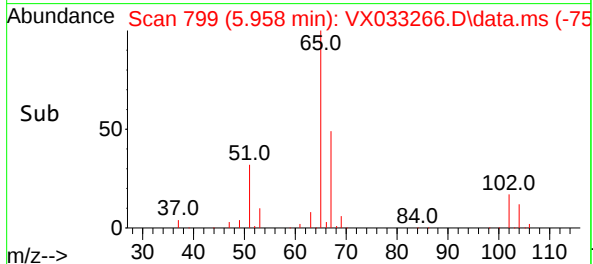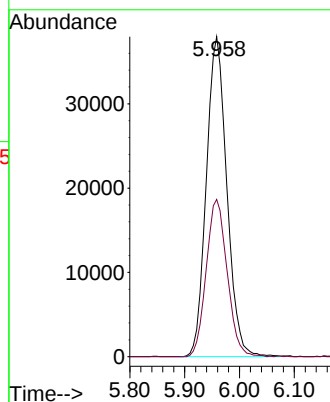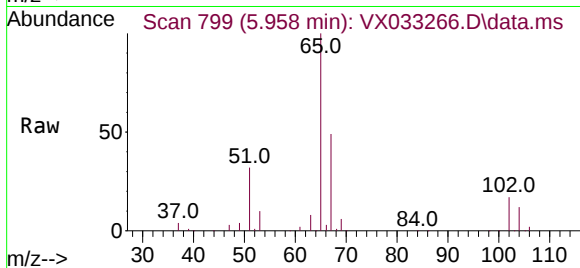

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX033266.D

Acq: 06 Dec 2022 18:08




Tgt Ion: 114 Resp: 163262


Ion Ratio Lower Upper

114 100

63 19.6 0.0 41.6

88 15.9 0.0 33.4


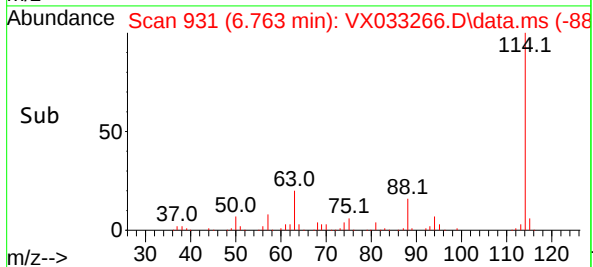

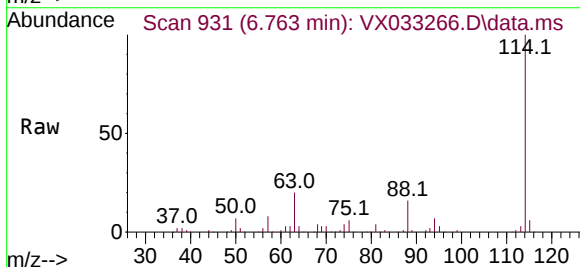




#35
Dibromofluoromethane
Concen: 83.521 ug/l
RT: 5.391 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX033266.D
Acq: 06 Dec 2022 18:08




Instrument :
MSVOA_X
ClientSampleId :
MW-42DL


Tgt Ion:113 Resp: 76874
Ion Ratio Lower Upper
113 100
111 102.0 82.4 123.6
192 19.6 15.4 23.2

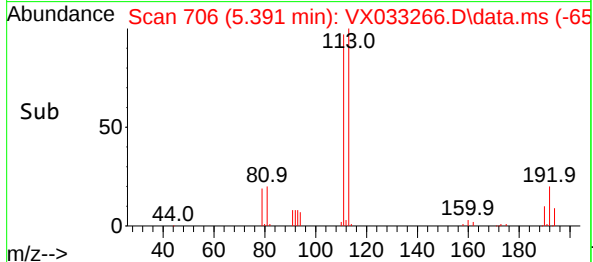

#36
1,1-Dichloropropene
Concen: 5.473 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.140 min
Lab File: VX033266.D
Acq: 06 Dec 2022 18:08

Tgt Ion: 75 Resp: 8054
Ion Ratio Lower Upper
75 100
110 9.7 18.4 55.2#
77 0.0 24.5 36.7#


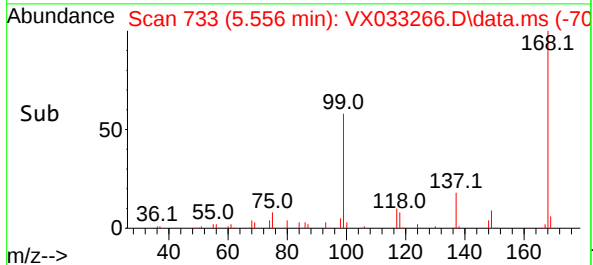

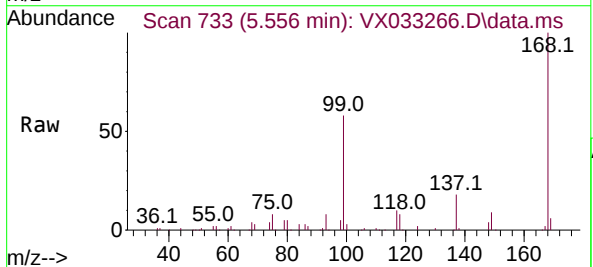


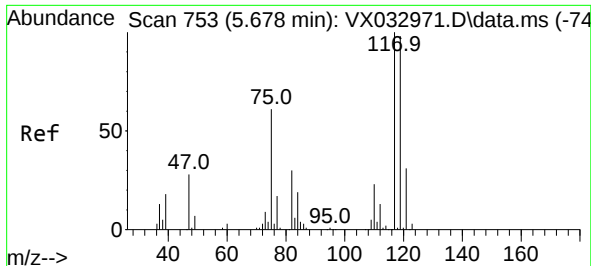

#38
Carbon Tetrachloride
Concen: 6.658 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX033266.D
Acq: 06 Dec 2022 18:08




Instrument :
MSVOA_X
ClientSampleId :
MW-42DL


Tgt Ion:117 Resp: 10870
Ion Ratio Lower Upper
117 100
119 4.8 77.2 115.8#
121 0.0 25.8 38.6#

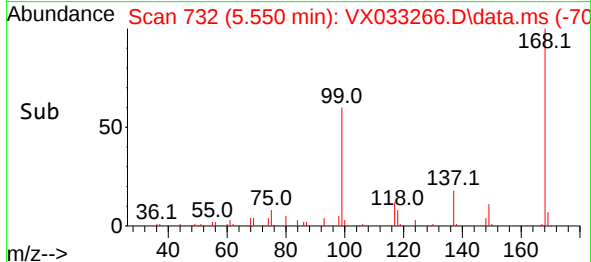

#39
Methylcyclohexane
Concen: 0.580 ug/l
RT: 7.361 min Scan# 1029
Delta R.T. -0.024 min
Lab File: VX033266.D
Acq: 06 Dec 2022 18:08

Tgt Ion: 83 Resp: 974
Ion Ratio Lower Upper
83 100
55 171.6 58.4 87.6#
98 19.1 37.2 55.8#


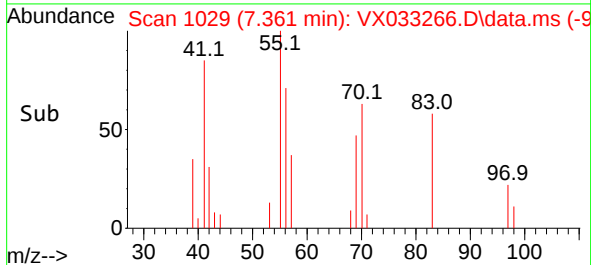

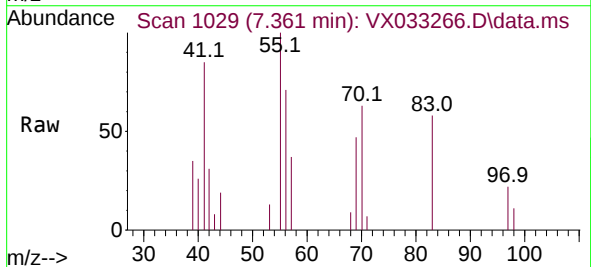




#40
Benzene
Concen: 32.690 ug/l
RT: 6.044 min Scan# 812
Delta R.T. 0.007 min
Lab File: VX033266.D
Acq: 06 Dec 2022 18:08




Instrument :
MSVOA_X
ClientSampleId :
MW-42DL


Tgt Ion: 78 Resp: 134888
Ion Ratio Lower Upper
78 100
77 24.6 19.0 28.4

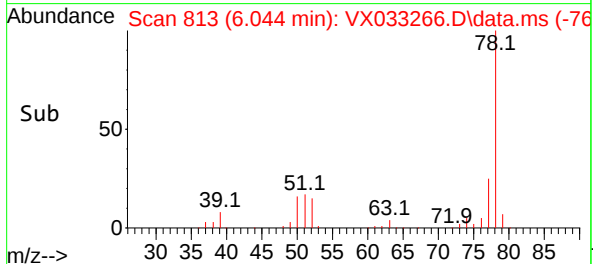

#41
Methacrylonitrile
Concen: 0.493 ug/l
RT: 5.135 min Scan# 664
Delta R.T. 0.213 min
Lab File: VX033266.D
Acq: 06 Dec 2022 18:08

Tgt Ion: 41 Resp: 356
Ion Ratio Lower Upper
41 100
39 22.2 47.5 71.3#
67 0.0 60.5 90.7#
52 0.0 27.0 40.6#

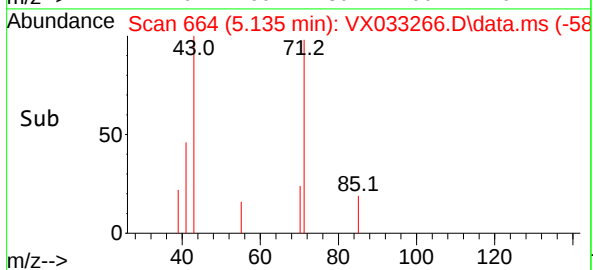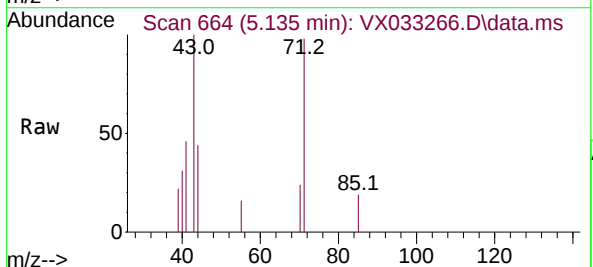



#42

1,2-Dichloroethane

Concen: 0.917 ug/l

RT: 6.038 min Scan# 81

Delta R.T. -0.048 min

Lab File: VX033266.D

Acq: 06 Dec 2022 18:08

Instrument :

MSVOA_X

ClientSampleId :





MW-42DL

Tgt Ion: 62 Resp: 1524

Ion Ratio Lower Upper

62 100

98 0.0 0.0 16.0

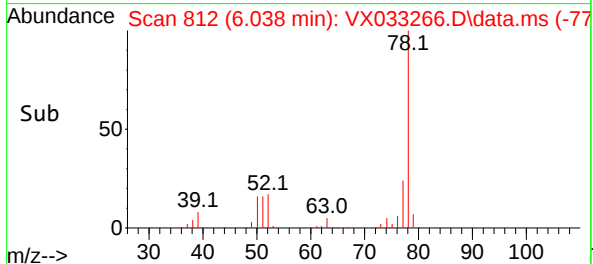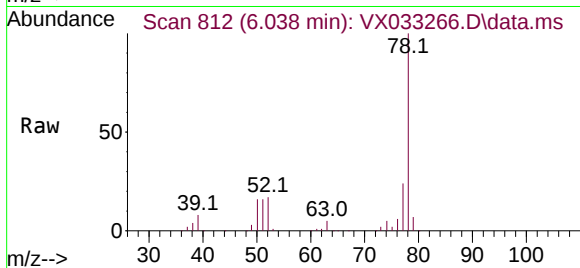

#43

Isopropyl Acetate

Concen: 0.209 ug/l

RT: 6.349 min Scan# 863

Delta R.T. 0.007 min

Lab File: VX033266.D

Acq: 06 Dec 2022 18:08




Tgt Ion: 43 Resp: 443


Ion Ratio Lower Upper

43 100

61 0.0 15.4 23.0#

87 0.0 10.8 16.2#

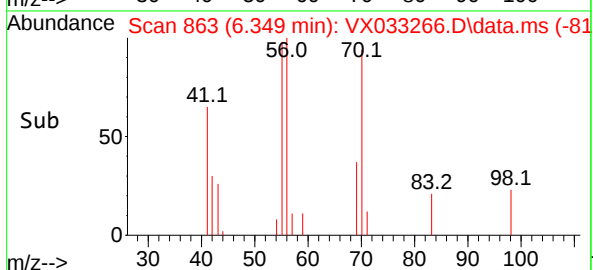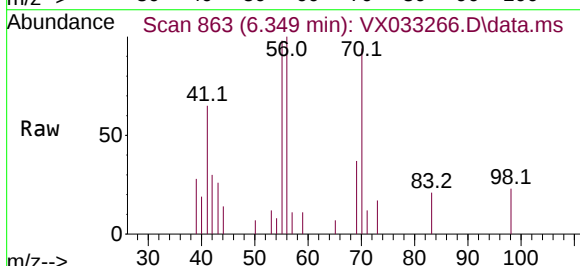



#48

Methyl methacrylate

Concen: 0.474 ug/l

RT: 7.775 min Scan# 1097

Delta R.T. 0.079 min

Lab File: VX033266.D

Acq: 06 Dec 2022 18:08

Instrument :

MSVOA_X

ClientSampleId :

MW-42DL





Tgt Ion: 41 Resp: 518

Ion Ratio Lower Upper

41 100

69 72.6 65.1 97.7

39 44.6 51.9 77.9#

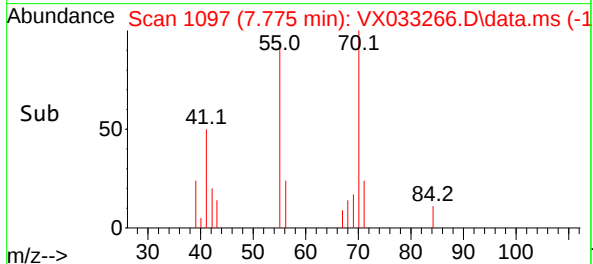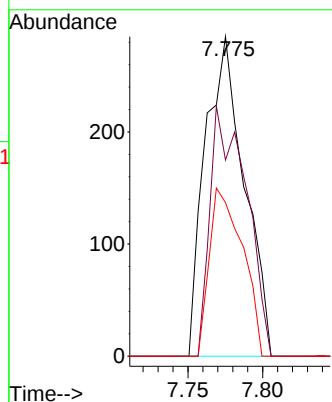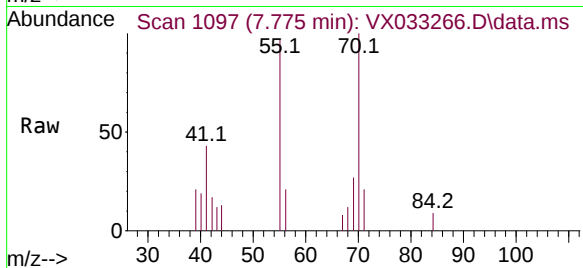

#50

Toluene-d8

Concen: 99.290 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.006 min

Lab File: VX033266.D




Acq: 06 Dec 2022 18:08


Tgt Ion: 98 Resp: 269078

Ion Ratio Lower Upper

98 100

100 64.0 50.9 76.3


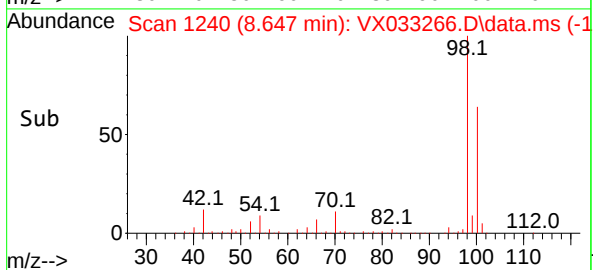
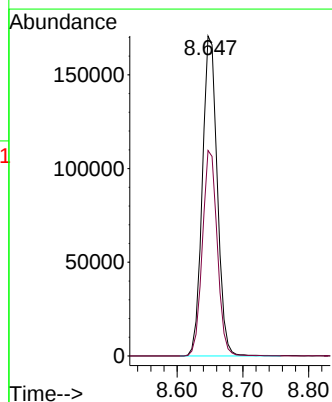
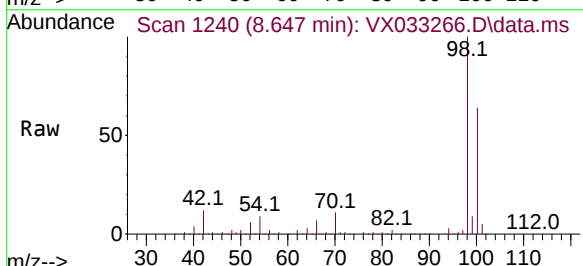




#51
4-Methyl-2-Pentanone
Concen: 0.885 ug/l
RT: 8.507 min Scan# 11
Delta R.T. -0.067 min
Lab File: VX033266.D
Acq: 06 Dec 2022 18:08




Instrument :
MSVOA_X
ClientSampleId :
MW-42DL


Tgt Ion: 43 Resp: 1160
Ion Ratio Lower Upper
43 100
58 11.8 30.9 46.3#

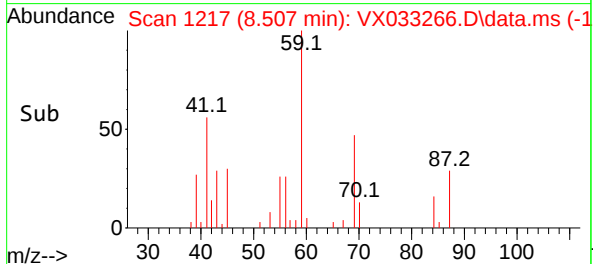

#55
1,1,2-Trichloroethane
Concen: 1.238 ug/l
RT: 9.104 min Scan# 1315
Delta R.T. -0.049 min
Lab File: VX033266.D
Acq: 06 Dec 2022 18:08

Tgt Ion: 97 Resp: 1368
Ion Ratio Lower Upper
97 100
83 8.4 68.1 102.1#
85 0.0 43.3 64.9#
99 0.0 50.4 75.6#


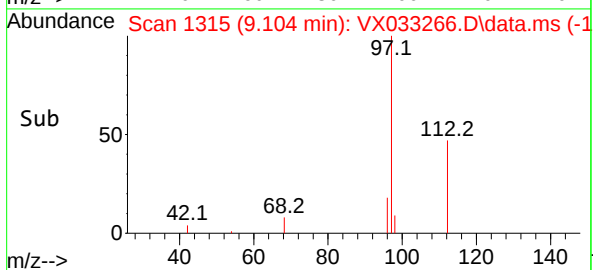

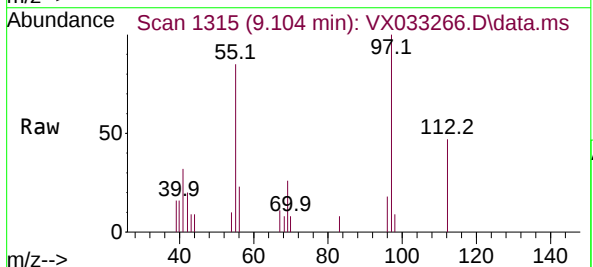




#56
Ethyl methacrylate
Concen: 0.209 ug/l
RT: 9.104 min Scan# 11
Delta R.T. -0.012 min
Lab File: VX033266.D
Acq: 06 Dec 2022 18:08




Instrument :
MSVOA_X
ClientSampleId :
MW-42DL


Tgt Ion: 69 Resp: 318
Ion Ratio Lower Upper
69 100
41 136.2 54.3 81.5#
39 102.8 35.2 52.8#

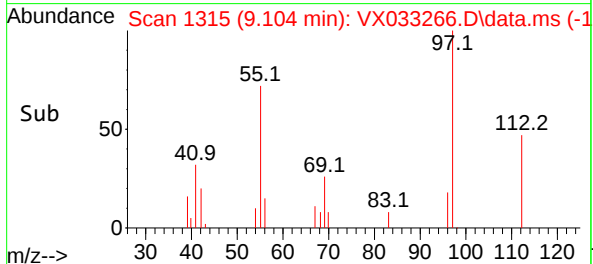

#59
2-Hexanone
Concen: 0.582 ug/l
RT: 9.580 min Scan# 1393
Delta R.T. 0.147 min
Lab File: VX033266.D
Acq: 06 Dec 2022 18:08

Tgt Ion: 43 Resp: 563
Ion Ratio Lower Upper
43 100
58 72.6 26.5 79.5


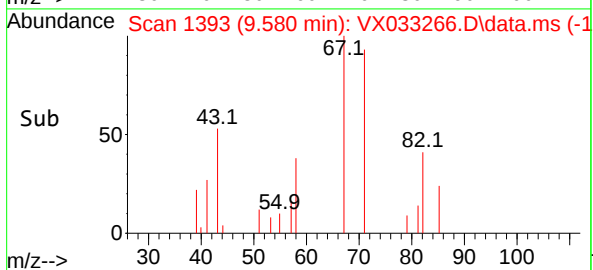

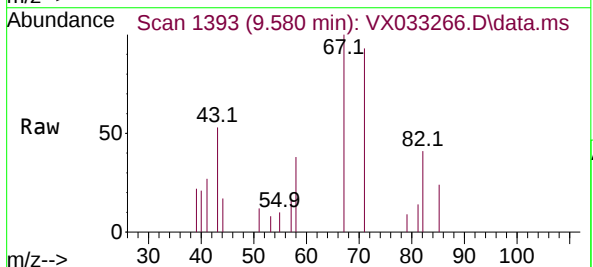




#62
4-Bromofluorobenzene
Concen: 76.215 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX033266.D
Acq: 06 Dec 2022 18:08




Instrument :
MSVOA_X
ClientSampleId :
MW-42DL


Tgt Ion: 95 Resp: 92148
Ion Ratio Lower Upper
95 100
174 83.6 0.0 164.0
176 79.5 0.0 154.4

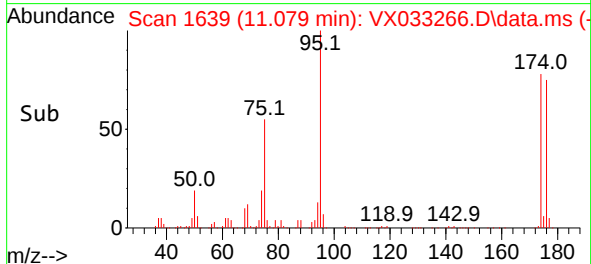

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX033266.D
Acq: 06 Dec 2022 18:08

Tgt Ion: 117 Resp: 164660
Ion Ratio Lower Upper
117 100
82 53.6 44.3 66.5
119 31.8 25.7 38.5


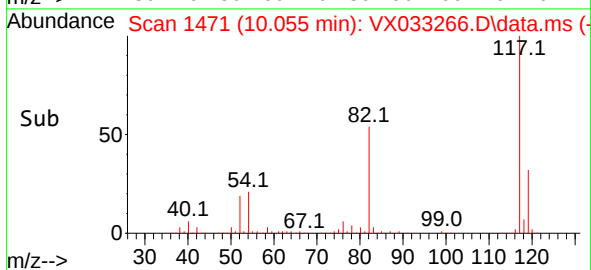

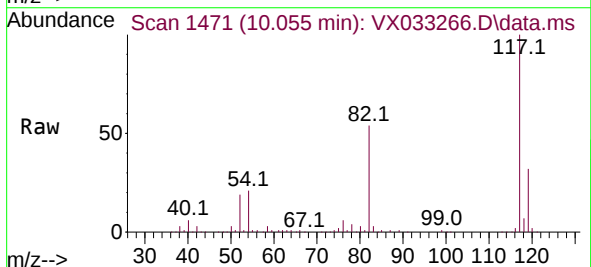




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX033266.D
 Acq: 06 Dec 2022 18:08




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-42DL


Tgt Ion:152 Resp: 97982
 Ion Ratio Lower Upper
 152 100
 115 59.6 44.0 132.0
 150 157.0 0.0 351.8

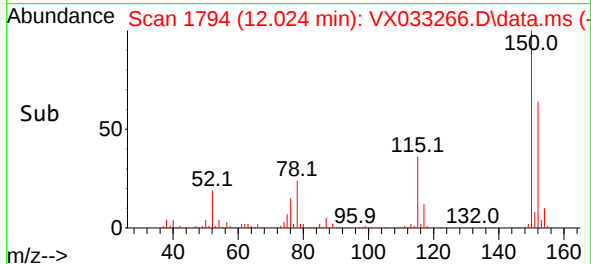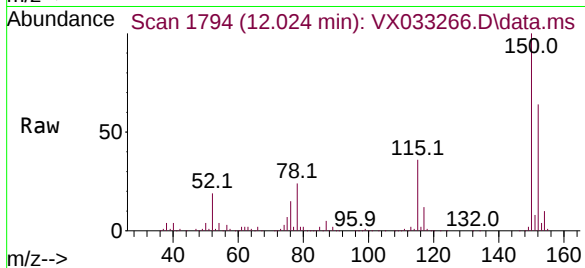

#76
 1,2,3-Trichloropropane
 Concen: 26.302 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. -0.165 min
 Lab File: VX033266.D
 Acq: 06 Dec 2022 18:08

Tgt Ion: 75 Resp: 48806
 Ion Ratio Lower Upper
 75 100
 77 1.1 20.0 60.0#

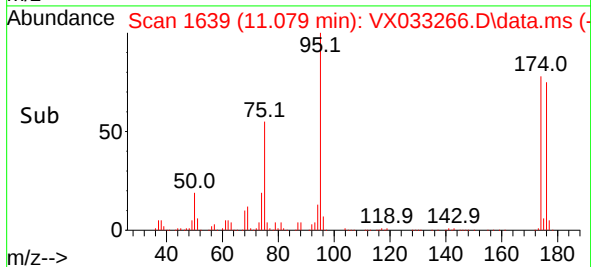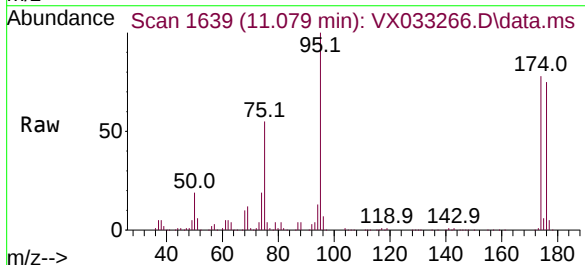



#80

1,3,5-Trimethylbenzene

Concen: 0.246 ug/l

RT: 11.616 min Scan# 11

Delta R.T. 0.165 min

Lab File: VX033266.D

Acq: 06 Dec 2022 18:08

Instrument :

MSVOA_X

ClientSampleId :





MW-42DL

Tgt Ion:105 Resp: 1449

Ion Ratio Lower Upper

105 100

120 32.2 23.6 71.0

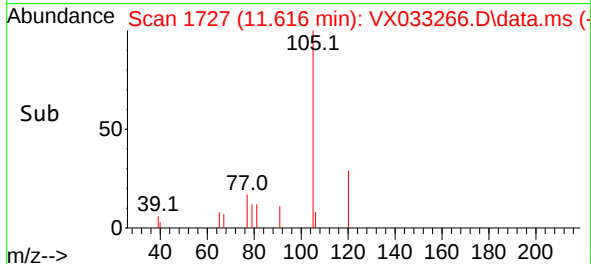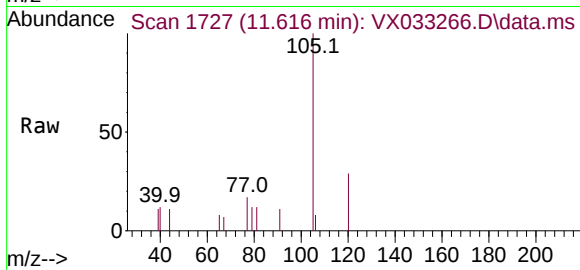

#81

trans-1,4-Dichloro-2-butene

Concen: 85.493 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX033266.D

Acq: 06 Dec 2022 18:08




Tgt Ion: 75 Resp: 48806


Ion Ratio Lower Upper

75 100

53 0.0 86.9 130.3#

89 0.0 38.3 57.5#

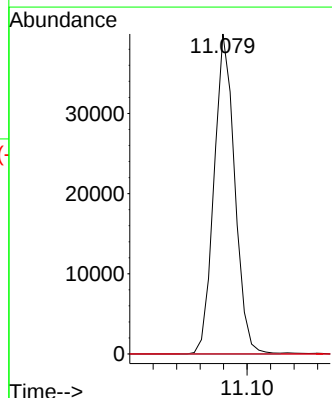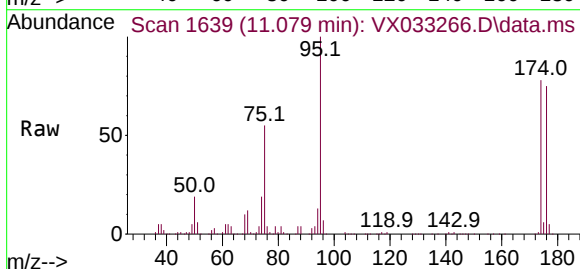



#85

sec-Butylbenzene

Concen: 0.313 ug/l

RT: 11.890 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX033266.D

Acq: 06 Dec 2022 18:08

Instrument :

MSVOA_X

ClientSampleId :





MW-42DL

Tgt Ion:105 Resp: 2192

Ion Ratio Lower Upper

105 100

134 34.0 9.9 29.7#

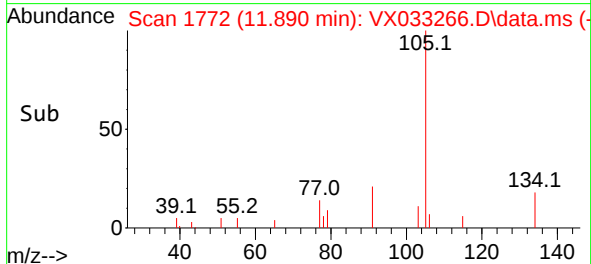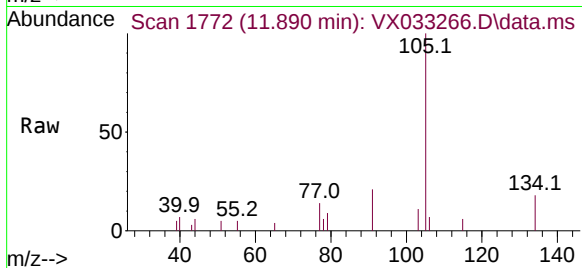

#89

n-Butylbenzene

Concen: 0.291 ug/l

RT: 12.317 min Scan# 1842

Delta R.T. -0.018 min

Lab File: VX033266.D

Acq: 06 Dec 2022 18:08




Tgt Ion: 91 Resp: 1490


Ion Ratio Lower Upper

91 100

92 0.0 26.2 78.6#

134 102.7 12.9 38.6#

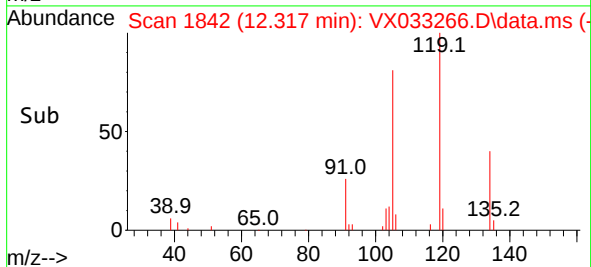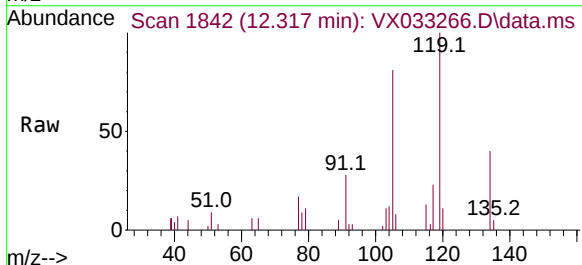



#90
 Hexachloroethane
 Concen: 45.283 ug/l
 RT: 12.701 min Scan# 1905
 Delta R.T. 0.159 min
 Lab File: VX033266.D
 Acq: 06 Dec 2022 18:08

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-42DL

Tgt Ion:117 Resp: 44152
 Ion Ratio Lower Upper
 117 100
 201 0.0 37.6 112.9#

