

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120624\
 Data File : VX044163.D
 Acq On : 06 Dec 2024 09:38
 Operator : JC/MD
 Sample : VX1206MBL01
 Misc : 5.00g/5.0ml/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 07 03:56:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 07 03:56:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.751	114	258462	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	221792	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	89494	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	94919	40.131	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.260%
7) Chloroethane-d5	1.660	69	79364	43.316	ug/L	0.01
Spiked Amount	50.000	Range	70 - 130	Recovery	=	86.640%
11) 1,1-Dichloroethene-d2	2.300	65	41316	40.845	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.680%
21) 2-Butanone-d5	4.446	46	145121	100.214	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.210%
24) Chloroform-d	5.044	84	179284	39.922	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.840%
26) 1,2-Dichloroethane-d4	5.940	65	127228	40.061	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.120%
32) Benzene-d6	5.964	84	321484	41.950	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.900%
36) 1,2-Dichloropropane-d6	7.300	67	101369	42.599	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	85.200%
41) Toluene-d8	8.641	98	285094	40.234	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.460%
43) trans-1,3-Dichloroprop...	8.946	79	45970	40.200	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.400%
47) 2-Hexanone-d5	9.378	63	87913	94.751	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	94.750%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	135606	42.499	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.000%
66) 1,2-Dichlorobenzene-d4	12.317	152	84920	40.726	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.460%
Target Compounds						
44) trans-1,3-Dichloropropene	8.946	75	2754	1.026	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120624\
Data File : VX044163.D
Acq On : 06 Dec 2024 09:38
Operator : JC/MD
Sample : VX1206MBL01
Misc : 5.00g/5.0ml/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Dec 07 03:56:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 03:56:15 2024
Response via : Initial Calibration

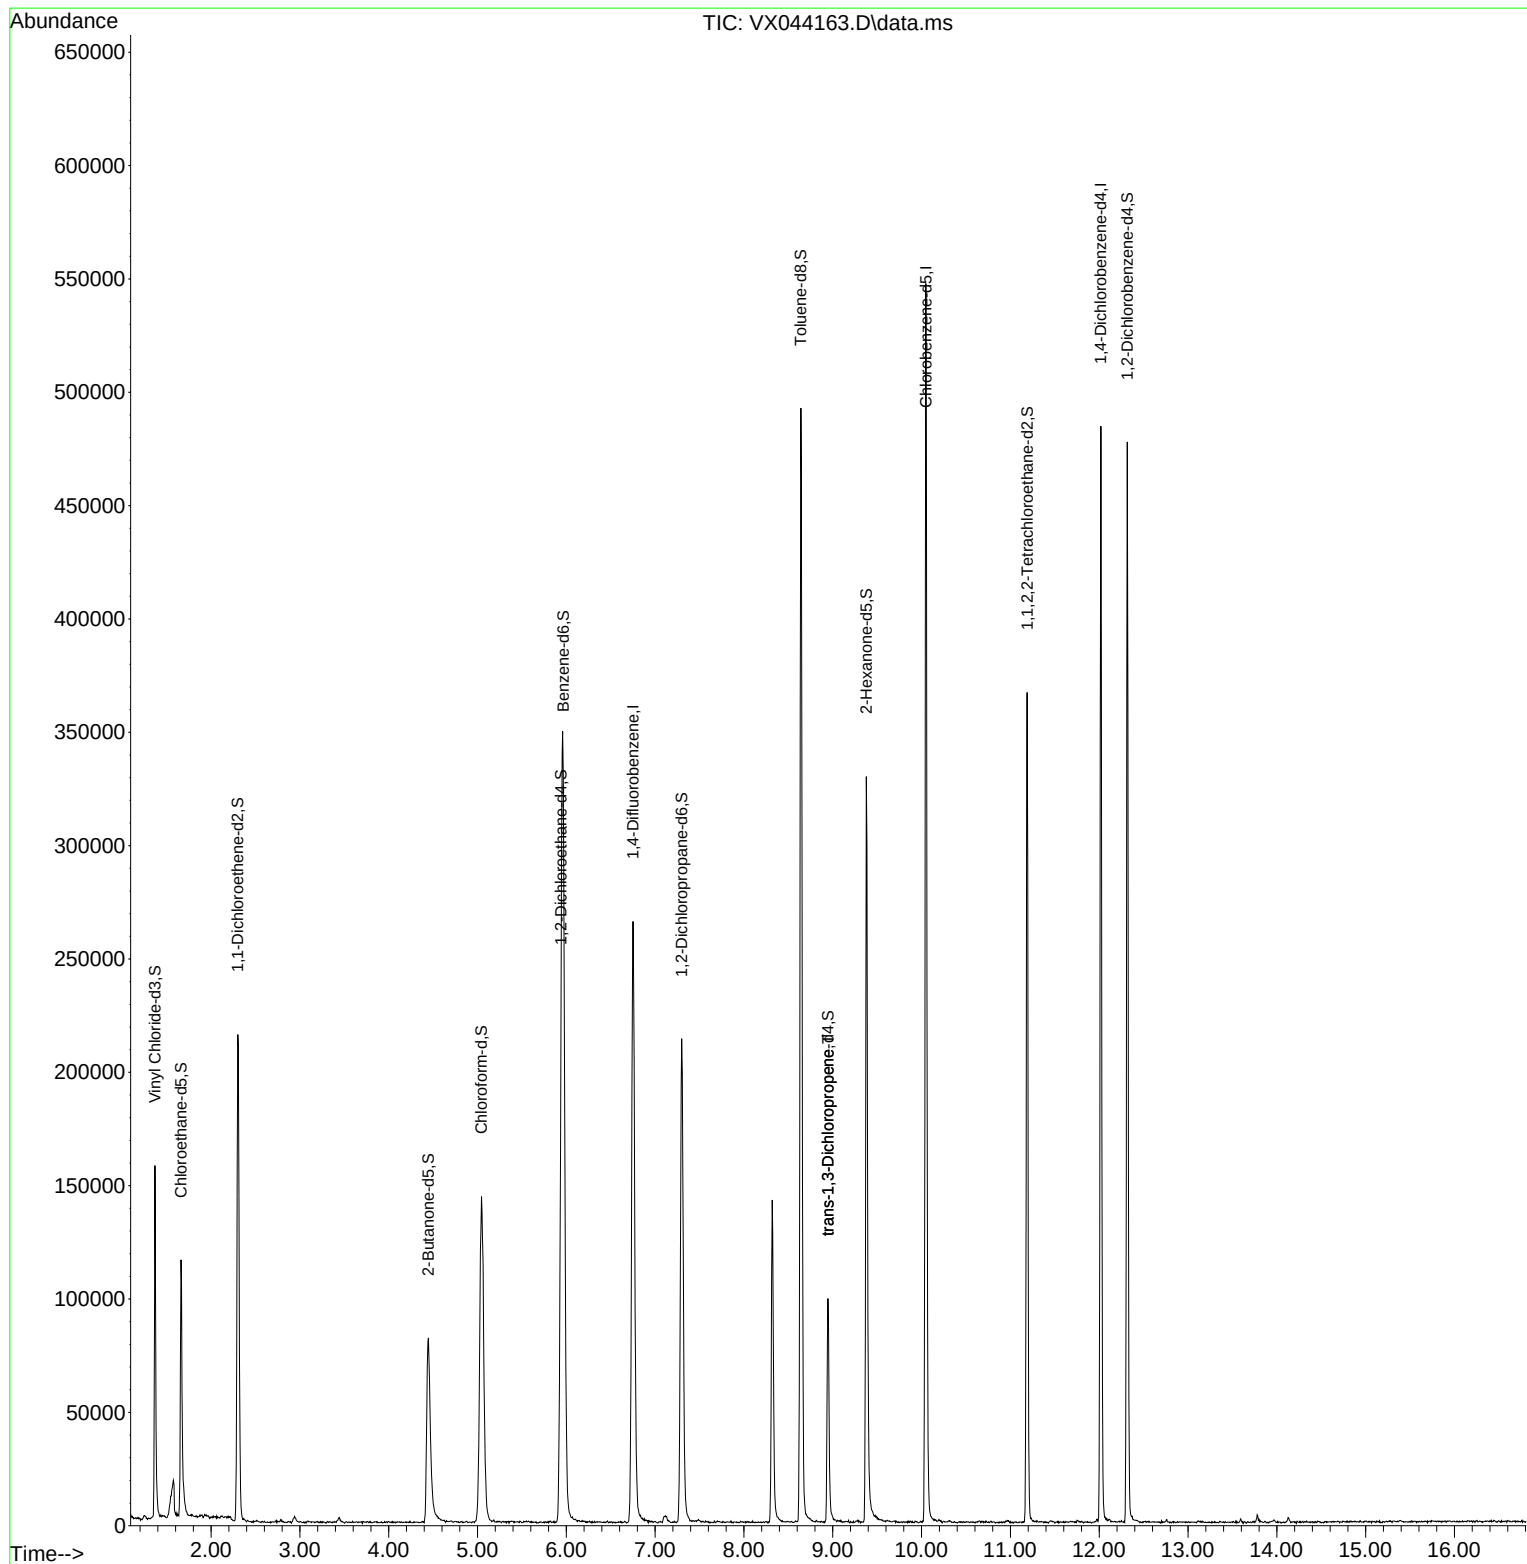

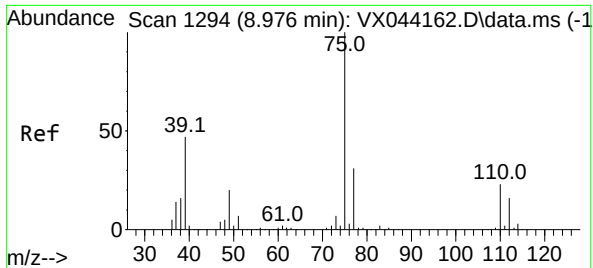

#44
 trans-1,3-Dichloropropene
 Concen: 1.026 ug/L
 RT: 8.946 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VX044163.D
 Acq: 06 Dec 2024 09:38

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 75 Resp: 2754
 Ion Ratio Lower Upper
 75 100
 77 26.2 21.8 40.6

