

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120624\
Data File : VX044170.D
Acq On : 06 Dec 2024 12:45
Operator : JC/MD
Sample : P5066-02
Misc : 5.89g/5.0ml/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1




Instrument :
MSVOA_X
ClientSampleId :
E28M1

Manual IntegrationsAPPROVED

Quant Time: Dec 07 03:58:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 03:56:15 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

12/09/2024
Supervised By :Semsettin
Yesilyurt

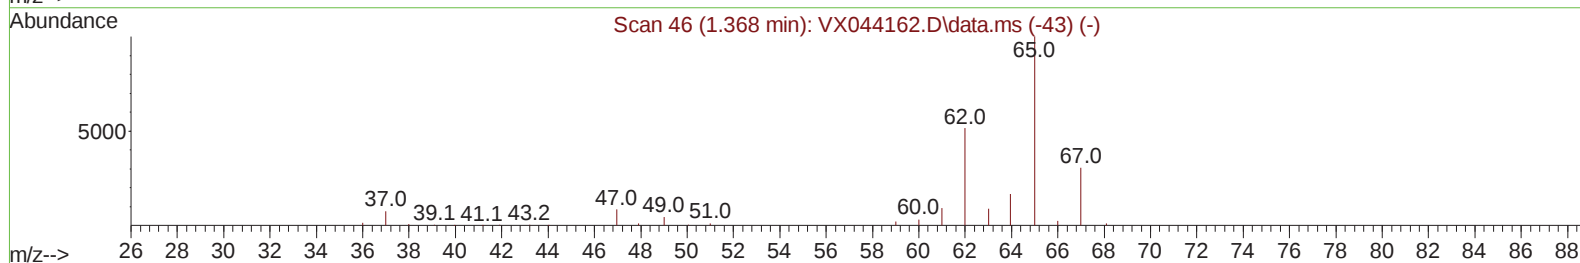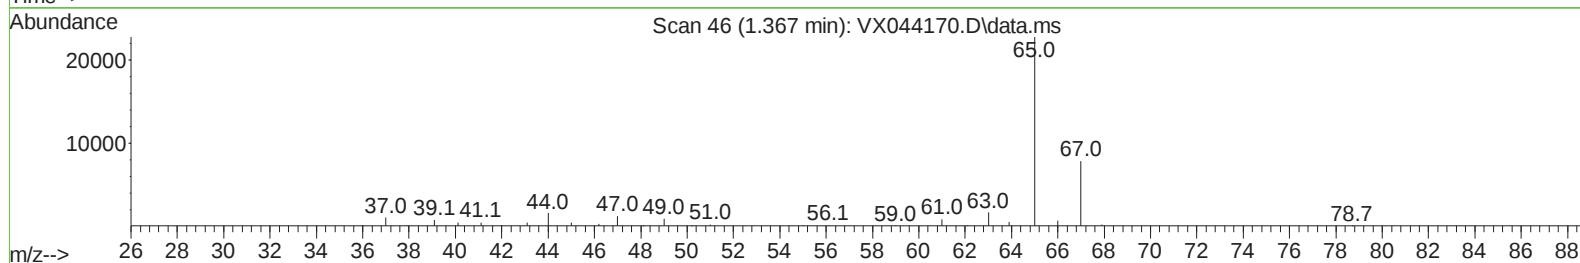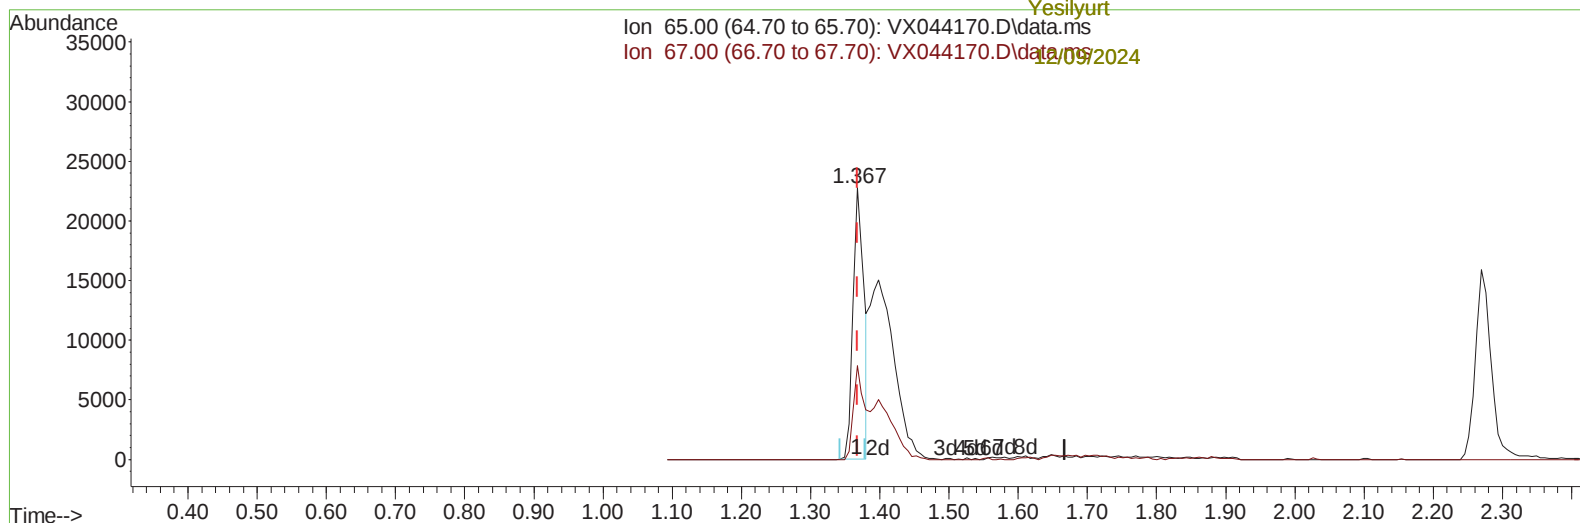

TIC: VX044170.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.367min (-0.000) 14.62 ug/L

response 25075

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	32.10	38.39
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120624\
Data File : VX044170.D
Acq On : 06 Dec 2024 12:45
Operator : JC/MD
Sample : P5066-02
Misc : 5.89g/5.0ml/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1




Instrument :
MSVOA_X
ClientSampleId :
E28M1

Manual IntegrationsAPPROVED

Reviewed By :Mahesh
Dadoda

12/09/2024
Supervised By :Semsettin
Yesilvurt

Quant Time: Dec 07 03:58:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 03:56:15 2024
Response via : Initial Calibration

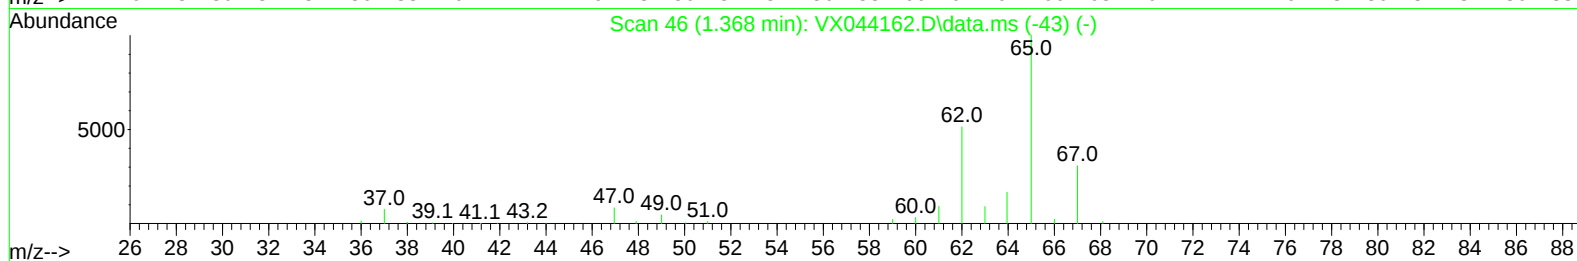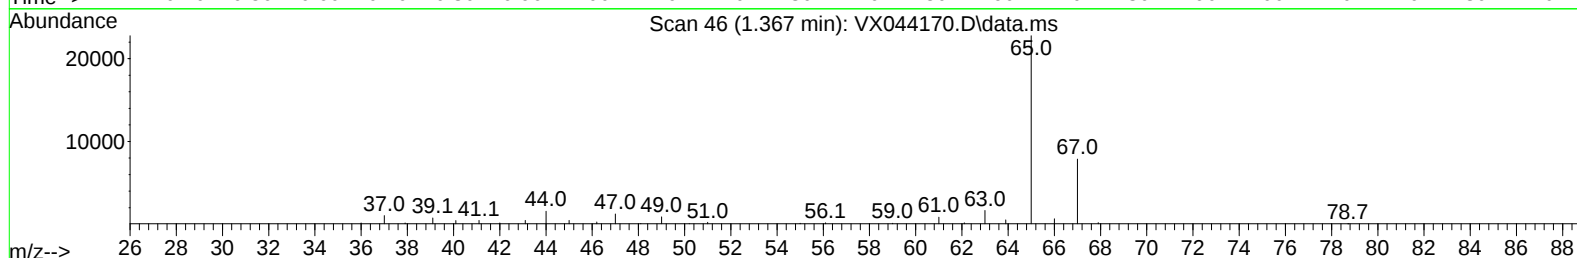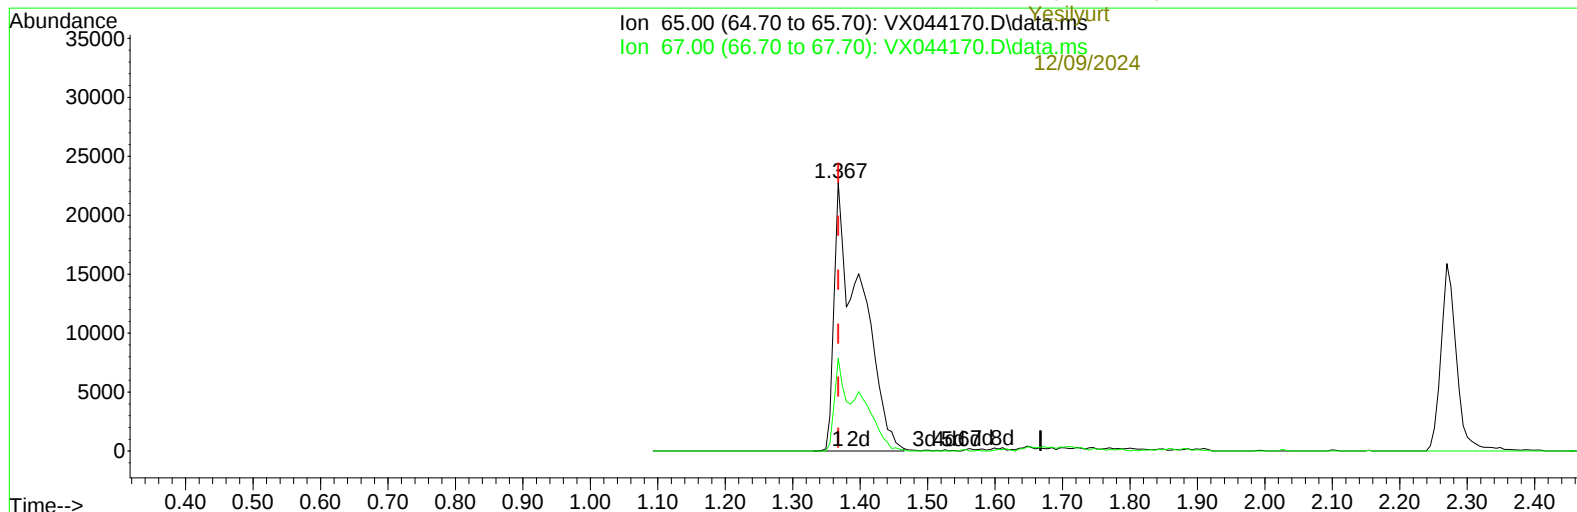

TIC: VX044170.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.367min (-0.000) 36.28 ug/L m

response 62227

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	32.10	15.47#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120624\
Data File : VX044170.D
Acq On : 06 Dec 2024 12:45
Operator : JC/MD
Sample : P5066-02
Misc : 5.89g/5.0ml/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E28M1


Manual IntegrationsAPPROVED

Reviewed By :Mahesh
Dadoda


12/09/2024
Supervised By :Semsettin
Yesilyurt

Quant Time: Dec 07 03:58:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 03:56:15 2024
Response via : Initial Calibration


Ion 69.00 (68.70 to 69.70): VX044170.D\data.ms
Ion 71.00 (70.70 to 71.70): VX044170.D\data.ms
Ion 51.00 (50.70 to 51.70): VX044170.D\data.ms

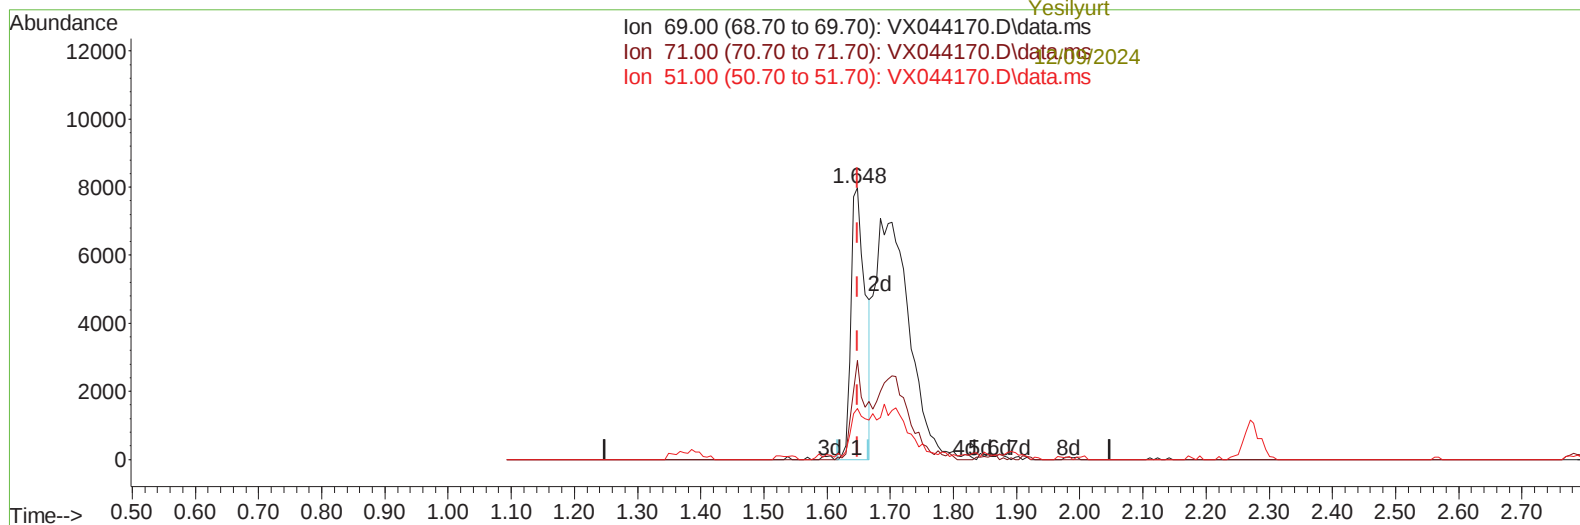

Scan 92 (1.648 min): VX044170.D\data.ms

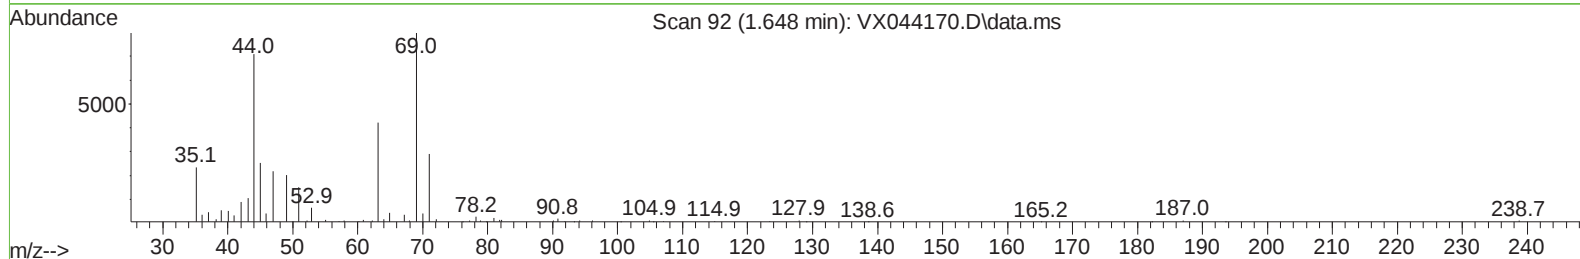

Scan 92 (1.648 min): VX044162.D\data.ms (-88) (-)

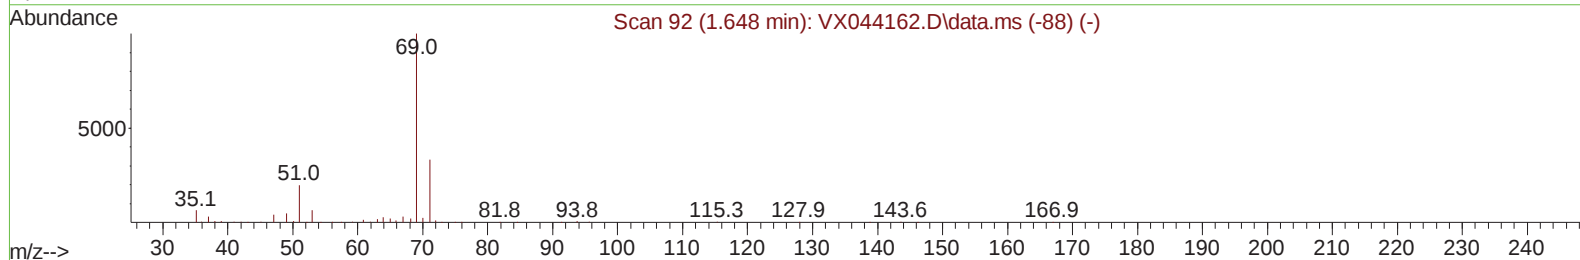

TIC: VX044170.D\data.ms

(7) Chloroethane-d5 (S)

1.648min (-0.000) 9.56 ug/L

response 12707

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	27.61
51.00	28.20	21.36
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120624\
 Data File : VX044170.D
 Acq On : 06 Dec 2024 12:45
 Operator : JC/MD
 Sample : P5066-02
 Misc : 5.89g/5.0ml/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1




Instrument :
 MSVOA_X
 ClientSampleId :
 E28M1

Manual IntegrationsAPPROVED

Quant Time: Dec 07 03:58:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 07 03:56:15 2024
 Response via : Initial Calibration

Reviewed By :Mahesh
 Dadoda

12/09/2024
 Supervised By :Semsettin
 Yesilyurt

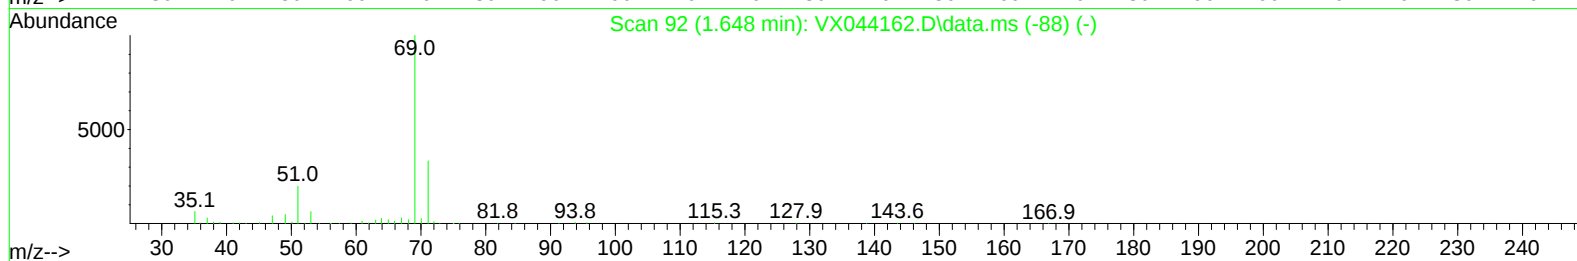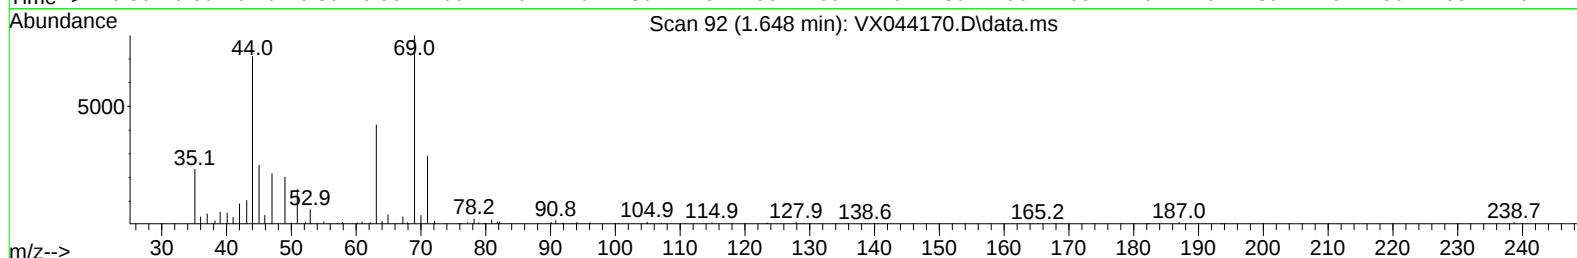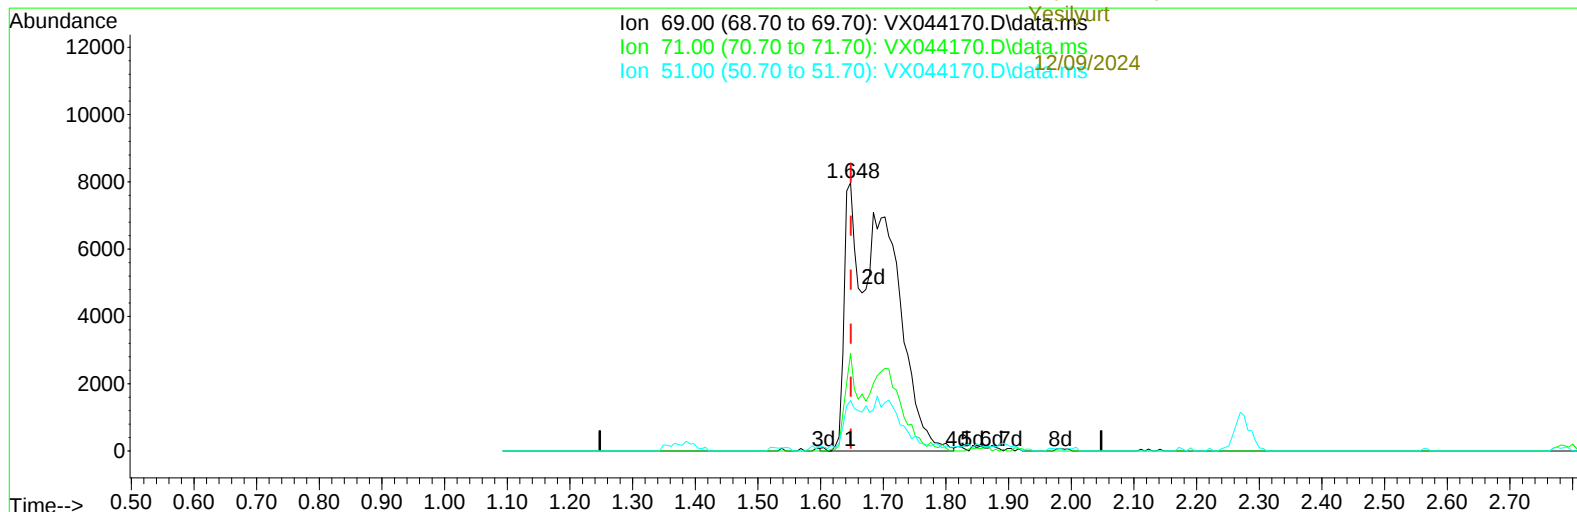

TIC: VX044170.D\data.ms

(7) Chloroethane-d5 (S)

1.648min (-0.000) 29.93 ug/L m

response 39770

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	8.82#
51.00	28.20	6.82#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120624\
Data File : VX044170.D
Acq On : 06 Dec 2024 12:45
Operator : JC/MD
Sample : P5066-02
Misc : 5.89g/5.0ml/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1




Instrument :
MSVOA_X
ClientSampleId :
E28M1

Manual IntegrationsAPPROVED

Reviewed By :Mahesh
Dadoda

12/09/2024
Supervised By :Semsettin
Yesilyurt

Quant Time: Dec 07 03:58:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 03:56:15 2024
Response via : Initial Calibration

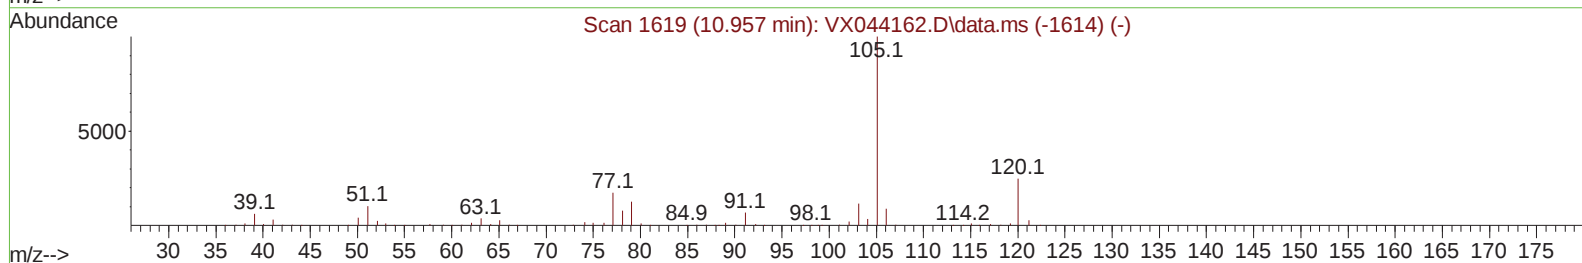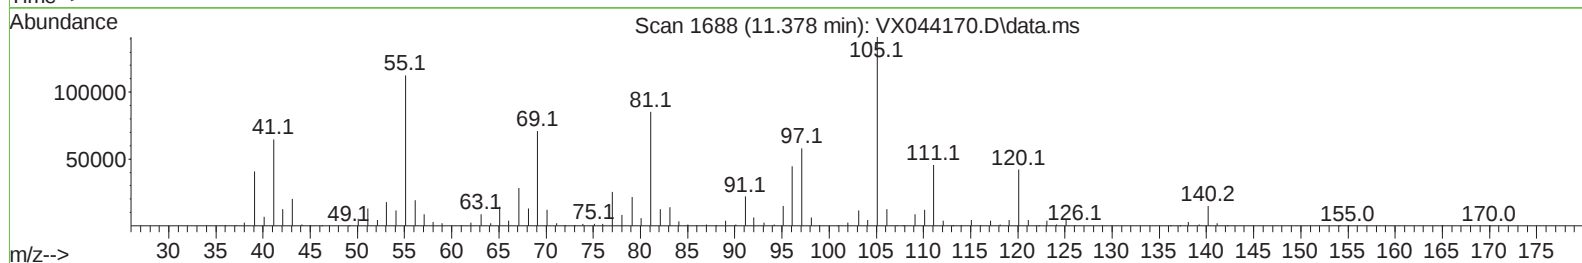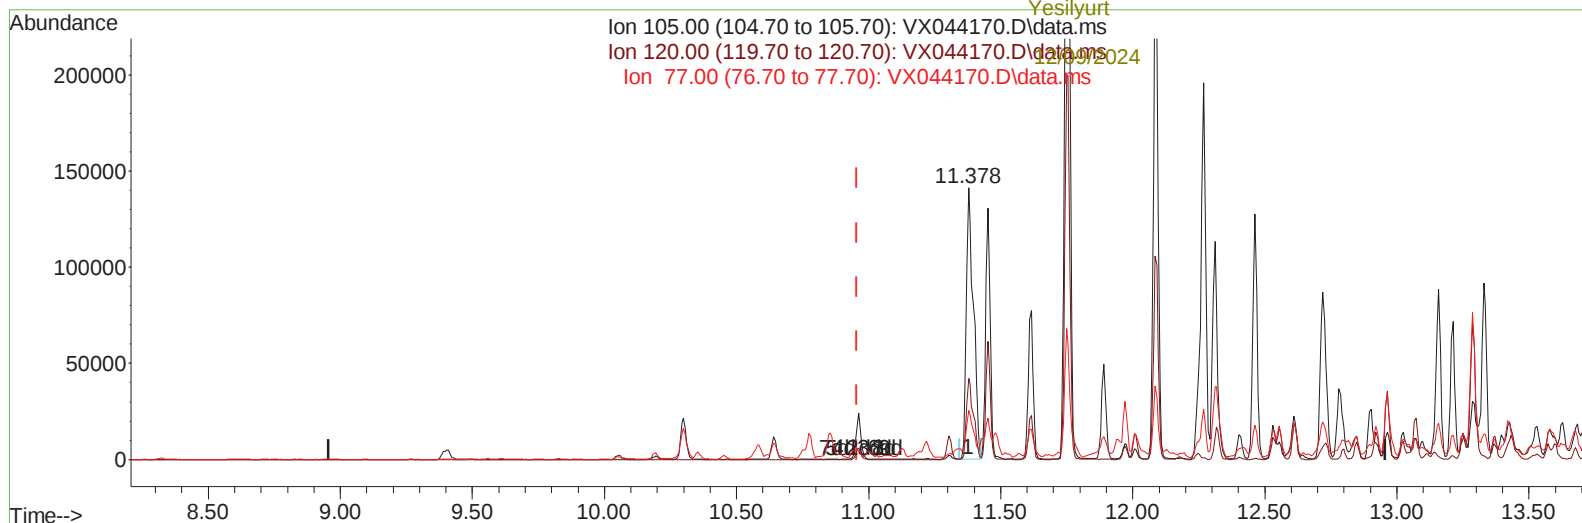

TIC: VX044170.D\data.ms

(60) Isopropylbenzene

11.378min (+ 0.420) 43.15 ug/L

response 261338

Ion	Exp%	Act%
105.00	100.00	100.00
120.00	25.80	29.47
77.00	16.70	16.26
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120624\
Data File : VX044170.D
Acq On : 06 Dec 2024 12:45
Operator : JC/MD
Sample : P5066-02
Misc : 5.89g/5.0ml/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1




Instrument :
MSVOA_X
ClientSampleId :
E28M1

Manual IntegrationsAPPROVED

Quant Time: Dec 07 03:58:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 03:56:15 2024
Response via : Initial Calibration

Reviewed By :Mahesh
Dadoda

12/09/2024
Supervised By :Semsettin
Yesilyurt

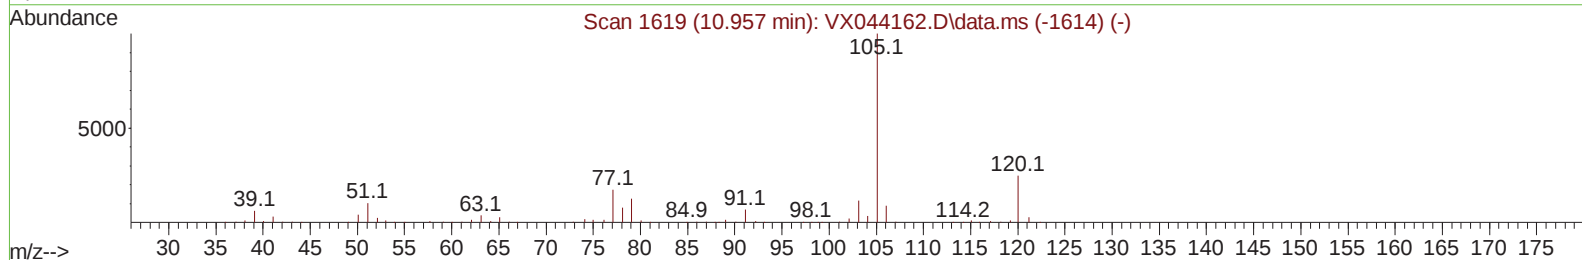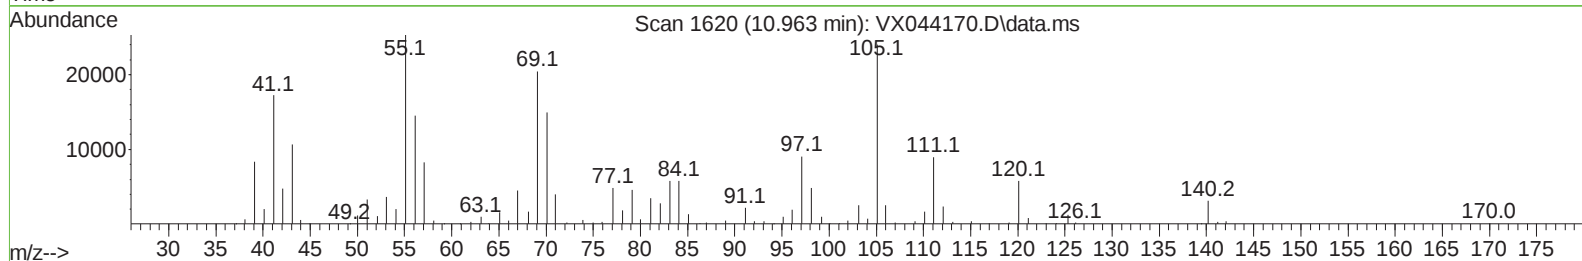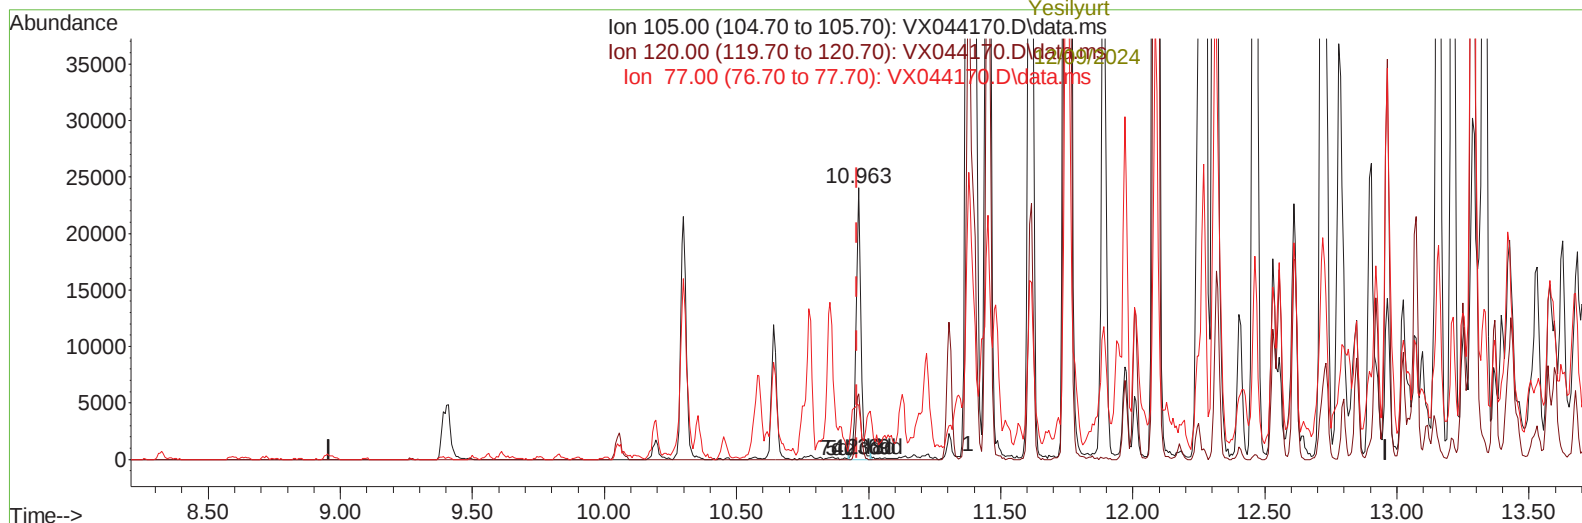

TIC: VX044170.D\data.ms

(60) Isopropylbenzene

10.963min (+ 0.006) 4.93 ug/L m

response 29866

Ion	Exp%	Act%
105.00	100.00	100.00
120.00	25.80	257.86#
77.00	16.70	142.32#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120624\
 Data File : VX044170.D
 Acq On : 06 Dec 2024 12:45
 Operator : JC/MD
 Sample : P5066-02
 Misc : 5.89g/5.0ml/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E28M1

Manual IntegrationsAPPROVED

Reviewed By :Mahesh
 Dadoda

12/09/2024
 Supervised By :Semsettin
 Yesilyurt

Quant Time: Dec 07 03:58:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 07 03:56:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----12/09/2024						
Internal Standards						
1) 1,4-Difluorobenzene	6.751	114	187419	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	169216	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	78496	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	62227m	36.282	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	72.560%	
7) Chloroethane-d5	1.648	69	39770m	29.934	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	59.860%#	
11) 1,1-Dichloroethene-d2	2.270	65	25084	34.198	ug/L	-0.02
Spiked Amount 50.000	Range 60	- 125	Recovery	=	68.400%	
21) 2-Butanone-d5	4.495	46	82289	78.365	ug/L	0.04
Spiked Amount 100.000	Range 40	- 130	Recovery	=	78.370%	
24) Chloroform-d	5.050	84	114396	35.129	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	70.260%	
26) 1,2-Dichloroethane-d4	5.946	65	84702	36.781	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	73.560%	
32) Benzene-d6	5.958	84	219322	37.511	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	75.020%	
36) 1,2-Dichloropropane-d6	7.299	67	70324	38.735	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	77.460%	
41) Toluene-d8	8.647	98	210310	38.901	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	77.800%#	
43) trans-1,3-Dichloroprop...	8.945	79	27304	31.295	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	62.600%	
47) 2-Hexanone-d5	9.396	63	51128	72.226	ug/L	0.01
Spiked Amount 100.000	Range 45	- 130	Recovery	=	72.230%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	121595	49.949	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	99.900%	
66) 1,2-Dichlorobenzene-d4	12.323	152	74383	40.670	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	81.340%	
Target Compounds						
					Qvalue	
34) Trichloroethene	7.116	95	24729	17.627	ug/L	88
35) Methylcyclohexane	7.366	83	15484	7.619	ug/L	92
42) Toluene	8.714	91	31944	5.867	ug/L	90
46) Tetrachloroethene	9.268	164	602245	643.522	ug/L	96
52) Ethylbenzene	10.189	91	53716	8.956	ug/L	98
53) m,p-Xylene	10.299	106	68159	31.377	ug/L	93
54) o-Xylene	10.640	106	38308	17.149	ug/L	99
60) Isopropylbenzene	10.963	105	29866m	4.931	ug/L	
62) 1,3,5-Trimethylbenzene	11.451	105	154058	30.648	ug/L	99
63) 1,2,4-Trimethylbenzene	11.750	105	593135	120.232	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120624\
Data File : VX044170.D
Acq On : 06 Dec 2024 12:45
Operator : JC/MD
Sample : P5066-02
Misc : 5.89g/5.0ml/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E28M1

Manual IntegrationsAPPROVED

Reviewed By :Mahesh
Dadoda

12/09/2024
Supervised By :Semsettin
Yesilyurt

12/09/2024

