

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120624\
 Data File : VX044163.D
 Acq On : 06 Dec 2024 09:38
 Operator : JC/MD
 Sample : VX1206MBL01
 Misc : 5.00g/5.0ml/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK734

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044163.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rBV	154994	160724	15.19%	2.073%
2	1.660	90	94	107	rBV	112875	161831	15.30%	2.087%
3	2.300	193	199	208	rBV	214485	350950	33.17%	4.526%
4	2.410	215	217	221	rBV4	717	939	0.09%	0.012%
5	2.575	242	244	246	rBV2	624	616	0.06%	0.008%
6	2.684	260	262	265	rBV3	514	802	0.08%	0.010%
7	2.733	268	270	271	rVB2	996	593	0.06%	0.008%
8	2.745	271	272	275	rBV2	695	726	0.07%	0.009%
9	2.782	276	278	283	rVB4	1017	1339	0.13%	0.017%
10	2.867	290	292	295	rBV4	543	662	0.06%	0.009%
11	2.941	298	304	312	rBV5	2914	7134	0.67%	0.092%
12	3.093	326	329	330	rBV3	854	1026	0.10%	0.013%
13	3.312	362	365	367	rBV2	838	950	0.09%	0.012%
14	3.337	367	369	371	rVV2	624	594	0.06%	0.008%
15	3.447	381	387	390	rVV5	2058	3731	0.35%	0.048%
16	3.526	396	400	402	rBV	619	850	0.08%	0.011%
17	3.709	429	430	434	rBV4	885	1253	0.12%	0.016%
18	3.837	447	451	452	rBV4	519	532	0.05%	0.007%
19	3.953	466	470	472	rBV3	658	618	0.06%	0.008%
20	3.995	475	477	481	rVV4	523	654	0.06%	0.008%
21	4.446	543	551	574	rBV	81537	246999	23.34%	3.186%
22	4.648	583	584	586	rBV2	789	654	0.06%	0.008%
23	4.824	609	613	615	rVB3	621	773	0.07%	0.010%
24	4.958	631	635	636	rBV3	496	617	0.06%	0.008%
25	5.044	638	649	668	rVB	143601	453882	42.90%	5.854%
26	5.288	686	689	691	rBV4	723	909	0.09%	0.012%
27	5.318	691	694	695	rVB	638	627	0.06%	0.008%
28	5.367	700	702	703	rBV2	760	745	0.07%	0.010%
29	5.477	719	720	723	rVB4	745	606	0.06%	0.008%
30	5.702	754	757	758	rVV	519	524	0.05%	0.007%
31	5.958	787	799	816	rBV3	348997	1058044	100.00%	13.646%
32	6.294	853	854	857	rBV2	760	685	0.06%	0.009%
33	6.348	860	863	864	rBV3	465	520	0.05%	0.007%
34	6.464	878	882	884	rVB3	825	819	0.08%	0.011%
35	6.751	920	929	942	rBV	264935	639656	60.46%	8.250%
36	6.928	957	958	962	rBV3	1078	1280	0.12%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120624\
 Data File : VX044163.D
 Acq On : 06 Dec 2024 09:38
 Operator : JC/MD
 Sample : VX1206MBL01
 Misc : 5.00g/5.0ml/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK734

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	7.043	975	977	979	rBV	621	706	0.07%	0.009%
38	7.104	983	987	988	rBV3	2781	3789	0.36%	0.049%
39	7.300	1011	1019	1034	rVV2	213102	478116	45.19%	6.166%
40	7.537	1056	1058	1062	rVB2	591	512	0.05%	0.007%
41	7.568	1062	1063	1065	rVV2	677	493	0.05%	0.006%
42	7.665	1078	1079	1082	rVB2	815	501	0.05%	0.006%
43	7.702	1082	1085	1087	rBV3	810	1035	0.10%	0.013%
44	7.885	1114	1115	1118	rBV2	520	592	0.06%	0.008%
45	8.251	1172	1175	1178	rVB4	680	983	0.09%	0.013%
46	8.318	1180	1186	1204	rVV	142298	240925	22.77%	3.107%
47	8.580	1227	1229	1233	rBV3	586	679	0.06%	0.009%
48	8.641	1233	1239	1253	rBV	491161	782076	73.92%	10.087%
49	8.818	1266	1268	1270	rBV2	757	659	0.06%	0.008%
50	8.946	1284	1289	1301	rVV	98863	156214	14.76%	2.015%
51	9.055	1305	1307	1309	rVV2	932	954	0.09%	0.012%
52	9.177	1326	1327	1329	rVB	1195	571	0.05%	0.007%
53	9.378	1355	1360	1375	rBV	328894	494016	46.69%	6.371%
54	9.848	1436	1437	1440	rBV	746	665	0.06%	0.009%
55	9.878	1440	1442	1444	rVB3	739	519	0.05%	0.007%
56	9.927	1448	1450	1452	rBV2	794	694	0.07%	0.009%
57	9.988	1456	1460	1463	rBV3	699	899	0.08%	0.012%
58	10.049	1465	1470	1486	rVV	546061	745199	70.43%	9.611%
59	10.250	1500	1503	1505	rBV4	752	1102	0.10%	0.014%
60	10.628	1562	1565	1566	rBV3	575	606	0.06%	0.008%
61	10.878	1605	1606	1609	rBV2	627	623	0.06%	0.008%
62	11.049	1632	1634	1636	rBV2	594	672	0.06%	0.009%
63	11.110	1639	1644	1647	rBV5	456	852	0.08%	0.011%
64	11.189	1651	1657	1663	rBV	366033	490507	46.36%	6.326%
65	11.390	1688	1690	1693	rBV2	580	640	0.06%	0.008%
66	11.451	1696	1700	1704	rBV4	1042	2234	0.21%	0.029%
67	11.750	1748	1749	1751	rBV2	1074	979	0.09%	0.013%
68	11.805	1756	1758	1761	rVB	748	736	0.07%	0.009%
69	11.933	1776	1779	1780	rBV2	505	584	0.06%	0.008%
70	11.975	1784	1786	1788	rVV2	1280	1139	0.11%	0.015%
71	12.018	1788	1793	1803	rVV	483146	602350	56.93%	7.769%
72	12.250	1829	1831	1835	rVB4	755	596	0.06%	0.008%
73	12.317	1837	1842	1856	rBV	476611	607445	57.41%	7.834%
74	12.701	1903	1905	1906	rBV	1054	503	0.05%	0.006%
75	12.762	1912	1915	1917	rVB3	1159	874	0.08%	0.011%
76	12.829	1923	1926	1927	rBV2	595	492	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120624\
 Data File : VX044163.D
 Acq On : 06 Dec 2024 09:38
 Operator : JC/MD
 Sample : VX1206MBL01
 Misc : 5.00g/5.0ml/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK734

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	13.109	1970	1972	1973	rBV2	773	721	0.07%	0.009%
78	13.146	1976	1978	1980	rVV	815	551	0.05%	0.007%
79	13.164	1980	1981	1984	rVV2	670	566	0.05%	0.007%
80	13.359	2010	2013	2016	rBV	687	828	0.08%	0.011%
81	13.420	2021	2023	2026	rBV3	618	593	0.06%	0.008%
82	13.591	2047	2051	2056	rVB2	2043	3038	0.29%	0.039%
83	13.640	2056	2059	2062	rBV2	824	1068	0.10%	0.014%
84	13.676	2062	2065	2068	rBV4	748	1022	0.10%	0.013%
85	13.743	2072	2076	2077	rBV3	603	605	0.06%	0.008%
86	13.780	2078	2082	2086	rBV2	3245	4046	0.38%	0.052%
87	13.865	2094	2096	2100	rVB3	778	874	0.08%	0.011%
88	14.128	2133	2139	2144	rBV3	2309	3890	0.37%	0.050%
89	14.225	2154	2155	2158	rBV2	919	1013	0.10%	0.013%
90	14.402	2181	2184	2185	rVB3	599	568	0.05%	0.007%
91	14.457	2191	2193	2195	rBV	780	723	0.07%	0.009%
92	14.713	2234	2235	2239	rBV3	507	700	0.07%	0.009%
93	14.743	2239	2240	2243	rBV	568	613	0.06%	0.008%
94	14.938	2270	2272	2274	rBV4	783	645	0.06%	0.008%
95	15.194	2313	2314	2317	rBV2	558	555	0.05%	0.007%
96	15.871	2423	2425	2427	rBV3	609	647	0.06%	0.008%
97	15.920	2431	2433	2435	rBV2	633	646	0.06%	0.008%
98	16.213	2480	2481	2484	rBV3	686	639	0.06%	0.008%
99	16.603	2543	2545	2547	rBV2	801	937	0.09%	0.012%
100	16.780	2572	2574	2575	rBV2	641	569	0.05%	0.007%

Sum of corrected areas: 7753652




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120624\
Data File : VX044163.D
Acq On : 06 Dec 2024 09:38
Operator : JC/MD
Sample : VX1206MBL01
Misc : 5.00g/5.0ml/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK734

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

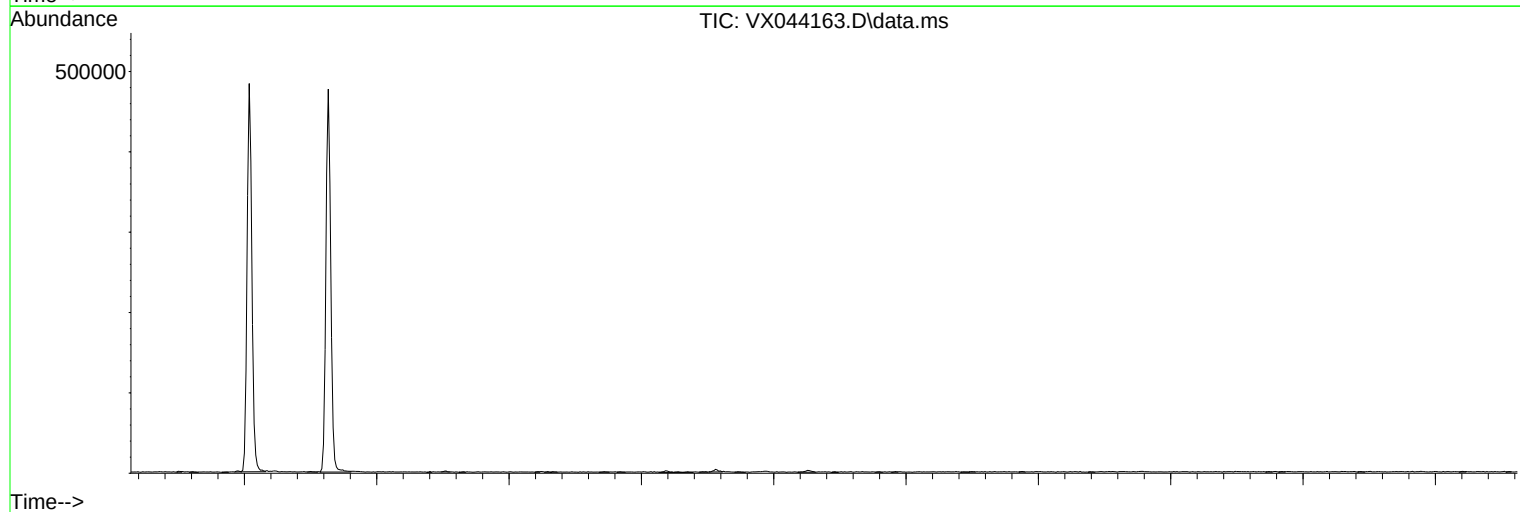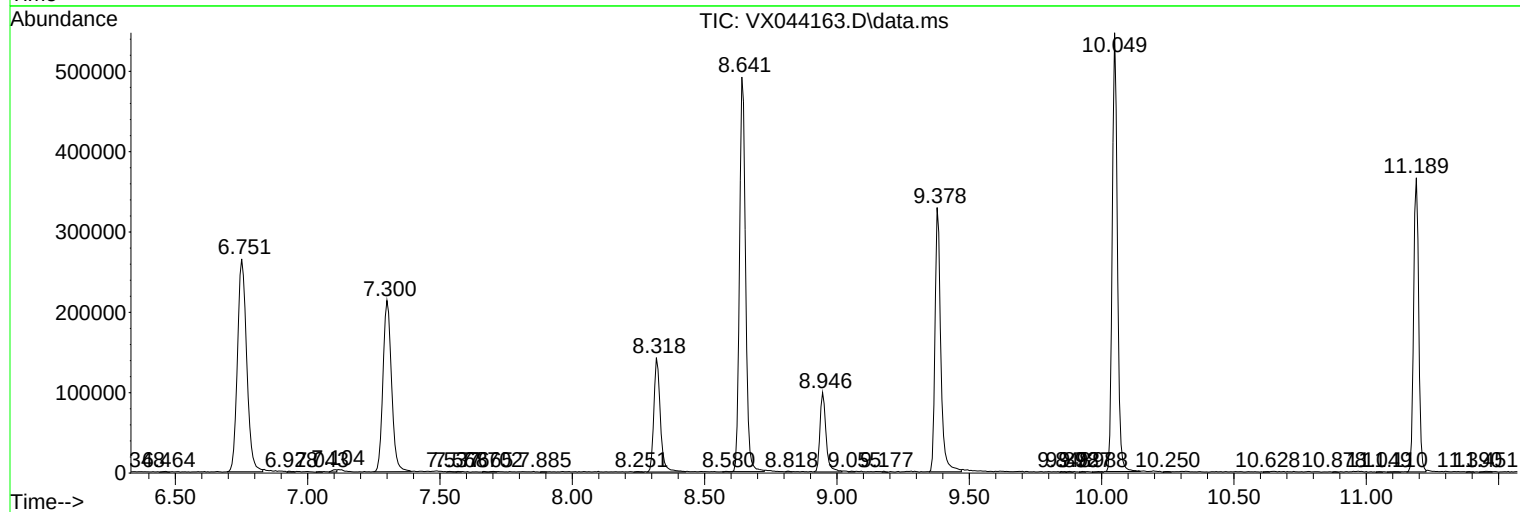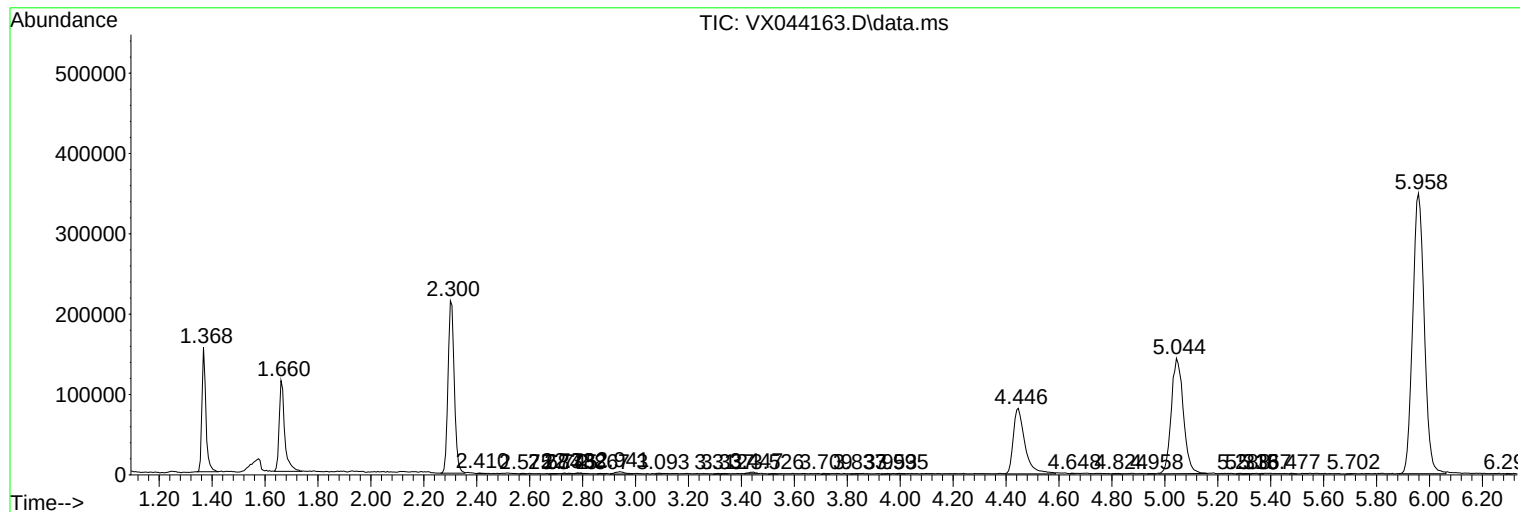

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120624\
Data File : VX044163.D
Acq On : 06 Dec 2024 09:38
Operator : JC/MD
Sample : VX1206MBL01
Misc : 5.00g/5.0ml/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK734

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120624\
Data File : VX044163.D
Acq On : 06 Dec 2024 09:38
Operator : JC/MD
Sample : VX1206MBL01
Misc : 5.00g/5.0ml/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK734

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc