
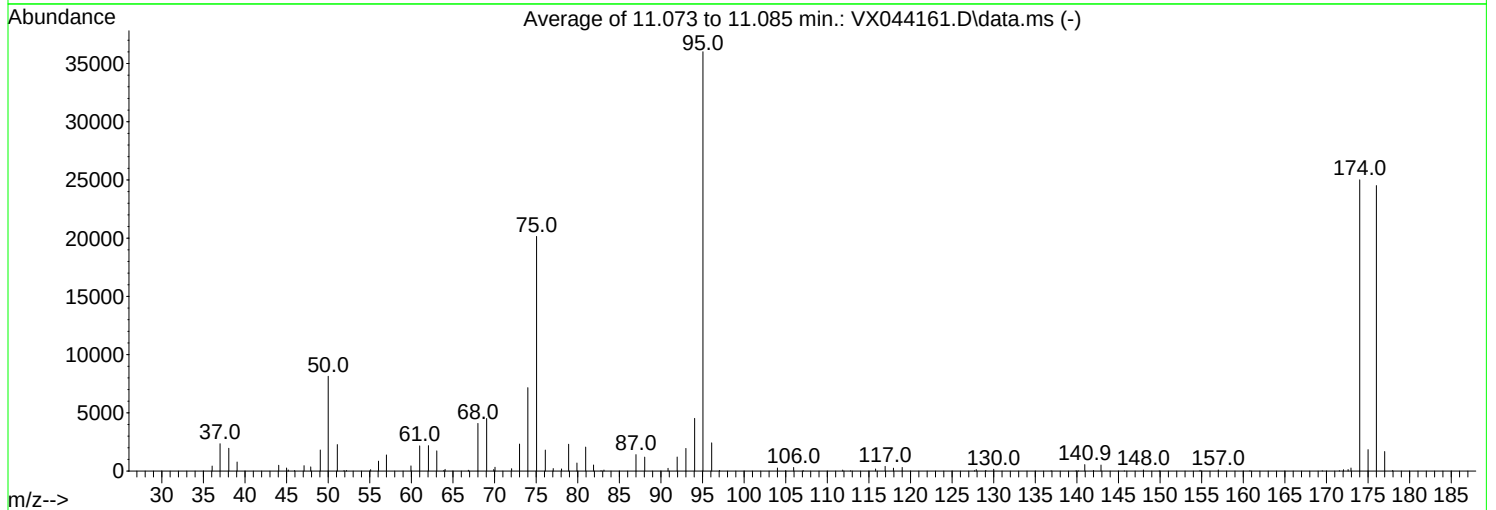


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120624\
Data File : VX044161.D
Acq On : 06 Dec 2024 08:08
Operator : JC/MD
Sample : BFB704
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB704

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Title : VOC Analysis
Last Update : Sat Dec 07 03:56:15 2024

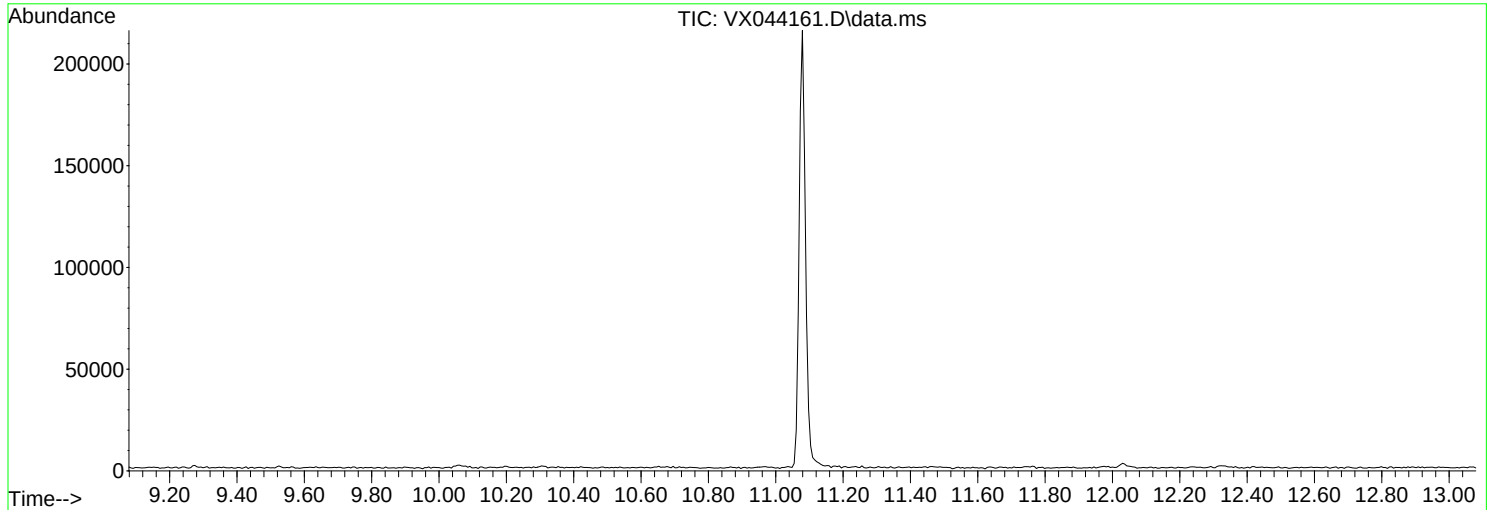

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	8141	PASS
75	95	30	80	56.0	20154	PASS
95	95	100	100	100.0	36011	PASS
96	95	5	9	6.7	2423	PASS
173	174	0.00	2	1.1	264	PASS
174	95	50	120	69.5	25013	PASS
175	174	5	9	7.4	1842	PASS
176	174	95	101	98.0	24520	PASS
177	176	5	9	6.8	1676	PASS

m/z	Abundance
38.80	399.0
39.10	433.0
40.00	703.0
41.10	161.0
44.10	204.0

Instrument :
MSVOA_X
ClientSampleId :
BFB704

m/z	Abundance
36.00	529.0
37.00	2212.0
38.00	1947.0
39.10	1441.0
40.00	631.0
41.00	56.0
44.00	794.0
45.00	441.0
45.90	74.0
47.10	366.0
47.90	276.0
49.10	1865.0
50.00	8911.0
51.10	2380.0
52.30	58.0
55.10	227.0
56.00	835.0
57.00	1297.0
59.90	390.0
61.00	2255.0
62.10	1933.0
63.00	2014.0
63.90	177.0
66.80	128.0
68.00	4147.0
69.00	4700.0
69.90	414.0
72.10	187.0
73.00	2153.0
74.00	7066.0
75.10	20176.0
76.10	1955.0
77.00	209.0
78.10	221.0
78.90	2268.0
79.90	642.0
80.90	1873.0
81.90	479.0
83.20	102.0
87.00	1464.0
88.00	1242.0
91.00	298.0
91.90	1154.0
93.00	2000.0
94.00	4810.0
95.00	36776.0
96.00	2657.0
97.00	81.0
104.00	202.0
105.90	397.0
107.10	70.0
111.90	154.0
115.80	184.0
117.00	492.0
118.00	214.0
119.00	336.0
127.70	117.0
129.00	83.0
130.10	155.0
140.90	585.0
142.90	473.0
145.70	56.0
149.90	53.0
169.50	85.0
171.50	63.0
172.00	73.0
172.60	182.0
173.00	221.0
174.00	21360.0
175.00	1791.0
176.00	20048.0
177.00	1395.0

Instrument :
MSVOA_X
ClientSampleId :
BFB704

m/z	Abundance
36.00	448.0
37.00	3133.0
38.00	2418.0
39.10	1228.0
40.00	522.0
44.00	728.0
45.20	288.0
46.00	53.0
46.90	301.0
47.20	400.0
47.90	551.0
49.00	2019.0
50.00	9506.0
51.10	2844.0
51.90	121.0
55.10	130.0
56.10	1053.0
57.00	1723.0
60.00	524.0
61.00	2779.0
62.00	2891.0
63.10	1908.0
64.10	296.0
66.90	97.0
68.00	5045.0
69.10	5249.0
70.10	625.0
72.00	263.0
73.00	2814.0
74.00	8544.0
75.10	24512.0
76.10	1902.0
77.10	267.0
78.00	167.0
78.90	2908.0
79.90	711.0
81.00	2582.0
82.00	570.0
82.80	118.0
83.20	109.0
86.90	1577.0
88.10	1405.0
90.80	231.0
92.00	1454.0
93.00	2427.0
94.10	5321.0
95.00	40696.0
96.10	2364.0
97.10	84.0
104.00	376.0
105.00	75.0
105.90	204.0
107.10	56.0
111.80	106.0
112.80	71.0
115.80	221.0
117.00	336.0
117.90	283.0
119.10	402.0
127.90	221.0
129.10	90.0
129.90	153.0
140.90	587.0
142.00	78.0
143.00	557.0
148.10	150.0
154.90	85.0
157.00	220.0
160.80	95.0
172.00	188.0
172.60	216.0
173.00	314.0
174.00	29176.0
175.00	2015.0
176.00	30128.0
177.00	2017.0
177.90	70.0

Instrument :
MSVOA_X
ClientSampleId :
BFB704

m/z	Abundance
36.10	328.0
37.10	1704.0
38.10	1514.0
39.00	964.0
40.00	431.0
44.10	587.0
45.00	361.0
47.10	334.0
47.90	246.0
49.00	1547.0
50.10	6006.0
51.10	1605.0
52.10	85.0
56.00	671.0
57.00	1136.0
60.00	428.0
61.10	1462.0
62.00	1732.0
63.00	1284.0
64.00	156.0
68.00	3088.0
69.00	3591.0
70.00	369.0
72.00	172.0
73.00	1995.0
74.00	5890.0
75.00	15774.0
76.10	1562.0
77.10	187.0
78.00	163.0
78.90	1741.0
79.80	362.0
80.00	361.0
81.00	1731.0
81.80	516.0
83.00	64.0
87.10	1208.0
88.10	954.0
90.80	193.0
92.00	1018.0
93.10	1408.0
94.00	3453.0
95.10	30560.0
96.20	2249.0
104.00	214.0
106.00	322.0
115.80	141.0
116.90	391.0
117.90	257.0
118.90	207.0
127.90	183.0
130.00	162.0
136.90	68.0
139.90	65.0
140.20	55.0
141.00	496.0
142.00	72.0
142.80	525.0
147.90	139.0
154.70	116.0
157.00	75.0
171.60	55.0
172.10	91.0
172.90	257.0
174.00	24504.0
175.00	1720.0
176.00	23384.0
177.00	1615.0
178.00	70.0

Instrument :
MSVOA_X
ClientSampleId :
BFB704