

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX120718\
 Data File : VX006346.D
 Acq On : 07 Dec 2018 14:45
 Operator : JC/MD
 Sample : J6252-17
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CPA-CPMW11S-M16W4-11-27-18

Quant Time: Dec 08 01:05:04 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 30 03:55:33 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	808773	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	1235442	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	1127019	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	557536	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	408038	49.42	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.84%	
35) Dibromofluoromethane	5.51	113	382510	47.82	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.64%	
50) Toluene-d8	8.71	98	1447665	49.76	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.52%	
62) 4-Bromofluorobenzene	11.13	95	546819	49.87	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.74%	
Target Compounds						
44) Trichloroethene	7.21	130	5195	0.550	ug/l	96
64) Tetrachloroethene	9.34	164	111053	13.084	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX120718\
Data File : VX006346.D
Acq On : 07 Dec 2018 14:45
Operator : JC/MD
Sample : J6252-17
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CPA-CPMW11S-M16W4-11-27-18

Quant Time: Dec 08 01:05:04 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 30 03:55:33 2018
Response via : Initial Calibration

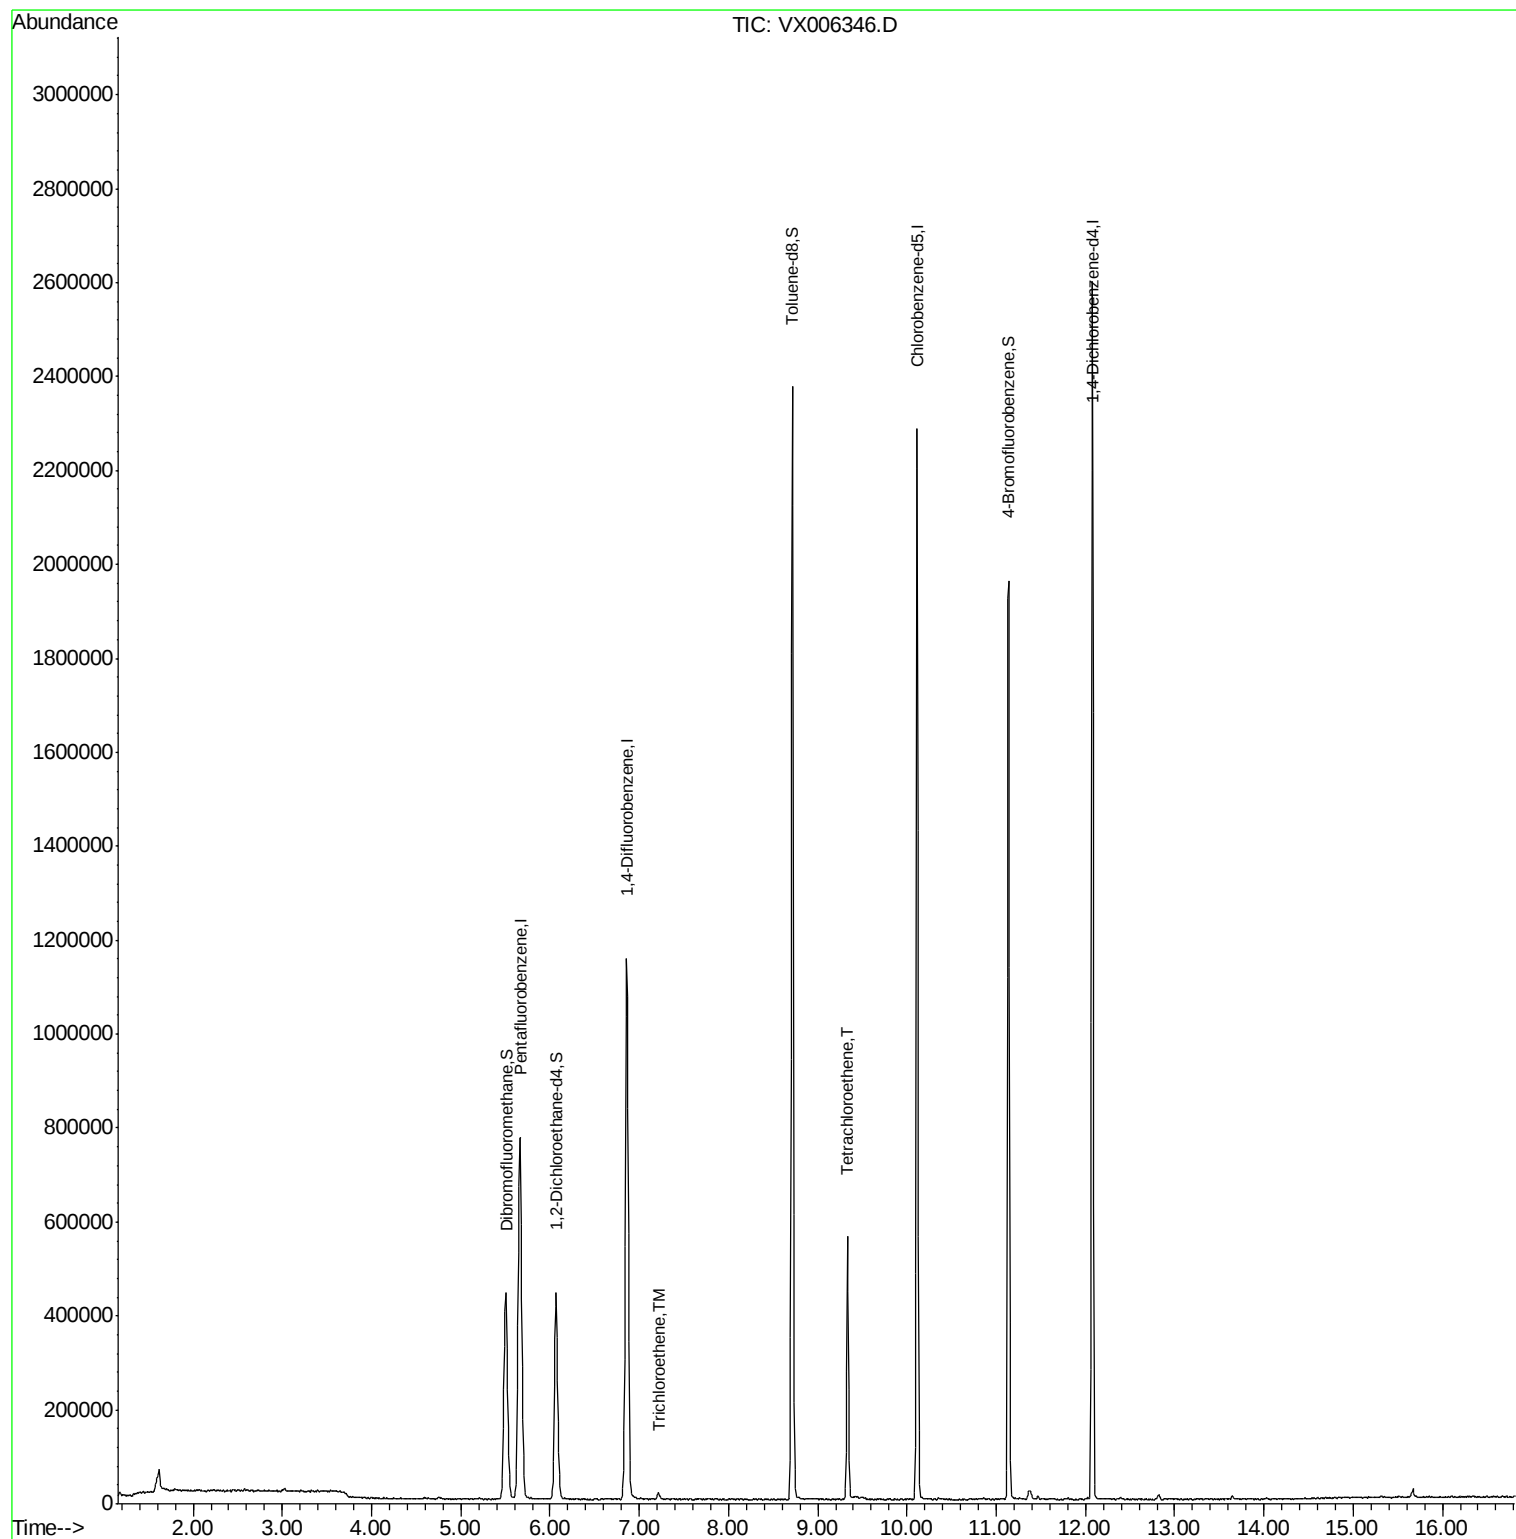

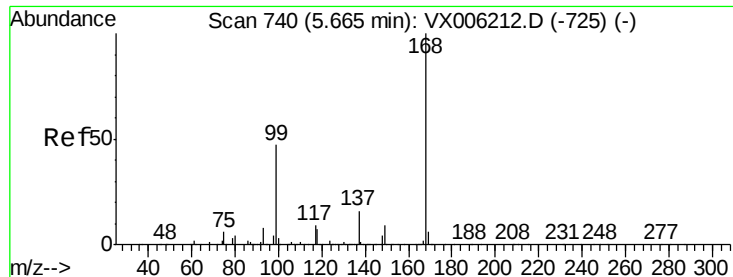

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.00 min

Lab File: VX006346.D

Acq: 07 Dec 2018 14:45

Instrument :

MSVOA_X

ClientSampleId :


CPA-CPMW11S-M16W4-11-27-18

Tot Ion:168 Resp: 808773

Ion Ratio Lower Upper

168 100

99 51.0 37.8 56.8

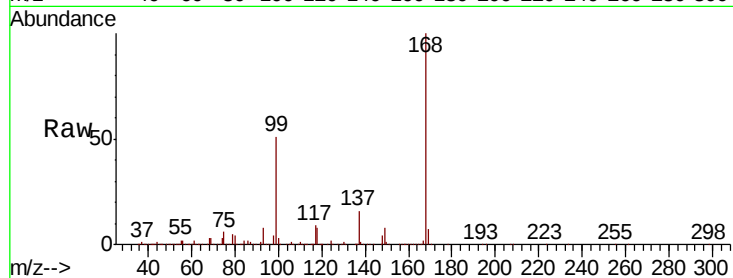

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

300000



200000

100000

0

Time-->

5.50 5.60 5.70 5.80

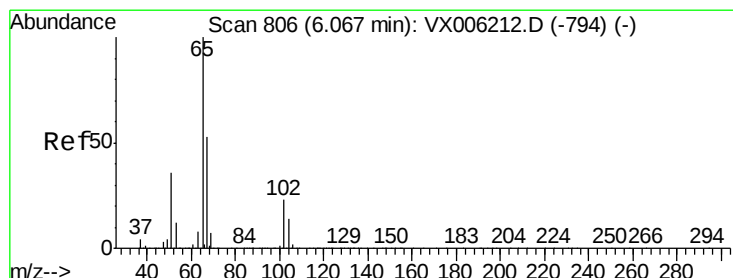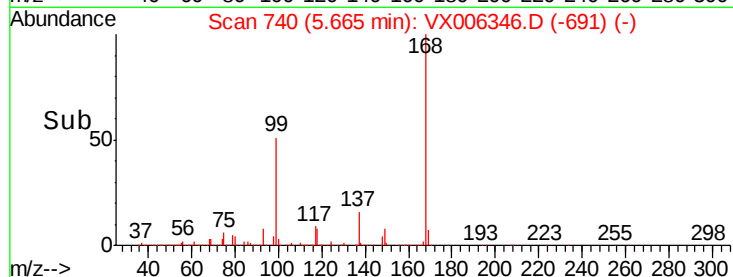

#33

1,2-Dichloroethane-d4

Concen: 49.422 ug/l

RT: 6.07 min Scan# 806

Delta R.T. -0.00 min

Lab File: VX006346.D


Acq: 07 Dec 2018 14:45

Tgt Ion: 65 Resp: 408038

Ion Ratio Lower Upper

65 100

67 53.4 0.0 107.2

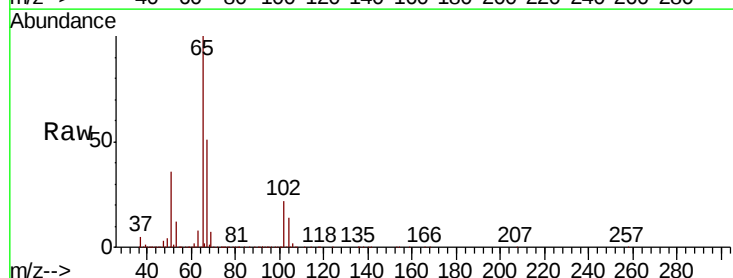

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07

150000


100000


50000

0

Time-->

6.00 6.10 6.20

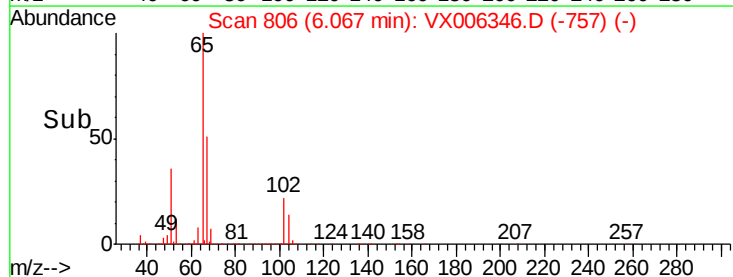

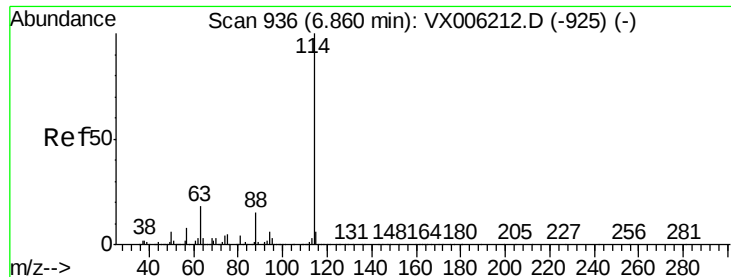

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX006346.D

Acq: 07 Dec 2018 14:45

Instrument :

MSVOA_X

ClientSampleId :

CPA-CPMW11S-M16W4-11-27-18


Tot Ion:114 Resp: 1235442

Ion Ratio Lower Upper

114 100

63 17.7 0.0 36.6




88 15.3 0.0 29.0

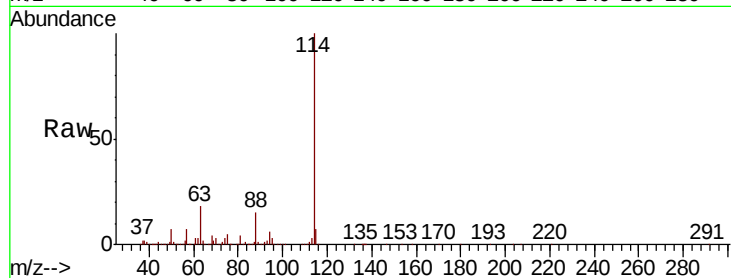

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

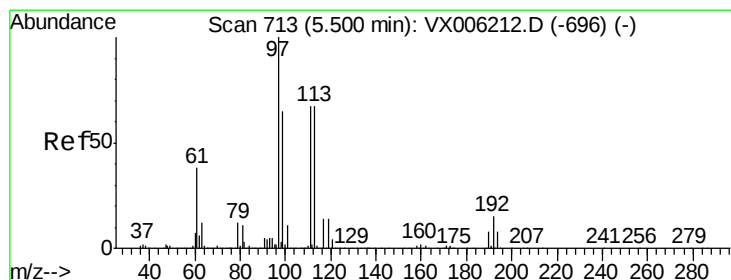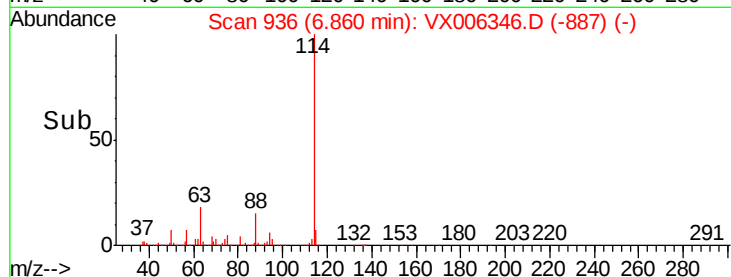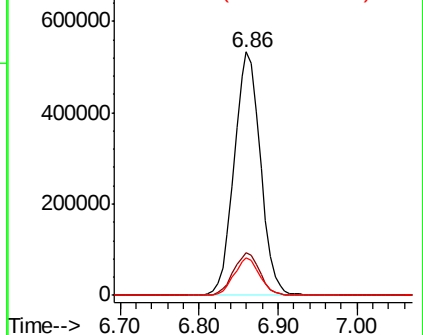

#35

Dibromofluoromethane

Concen: 47.820 ug/l

RT: 5.51 min Scan# 714

Delta R.T. 0.01 min

Lab File: VX006346.D

Acq: 07 Dec 2018 14:45


Tgt Ion:113 Resp: 382510

Ion Ratio Lower Upper

113 100

111 102.2 81.1 121.7



192 21.4 18.2 27.2

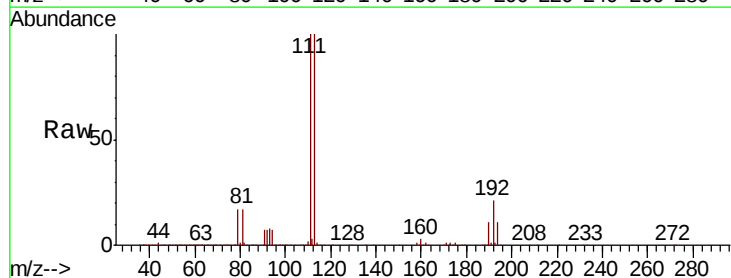


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

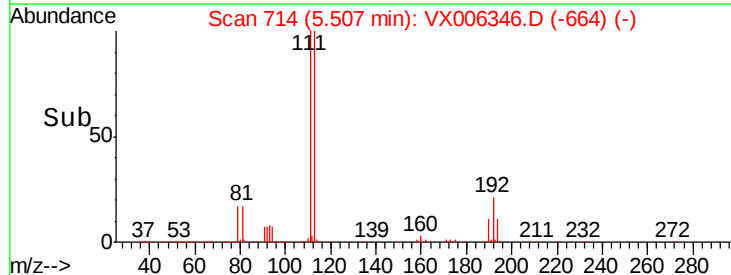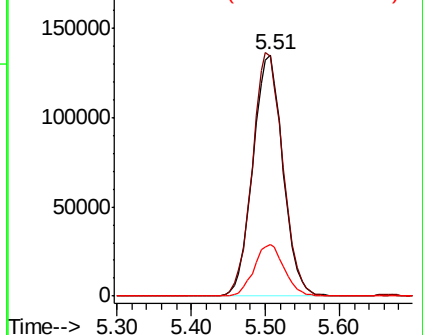

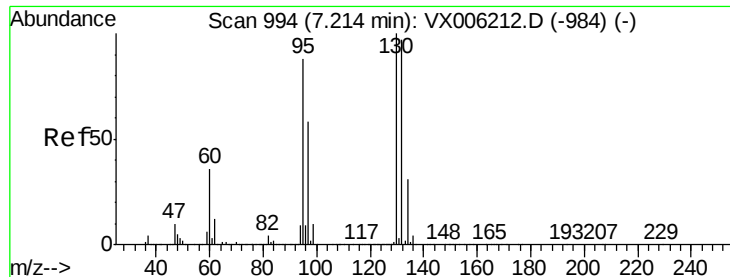

#44

Trichloroethene

Concen: 0.550 ug/l

RT: 7.21 min Scan# 994

Delta R.T. -0.00 min

Lab File: VX006346.D

Acq: 07 Dec 2018 14:45

Instrument :

MSVOA_X

ClientSampleId :


CPA-CPMW11S-M16W4-11-27-18

Tot Ion:130 Resp: 5195




Ion Ratio Lower Upper

130 100

95 84.2 0.0 175.8

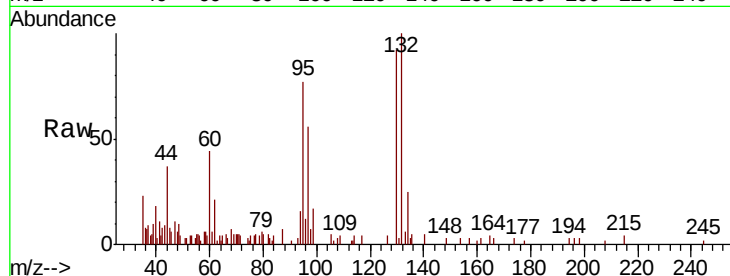

Abundance Ion 129.80 (129.50 to 130.50): V

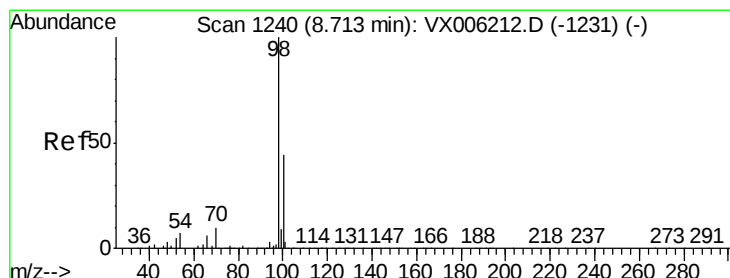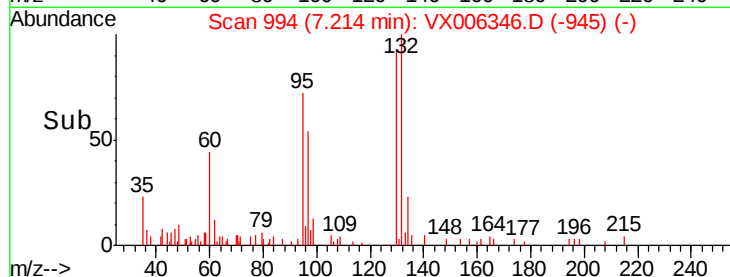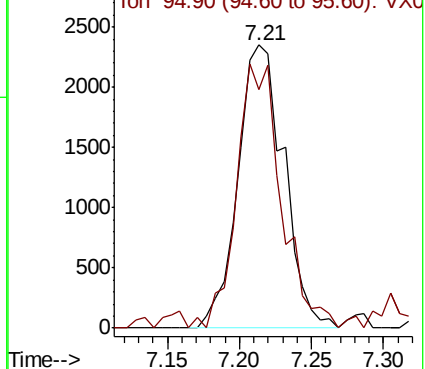

#50

Toluene-d8

Concen: 49.755 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX006346.D


Acq: 07 Dec 2018 14:45

Tgt Ion: 98 Resp: 1447665



Ion Ratio Lower Upper


98 100

100 64.5 52.2 78.2

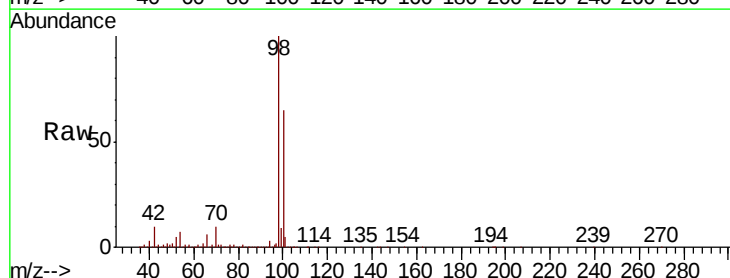

Abundance Ion 98.00 (97.70 to 98.70): VX0

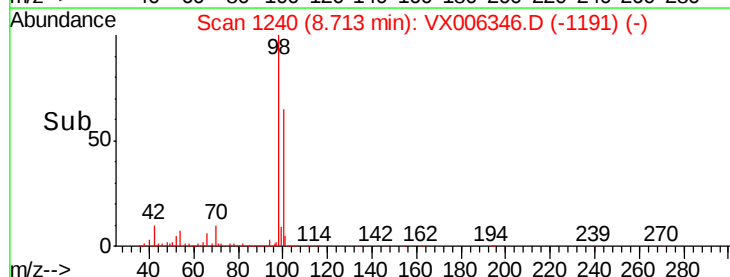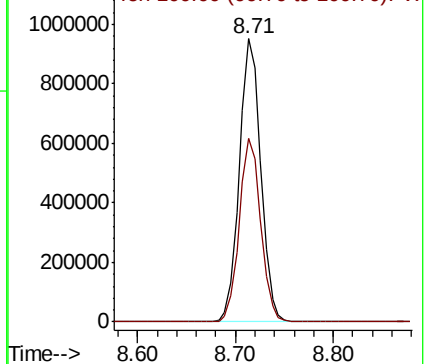

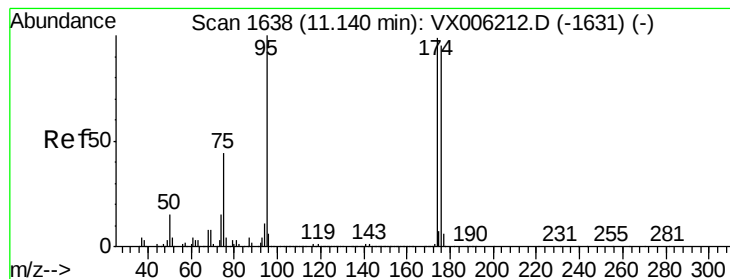

#62

4-Bromofluorobenzene

Concen: 49.874 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.01 min

Lab File: VX006346.D

Acq: 07 Dec 2018 14:45

Instrument :

MSVOA_X

ClientSampleId :

CPA-CPMW11S-M16W4-11-27-18


Tot Ion: 95 Resp: 546819

Ion Ratio Lower Upper

95 100

174 87.9 0.0 187.0




176 85.0 0.0 181.8

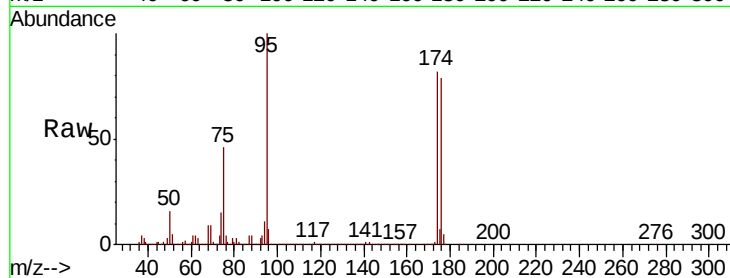

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

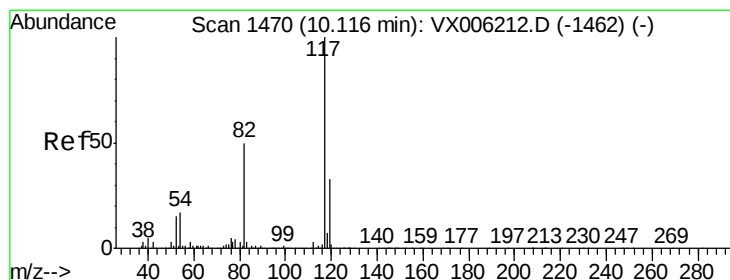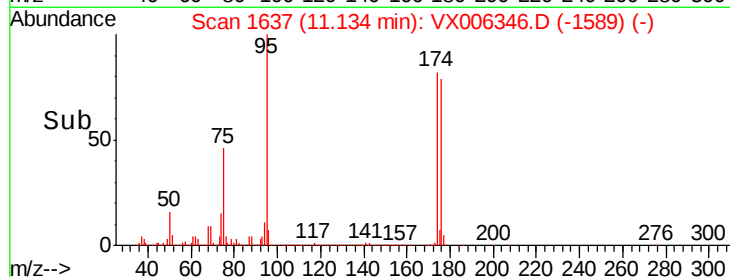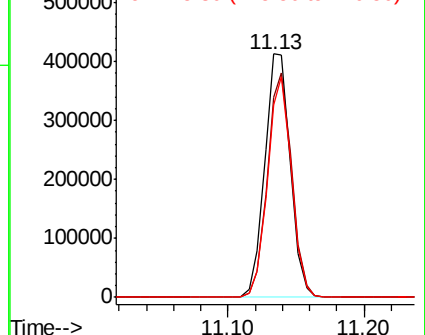

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.12 min Scan# 1470

Delta R.T. -0.00 min

Lab File: VX006346.D

Acq: 07 Dec 2018 14:45


Tgt Ion: 117 Resp: 1127019

Ion Ratio Lower Upper

117 100

82 49.8 39.6 59.4



119 32.1 26.3 39.5

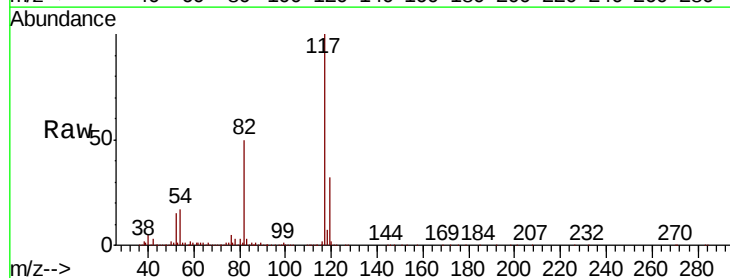


Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): V

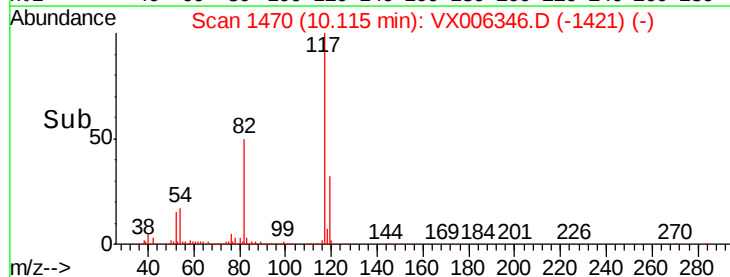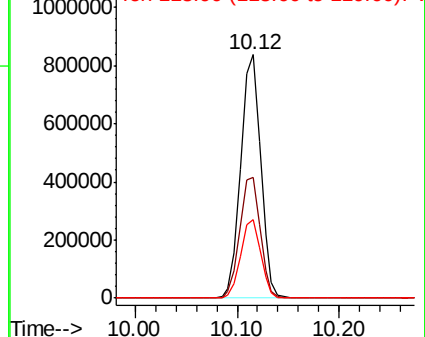

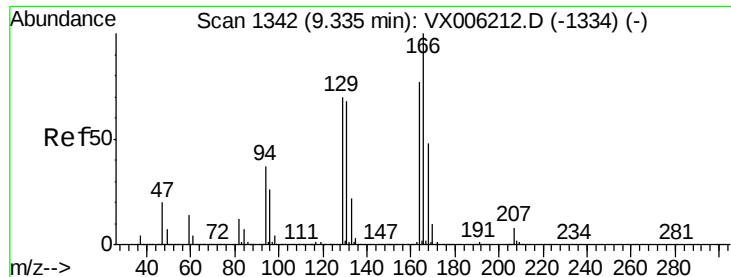

#64

Tetrachloroethene

Concen: 13.084 ug/l

RT: 9.34 min Scan# 1342

Delta R.T. -0.00 min

Lab File: VX006346.D

Acq: 07 Dec 2018 14:45

Instrument :

MSVOA_X

ClientSampleId :

CPA-CPMW11S-M16W4-11-27-18

Tot Ion:164 Resp: 111053


Ion Ratio Lower Upper

164 100

166 126.1 104.2 156.2

129 89.7 72.6 108.8

131 86.5 70.3 105.5



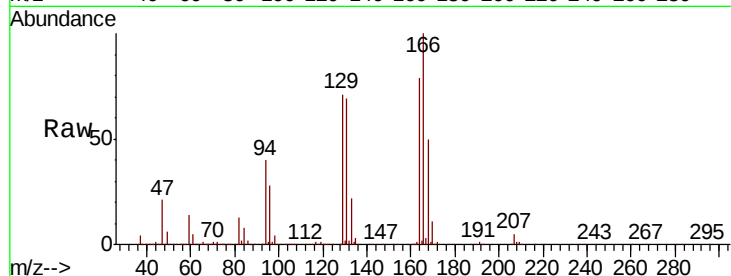


Abundance Ion 163.80 (163.50 to 164.50): V

Ion 165.80 (165.50 to 166.50): V

Ion 128.80 (128.50 to 129.50): V

Ion 130.80 (130.50 to 131.50): V

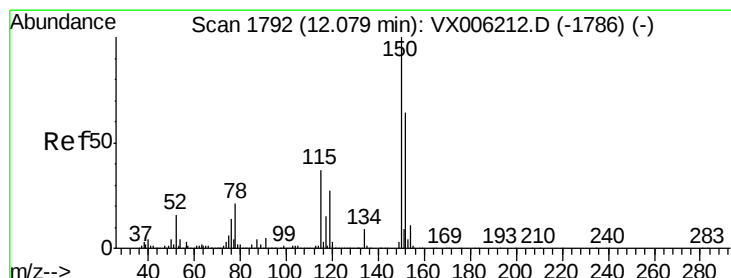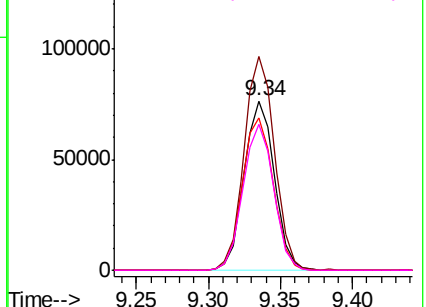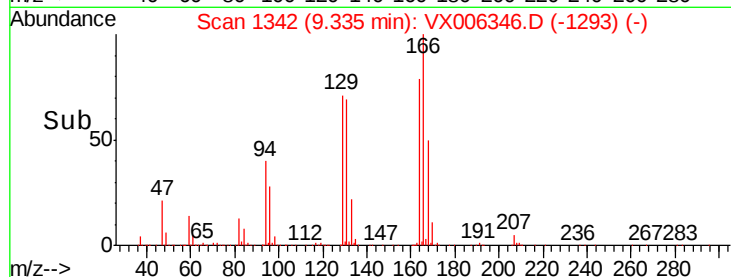

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX006346.D

Acq: 07 Dec 2018 14:45


Tgt Ion:152 Resp: 557536

Ion Ratio Lower Upper

152 100

115 55.8 39.0 116.9

150 156.1 0.0 345.8

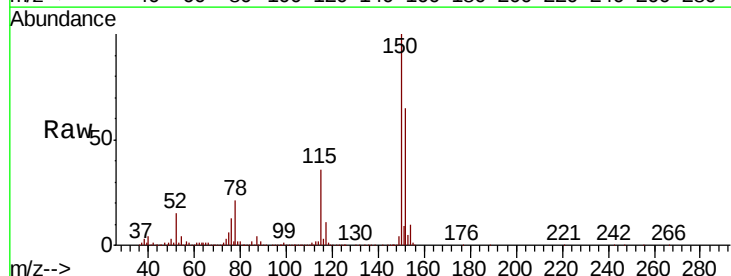

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

