


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX120718\  
 Data File : VX006334.D  
 Acq On : 07 Dec 2018 09:05  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X112918W.M  
 Title : SW846 8260  
 Last Update : Fri Nov 30 03:55:33 2018

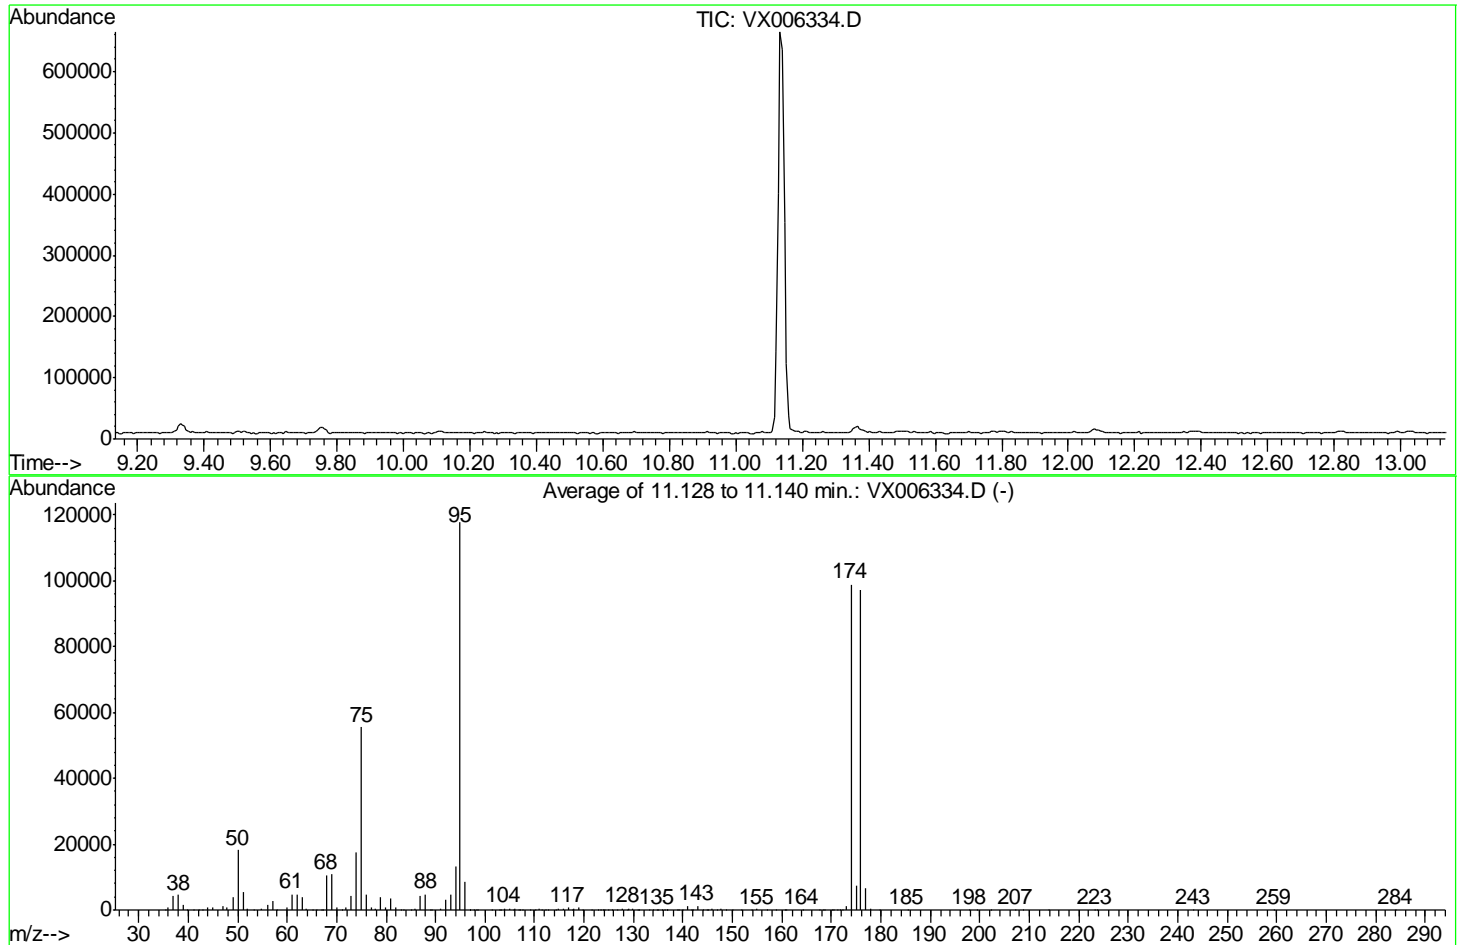

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	18270	PASS
75	95	30	60	47.1	55434	PASS
95	95	100	100	100.0	117776	PASS
96	95	5	9	7.3	8554	PASS
173	174	0.00	2	1.1	1085	PASS
174	95	50	100	84.0	98965	PASS
175	174	5	9	7.6	7505	PASS
176	174	95	101	98.1	97090	PASS
177	176	5	9	6.7	6551	PASS