


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX120720\
Data File : VX019745.D
Acq On : 07 Dec 2020 09:18
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
Title : SW846 8260
Last Update : Fri Dec 04 15:32:53 2020

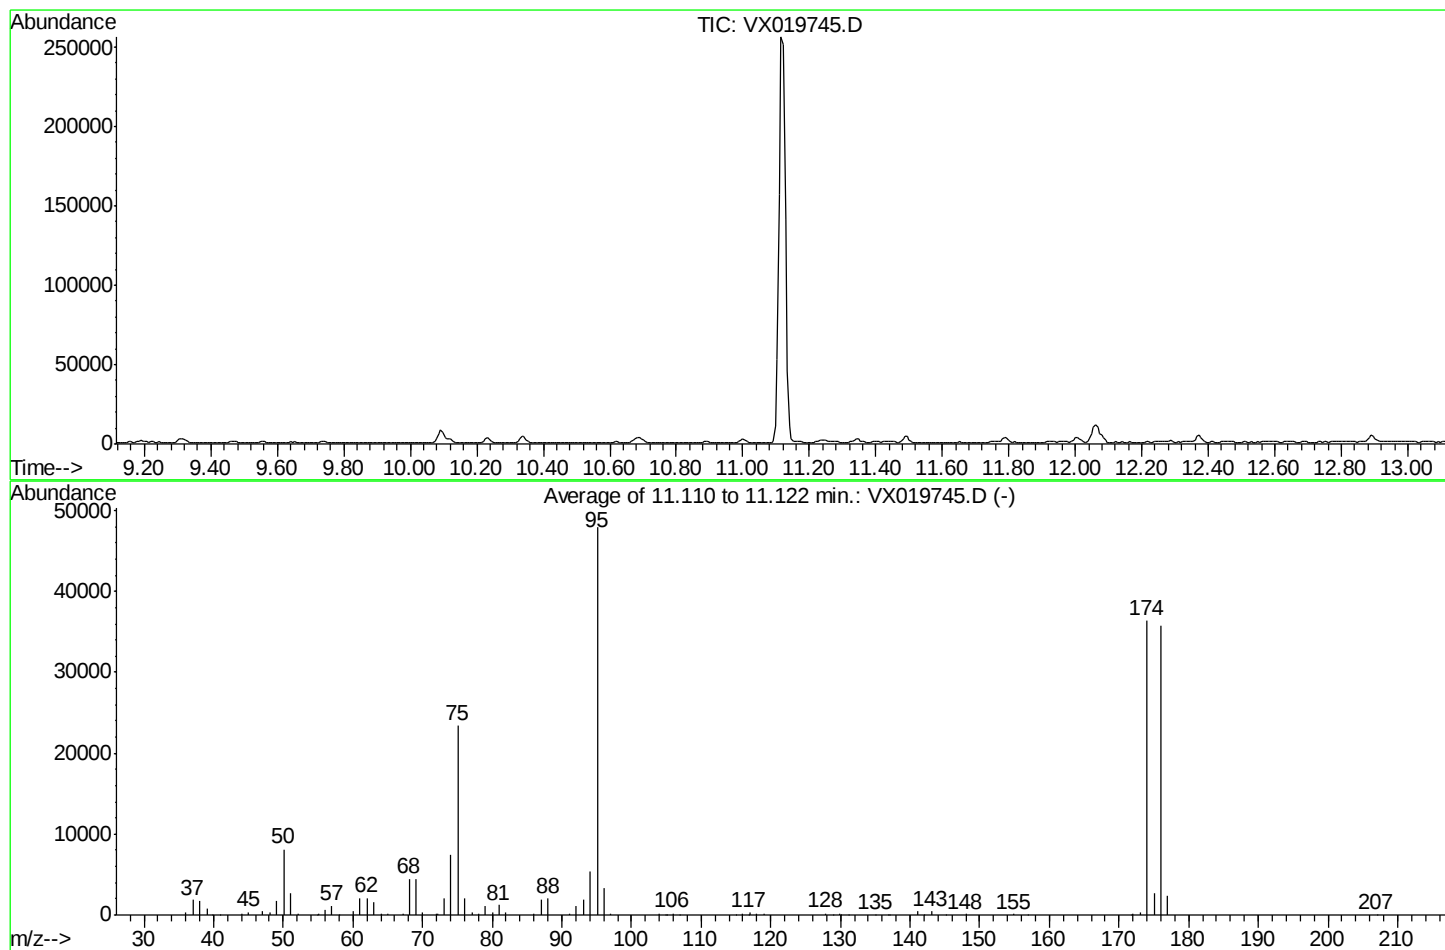

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	8120	PASS
75	95	30	60	48.8	23368	PASS
95	95	100	100	100.0	47920	PASS
96	95	5	9	6.8	3271	PASS
173	174	0.00	2	0.8	295	PASS
174	95	50	100	75.9	36389	PASS
175	174	5	9	7.6	2757	PASS
176	174	95	101	98.1	35696	PASS
177	176	5	9	6.7	2393	PASS