

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025580.D
 Acq On : 07 Dec 2021 15:30
 Operator : JC/MD
 Sample : M4883-04ME
 Misc : 4.67g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 08 05:35:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 08 05:26:42 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	103497	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.061	117	92076	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	45446	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	24241	34.320	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	68.640%		
7) Chloroethane-d5	1.648	69	13207	22.655	ug/L	-0.02
Spiked Amount 50.000	Range 70 - 130		Recovery =	45.320%#		
11) 1,1-Dichloroethene-d2	2.282	63	38222	33.939	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	67.880%		
21) 2-Butanone-d5	4.495	46	44105	83.884	ug/L	0.04
Spiked Amount 100.000	Range 40 - 130		Recovery =	83.880%		
24) Chloroform-d	5.068	84	54226	43.928	ug/L	0.01
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.860%		
26) 1,2-Dichloroethane-d4	5.964	65	35819	46.552	ug/L	0.01
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.100%		
32) Benzene-d6	5.971	84	116219	47.625	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.240%		
36) 1,2-Dichloropropane-d6	7.312	67	35066	46.411	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	92.820%		
41) Toluene-d8	8.653	98	105176	45.662	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.320%		
43) trans-1,3-Dichloroprop...	8.958	79	11931	31.409	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	62.820%		
47) 2-Hexanone-d5	9.403	63	31993	81.347	ug/L	0.02
Spiked Amount 100.000	Range 45 - 130		Recovery =	81.350%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	46569	43.612	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.220%		
66) 1,2-Dichlorobenzene-d4	12.323	152	42857	48.081	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.160%		
Target Compounds						Qvalue
29) Cyclohexane	5.471	56	1390	1.474	ug/L #	80
34) Trichloroethene	7.129	95	26757	41.357	ug/L	98
35) Methylcyclohexane	7.379	83	5850	5.745	ug/L	98
37) 1,2-Dichloropropane	7.318	63	3850	6.240	ug/L #	85
39) cis-1,3-Dichloropropene	8.330	75	898	0.894	ug/L #	76
42) Toluene	8.720	91	10123	3.732	ug/L	98
46) Tetrachloroethene	9.275	164	2289	4.172	ug/L	91
49) Dibromochloromethane	9.275	129	2025	2.683	ug/L #	12
52) Ethylbenzene	10.195	91	2354	0.807	ug/L	98
53) m,p-Xylene	10.305	106	2918	2.471	ug/L	90
54) o-Xylene	10.646	106	2678	2.265	ug/L	90
61) 1,2,3-Trichloropropane	12.024	75	5095	6.554	ug/L #	63
63) 1,2,4-Trimethylbenzene	11.756	105	3529	1.430	ug/L #	81
71) Naphthalene	13.780	128	6565	2.362	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025580.D
Acq On : 07 Dec 2021 15:30
Operator : JC/MD
Sample : M4883-04ME
Misc : 4.67g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Dec 08 05:35:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 08 05:26:42 2021
Response via : Initial Calibration

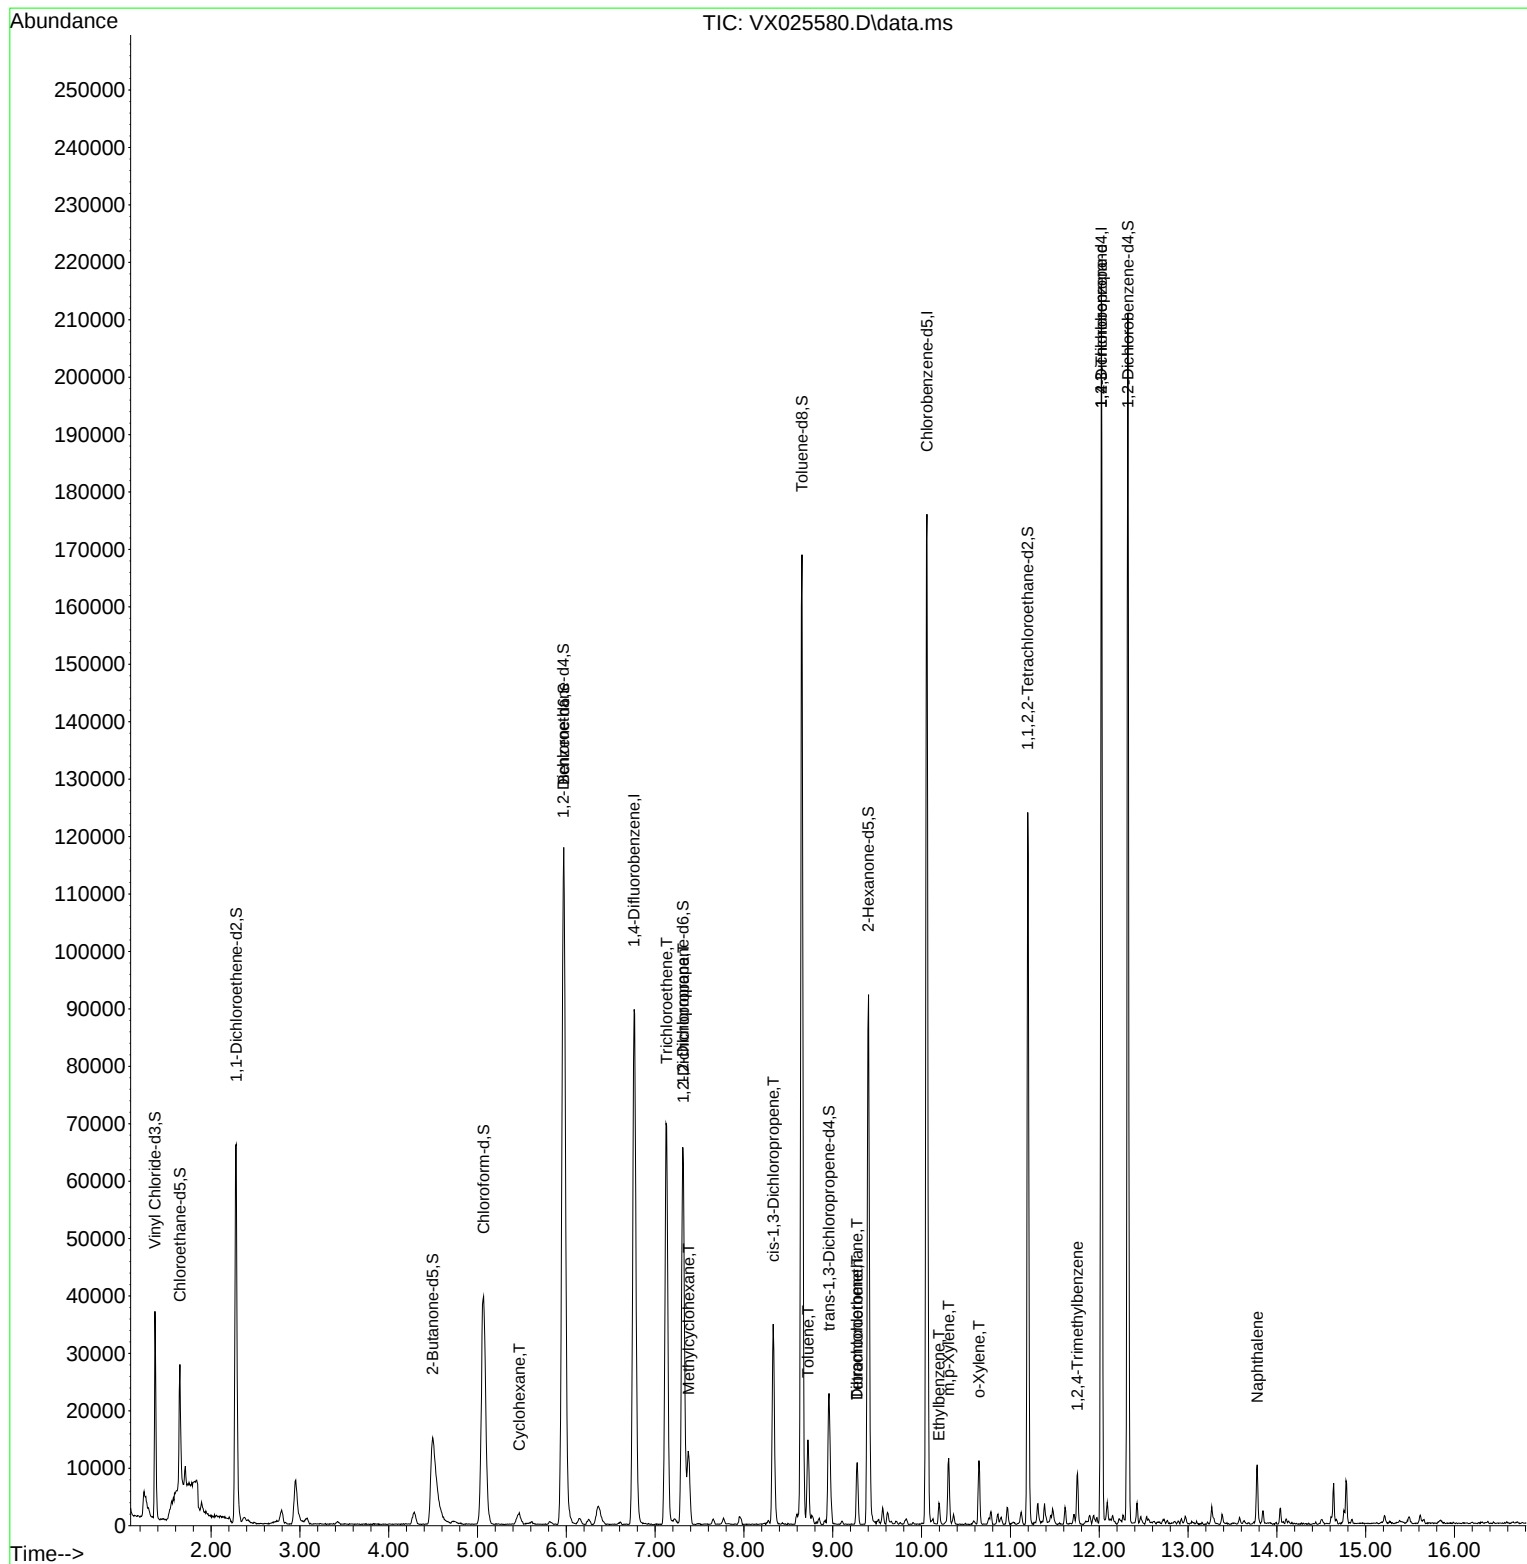






#29
Cyclohexane
Concen: 1.474 ug/L
RT: 5.471 min Scan# 719
Delta R.T. 0.000 min
Lab File: VX025580.D
Acq: 07 Dec 2021 15:30


Instrument :
MSVOA_X
ClientSampleId :

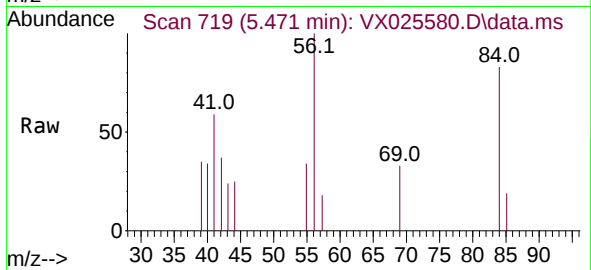



Tgt Ion: 56 Resp: 1390
Ion Ratio Lower Upper
56 100
69 13.7 25.4 38.2#
84 79.8 76.6 114.8

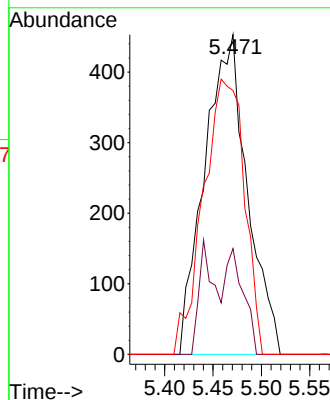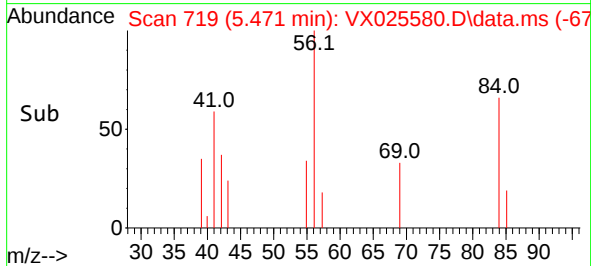


#34
Trichloroethene
Concen: 41.357 ug/L
RT: 7.129 min Scan# 991
Delta R.T. 0.006 min
Lab File: VX025580.D
Acq: 07 Dec 2021 15:30

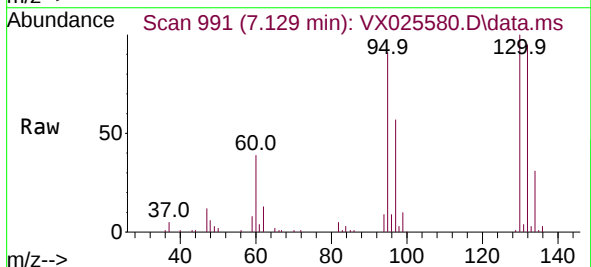

Tgt Ion: 95 Resp: 26757
Ion Ratio Lower Upper
95 100
97 63.1 46.0 85.4
132 104.7 75.0 139.2
130 109.8 77.9 144.7



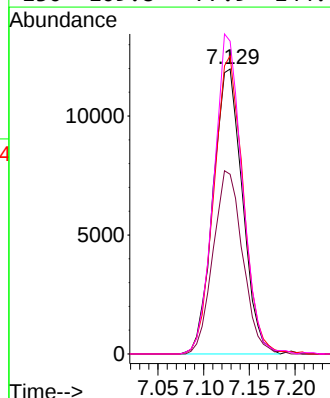



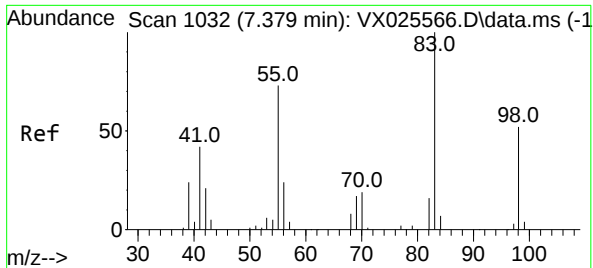

#35
Methylcyclohexane
Concen: 5.745 ug/L
RT: 7.379 min Scan# 1032
Delta R.T. 0.000 min
Lab File: VX025580.D
Acq: 07 Dec 2021 15:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 83 Resp: 5850
Ion Ratio Lower Upper
83 100
55 73.5 57.3 85.9
98 50.4 41.1 61.7

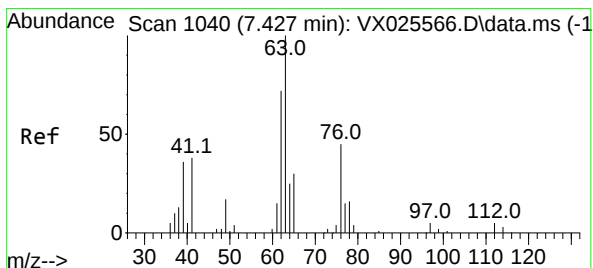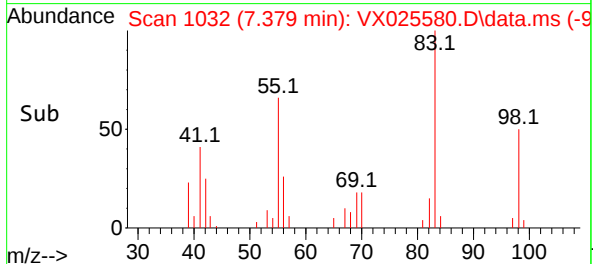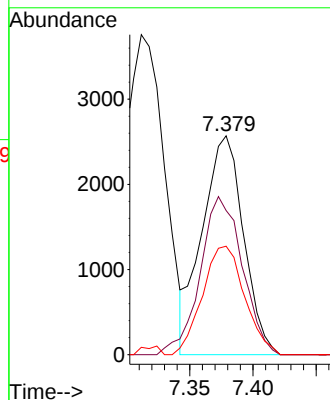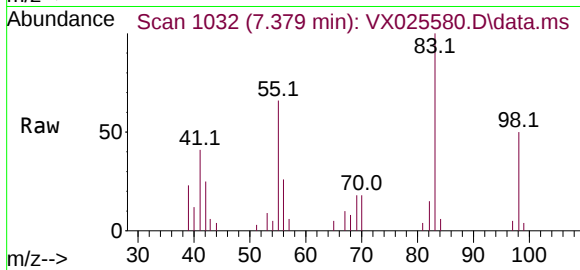

#37
1,2-Dichloropropane
Concen: 6.240 ug/L
RT: 7.318 min Scan# 1022
Delta R.T. -0.110 min
Lab File: VX025580.D
Acq: 07 Dec 2021 15:30

Tgt Ion: 63 Resp: 3850
Ion Ratio Lower Upper
63 100
112 0.0 4.0 6.0#

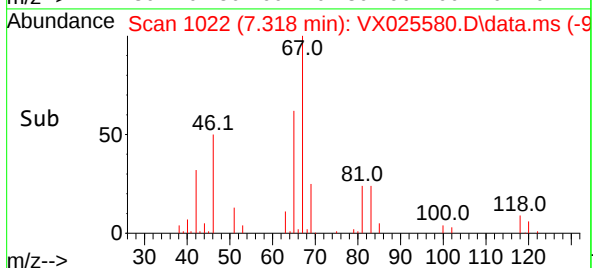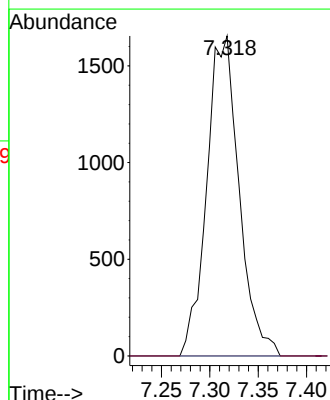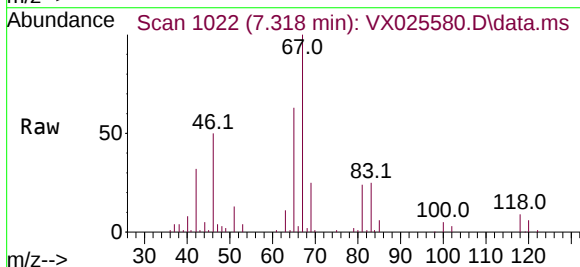

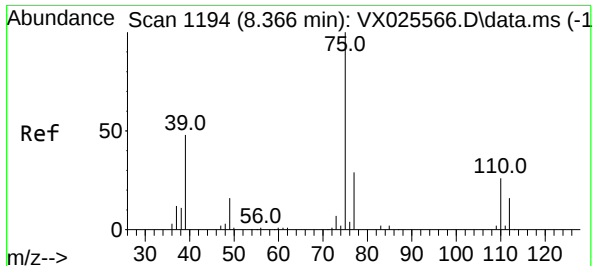

#39

cis-1,3-Dichloropropene

Concen: 0.894 ug/L

RT: 8.330 min Scan# 1194

Delta R.T. -0.036 min

Lab File: VX025580.D

Acq: 07 Dec 2021 15:30

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 898

Ion Ratio Lower Upper

75 100

77 45.2 22.3 41.3#

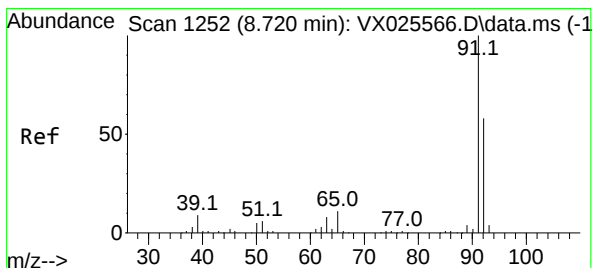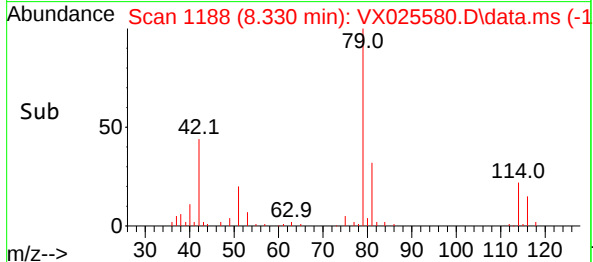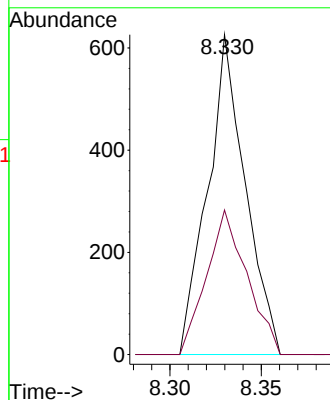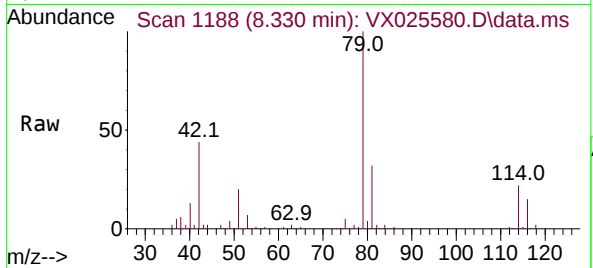

#42

Toluene

Concen: 3.732 ug/L

RT: 8.720 min Scan# 1252

Delta R.T. 0.000 min

Lab File: VX025580.D




Acq: 07 Dec 2021 15:30


Tgt Ion: 91 Resp: 10123

Ion Ratio Lower Upper

91 100


92 57.2 41.2 76.6

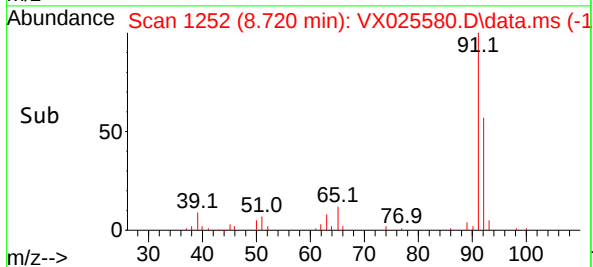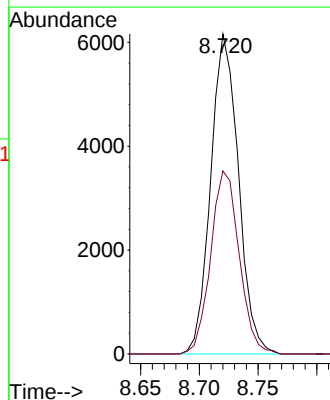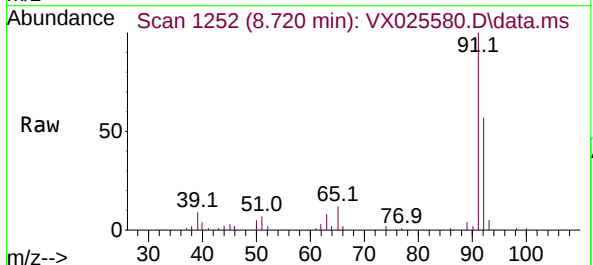






#46
Tetrachloroethene
Concen: 4.172 ug/L
RT: 9.275 min Scan# 1343
Delta R.T. 0.000 min
Lab File: VX025580.D
Acq: 07 Dec 2021 15:30

Instrument :
MSVOA_X
ClientSampleId :



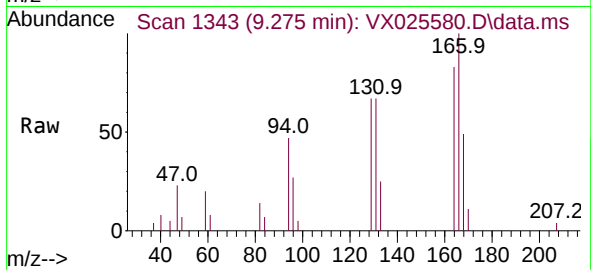



Tgt Ion:164 Resp: 2289
Ion Ratio Lower Upper
164 100
129 81.3 64.7 120.1
131 81.1 63.2 117.4
166 121.0 90.1 167.3

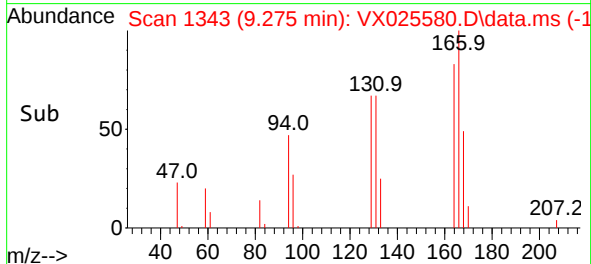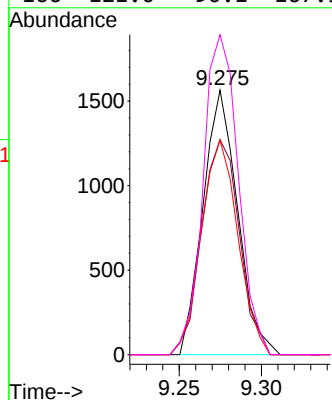

#49
Dibromochloromethane
Concen: 2.683 ug/L
RT: 9.275 min Scan# 1343
Delta R.T. -0.250 min
Lab File: VX025580.D
Acq: 07 Dec 2021 15:30

Tgt Ion:129 Resp: 2025
Ion Ratio Lower Upper
129 100
127 0.0 52.4 97.2#


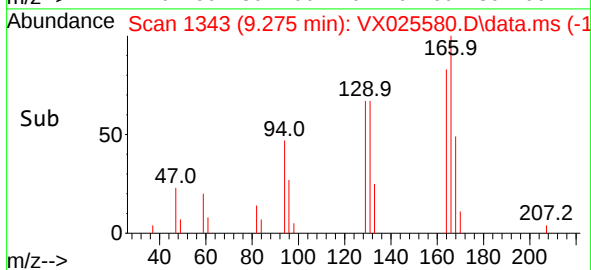
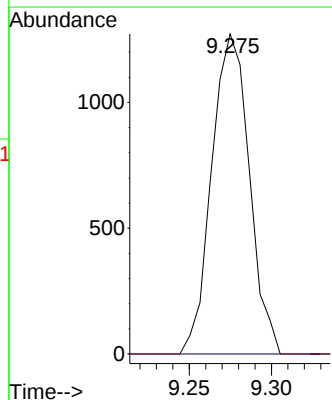
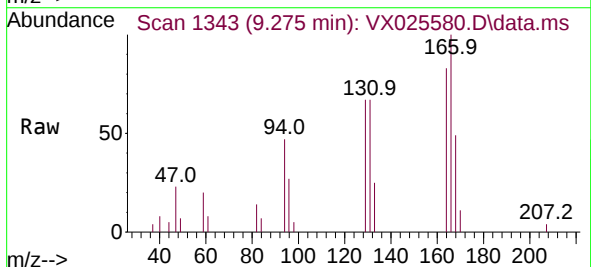




#52
Ethylbenzene
Concen: 0.807 ug/L
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX025580.D
Acq: 07 Dec 2021 15:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 2354
Ion Ratio Lower Upper
91 100
106 34.1 23.1 42.9

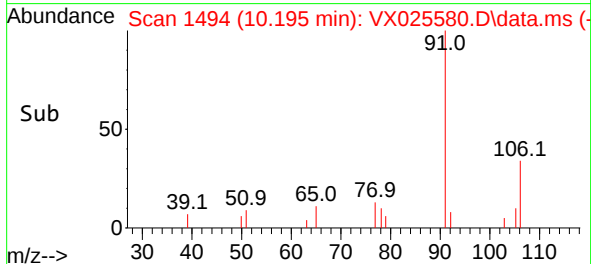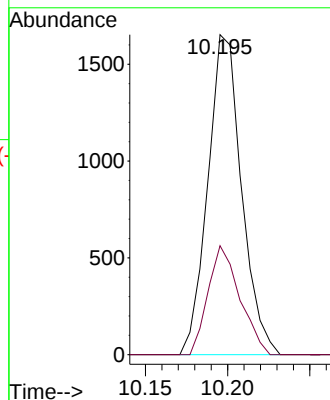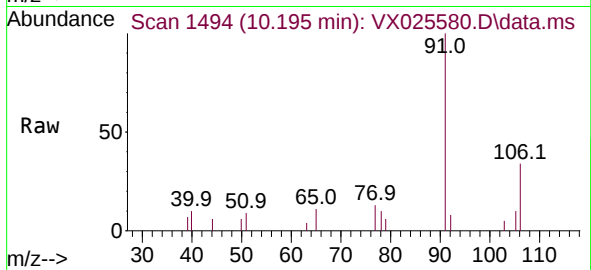

#53
m,p-Xylene
Concen: 2.471 ug/L
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX025580.D
Acq: 07 Dec 2021 15:30

Tgt Ion: 106 Resp: 2918
Ion Ratio Lower Upper
106 100
91 180.6 136.8 254.2



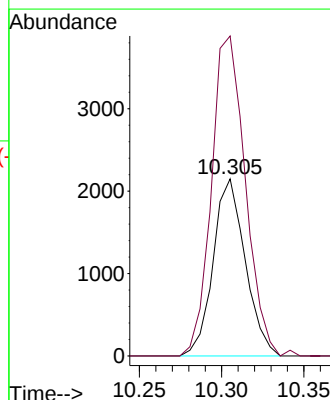
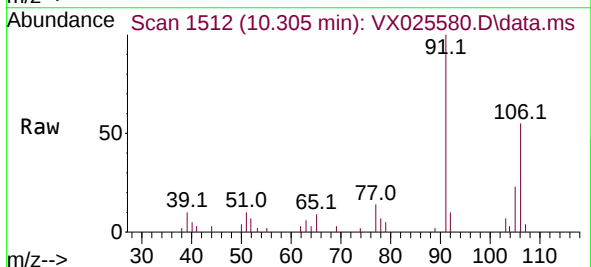


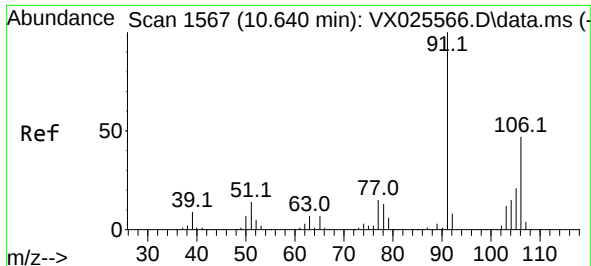

#54
o-Xylene
Concen: 2.265 ug/L
RT: 10.646 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX025580.D
Acq: 07 Dec 2021 15:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 2678
Ion Ratio Lower Upper
106 100
91 185.2 140.5 260.9

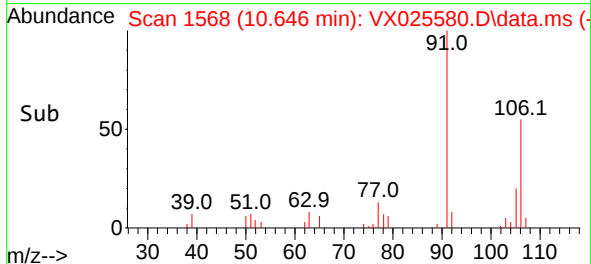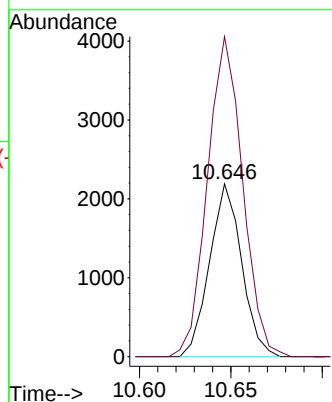

#61
1,2,3-Trichloropropane
Concen: 6.554 ug/L
RT: 12.024 min Scan# 1794
Delta R.T. 0.787 min
Lab File: VX025580.D
Acq: 07 Dec 2021 15:30

Tgt Ion: 75 Resp: 5095
Ion Ratio Lower Upper
75 100
77 34.2 25.8 38.8
110 3.7 34.7 52.1#


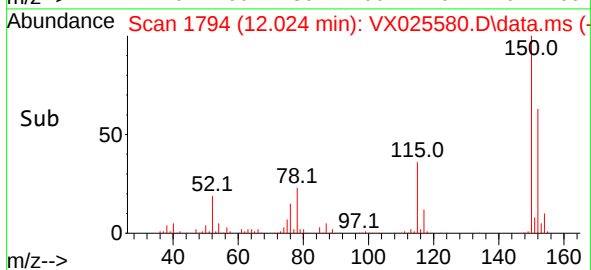
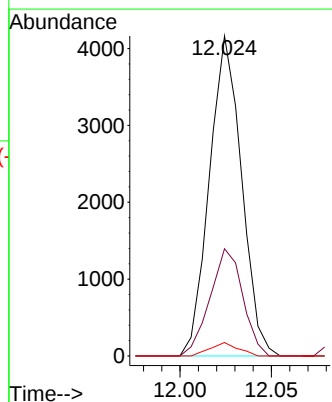
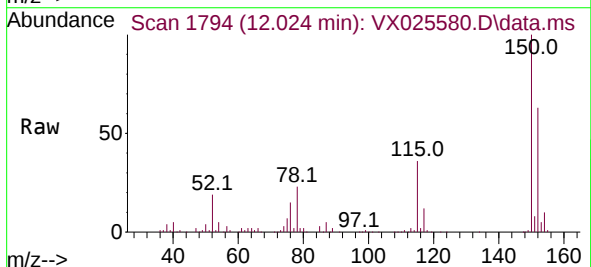


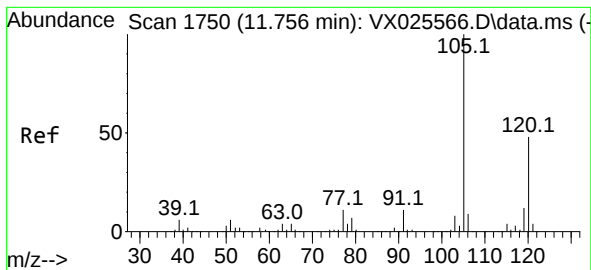

#63
1,2,4-Trimethylbenzene
Concen: 1.430 ug/L
RT: 11.756 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX025580.D
Acq: 07 Dec 2021 15:30

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion:105 Resp: 3529
Ion Ratio Lower Upper
105 100
120 44.1 0.1 0.1#

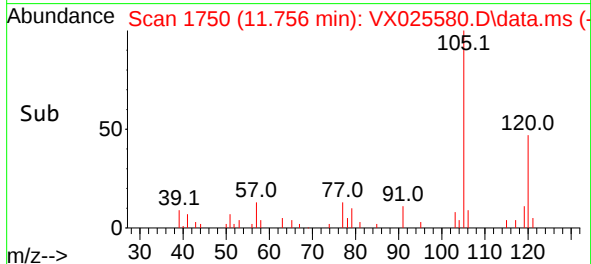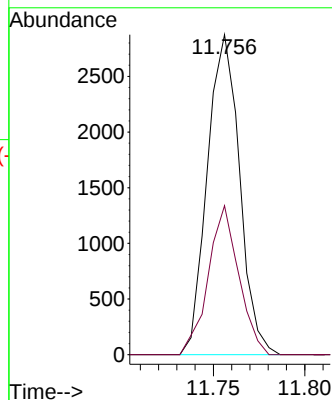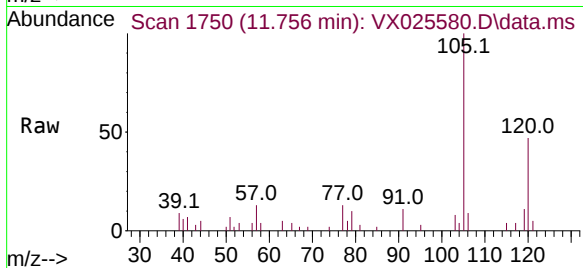

#71
Naphthalene
Concen: 2.362 ug/L
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX025580.D
Acq: 07 Dec 2021 15:30

Tgt Ion:128 Resp: 6565
Ion Ratio Lower Upper
128 100
127 13.4 10.1 15.1
129 12.5 8.7 13.1

