

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025569.D
 Acq On : 07 Dec 2021 11:14
 Operator : JC/MD
 Sample : M4881-02ME
 Misc : 4.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW9D8ME

Quant Time: Dec 08 05:33:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 08 05:26:42 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	91546	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.061	117	81638	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	40455	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	24624	39.414	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	78.820%
7) Chloroethane-d5	1.648	69	13893	26.943	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	53.880%#
11) 1,1-Dichloroethene-d2	2.282	63	38369	38.517	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.040%
21) 2-Butanone-d5	4.483	46	41082	88.335	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	88.340%
24) Chloroform-d	5.056	84	54085	49.533	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.060%
26) 1,2-Dichloroethane-d4	5.958	65	35342	51.928	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.860%
32) Benzene-d6	5.970	84	112637	52.058	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.120%
36) 1,2-Dichloropropane-d6	7.306	67	33989	50.738	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.480%
41) Toluene-d8	8.647	98	101116	49.512	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.020%
43) trans-1,3-Dichloroprop...	8.958	79	12278	36.455	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.920%
47) 2-Hexanone-d5	9.397	63	29794	85.441	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.440%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	45635	48.202	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.400%
66) 1,2-Dichlorobenzene-d4	12.323	152	40246	50.722	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.440%
Target Compounds						Qvalue
14) Carbon disulfide	2.483	76	1033	0.855	ug/L	97
42) Toluene	8.720	91	2378	0.989	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025569.D
Acq On : 07 Dec 2021 11:14
Operator : JC/MD
Sample : M4881-02ME
Misc : 4.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW9D8ME

Quant Time: Dec 08 05:33:04 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 08 05:26:42 2021
Response via : Initial Calibration




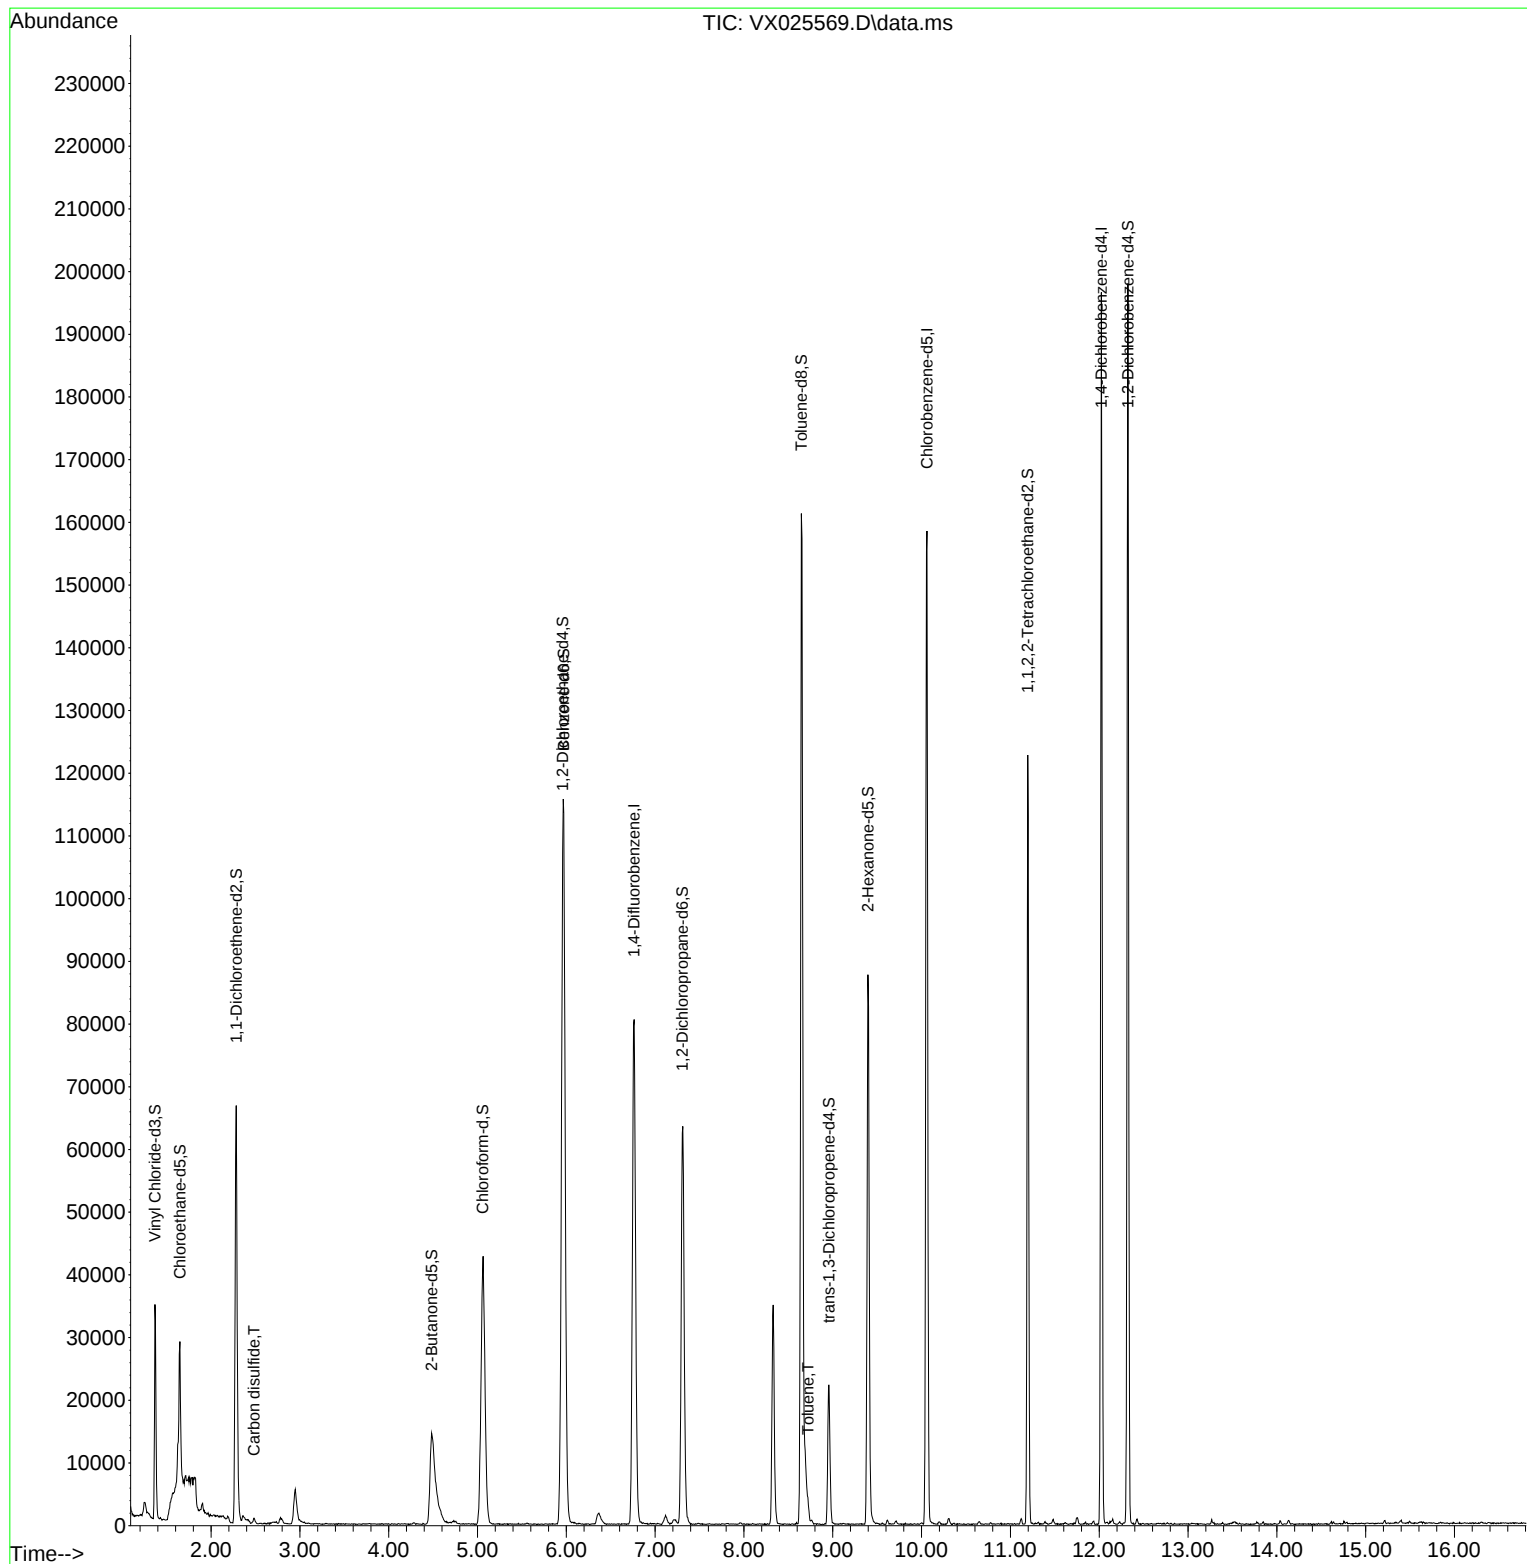


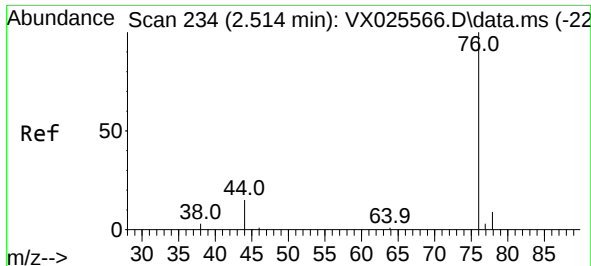

#14
Carbon disulfide
Concen: 0.855 ug/L
RT: 2.483 min Scan# 21
Delta R.T. -0.030 min
Lab File: VX025569.D
Acq: 07 Dec 2021 11:14

Instrument :
MSVOA_X
ClientSampleId :
EW9D8ME

Tgt Ion: 76 Resp: 1033
Ion Ratio Lower Upper
76 100
78 10.4 7.4 11.2

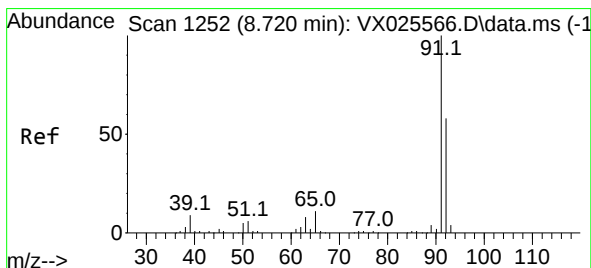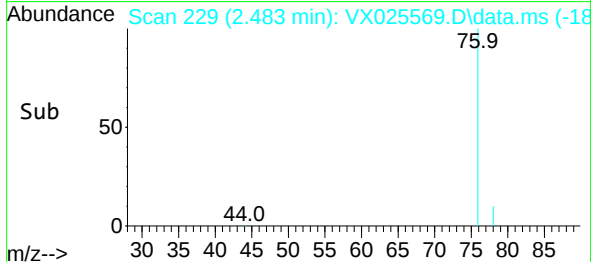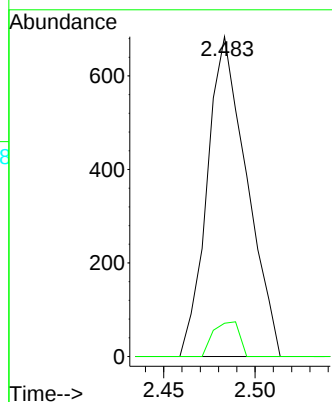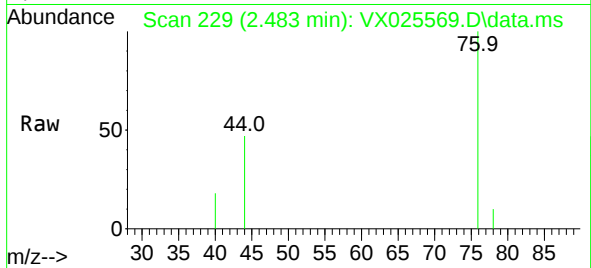

#42
Toluene
Concen: 0.989 ug/L
RT: 8.720 min Scan# 1252
Delta R.T. 0.000 min
Lab File: VX025569.D
Acq: 07 Dec 2021 11:14

Tgt Ion: 91 Resp: 2378
Ion Ratio Lower Upper
91 100
92 50.7 41.2 76.6

