

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025591.D
 Acq On : 07 Dec 2021 21:11
 Operator : JC/MD
 Sample : M4886-06ME
 Misc : 3.91g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EX887ME

Quant Time: Dec 08 13:54:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 08 07:24:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	138899	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.061	117	123384	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	61841	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	49014	51.707	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	103.420%
7) Chloroethane-d5	1.648	69	24401	31.189	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	62.380%#
11) 1,1-Dichloroethene-d2	2.282	63	68803	45.522	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.040%
21) 2-Butanone-d5	4.489	46	66123	93.708	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.710%
24) Chloroform-d	5.062	84	83751	50.553	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.100%
26) 1,2-Dichloroethane-d4	5.964	65	56105	54.332	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.660%
32) Benzene-d6	5.970	84	189032	57.807	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	115.620%
36) 1,2-Dichloropropane-d6	7.312	67	54953	54.277	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	108.560%
41) Toluene-d8	8.653	98	172473	55.879	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	111.760%
43) trans-1,3-Dichloroprop...	8.958	79	22074	43.366	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.740%
47) 2-Hexanone-d5	9.397	63	47374	89.890	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.890%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	71373	49.881	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.760%
66) 1,2-Dichlorobenzene-d4	12.323	152	66817	55.088	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	110.180%
Target Compounds						Qvalue
46) Tetrachloroethene	9.275	164	1504	2.046	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025591.D
Acq On : 07 Dec 2021 21:11
Operator : JC/MD
Sample : M4886-06ME
Misc : 3.91g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EX887ME


Quant Time: Dec 08 13:54:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 08 07:24:50 2021
Response via : Initial Calibration

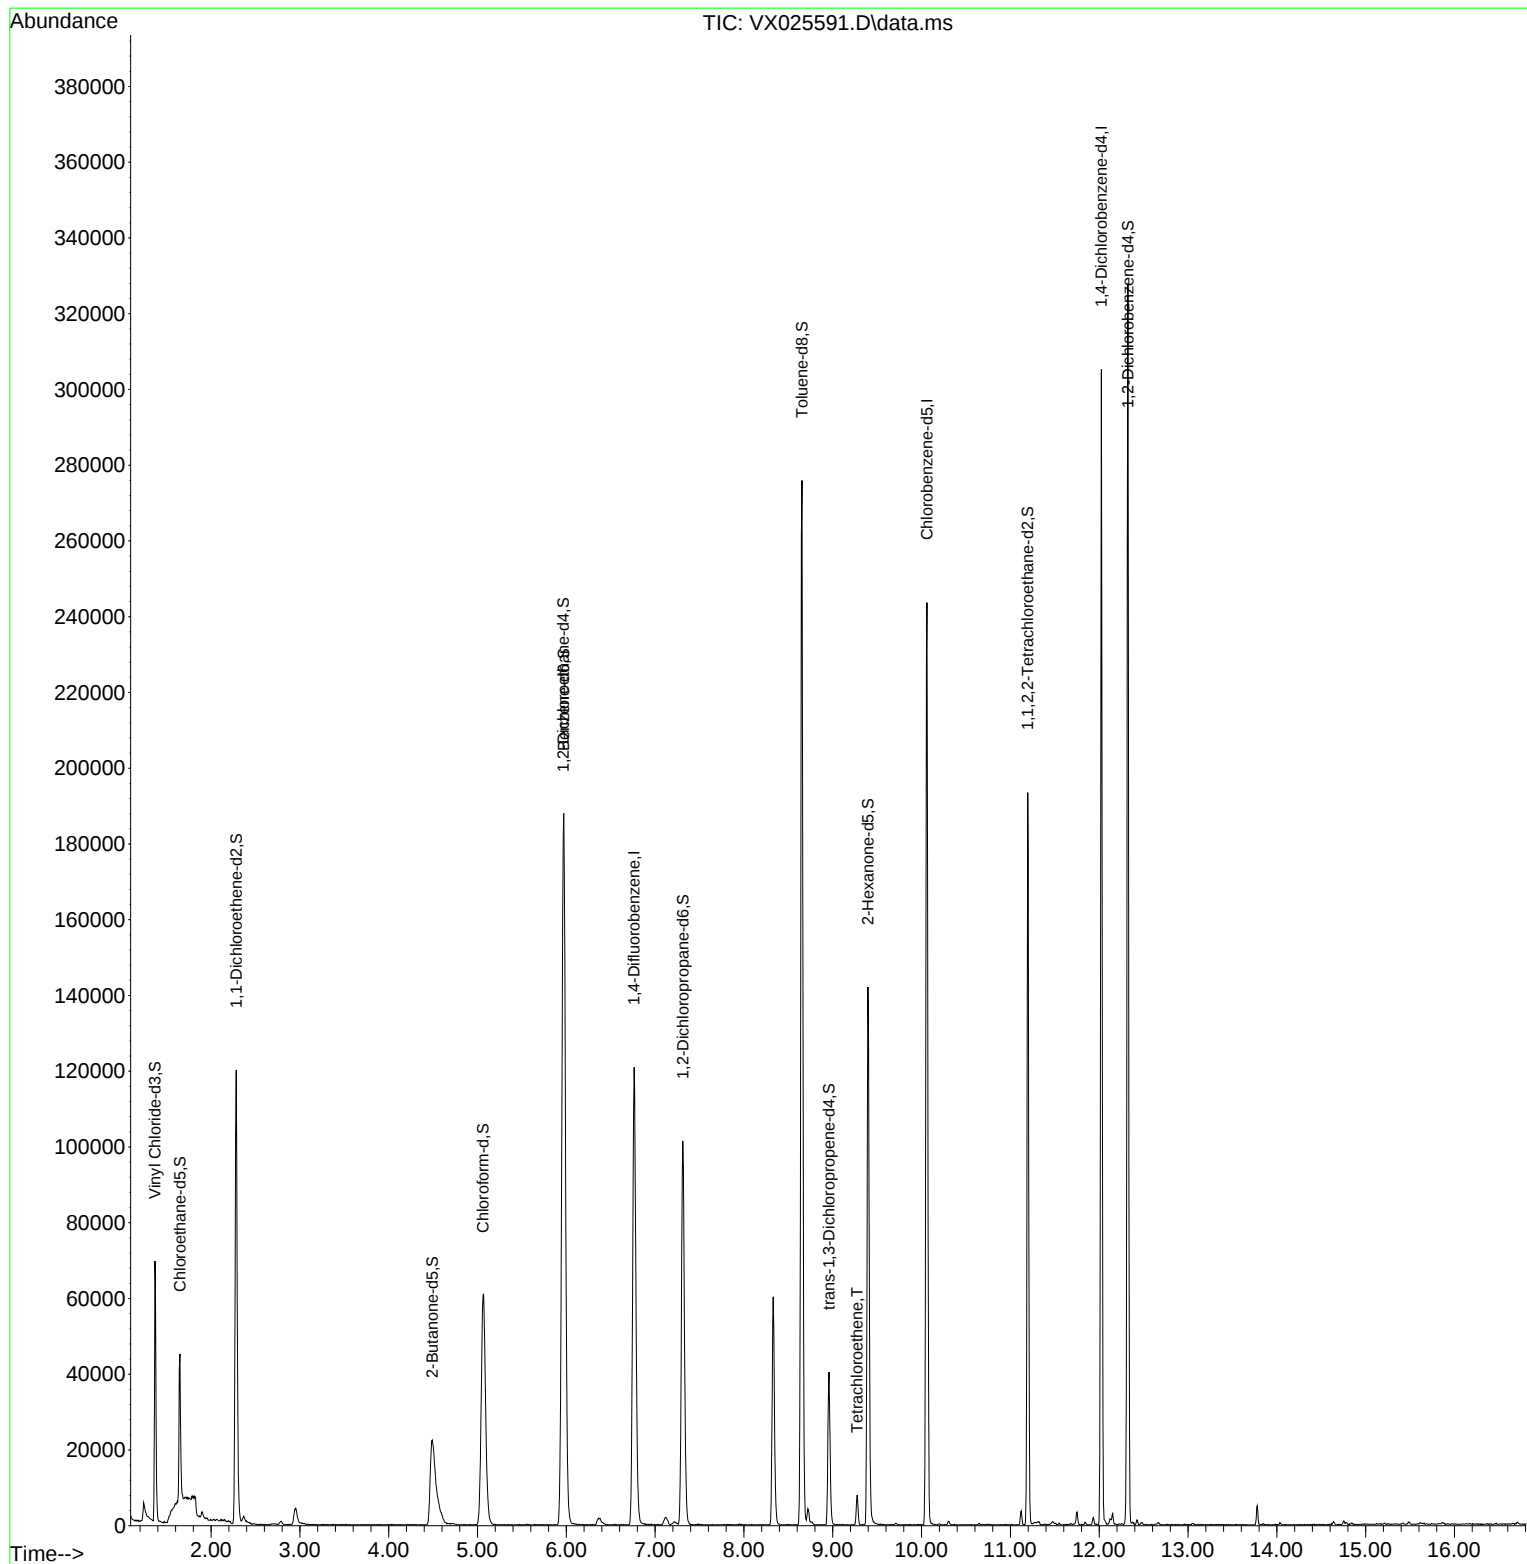

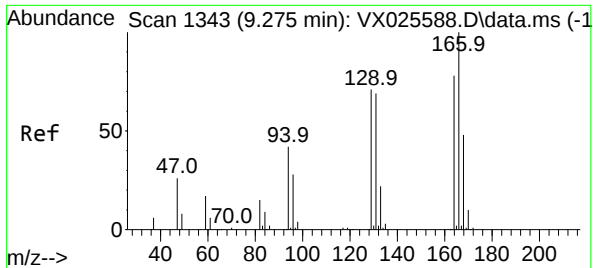

#46
 Tetrachloroethene
 Concen: 2.046 ug/L
 RT: 9.275 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX025591.D
 Acq: 07 Dec 2021 21:11

Instrument :
 MSVOA_X
 ClientSampleId :
 EX887ME

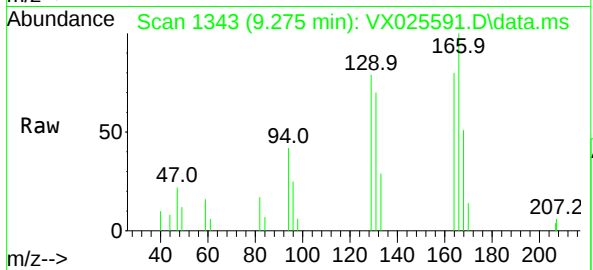

Tgt Ion:	164	Resp:	1504
Ion	Ratio	Lower	Upper
164	100		
129	98.1	64.7	120.1
131	87.4	63.2	117.4
166	124.7	90.1	167.3

