

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025592.D
 Acq On : 07 Dec 2021 21:34
 Operator : JC/MD
 Sample : M4886-07ME
 Misc : 5.48g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EX888ME

Quant Time: Dec 08 13:54:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 08 07:24:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	248733	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.061	117	225474	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	121291	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	84017	49.495	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	98.980%
7) Chloroethane-d5	1.648	69	42145	30.082	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	60.160%#
11) 1,1-Dichloroethene-d2	2.276	63	121338	44.831	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.660%
21) 2-Butanone-d5	4.495	46	123788	97.964	ug/L	0.04
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.960%
24) Chloroform-d	5.068	84	150294	50.660	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.320%
26) 1,2-Dichloroethane-d4	5.964	65	98805	53.431	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.860%
32) Benzene-d6	5.970	84	333747	55.850	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	111.700%
36) 1,2-Dichloropropane-d6	7.311	67	96857	52.350	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	104.700%
41) Toluene-d8	8.653	98	309282	54.833	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.660%
43) trans-1,3-Dichloroprop...	8.957	79	41280	44.378	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.760%
47) 2-Hexanone-d5	9.402	63	91722	95.237	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.240%
56) 1,1,2,2-Tetrachloroeth...	11.201	84	129183	49.404	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.800%
66) 1,2-Dichlorobenzene-d4	12.323	152	125486	52.749	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.500%
Target Compounds						
					Qvalue	
42) Toluene	8.720	91	6035	0.908	ug/L	99
53) m,p-Xylene	10.305	106	6402	2.214	ug/L	99
54) o-Xylene	10.646	106	3244	1.121	ug/L	93
62) 1,3,5-Trimethylbenzene	11.457	105	12152	1.864	ug/L	99
63) 1,2,4-Trimethylbenzene	11.756	105	34425	5.226	ug/L #	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025592.D
Acq On : 07 Dec 2021 21:34
Operator : JC/MD
Sample : M4886-07ME
Misc : 5.48g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EX888ME

Quant Time: Dec 08 13:54:49 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 08 07:24:50 2021
Response via : Initial Calibration

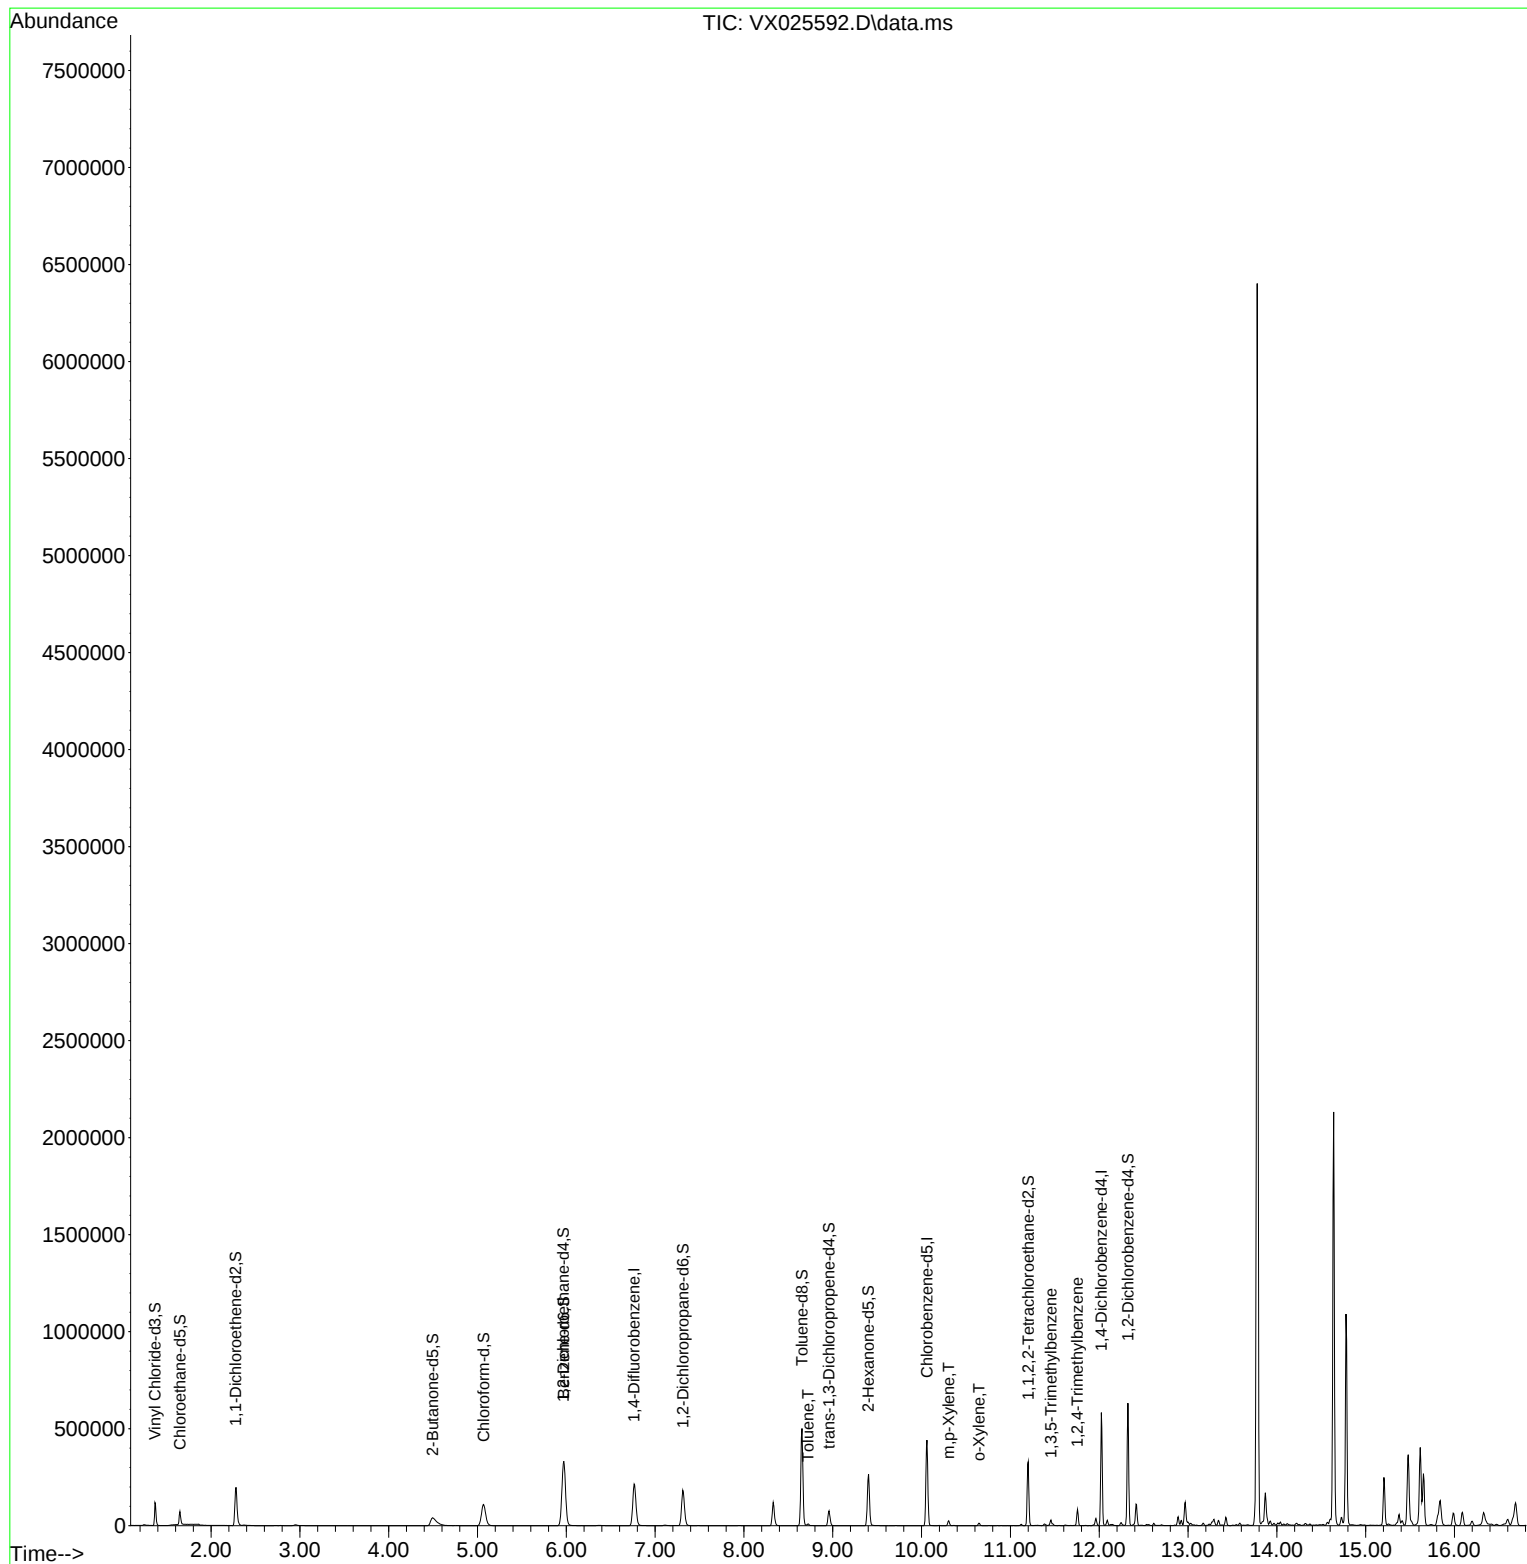

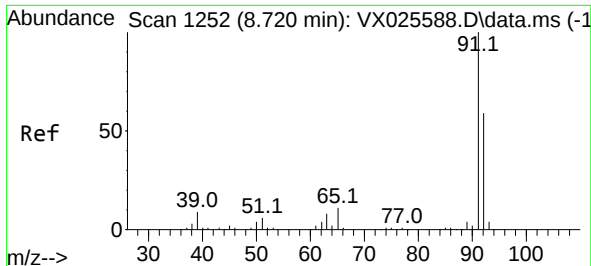

#42

Toluene

Concen: 0.908 ug/L

RT: 8.720 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX025592.D

Acq: 07 Dec 2021 21:34

Instrument :

MSVOA_X

ClientSampleId :





EX888ME

Tgt Ion: 91 Resp: 6035

Ion Ratio Lower Upper

91 100

92 58.4 41.2 76.6

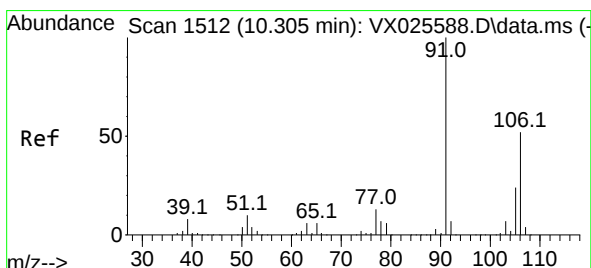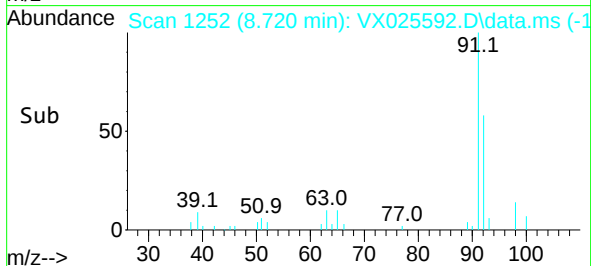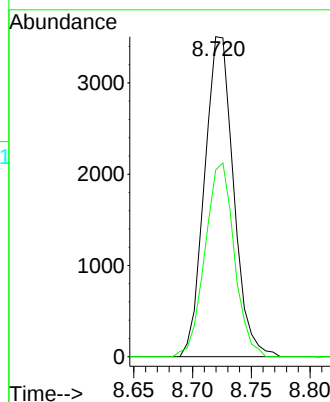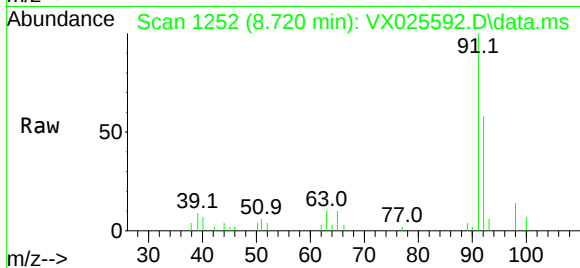

#53

m,p-Xylene

Concen: 2.214 ug/L

RT: 10.305 min Scan# 1512

Delta R.T. -0.000 min

Lab File: VX025592.D




Acq: 07 Dec 2021 21:34


Tgt Ion:106 Resp: 6402

Ion Ratio Lower Upper

106 100

91 193.8 136.8 254.2


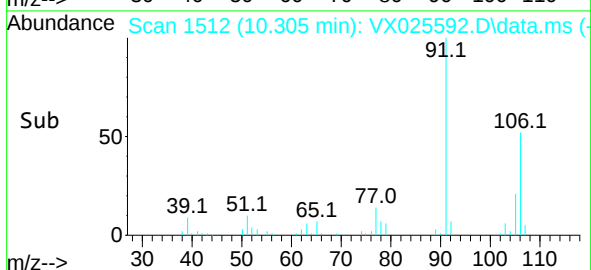
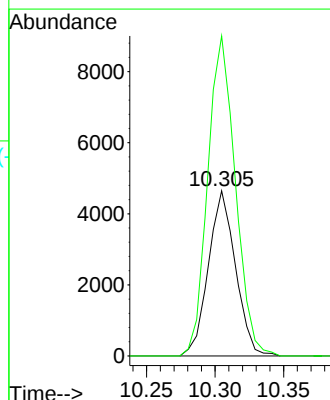
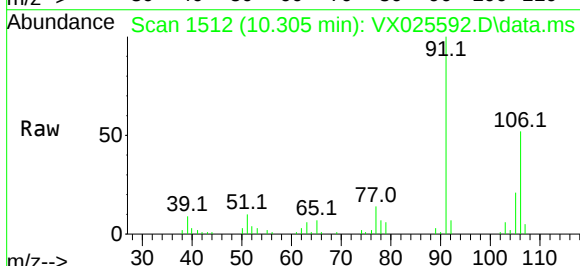


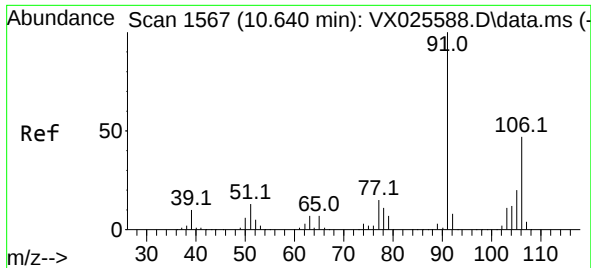

#54
o-Xylene
Concen: 1.121 ug/L
RT: 10.646 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX025592.D
Acq: 07 Dec 2021 21:34




Instrument :
MSVOA_X
ClientSampleId :
EX888ME


Tgt Ion:106 Resp: 3244
Ion Ratio Lower Upper
106 100
91 189.6 140.5 260.9

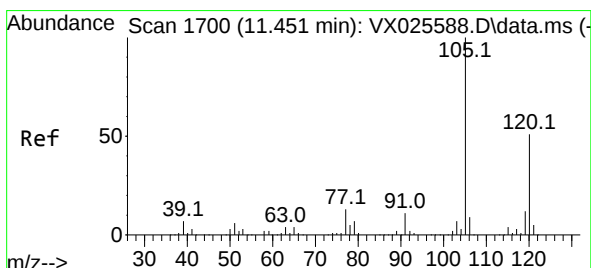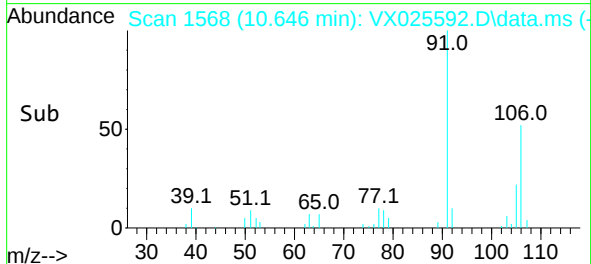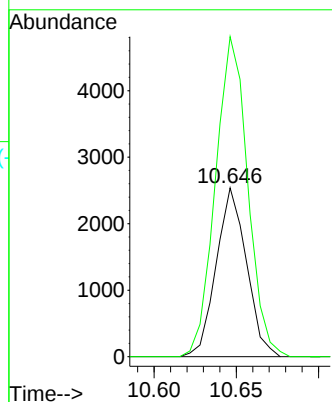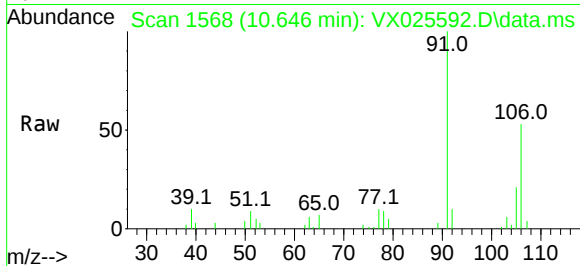

#62
1,3,5-Trimethylbenzene
Concen: 1.864 ug/L
RT: 11.457 min Scan# 1701
Delta R.T. 0.006 min
Lab File: VX025592.D
Acq: 07 Dec 2021 21:34

Tgt Ion:105 Resp: 12152
Ion Ratio Lower Upper
105 100
120 50.7 41.0 61.4

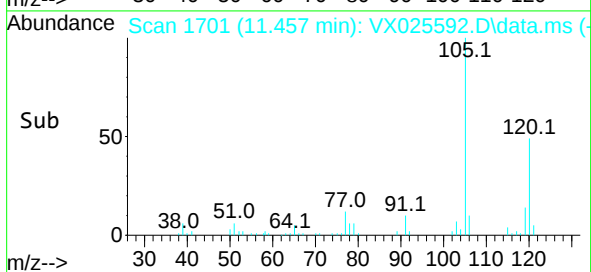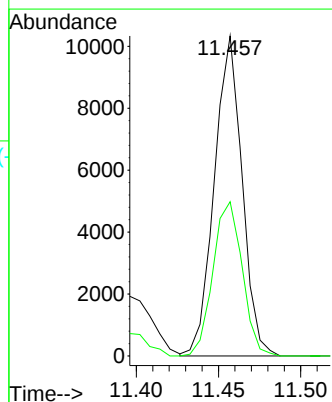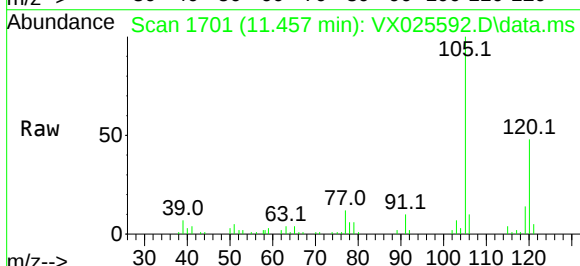

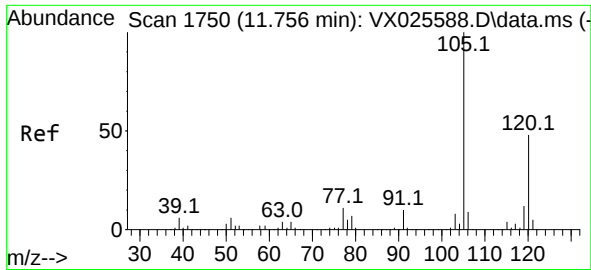

#63
 1,2,4-Trimethylbenzene
 Concen: 5.226 ug/L
 RT: 11.756 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX025592.D
 Acq: 07 Dec 2021 21:34

Instrument :
 MSVOA_X
 ClientSampleId :
 EX888ME

Tgt Ion:105 Resp: 34425
 Ion Ratio Lower Upper
 105 100
 120 46.2 0.1 0.1#

