

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025604.D
 Acq On : 08 Dec 2021 02:13
 Operator : JC/MD
 Sample : M4885-13ME
 Misc : 6.72g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW9M0ME

Quant Time: Dec 08 13:58:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 08 07:24:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	147455	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.061	117	130097	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	66559	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	46446	46.155	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.300%
7) Chloroethane-d5	1.648	69	22829	27.487	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	54.980%#
11) 1,1-Dichloroethene-d2	2.282	63	65050	40.542	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.080%
21) 2-Butanone-d5	4.501	46	64918	86.662	ug/L	0.04
Spiked Amount	100.000	Range	40 - 130	Recovery	=	86.660%
24) Chloroform-d	5.068	84	83586	47.526	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.060%
26) 1,2-Dichloroethane-d4	5.958	65	55944	51.032	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.060%
32) Benzene-d6	5.970	84	185287	53.738	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.480%
36) 1,2-Dichloropropane-d6	7.312	67	54272	50.839	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.680%
41) Toluene-d8	8.653	98	167242	51.388	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.780%
43) trans-1,3-Dichloroprop...	8.958	79	20781	38.719	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.440%
47) 2-Hexanone-d5	9.403	63	47616	85.687	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.690%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	69947	46.362	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.720%
66) 1,2-Dichlorobenzene-d4	12.323	152	66367	50.838	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.680%
Target Compounds						
					Qvalue	
46) Tetrachloroethene	9.275	164	3820	4.927	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025604.D
Acq On : 08 Dec 2021 02:13
Operator : JC/MD
Sample : M4885-13ME
Misc : 6.72g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW9M0ME


Quant Time: Dec 08 13:58:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 08 07:24:50 2021
Response via : Initial Calibration

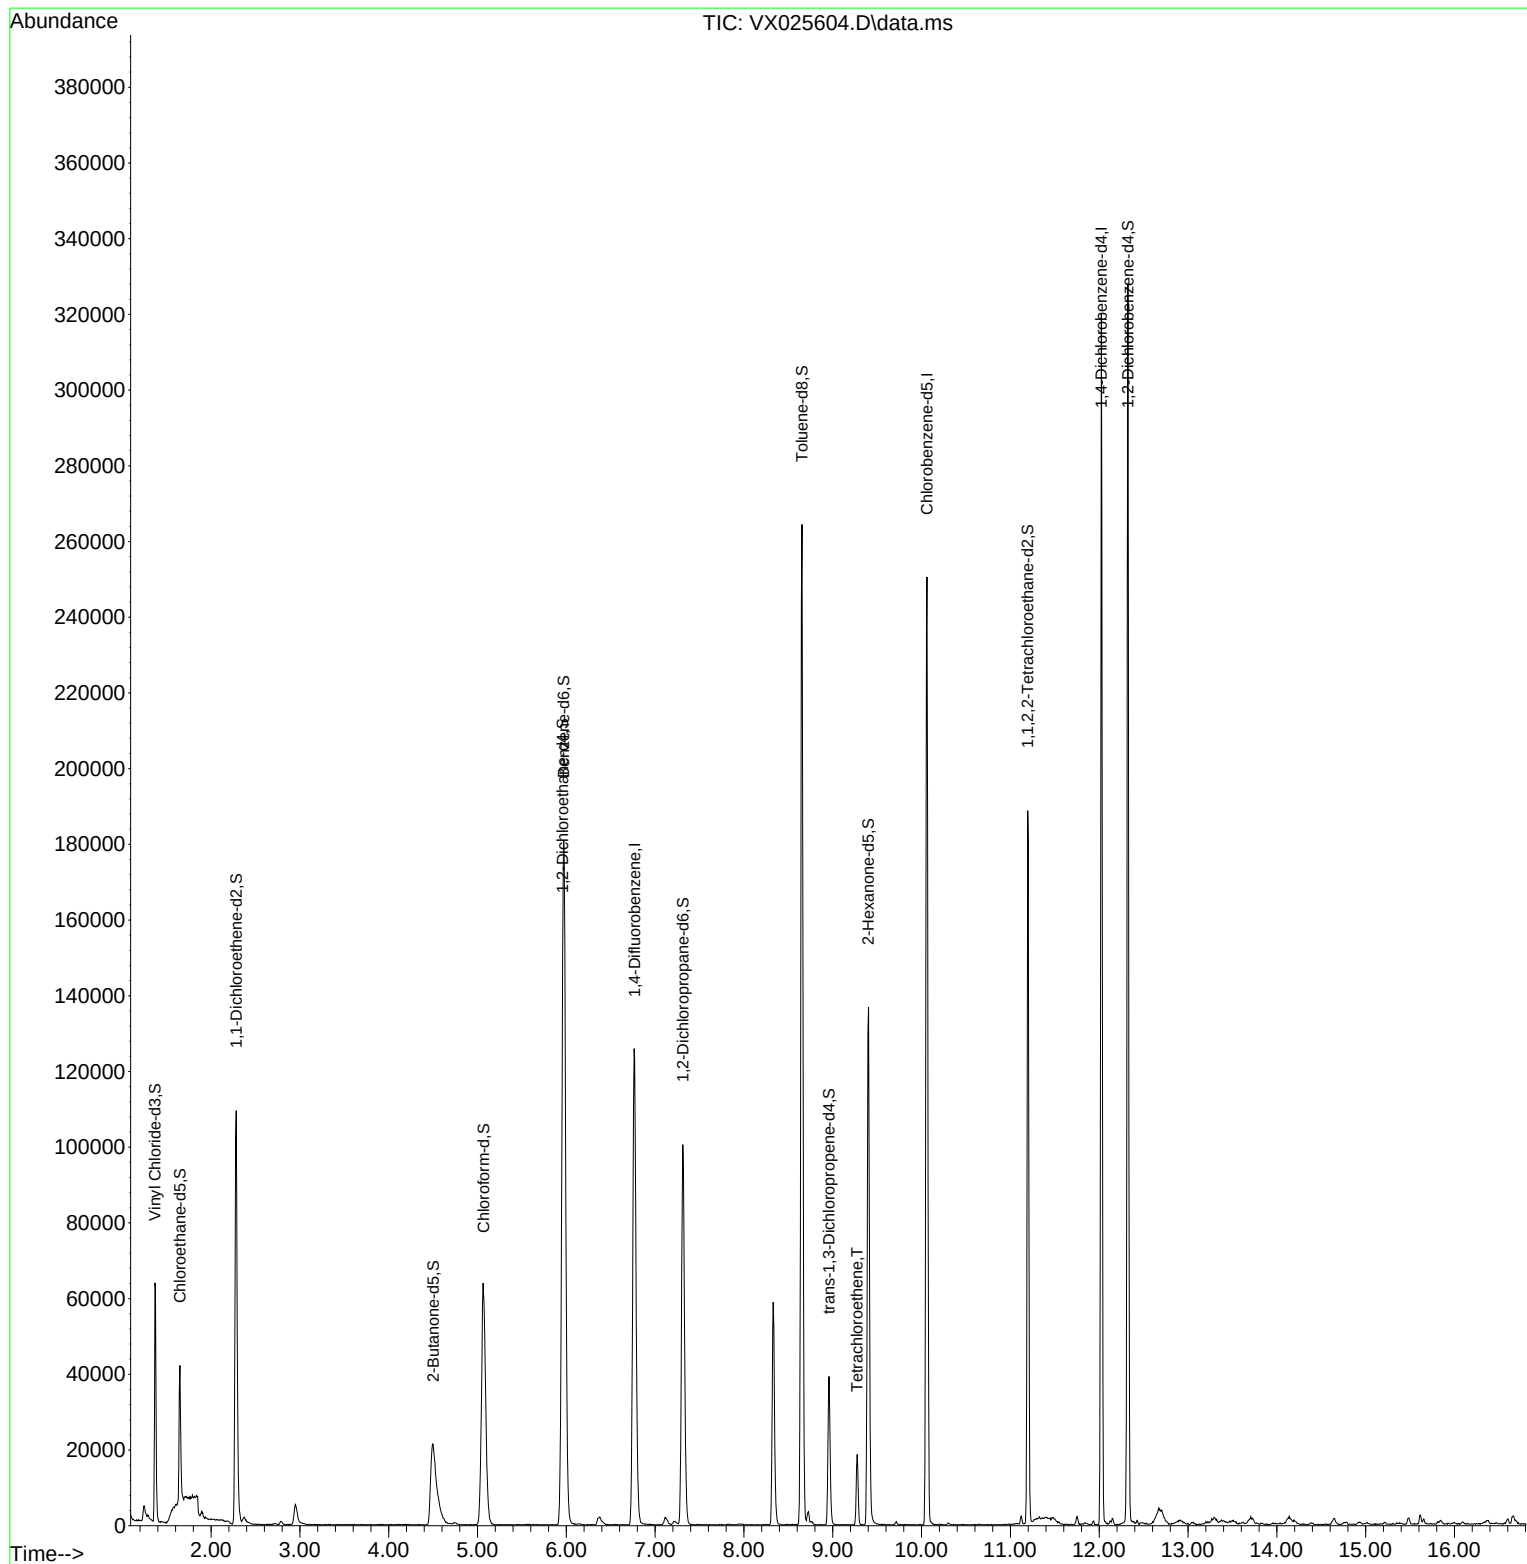

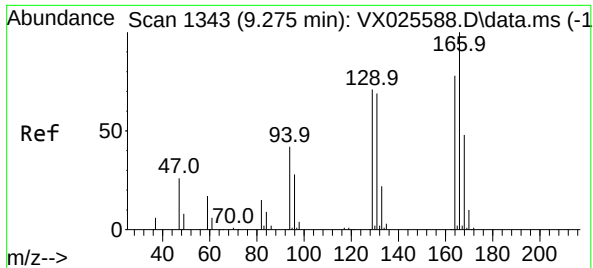

#46
 Tetrachloroethene
 Concen: 4.927 ug/L
 RT: 9.275 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX025604.D
 Acq: 08 Dec 2021 02:13

Instrument :
 MSVOA_X
 ClientSampleId :
 EW9M0ME

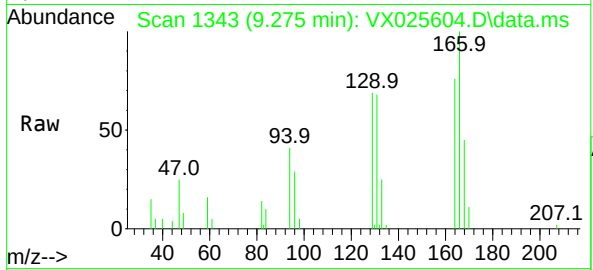

Tgt Ion:	164	Resp:	3820
Ion	Ratio	Lower	Upper
164	100		
129	90.9	64.7	120.1
131	89.7	63.2	117.4
166	131.5	90.1	167.3

