

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025572.D
 Acq On : 07 Dec 2021 12:24
 Operator : JC/MD
 Sample : M4881-06ME
 Misc : 4.42g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW9E2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025572.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	41	rVB3	3233	9242	2.71%	0.357%
2	1.368	43	46	53	rVB	36734	41283	12.13%	1.594%
3	1.605	70	85	86	rBV6	5298	18978	5.57%	0.733%
4	1.648	88	92	98	rVV	22533	30671	9.01%	1.184%
5	2.282	190	196	206	rBV	63625	107740	31.65%	4.160%
6	2.532	232	237	238	rBV2	137	177	0.05%	0.007%
7	2.788	273	279	285	rVB5	952	2023	0.59%	0.078%
8	2.953	297	306	316	rBV	5153	14151	4.16%	0.546%
9	3.587	409	410	413	rVB	150	132	0.04%	0.005%
10	3.989	473	476	477	rBV	131	120	0.04%	0.005%
11	4.203	508	511	516	rVB2	130	213	0.06%	0.008%
12	4.489	549	558	583	rBV	15223	69897	20.53%	2.699%
13	4.690	590	591	593	rVB2	279	157	0.05%	0.006%
14	4.715	593	595	596	rBV2	246	212	0.06%	0.008%
15	5.062	640	652	671	rVB	43779	136975	40.24%	5.288%
16	5.300	688	691	692	rBV	220	187	0.05%	0.007%
17	5.727	758	761	762	rBV	101	112	0.03%	0.004%
18	5.971	790	801	817	rVV2	118498	340434	100.00%	13.143%
19	6.214	838	841	843	rVB2	126	114	0.03%	0.004%
20	6.367	859	866	874	rBV6	1943	5985	1.76%	0.231%
21	6.763	922	931	945	rVV	80288	203026	59.64%	7.838%
22	7.001	968	970	973	rBV2	123	121	0.04%	0.005%
23	7.111	981	988	991	rBV3	887	1843	0.54%	0.071%
24	7.220	999	1006	1013	rBV4	897	2343	0.69%	0.090%
25	7.312	1013	1021	1039	rVB	65390	155213	45.59%	5.992%
26	7.452	1042	1044	1046	rVB2	131	117	0.03%	0.005%
27	7.476	1046	1048	1053	rBV2	203	319	0.09%	0.012%
28	7.592	1065	1067	1069	rVB2	161	109	0.03%	0.004%
29	7.647	1072	1076	1078	rBV2	108	123	0.04%	0.005%
30	7.769	1094	1096	1098	rBV	97	115	0.03%	0.004%
31	7.934	1121	1123	1125	rVV	187	162	0.05%	0.006%
32	7.964	1126	1128	1132	rVB2	297	326	0.10%	0.013%
33	8.330	1182	1188	1198	rBV2	34997	63915	18.77%	2.468%
34	8.476	1208	1212	1217	rBV2	95	241	0.07%	0.009%
35	8.537	1220	1222	1225	rVB2	115	110	0.03%	0.004%
36	8.653	1233	1241	1248	rBV	165588	275842	81.03%	10.649%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025572.D
 Acq On : 07 Dec 2021 12:24
 Operator : JC/MD
 Sample : M4881-06ME
 Misc : 4.42g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW9E2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	8.720	1248	1252	1258	rVB	1993	3163	0.93%	0.122%
38	8.958	1285	1291	1299	rVV	22121	39051	11.47%	1.508%
39	9.116	1314	1317	1320	rBV2	144	184	0.05%	0.007%
40	9.202	1329	1331	1334	rVV	105	125	0.04%	0.005%
41	9.275	1340	1343	1345	rVB2	140	165	0.05%	0.006%
42	9.397	1355	1363	1377	rBV	87572	153585	45.11%	5.929%
43	9.561	1388	1390	1392	rVB2	187	146	0.04%	0.006%
44	9.720	1412	1416	1419	rVB4	539	836	0.25%	0.032%
45	9.756	1419	1422	1425	rBV2	147	189	0.06%	0.007%
46	9.817	1430	1432	1435	rVB2	224	177	0.05%	0.007%
47	10.055	1465	1471	1484	rVV	159360	237380	69.73%	9.165%
48	10.201	1491	1495	1497	rVB2	318	327	0.10%	0.013%
49	10.305	1508	1512	1520	rBV2	897	1361	0.40%	0.053%
50	10.604	1559	1561	1564	rBV	130	121	0.04%	0.005%
51	10.646	1564	1568	1574	rVB3	677	999	0.29%	0.039%
52	10.695	1574	1576	1578	rBV2	115	120	0.04%	0.005%
53	10.970	1615	1621	1623	rBV3	223	379	0.11%	0.015%
54	11.000	1623	1626	1628	rVB	146	170	0.05%	0.007%
55	11.018	1628	1629	1633	rBV	179	168	0.05%	0.006%
56	11.122	1643	1646	1649	rVB	861	996	0.29%	0.038%
57	11.195	1653	1658	1666	rVV	124406	164738	48.39%	6.360%
58	11.281	1669	1672	1673	rBV	273	249	0.07%	0.010%
59	11.354	1681	1684	1686	rBV2	129	144	0.04%	0.006%
60	11.384	1687	1689	1693	rVB3	221	295	0.09%	0.011%
61	11.476	1702	1704	1707	rBV2	348	349	0.10%	0.013%
62	11.537	1713	1714	1718	rVB	108	108	0.03%	0.004%
63	11.616	1725	1727	1728	rVV2	256	188	0.06%	0.007%
64	11.707	1741	1742	1744	rBV	309	153	0.04%	0.006%
65	11.750	1745	1749	1755	rVB3	1408	2128	0.63%	0.082%
66	11.823	1759	1761	1763	rBV2	125	120	0.04%	0.005%
67	11.847	1763	1765	1768	rBV2	99	109	0.03%	0.004%
68	11.902	1770	1774	1775	rVB2	144	153	0.04%	0.006%
69	11.933	1776	1779	1783	rVB3	595	620	0.18%	0.024%
70	11.976	1783	1786	1789	rBV	152	155	0.05%	0.006%
71	12.024	1789	1794	1802	rBV	195407	234105	68.77%	9.038%
72	12.128	1808	1811	1812	rBV	449	441	0.13%	0.017%
73	12.152	1812	1815	1818	rVB2	883	1058	0.31%	0.041%
74	12.323	1837	1843	1851	rVB	202414	252743	74.24%	9.758%
75	12.427	1857	1860	1865	rVB2	704	784	0.23%	0.030%
76	12.482	1865	1869	1872	rVB2	225	284	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025572.D
 Acq On : 07 Dec 2021 12:24
 Operator : JC/MD
 Sample : M4881-06ME
 Misc : 4.42g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW9E2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	12.628	1891	1893	1896	rVB2	236	173	0.05%	0.007%
78	12.671	1896	1900	1904	rVB3	253	399	0.12%	0.015%
79	12.731	1904	1910	1912	rBV2	145	241	0.07%	0.009%
80	12.768	1912	1916	1918	rVV2	342	429	0.13%	0.017%
81	12.872	1931	1933	1936	rBV	118	111	0.03%	0.004%
82	13.018	1955	1957	1960	rBV2	108	154	0.05%	0.006%
83	13.061	1960	1964	1966	rVV2	191	288	0.08%	0.011%
84	13.274	1994	1999	2003	rVB3	285	557	0.16%	0.022%
85	13.384	2015	2017	2022	rVB2	208	154	0.05%	0.006%
86	13.481	2031	2033	2035	rBV2	182	149	0.04%	0.006%
87	13.780	2076	2082	2088	rVB3	409	692	0.20%	0.027%
88	14.042	2122	2125	2127	rBV2	378	292	0.09%	0.011%
89	14.128	2133	2139	2146	rVB4	839	1392	0.41%	0.054%
90	14.207	2150	2152	2154	rBV	135	108	0.03%	0.004%
91	14.280	2163	2164	2168	rBV2	105	119	0.03%	0.005%
92	14.603	2214	2217	2218	rVV2	151	158	0.05%	0.006%
93	14.640	2221	2223	2228	rVB3	380	539	0.16%	0.021%
94	14.756	2239	2242	2244	rBV2	344	394	0.12%	0.015%
95	14.780	2244	2246	2250	rVB3	370	464	0.14%	0.018%
96	14.816	2250	2252	2254	rBV2	166	141	0.04%	0.005%
97	15.066	2291	2293	2295	rBV2	166	151	0.04%	0.006%
98	15.213	2315	2317	2322	rVB2	603	628	0.18%	0.024%
99	15.396	2343	2347	2354	rVB3	614	1000	0.29%	0.039%
100	16.298	2493	2495	2497	rVB3	256	183	0.05%	0.007%




Sum of corrected areas: 2590210

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025572.D
Acq On : 07 Dec 2021 12:24
Operator : JC/MD
Sample : M4881-06ME
Misc : 4.42g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW9E2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

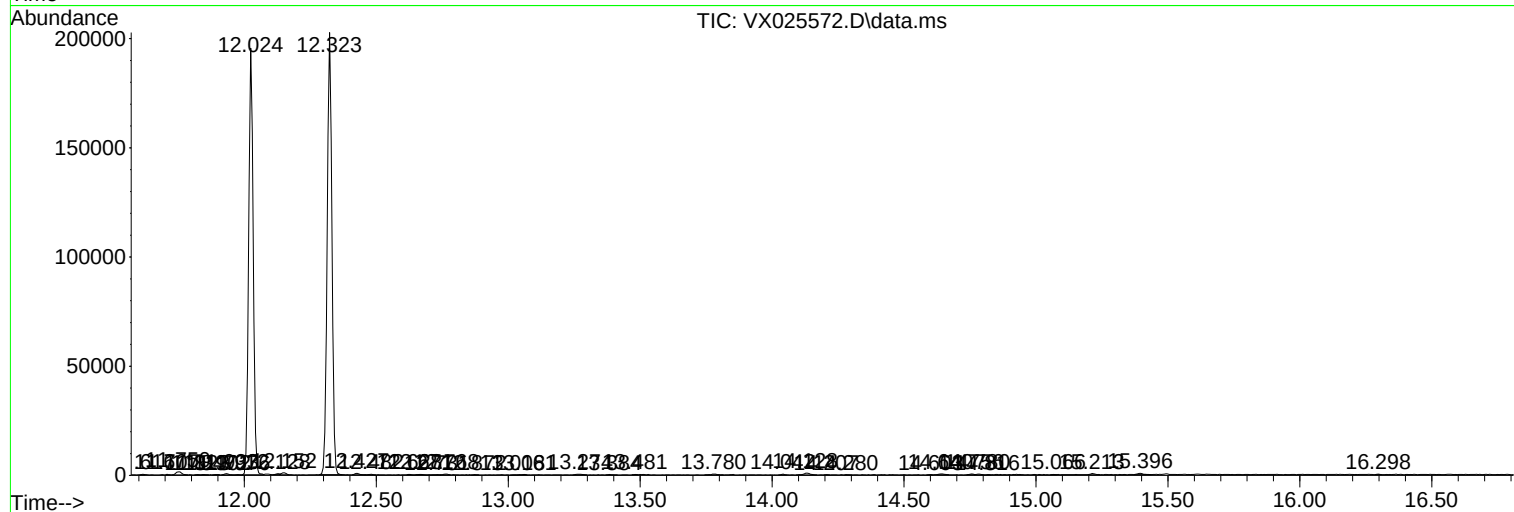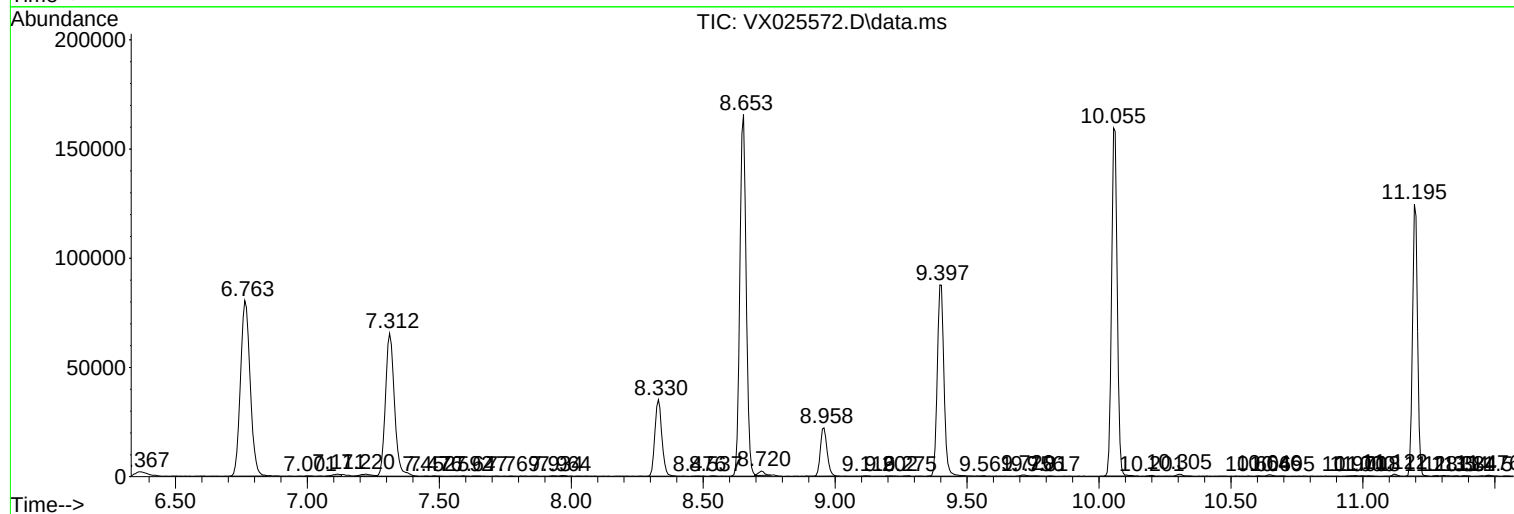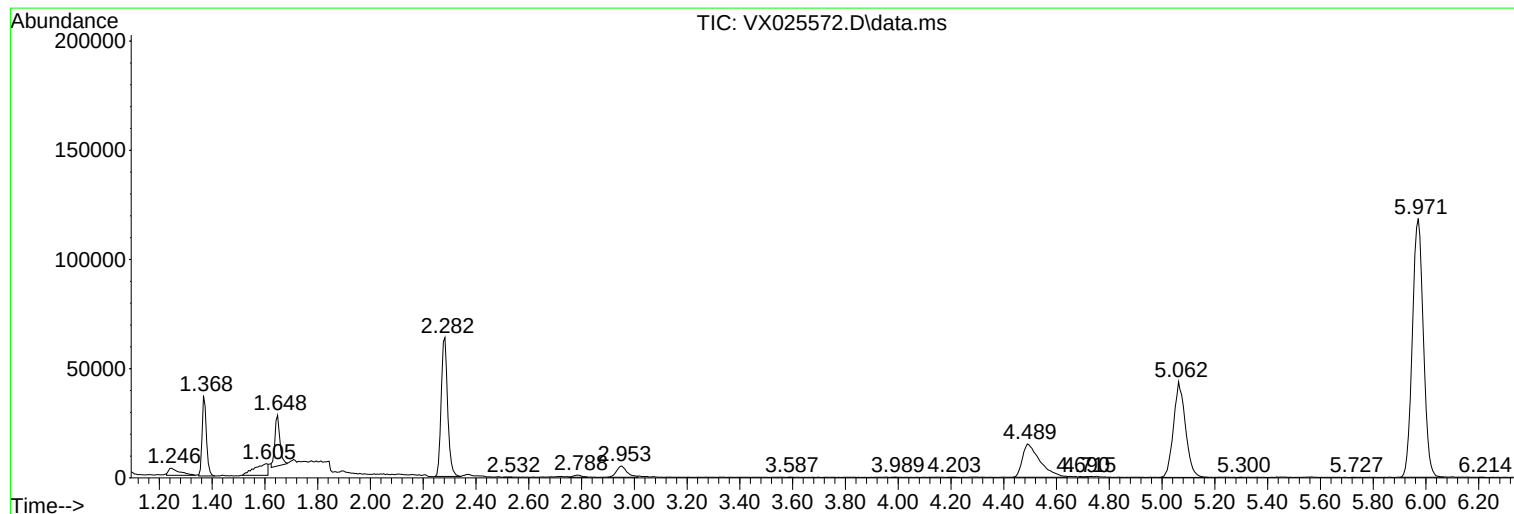

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025572.D
Acq On : 07 Dec 2021 12:24
Operator : JC/MD
Sample : M4881-06ME
Misc : 4.42g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW9E2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025572.D
Acq On : 07 Dec 2021 12:24
Operator : JC/MD
Sample : M4881-06ME
Misc : 4.42g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW9E2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc