

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025590.D
 Acq On : 07 Dec 2021 20:47
 Operator : JC/MD
 Sample : M4886-03ME
 Misc : 4.64g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW9M9ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025590.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	32	rBV	4697	8863	1.67%	0.218%
2	1.373	43	47	57	rVB	66568	77567	14.59%	1.911%
3	1.562	69	78	79	rBV5	3249	7308	1.37%	0.180%
4	1.648	88	92	98	rBV	39992	47374	8.91%	1.167%
5	2.282	190	196	205	rBV	120286	192536	36.22%	4.743%
6	2.654	255	257	258	rBV	159	137	0.03%	0.003%
7	2.794	275	280	286	rVB4	1152	2630	0.49%	0.065%
8	2.952	298	306	314	rBV	4234	10174	1.91%	0.251%
9	3.117	331	333	334	rBV	179	137	0.03%	0.003%
10	3.714	427	431	433	rVB2	110	142	0.03%	0.003%
11	4.086	488	492	493	rBV	116	138	0.03%	0.003%
12	4.245	514	518	519	rBV2	147	182	0.03%	0.004%
13	4.263	519	521	522	rVV	209	135	0.03%	0.003%
14	4.294	522	526	528	rVB3	300	446	0.08%	0.011%
15	4.312	528	529	532	rBV2	142	164	0.03%	0.004%
16	4.489	547	558	580	rBV	22773	100762	18.96%	2.482%
17	4.793	606	608	611	rBV2	138	189	0.04%	0.005%
18	5.068	640	653	670	rBV	63949	205217	38.61%	5.056%
19	5.446	713	715	721	rVB2	399	627	0.12%	0.015%
20	5.562	727	734	736	rVB2	155	277	0.05%	0.007%
21	5.629	744	745	747	rBV2	160	149	0.03%	0.004%
22	5.970	788	801	817	rBV2	186453	531571	100.00%	13.096%
23	6.299	852	855	857	rBV2	104	140	0.03%	0.003%
24	6.360	858	865	875	rBV4	2189	6193	1.17%	0.153%
25	6.543	894	895	898	rBV2	138	151	0.03%	0.004%
26	6.763	921	931	947	rVV	132912	337781	63.54%	8.322%
27	7.116	983	989	996	rBV6	1724	4517	0.85%	0.111%
28	7.208	1001	1004	1005	rBV	525	576	0.11%	0.014%
29	7.311	1012	1021	1038	rVB	100051	234934	44.20%	5.788%
30	7.488	1048	1050	1052	rVB2	219	169	0.03%	0.004%
31	7.750	1090	1093	1094	rBV	144	153	0.03%	0.004%
32	7.964	1126	1128	1134	rVB3	406	504	0.09%	0.012%
33	8.329	1181	1188	1204	rVB	60167	108098	20.34%	2.663%
34	8.482	1210	1213	1214	rBV	145	123	0.02%	0.003%
35	8.592	1229	1231	1234	rBV2	185	279	0.05%	0.007%
36	8.653	1234	1241	1248	rVV	269019	439238	82.63%	10.821%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025590.D
 Acq On : 07 Dec 2021 20:47
 Operator : JC/MD
 Sample : M4886-03ME
 Misc : 4.64g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW9M9ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	8.720	1249	1252	1257	rVB	4106	5722	1.08%	0.141%
38	8.957	1285	1291	1301	rVV	38538	67219	12.65%	1.656%
39	9.104	1314	1315	1320	rVB2	99	134	0.03%	0.003%
40	9.274	1340	1343	1347	rVB3	272	323	0.06%	0.008%
41	9.396	1357	1363	1375	rBV	135909	221752	41.72%	5.463%
42	9.616	1396	1399	1404	rBV3	488	644	0.12%	0.016%
43	9.713	1411	1415	1420	rVB2	365	557	0.10%	0.014%
44	9.756	1420	1422	1424	rBV	146	102	0.02%	0.003%
45	9.811	1429	1431	1434	rBV	153	136	0.03%	0.003%
46	9.988	1456	1460	1462	rBV2	111	113	0.02%	0.003%
47	10.061	1466	1472	1482	rVV	264556	390033	73.37%	9.609%
48	10.201	1491	1495	1500	rVB2	458	725	0.14%	0.018%
49	10.305	1508	1512	1517	rVB	1634	2087	0.39%	0.051%
50	10.360	1520	1521	1526	rVB2	317	230	0.04%	0.006%
51	10.561	1552	1554	1555	rBV	137	120	0.02%	0.003%
52	10.646	1564	1568	1572	rBV3	1031	1457	0.27%	0.036%
53	10.756	1585	1586	1589	rVV2	354	214	0.04%	0.005%
54	10.969	1617	1621	1625	rBV2	320	425	0.08%	0.010%
55	11.122	1642	1646	1650	rBV	3392	4396	0.83%	0.108%
56	11.195	1653	1658	1668	rBV	178224	236422	44.48%	5.825%
57	11.286	1669	1673	1674	rBV3	402	443	0.08%	0.011%
58	11.384	1686	1689	1693	rBV3	255	364	0.07%	0.009%
59	11.481	1698	1705	1708	rBV5	1226	2305	0.43%	0.057%
60	11.548	1713	1716	1719	rBV2	449	412	0.08%	0.010%
61	11.682	1735	1738	1741	rBV3	229	378	0.07%	0.009%
62	11.713	1741	1743	1745	rVV	590	584	0.11%	0.014%
63	11.750	1745	1749	1754	rVB2	3397	4458	0.84%	0.110%
64	11.847	1761	1765	1769	rBV2	713	782	0.15%	0.019%
65	11.932	1775	1779	1783	rVB2	1698	1984	0.37%	0.049%
66	11.975	1783	1786	1789	rBV2	281	248	0.05%	0.006%
67	12.024	1789	1794	1800	rBV	310782	391574	73.66%	9.647%
68	12.121	1808	1810	1811	rBV2	706	585	0.11%	0.014%
69	12.268	1832	1834	1836	rBV2	272	219	0.04%	0.005%
70	12.323	1836	1843	1851	rVV	317194	387651	72.93%	9.550%
71	12.426	1856	1860	1864	rBV3	1737	2183	0.41%	0.054%
72	12.475	1864	1868	1873	rVB3	761	1297	0.24%	0.032%
73	12.664	1896	1899	1903	rVB4	647	794	0.15%	0.020%
74	12.762	1913	1915	1918	rBV	201	194	0.04%	0.005%
75	12.847	1927	1929	1931	rBV2	102	128	0.02%	0.003%
76	13.048	1959	1962	1968	rVB3	549	656	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025590.D
 Acq On : 07 Dec 2021 20:47
 Operator : JC/MD
 Sample : M4886-03ME
 Misc : 4.64g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW9M9ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	13.268	1995	1998	2002	rVV2	521	586	0.11%	0.014%
78	13.298	2002	2003	2006	rVV2	144	115	0.02%	0.003%
79	13.329	2006	2008	2010	rVB	156	105	0.02%	0.003%
80	13.390	2015	2018	2020	rBV2	320	355	0.07%	0.009%
81	13.450	2026	2028	2033	rVB2	128	152	0.03%	0.004%
82	13.780	2079	2082	2088	rVB	1058	1236	0.23%	0.030%
83	13.847	2090	2093	2097	rVV4	554	612	0.12%	0.015%
84	13.883	2097	2099	2103	rVB	193	189	0.04%	0.005%
85	13.938	2106	2108	2110	rBV	176	131	0.02%	0.003%
86	13.969	2110	2113	2116	rBV2	233	221	0.04%	0.005%
87	14.042	2119	2125	2128	rBV2	647	805	0.15%	0.020%
88	14.127	2135	2139	2146	rBV2	398	759	0.14%	0.019%
89	14.432	2188	2189	2194	rVB2	130	140	0.03%	0.003%
90	14.615	2217	2219	2220	rBV2	143	131	0.02%	0.003%
91	14.639	2220	2223	2228	rVV3	632	946	0.18%	0.023%
92	14.755	2239	2242	2244	rBV3	532	557	0.10%	0.014%
93	14.780	2244	2246	2253	rVB2	607	795	0.15%	0.020%
94	15.212	2315	2317	2320	rBV3	261	334	0.06%	0.008%
95	15.383	2343	2345	2346	rBV	243	124	0.02%	0.003%
96	15.615	2381	2383	2387	rVB2	396	434	0.08%	0.011%
97	15.657	2387	2390	2392	rBV2	258	247	0.05%	0.006%
98	15.944	2436	2437	2441	rBV2	183	186	0.03%	0.005%
99	16.157	2471	2472	2474	rBV	288	158	0.03%	0.004%
100	16.499	2526	2528	2530	rBV	185	107	0.02%	0.003%




Sum of corrected areas: 4059056

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025590.D
Acq On : 07 Dec 2021 20:47
Operator : JC/MD
Sample : M4886-03ME
Misc : 4.64g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW9M9ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

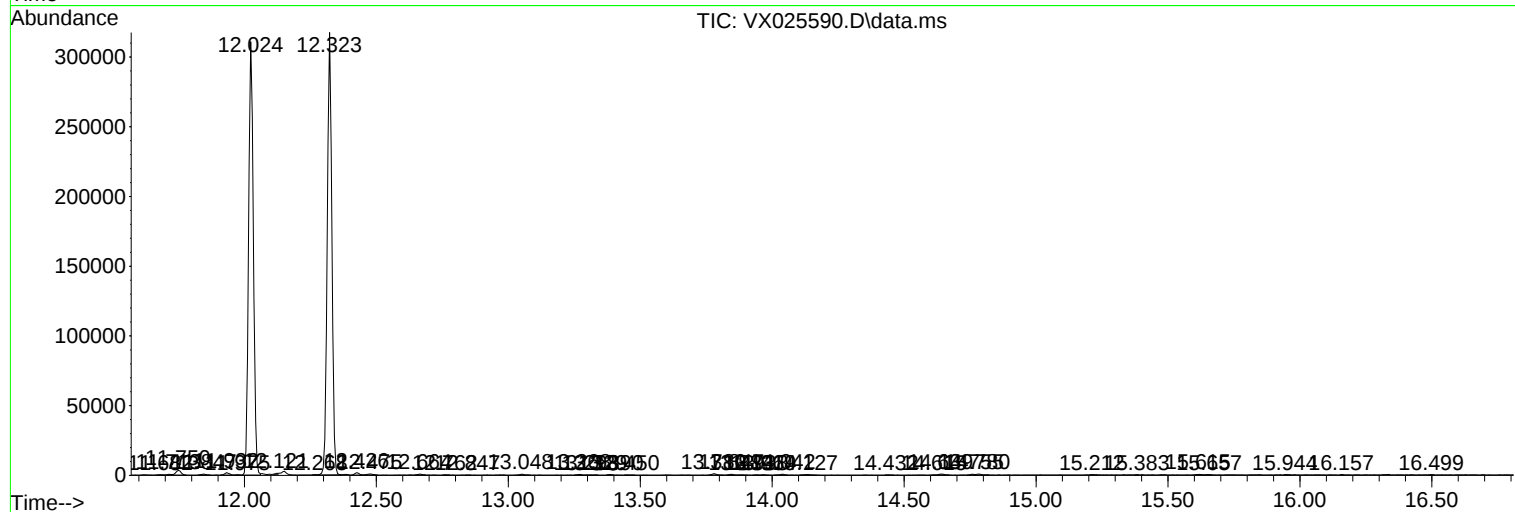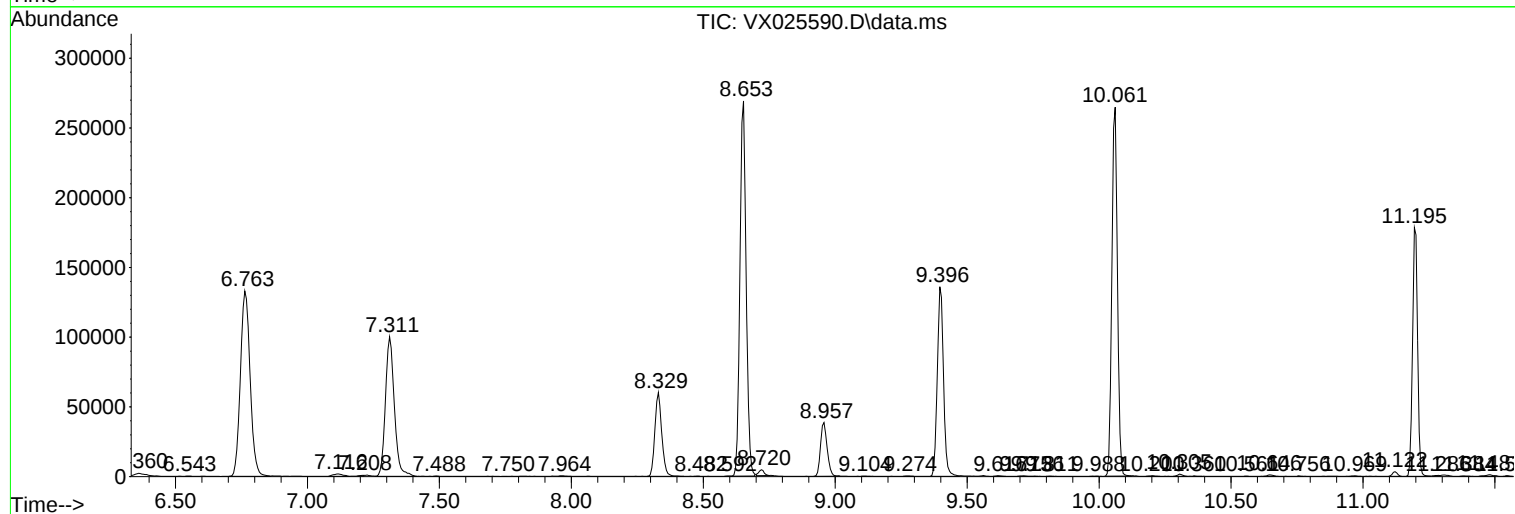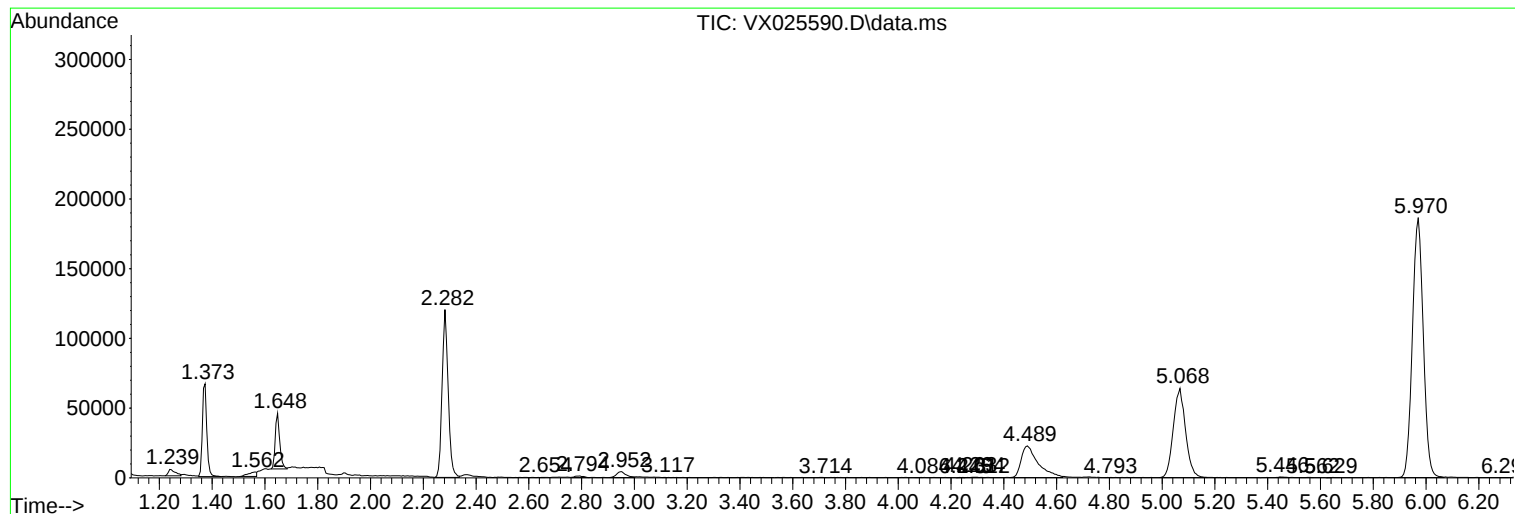

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025590.D
Acq On : 07 Dec 2021 20:47
Operator : JC/MD
Sample : M4886-03ME
Misc : 4.64g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW9M9ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025590.D
Acq On : 07 Dec 2021 20:47
Operator : JC/MD
Sample : M4886-03ME
Misc : 4.64g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW9M9ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc