

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025591.D
 Acq On : 07 Dec 2021 21:11
 Operator : JC/MD
 Sample : M4886-06ME
 Misc : 3.91g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EX887ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025591.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	43	rVV2	4858	11416	2.09%	0.279%
2	1.368	43	46	53	rVB	68681	77494	14.17%	1.895%
3	1.599	69	84	85	rBV6	5025	18451	3.37%	0.451%
4	1.648	88	92	98	rVV	39409	50855	9.30%	1.244%
5	2.282	189	196	205	rBV	119811	194850	35.64%	4.766%
6	2.538	235	238	240	rBV2	131	154	0.03%	0.004%
7	2.788	274	279	286	rVB4	886	1767	0.32%	0.043%
8	2.953	298	306	316	rBV	4310	11713	2.14%	0.286%
9	3.514	396	398	403	rVB2	168	217	0.04%	0.005%
10	3.556	403	405	407	rBV2	115	125	0.02%	0.003%
11	3.605	410	413	417	rBV2	112	179	0.03%	0.004%
12	3.648	417	420	424	rVB2	106	155	0.03%	0.004%
13	3.989	474	476	478	rVV2	122	118	0.02%	0.003%
14	4.050	484	486	488	rBV2	144	138	0.03%	0.003%
15	4.135	498	500	504	rVB2	123	149	0.03%	0.004%
16	4.233	513	516	520	rVB2	120	143	0.03%	0.003%
17	4.489	548	558	585	rBV2	22427	106014	19.39%	2.593%
18	5.068	640	653	672	rBV	60847	207289	37.91%	5.070%
19	5.342	695	698	701	rBV2	137	179	0.03%	0.004%
20	5.391	703	706	708	rVB2	129	155	0.03%	0.004%
21	5.440	708	714	715	rBV2	125	213	0.04%	0.005%
22	5.470	715	719	721	rBV2	141	201	0.04%	0.005%
23	5.556	729	733	737	rVV3	180	248	0.05%	0.006%
24	5.733	760	762	763	rBV	121	126	0.02%	0.003%
25	5.970	788	801	819	rBV2	187906	546748	100.00%	13.373%
26	6.361	860	865	866	rBV2	1736	2612	0.48%	0.064%
27	6.617	902	907	909	rBV2	119	191	0.03%	0.005%
28	6.763	921	931	948	rBV	120856	307302	56.21%	7.517%
29	7.031	973	975	977	rVV2	130	133	0.02%	0.003%
30	7.123	982	990	998	rVB9	1999	5722	1.05%	0.140%
31	7.214	998	1005	1012	rBV3	837	2413	0.44%	0.059%
32	7.312	1012	1021	1036	rVB	101372	237112	43.37%	5.800%
33	7.415	1036	1038	1043	rVB2	153	184	0.03%	0.005%
34	7.818	1100	1104	1107	rBV3	112	175	0.03%	0.004%
35	7.933	1120	1123	1124	rVV3	153	158	0.03%	0.004%
36	7.946	1124	1125	1128	rVB2	255	219	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025591.D
 Acq On : 07 Dec 2021 21:11
 Operator : JC/MD
 Sample : M4886-06ME
 Misc : 3.91g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EX887ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	8.330	1181	1188	1201	rVB	60200	110131	20.14%	2.694%
38	8.561	1223	1226	1228	rBV2	106	146	0.03%	0.004%
39	8.653	1234	1241	1249	rBV	275673	455817	83.37%	11.149%
40	8.720	1249	1252	1257	rVB	3532	5167	0.95%	0.126%
41	8.854	1270	1274	1276	rVB2	93	140	0.03%	0.003%
42	8.958	1285	1291	1300	rBV	40317	69443	12.70%	1.699%
43	9.275	1338	1343	1350	rVB	7928	11215	2.05%	0.274%
44	9.336	1350	1353	1355	rBV2	99	159	0.03%	0.004%
45	9.397	1357	1363	1377	rBV	141873	231418	42.33%	5.660%
46	9.628	1399	1401	1403	rVB2	163	132	0.02%	0.003%
47	9.714	1411	1415	1418	rVV2	450	683	0.12%	0.017%
48	9.866	1437	1440	1441	rBV	145	119	0.02%	0.003%
49	9.970	1454	1457	1458	rBV	140	132	0.02%	0.003%
50	10.061	1465	1472	1480	rBV	243515	359046	65.67%	8.782%
51	10.195	1489	1494	1499	rBV3	276	523	0.10%	0.013%
52	10.305	1508	1512	1517	rVV2	984	1424	0.26%	0.035%
53	10.439	1530	1534	1536	rBV2	114	170	0.03%	0.004%
54	10.646	1564	1568	1573	rVB	468	592	0.11%	0.014%
55	10.689	1573	1575	1576	rBV	153	124	0.02%	0.003%
56	10.744	1582	1584	1587	rVB2	150	165	0.03%	0.004%
57	11.122	1641	1646	1650	rVB	3651	4467	0.82%	0.109%
58	11.195	1653	1658	1666	rBV	193340	245526	44.91%	6.005%
59	11.384	1687	1689	1691	rBV	203	227	0.04%	0.006%
60	11.476	1698	1704	1708	rBV4	873	1755	0.32%	0.043%
61	11.549	1713	1716	1723	rVB3	466	500	0.09%	0.012%
62	11.634	1729	1730	1731	rBV	212	115	0.02%	0.003%
63	11.750	1745	1749	1753	rVB2	3407	4433	0.81%	0.108%
64	11.805	1753	1758	1761	rBV2	148	272	0.05%	0.007%
65	11.841	1761	1764	1769	rVB2	665	711	0.13%	0.017%
66	11.933	1774	1779	1782	rBV3	1923	2296	0.42%	0.056%
67	12.024	1789	1794	1800	rBV	305043	365349	66.82%	8.936%
68	12.122	1807	1810	1812	rBV2	1355	1767	0.32%	0.043%
69	12.152	1812	1815	1818	rVB	2820	3159	0.58%	0.077%
70	12.323	1835	1843	1849	rBV	327683	406651	74.38%	9.947%
71	12.427	1856	1860	1863	rBV3	1341	1587	0.29%	0.039%
72	12.475	1866	1868	1873	rVB3	626	941	0.17%	0.023%
73	12.524	1873	1876	1879	rVB	179	226	0.04%	0.006%
74	12.634	1891	1894	1895	rBV2	193	205	0.04%	0.005%
75	12.664	1896	1899	1905	rVB2	622	931	0.17%	0.023%
76	12.762	1913	1915	1917	rBV	203	168	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025591.D
 Acq On : 07 Dec 2021 21:11
 Operator : JC/MD
 Sample : M4886-06ME
 Misc : 3.91g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EX887ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	12.823	1922	1925	1926	rVV	158	119	0.02%	0.003%
78	13.000	1952	1954	1957	rVB2	119	138	0.03%	0.003%
79	13.054	1960	1963	1970	rVB4	398	754	0.14%	0.018%
80	13.292	2000	2002	2005	rVB2	147	162	0.03%	0.004%
81	13.536	2040	2042	2043	rBV	154	127	0.02%	0.003%
82	13.780	2077	2082	2088	rVV	5021	6151	1.13%	0.150%
83	13.847	2090	2093	2095	rVV2	285	254	0.05%	0.006%
84	14.036	2122	2124	2129	rVB2	627	558	0.10%	0.014%
85	14.286	2164	2165	2168	rBV2	135	165	0.03%	0.004%
86	14.408	2183	2185	2187	rBV	163	195	0.04%	0.005%
87	14.524	2203	2204	2207	rVB	155	141	0.03%	0.003%
88	14.640	2220	2223	2228	rVB2	867	1165	0.21%	0.028%
89	14.755	2238	2242	2244	rBV5	945	1253	0.23%	0.031%
90	14.847	2254	2257	2258	rVV2	322	304	0.06%	0.007%
91	14.963	2275	2276	2278	rBV2	217	200	0.04%	0.005%
92	15.121	2300	2302	2305	rBV3	246	237	0.04%	0.006%
93	15.396	2345	2347	2348	rBV2	199	138	0.03%	0.003%
94	15.420	2348	2351	2355	rVV3	382	524	0.10%	0.013%
95	15.481	2359	2361	2368	rVB3	639	976	0.18%	0.024%
96	15.578	2375	2377	2379	rBV2	159	136	0.02%	0.003%
97	15.743	2402	2404	2405	rBV	301	206	0.04%	0.005%
98	15.969	2439	2441	2443	rBV	197	194	0.04%	0.005%
99	16.688	2557	2559	2560	rBV2	209	173	0.03%	0.004%
100	16.712	2560	2563	2569	rVB4	513	742	0.14%	0.018%




Sum of corrected areas: 4088362

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025591.D
Acq On : 07 Dec 2021 21:11
Operator : JC/MD
Sample : M4886-06ME
Misc : 3.91g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EX887ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

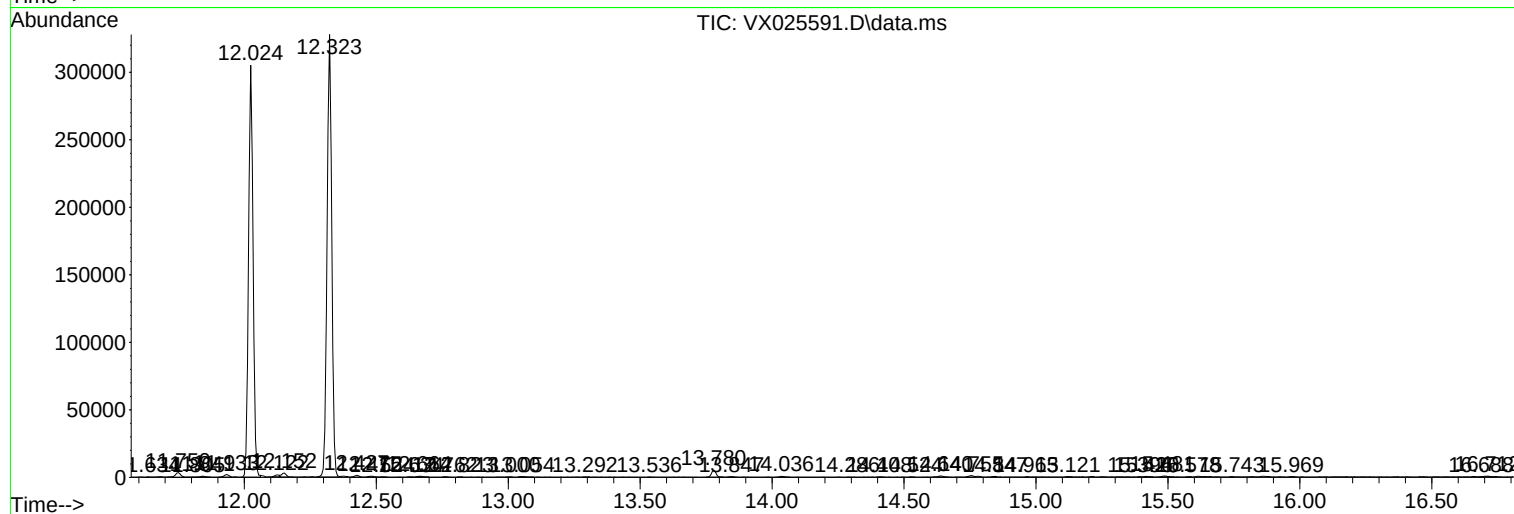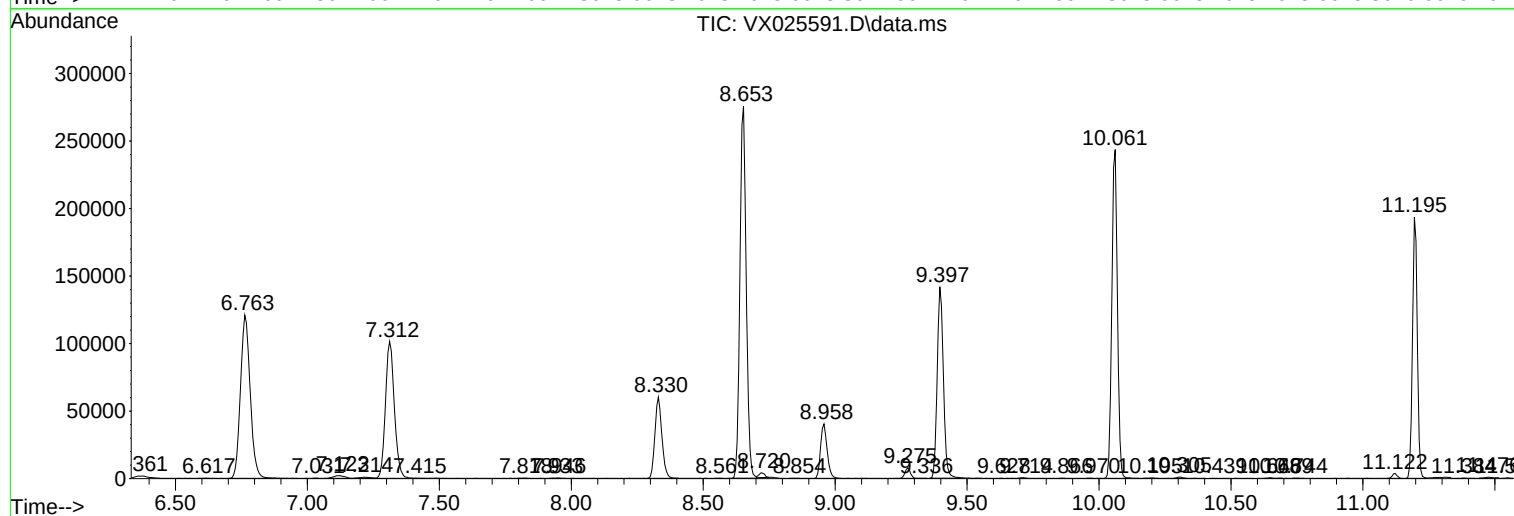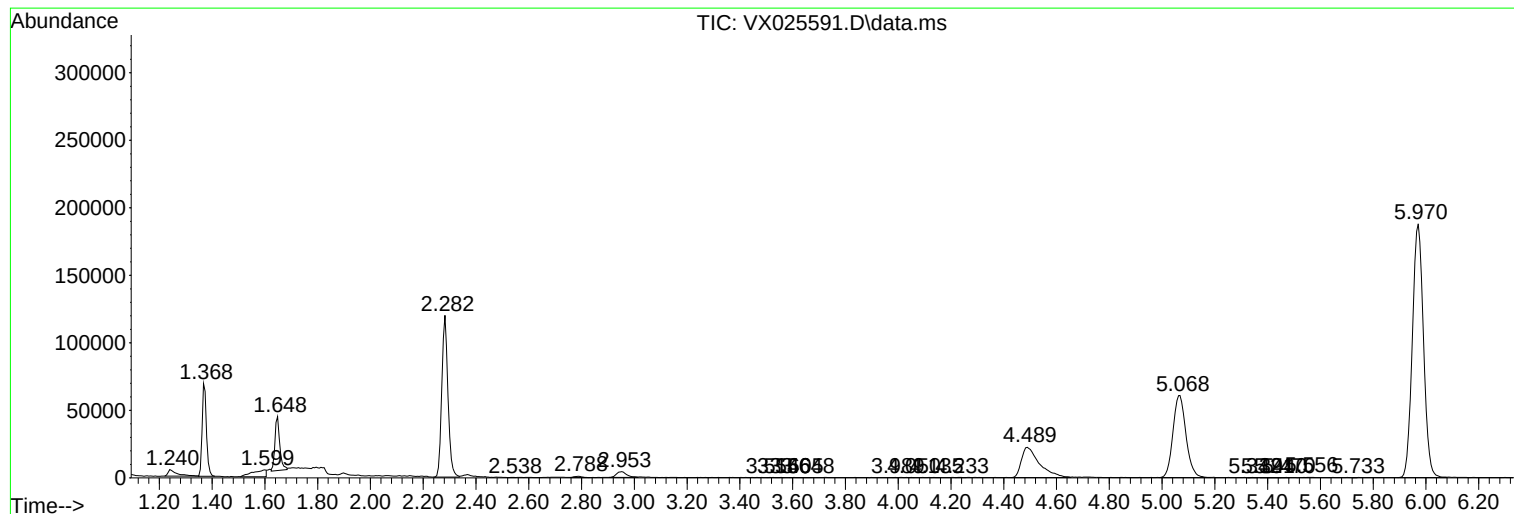

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025591.D
Acq On : 07 Dec 2021 21:11
Operator : JC/MD
Sample : M4886-06ME
Misc : 3.91g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EX887ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025591.D
Acq On : 07 Dec 2021 21:11
Operator : JC/MD
Sample : M4886-06ME
Misc : 3.91g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EX887ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc