

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025594.D
 Acq On : 07 Dec 2021 22:21
 Operator : JC/MD
 Sample : M4886-09ME
 Misc : 4.40g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EX890ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025594.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	33	rBV2	4120	8199	1.59%	0.207%
2	1.368	43	46	53	rVB	65393	74080	14.33%	1.872%
3	1.569	70	79	80	rBV2	3852	8860	1.71%	0.224%
4	1.648	88	92	99	rBV	37714	46303	8.96%	1.170%
5	2.282	190	196	206	rBV	119050	187811	36.33%	4.747%
6	2.605	246	249	251	rBV	177	164	0.03%	0.004%
7	2.782	274	278	286	rVB2	970	1758	0.34%	0.044%
8	2.947	298	305	313	rBV	3738	9614	1.86%	0.243%
9	3.569	405	407	410	rBV2	136	156	0.03%	0.004%
10	3.843	450	452	453	rBV	133	99	0.02%	0.003%
11	3.953	469	470	474	rVB2	168	157	0.03%	0.004%
12	4.117	494	497	500	rBV2	197	333	0.06%	0.008%
13	4.410	542	545	548	rBV2	116	158	0.03%	0.004%
14	4.489	548	558	584	rBV	21425	99505	19.25%	2.515%
15	4.794	606	608	612	rVB2	77	83	0.02%	0.002%
16	4.946	631	633	634	rBV2	139	102	0.02%	0.003%
17	4.965	634	636	638	rVB	255	198	0.04%	0.005%
18	5.062	638	652	672	rBV	62510	203877	39.44%	5.153%
19	5.416	708	710	713	rBV	95	108	0.02%	0.003%
20	5.971	789	801	818	rBV2	177342	516893	100.00%	13.064%
21	6.367	859	866	868	rBV4	1872	3822	0.74%	0.097%
22	6.647	911	912	914	rBV	116	103	0.02%	0.003%
23	6.690	916	919	921	rVB2	99	112	0.02%	0.003%
24	6.763	921	931	946	rBV	122482	314587	60.86%	7.951%
25	7.025	972	974	975	rBV	188	92	0.02%	0.002%
26	7.111	982	988	998	rVV9	1855	4667	0.90%	0.118%
27	7.214	998	1005	1012	rVV3	833	2233	0.43%	0.056%
28	7.312	1012	1021	1038	rVB	96764	227354	43.98%	5.746%
29	7.428	1038	1040	1042	rBV	160	138	0.03%	0.003%
30	7.470	1045	1047	1048	rBV2	115	118	0.02%	0.003%
31	7.769	1092	1096	1098	rBV2	91	144	0.03%	0.004%
32	7.970	1126	1129	1130	rVB	346	286	0.06%	0.007%
33	8.098	1147	1150	1151	rBV2	128	129	0.02%	0.003%
34	8.159	1157	1160	1161	rBV2	82	103	0.02%	0.003%
35	8.244	1172	1174	1177	rBV2	102	135	0.03%	0.003%
36	8.330	1181	1188	1199	rBV	55630	103917	20.10%	2.626%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025594.D
 Acq On : 07 Dec 2021 22:21
 Operator : JC/MD
 Sample : M4886-09ME
 Misc : 4.40g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EX890ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

37	8.574	1226	1228	1230	rVB	110	105	0.02%	0.003%
38	8.598	1230	1232	1234	rBV	197	225	0.04%	0.006%
39	8.653	1234	1241	1249	rBV	256259	433485	83.86%	10.956%
40	8.720	1249	1252	1257	rVB	3645	5151	1.00%	0.130%
41	8.958	1285	1291	1306	rVB2	37039	64999	12.57%	1.643%
42	9.275	1339	1343	1347	rVB3	747	917	0.18%	0.023%
43	9.397	1357	1363	1377	rBV	133631	223873	43.31%	5.658%
44	9.708	1412	1414	1420	rVB4	586	855	0.17%	0.022%
45	9.805	1427	1430	1431	rBV	140	137	0.03%	0.003%
46	9.878	1440	1442	1443	rBV	113	86	0.02%	0.002%
47	9.921	1447	1449	1451	rBV2	96	89	0.02%	0.002%
48	10.061	1465	1472	1483	rBV	247028	370755	71.73%	9.371%
49	10.195	1492	1494	1498	rBV2	302	344	0.07%	0.009%
50	10.232	1498	1500	1501	rBV	126	82	0.02%	0.002%
51	10.305	1508	1512	1517	rBV	879	1126	0.22%	0.028%
52	10.439	1532	1534	1538	rBV2	115	150	0.03%	0.004%
53	10.647	1564	1568	1572	rBV2	322	484	0.09%	0.012%
54	10.799	1589	1593	1594	rBV2	112	153	0.03%	0.004%
55	11.122	1642	1646	1650	rVB	2561	2823	0.55%	0.071%
56	11.195	1653	1658	1666	rBV	178980	232509	44.98%	5.876%
57	11.287	1669	1673	1674	rBV2	264	328	0.06%	0.008%
58	11.409	1691	1693	1694	rVB2	273	154	0.03%	0.004%
59	11.457	1698	1701	1702	rBV2	322	321	0.06%	0.008%
60	11.482	1702	1705	1707	rVV2	1029	1084	0.21%	0.027%
61	11.549	1714	1716	1719	rBV2	131	114	0.02%	0.003%
62	11.616	1725	1727	1731	rVB2	178	162	0.03%	0.004%
63	11.683	1736	1738	1741	rBV2	223	169	0.03%	0.004%
64	11.719	1742	1744	1746	rVV3	291	336	0.07%	0.008%
65	11.750	1746	1749	1753	rVB2	2303	2917	0.56%	0.074%
66	11.841	1761	1764	1768	rBV	396	435	0.08%	0.011%
67	11.933	1775	1779	1783	rBV4	1080	1304	0.25%	0.033%
68	12.024	1789	1794	1800	rBV	301085	374044	72.36%	9.454%
69	12.122	1808	1810	1812	rBV2	670	750	0.15%	0.019%
70	12.152	1812	1815	1818	rVB	1838	2026	0.39%	0.051%
71	12.232	1826	1828	1829	rBV2	263	170	0.03%	0.004%
72	12.256	1829	1832	1834	rVB3	219	239	0.05%	0.006%
73	12.323	1836	1843	1850	rBV	312221	383275	74.15%	9.687%
74	12.427	1856	1860	1864	rVB3	904	1249	0.24%	0.032%
75	12.664	1895	1899	1902	rBV5	575	912	0.18%	0.023%
76	12.762	1913	1915	1919	rVB2	189	211	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025594.D
 Acq On : 07 Dec 2021 22:21
 Operator : JC/MD
 Sample : M4886-09ME
 Misc : 4.40g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EX890ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	12.896	1923	1937	1950	rBV2	2024	9230	1.79%	0.233%
78	13.049	1957	1962	1967	rBV3	415	713	0.14%	0.018%
79	13.097	1967	1970	1971	rBV2	166	147	0.03%	0.004%
80	13.213	1987	1989	1992	rBV2	101	117	0.02%	0.003%
81	13.244	1992	1994	1996	rBV2	120	121	0.02%	0.003%
82	13.268	1996	1998	2001	rVV2	279	277	0.05%	0.007%
83	13.329	2007	2008	2011	rBV	247	185	0.04%	0.005%
84	13.396	2017	2019	2021	rVB2	234	140	0.03%	0.004%
85	13.707	2059	2070	2071	rBV2	1406	2997	0.58%	0.076%
86	13.780	2078	2082	2089	rVB	3497	4874	0.94%	0.123%
87	13.841	2090	2092	2096	rVB	432	323	0.06%	0.008%
88	14.146	2134	2142	2143	rBV3	1994	3355	0.65%	0.085%
89	14.329	2170	2172	2174	rVB	157	98	0.02%	0.002%
90	14.390	2178	2182	2186	rBV2	430	832	0.16%	0.021%
91	14.493	2197	2199	2201	rBV2	154	139	0.03%	0.004%
92	14.597	2213	2216	2217	rVB2	183	148	0.03%	0.004%
93	14.640	2217	2223	2231	rBV2	2004	3529	0.68%	0.089%
94	14.756	2239	2242	2243	rBV3	455	366	0.07%	0.009%
95	14.780	2244	2246	2251	rVB3	994	1296	0.25%	0.033%
96	15.012	2282	2284	2289	rBV3	308	435	0.08%	0.011%
97	15.219	2312	2318	2321	rVB3	679	996	0.19%	0.025%
98	15.487	2358	2362	2366	rVB5	541	913	0.18%	0.023%
99	15.737	2401	2403	2405	rBV2	260	177	0.03%	0.004%
100	15.926	2431	2434	2435	rBV	237	250	0.05%	0.006%




Sum of corrected areas: 3956604

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025594.D
Acq On : 07 Dec 2021 22:21
Operator : JC/MD
Sample : M4886-09ME
Misc : 4.40g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EX890ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

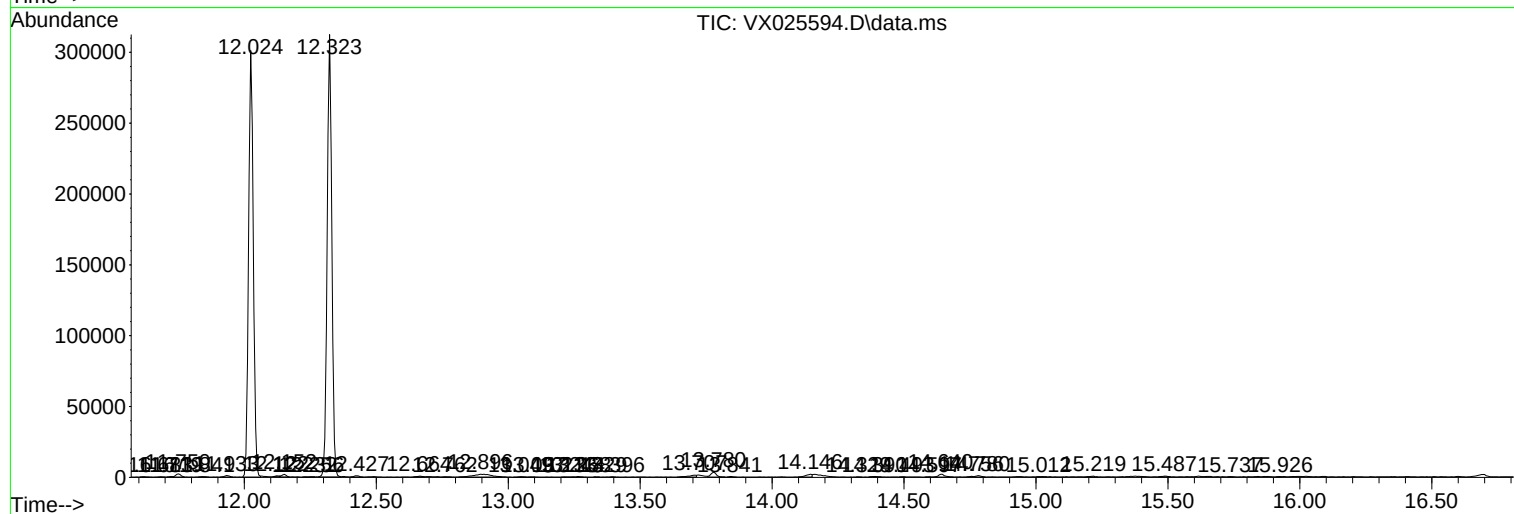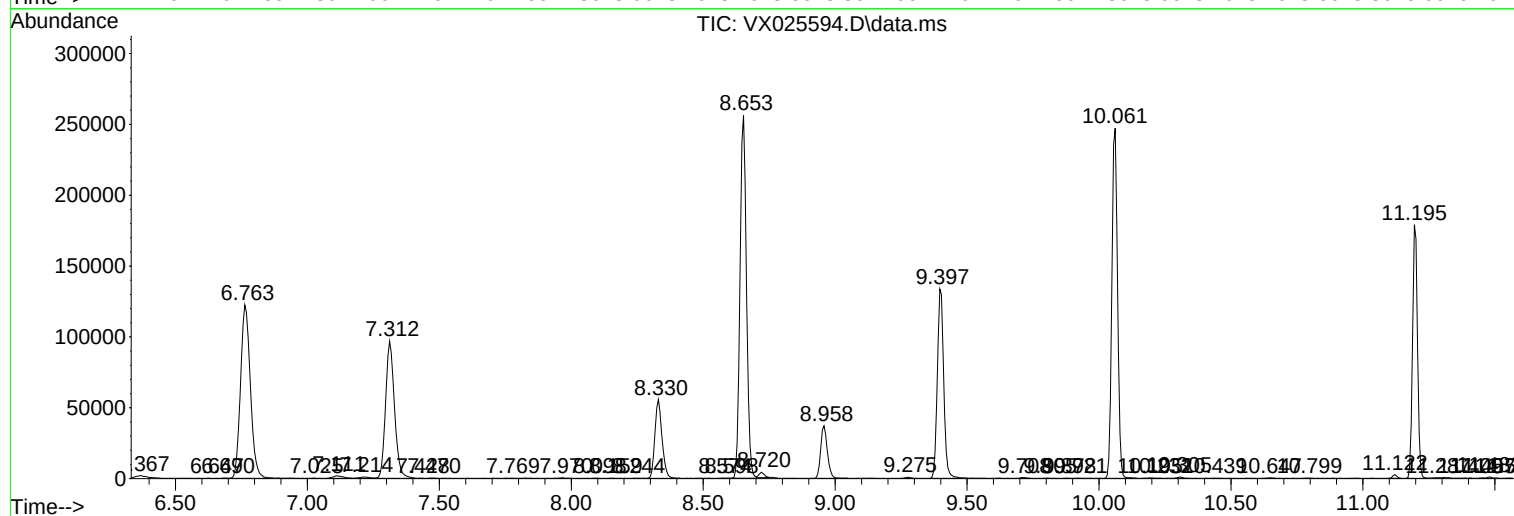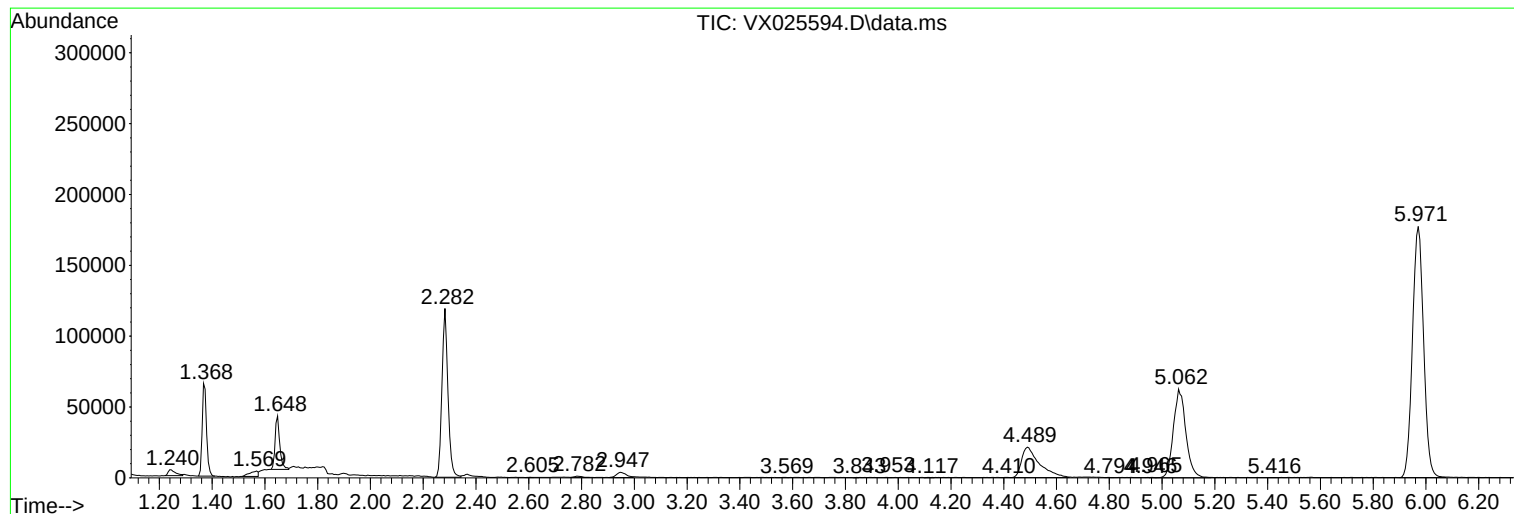

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025594.D
Acq On : 07 Dec 2021 22:21
Operator : JC/MD
Sample : M4886-09ME
Misc : 4.40g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EX890ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025594.D
Acq On : 07 Dec 2021 22:21
Operator : JC/MD
Sample : M4886-09ME
Misc : 4.40g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EX890ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc