

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025598.D
 Acq On : 07 Dec 2021 23:53
 Operator : JC/MD
 Sample : M4886-16ME
 Misc : 5.90g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EX895ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025598.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	32	rBV2	4215	7921	1.54%	0.185%
2	1.368	42	46	56	rVB	64168	73771	14.39%	1.720%
3	1.648	88	92	100	rBV	36363	43608	8.51%	1.017%
4	2.282	189	196	205	rBV	106966	181151	35.33%	4.224%
5	2.685	260	262	263	rBV	110	68	0.01%	0.002%
6	2.715	263	267	270	rBV2	388	528	0.10%	0.012%
7	2.788	275	279	285	rVB5	805	1743	0.34%	0.041%
8	2.874	291	293	294	rBV	149	104	0.02%	0.002%
9	2.953	299	306	318	rBV	3660	9815	1.91%	0.229%
10	3.178	342	343	344	rVB	155	57	0.01%	0.001%
11	3.459	388	389	390	rVB	134	49	0.01%	0.001%
12	3.800	444	445	448	rVB	151	89	0.02%	0.002%
13	3.886	457	459	462	rVB2	155	122	0.02%	0.003%
14	4.032	480	483	484	rBV	109	82	0.02%	0.002%
15	4.184	506	508	510	rBV	97	55	0.01%	0.001%
16	4.233	514	516	517	rVB	146	78	0.02%	0.002%
17	4.251	517	519	521	rBV2	126	106	0.02%	0.002%
18	4.404	543	544	547	rBV	137	148	0.03%	0.003%
19	4.489	549	558	589	rVV2	20351	97617	19.04%	2.276%
20	4.830	613	614	615	rVB	132	48	0.01%	0.001%
21	5.062	640	652	675	rBV	61131	198063	38.63%	4.618%
22	5.623	742	744	746	rBV	98	81	0.02%	0.002%
23	5.782	768	770	772	rBV	116	110	0.02%	0.003%
24	5.971	789	801	819	rBV2	177706	512717	100.00%	11.954%
25	6.190	835	837	840	rVB2	125	109	0.02%	0.003%
26	6.263	847	849	852	rBV2	106	129	0.03%	0.003%
27	6.373	858	867	879	rBV4	2061	7313	1.43%	0.171%
28	6.495	886	887	890	rBV	119	120	0.02%	0.003%
29	6.538	890	894	896	rBV	194	309	0.06%	0.007%
30	6.623	907	908	910	rBV	127	113	0.02%	0.003%
31	6.763	921	931	948	rBV	132413	342939	66.89%	7.996%
32	7.037	974	976	979	rVB	214	257	0.05%	0.006%
33	7.062	979	980	981	rBV	116	76	0.01%	0.002%
34	7.129	981	991	1000	rVV3	18155	43273	8.44%	1.009%
35	7.312	1013	1021	1037	rVB	96574	223743	43.64%	5.217%
36	7.421	1037	1039	1041	rVB	132	73	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025598.D
 Acq On : 07 Dec 2021 23:53
 Operator : JC/MD
 Sample : M4886-16ME
 Misc : 5.90g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EX895ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	7.482	1046	1049	1052	rBV3	148	186	0.04%	0.004%
38	7.787	1098	1099	1102	rBV	135	89	0.02%	0.002%
39	7.818	1102	1104	1105	rBV	229	133	0.03%	0.003%
40	7.934	1122	1123	1124	rBV	190	113	0.02%	0.003%
41	8.043	1140	1141	1142	rBV	75	35	0.01%	0.001%
42	8.226	1170	1171	1173	rBV	195	130	0.03%	0.003%
43	8.251	1173	1175	1178	rVV2	201	248	0.05%	0.006%
44	8.330	1181	1188	1202	rVB	56197	101911	19.88%	2.376%
45	8.653	1233	1241	1249	rBV	258115	433094	84.47%	10.098%
46	8.720	1249	1252	1256	rVB2	3186	4842	0.94%	0.113%
47	8.830	1268	1270	1275	rVB2	160	232	0.05%	0.005%
48	8.866	1275	1276	1279	rBV2	110	99	0.02%	0.002%
49	8.958	1285	1291	1303	rVB	37369	63927	12.47%	1.490%
50	9.043	1303	1305	1309	rVB2	197	249	0.05%	0.006%
51	9.275	1337	1343	1353	rVB	166202	243144	47.42%	5.669%
52	9.342	1353	1354	1355	rBV	124	48	0.01%	0.001%
53	9.403	1357	1364	1380	rVV	126641	215935	42.12%	5.035%
54	9.714	1411	1415	1417	rBV2	459	522	0.10%	0.012%
55	9.763	1422	1423	1424	rBV	145	85	0.02%	0.002%
56	9.781	1424	1426	1427	rBV	211	114	0.02%	0.003%
57	10.061	1466	1472	1486	rVB	265877	402616	78.53%	9.387%
58	10.256	1501	1504	1505	rBV	137	116	0.02%	0.003%
59	10.311	1508	1513	1517	rVV2	627	958	0.19%	0.022%
60	10.616	1561	1563	1565	rVB	106	71	0.01%	0.002%
61	10.640	1565	1567	1568	rBV	183	186	0.04%	0.004%
62	10.750	1583	1585	1586	rBV	229	171	0.03%	0.004%
63	10.921	1611	1613	1615	rBV2	118	150	0.03%	0.003%
64	10.957	1617	1619	1620	rBV	116	70	0.01%	0.002%
65	11.085	1638	1640	1642	rBV2	116	111	0.02%	0.003%
66	11.122	1642	1646	1650	rBV2	2846	3668	0.72%	0.086%
67	11.201	1653	1659	1666	rBV	169681	229003	44.66%	5.339%
68	11.281	1670	1672	1674	rBV2	500	628	0.12%	0.015%
69	11.366	1684	1686	1689	rBV	335	359	0.07%	0.008%
70	11.433	1695	1697	1700	rBV2	184	230	0.04%	0.005%
71	11.482	1700	1705	1712	rVV5	933	2073	0.40%	0.048%
72	11.543	1714	1715	1718	rVB2	535	472	0.09%	0.011%
73	11.573	1718	1720	1722	rBV	100	89	0.02%	0.002%
74	11.720	1742	1744	1745	rBV2	418	355	0.07%	0.008%
75	11.750	1745	1749	1754	rVV3	3191	4150	0.81%	0.097%
76	11.811	1757	1759	1761	rBV	197	141	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025598.D
 Acq On : 07 Dec 2021 23:53
 Operator : JC/MD
 Sample : M4886-16ME
 Misc : 5.90g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EX895ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

77	11.841	1761	1764	1768	rVB4	877	1055	0.21%	0.025%
78	11.939	1775	1780	1783	rBV3	1311	1990	0.39%	0.046%
79	12.024	1789	1794	1800	rBV	333311	416162	81.17%	9.703%
80	12.122	1807	1810	1812	rBV3	965	1190	0.23%	0.028%
81	12.256	1831	1832	1834	rBV2	542	481	0.09%	0.011%
82	12.323	1836	1843	1850	rVV	312075	392070	76.47%	9.141%
83	12.469	1865	1867	1874	rVB5	721	1403	0.27%	0.033%
84	12.530	1876	1877	1882	rVB3	343	485	0.09%	0.011%
85	12.579	1883	1885	1886	rBV2	323	209	0.04%	0.005%
86	12.597	1886	1888	1889	rBV2	358	176	0.03%	0.004%
87	12.664	1896	1899	1901	rBV4	524	647	0.13%	0.015%
88	12.817	1922	1924	1927	rVB3	602	523	0.10%	0.012%
89	12.853	1927	1930	1931	rBV3	541	710	0.14%	0.017%
90	13.049	1958	1962	1968	rVB5	799	1715	0.33%	0.040%
91	14.042	2121	2125	2128	rBV4	1275	1451	0.28%	0.034%
92	14.615	2216	2219	2222	rBV5	894	1302	0.25%	0.030%
93	14.756	2239	2242	2247	rBV4	2115	3077	0.60%	0.072%
94	15.213	2315	2317	2323	rVB4	1502	1564	0.31%	0.036%
95	15.487	2358	2362	2369	rBV4	2017	3297	0.64%	0.077%
96	15.737	2401	2403	2406	rBV2	741	799	0.16%	0.019%
97	16.328	2496	2500	2503	rBV5	465	801	0.16%	0.019%
98	16.432	2515	2517	2519	rVB2	422	266	0.05%	0.006%
99	16.755	2569	2570	2572	rVB3	333	228	0.04%	0.005%
100	16.780	2572	2574	2575	rBV	187	138	0.03%	0.003%




Sum of corrected areas: 4289077

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025598.D
Acq On : 07 Dec 2021 23:53
Operator : JC/MD
Sample : M4886-16ME
Misc : 5.90g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EX895ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

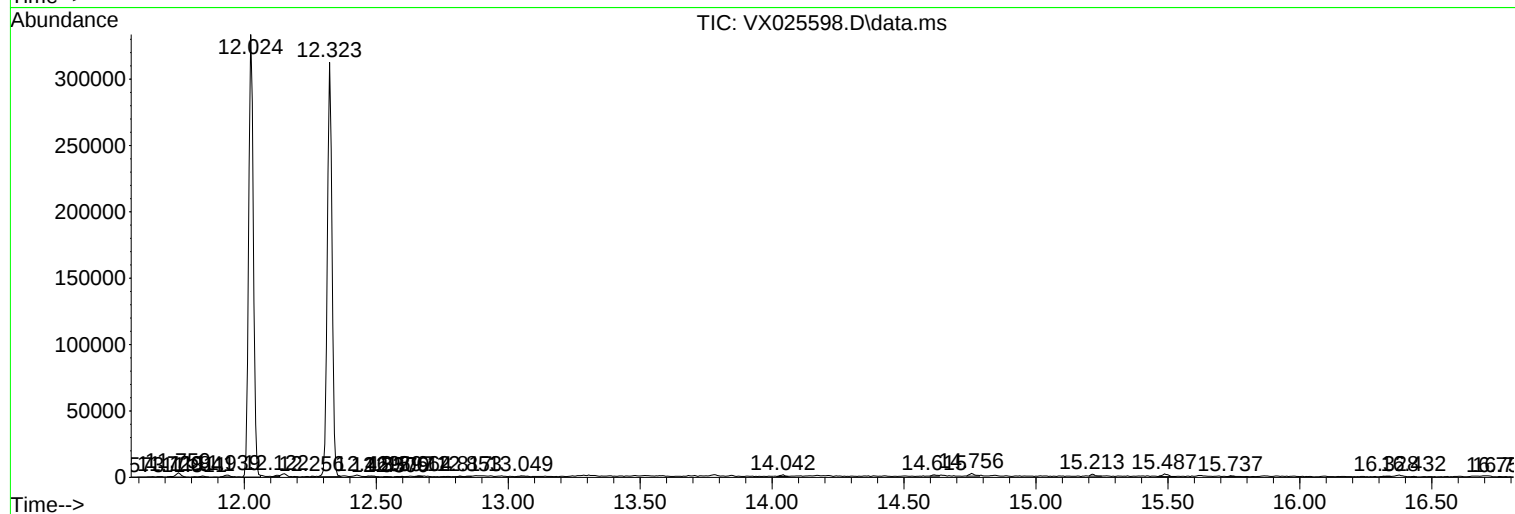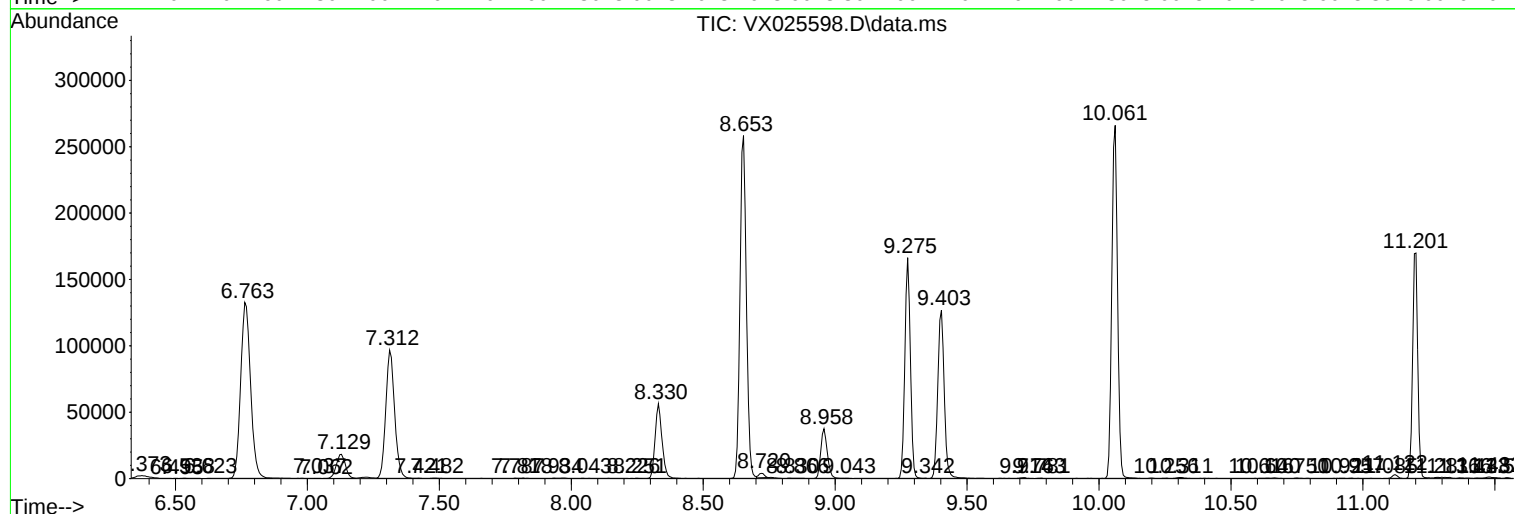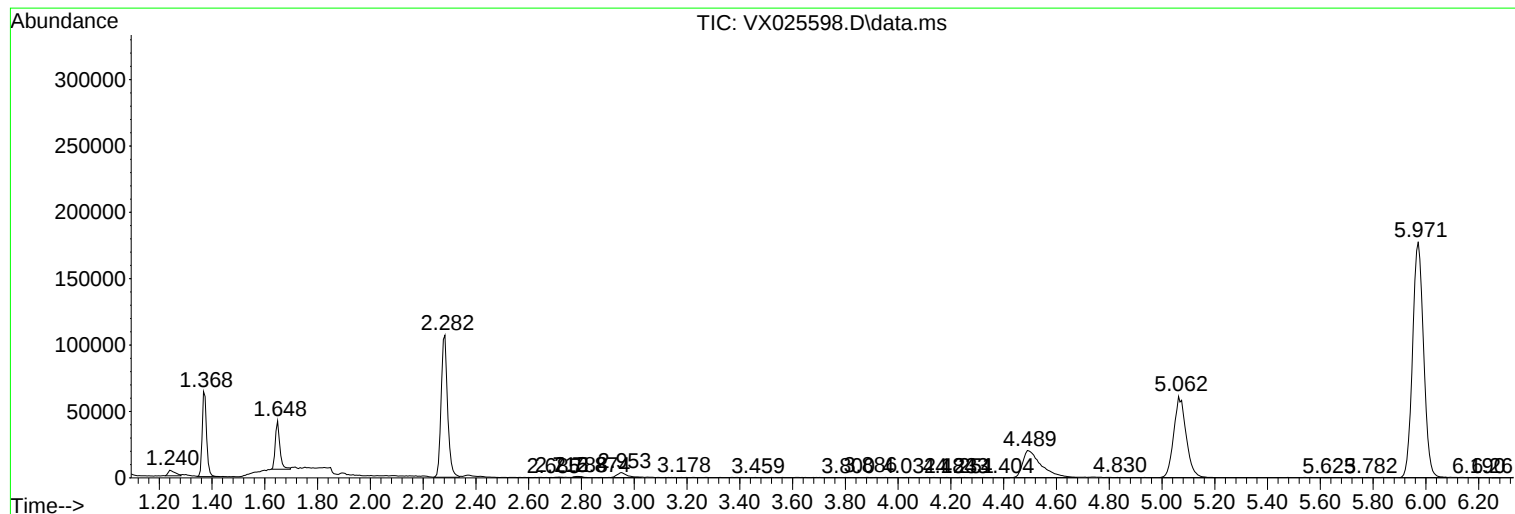

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025598.D
Acq On : 07 Dec 2021 23:53
Operator : JC/MD
Sample : M4886-16ME
Misc : 5.90g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EX895ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025598.D
Acq On : 07 Dec 2021 23:53
Operator : JC/MD
Sample : M4886-16ME
Misc : 5.90g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EX895ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc