

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025609.D
 Acq On : 08 Dec 2021 04:09
 Operator : JC/MD
 Sample : M4885-21ME
 Misc : 6.23g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW9M6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025609.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	32	rBV2	3680	7079	1.35%	0.172%
2	1.368	43	46	54	rVB	64687	73764	14.05%	1.793%
3	1.599	69	84	85	rBV7	4707	16953	3.23%	0.412%
4	1.648	88	92	97	rVV	35063	44043	8.39%	1.071%
5	2.282	189	196	207	rBV	104896	182349	34.72%	4.433%
6	2.361	207	209	219	rVB2	1139	2369	0.45%	0.058%
7	2.715	265	267	268	rBV	260	194	0.04%	0.005%
8	2.788	274	279	283	rBV3	885	1578	0.30%	0.038%
9	2.947	298	305	318	rBV	4480	11913	2.27%	0.290%
10	3.276	357	359	361	rBV	138	126	0.02%	0.003%
11	3.379	375	376	379	rBV2	102	113	0.02%	0.003%
12	3.428	382	384	386	rVB2	154	119	0.02%	0.003%
13	4.495	546	559	584	rBV	20506	100509	19.14%	2.443%
14	5.074	640	654	674	rBV2	59857	204802	39.00%	4.979%
15	5.550	730	732	735	rVB2	196	142	0.03%	0.003%
16	5.751	764	765	768	rBV2	134	154	0.03%	0.004%
17	5.897	787	789	790	rVB	204	120	0.02%	0.003%
18	5.970	790	801	818	rBV2	182513	525144	100.00%	12.766%
19	6.129	825	827	828	rBV	251	198	0.04%	0.005%
20	6.196	837	838	840	rBV	117	113	0.02%	0.003%
21	6.367	858	866	883	rBV6	2074	7294	1.39%	0.177%
22	6.653	911	913	917	rBV	171	166	0.03%	0.004%
23	6.690	917	919	921	rBV	150	147	0.03%	0.004%
24	6.769	921	932	948	rVV	135097	351543	66.94%	8.546%
25	7.129	982	991	999	rVV7	4974	13115	2.50%	0.319%
26	7.220	1002	1006	1013	rVV5	886	2456	0.47%	0.060%
27	7.312	1013	1021	1040	rVB	97528	230519	43.90%	5.604%
28	7.488	1046	1050	1052	rVB2	197	247	0.05%	0.006%
29	7.623	1069	1072	1074	rVB	162	143	0.03%	0.003%
30	7.671	1078	1080	1082	rBV	118	125	0.02%	0.003%
31	7.934	1121	1123	1125	rBV2	180	172	0.03%	0.004%
32	8.019	1135	1137	1140	rVB2	114	142	0.03%	0.003%
33	8.055	1140	1143	1146	rBV2	102	147	0.03%	0.004%
34	8.220	1168	1170	1173	rBV	154	175	0.03%	0.004%
35	8.257	1173	1176	1179	rBV2	127	206	0.04%	0.005%
36	8.330	1181	1188	1198	rBV	58265	103752	19.76%	2.522%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025609.D
 Acq On : 08 Dec 2021 04:09
 Operator : JC/MD
 Sample : M4885-21ME
 Misc : 6.23g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW9M6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	8.531	1218	1221	1223	rBV2	136	186	0.04%	0.005%
38	8.653	1234	1241	1249	rBV	262054	440655	83.91%	10.712%
39	8.720	1249	1252	1257	rVB3	3076	4497	0.86%	0.109%
40	8.842	1269	1272	1273	rBV2	108	116	0.02%	0.003%
41	8.958	1285	1291	1300	rBV	38034	64618	12.30%	1.571%
42	9.195	1329	1330	1333	rVB	158	123	0.02%	0.003%
43	9.275	1339	1343	1348	rVB3	1278	1799	0.34%	0.044%
44	9.403	1357	1364	1377	rBV	130588	222862	42.44%	5.418%
45	9.714	1412	1415	1418	rBV2	609	730	0.14%	0.018%
46	9.921	1447	1449	1452	rBV2	110	128	0.02%	0.003%
47	10.061	1466	1472	1480	rBV	271483	410866	78.24%	9.988%
48	10.311	1508	1513	1519	rVB3	754	1095	0.21%	0.027%
49	10.555	1551	1553	1556	rVV2	131	133	0.03%	0.003%
50	10.598	1558	1560	1565	rVB	185	193	0.04%	0.005%
51	10.646	1565	1568	1571	rBV2	256	336	0.06%	0.008%
52	10.835	1596	1599	1600	rBV	157	180	0.03%	0.004%
53	11.122	1642	1646	1650	rVB3	1864	2448	0.47%	0.060%
54	11.201	1653	1659	1666	rBV	174036	235007	44.75%	5.713%
55	11.280	1669	1672	1675	rBV2	320	435	0.08%	0.011%
56	11.482	1696	1705	1706	rBV5	456	742	0.14%	0.018%
57	11.543	1714	1715	1717	rVV	228	134	0.03%	0.003%
58	11.683	1735	1738	1741	rVB2	232	248	0.05%	0.006%
59	11.719	1741	1744	1745	rBV	285	226	0.04%	0.005%
60	11.750	1745	1749	1755	rVV2	2112	2875	0.55%	0.070%
61	11.841	1762	1764	1767	rVB	472	454	0.09%	0.011%
62	11.878	1768	1770	1773	rBV	132	121	0.02%	0.003%
63	11.933	1775	1779	1783	rBV2	1015	1266	0.24%	0.031%
64	12.024	1789	1794	1800	rBV	344415	415164	79.06%	10.092%
65	12.122	1808	1810	1812	rBV2	592	657	0.13%	0.016%
66	12.152	1812	1815	1819	rVB2	1916	2365	0.45%	0.057%
67	12.323	1835	1843	1849	rBV	311668	395697	75.35%	9.619%
68	12.427	1857	1860	1863	rVB3	877	1181	0.22%	0.029%
69	12.488	1864	1870	1871	rBV3	419	577	0.11%	0.014%
70	12.664	1896	1899	1902	rVV	370	417	0.08%	0.010%
71	12.762	1912	1915	1918	rBV2	111	143	0.03%	0.003%
72	12.884	1933	1935	1936	rBV	277	191	0.04%	0.005%
73	13.055	1959	1963	1967	rBV2	299	519	0.10%	0.013%
74	13.109	1970	1972	1973	rBV	149	117	0.02%	0.003%
75	13.268	1995	1998	2001	rVB2	562	563	0.11%	0.014%
76	13.390	2014	2018	2020	rVB3	485	559	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
 Data File : VX025609.D
 Acq On : 08 Dec 2021 04:09
 Operator : JC/MD
 Sample : M4885-21ME
 Misc : 6.23g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW9M6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

77	13.774	2079	2081	2085	rVB	677	870	0.17%	0.021%
78	13.847	2090	2093	2096	rVB3	808	1059	0.20%	0.026%
79	14.042	2120	2125	2128	rBV4	1245	1545	0.29%	0.038%
80	14.146	2135	2142	2154	rBV4	1086	4145	0.79%	0.101%
81	14.286	2163	2165	2166	rVB	215	127	0.02%	0.003%
82	14.377	2174	2180	2182	rBV3	282	443	0.08%	0.011%
83	14.432	2187	2189	2192	rBV2	275	328	0.06%	0.008%
84	14.506	2197	2201	2205	rVB3	273	399	0.08%	0.010%
85	14.615	2215	2219	2220	rBV3	725	685	0.13%	0.017%
86	14.755	2239	2242	2245	rBV3	1862	2243	0.43%	0.055%
87	14.847	2255	2257	2260	rVB2	602	457	0.09%	0.011%
88	14.944	2272	2273	2275	rBV2	270	176	0.03%	0.004%
89	14.969	2275	2277	2282	rVB2	207	208	0.04%	0.005%
90	15.012	2282	2284	2287	rBV	222	318	0.06%	0.008%
91	15.213	2312	2317	2324	rVB5	880	1491	0.28%	0.036%
92	15.347	2337	2339	2340	rBV2	393	391	0.07%	0.010%
93	15.457	2356	2357	2358	rBV	217	113	0.02%	0.003%
94	15.493	2358	2363	2366	rVB4	1310	2116	0.40%	0.051%
95	15.554	2372	2373	2375	rBV	196	139	0.03%	0.003%
96	15.615	2380	2383	2386	rVB4	812	941	0.18%	0.023%
97	15.810	2413	2415	2418	rBV3	318	352	0.07%	0.009%
98	15.841	2418	2420	2421	rBV2	381	248	0.05%	0.006%
99	15.981	2439	2443	2452	rVB3	712	2010	0.38%	0.049%
100	16.761	2569	2571	2573	rBB	200	139	0.03%	0.003%




Sum of corrected areas: 4113697

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025609.D
Acq On : 08 Dec 2021 04:09
Operator : JC/MD
Sample : M4885-21ME
Misc : 6.23g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW9M6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

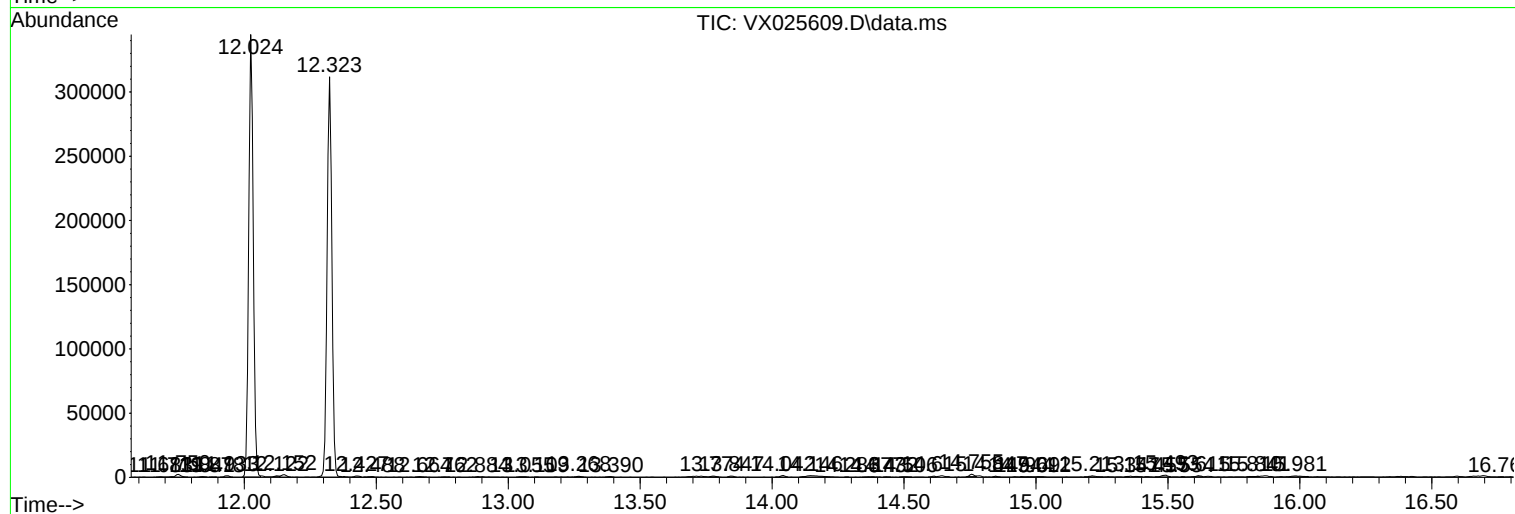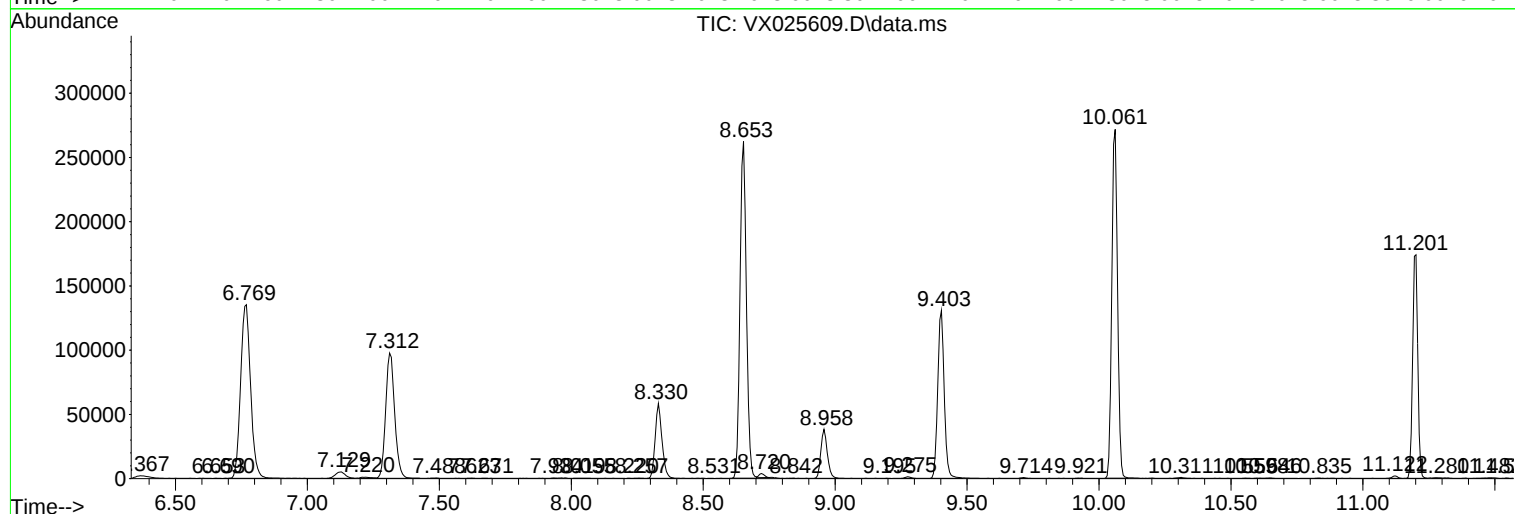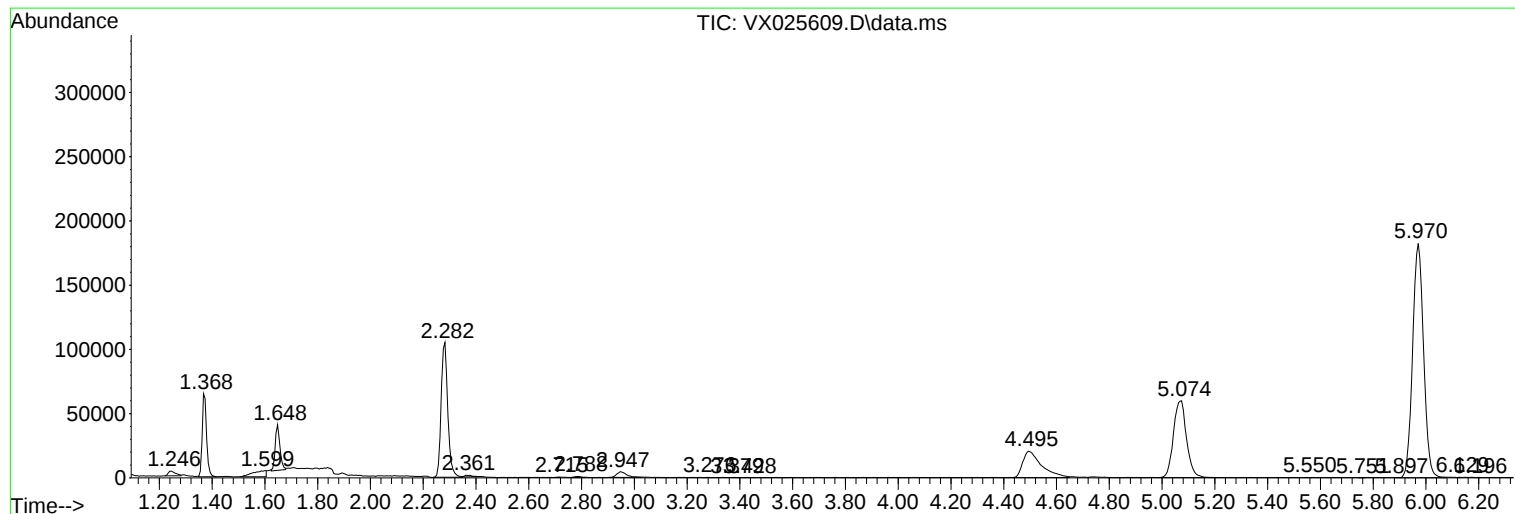

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025609.D
Acq On : 08 Dec 2021 04:09
Operator : JC/MD
Sample : M4885-21ME
Misc : 6.23g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW9M6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120721\
Data File : VX025609.D
Acq On : 08 Dec 2021 04:09
Operator : JC/MD
Sample : M4885-21ME
Misc : 6.23g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW9M6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc