

Quantitation Report (QT Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
 Data File : VX025632.D
 Acq On : 08 Dec 2021 20:16
 Operator : JC/MD
 Sample : M4885-15MEDL 10X
 Misc : 3.06g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 Client Sampled :
 EW9M2MEDL

Quant Time: Dec 09 03:30:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 09 03:12:30 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Mahesh Dadoda 12/15/2021
 Supervised By : Semsettin Yesilyurt 12/15/2021

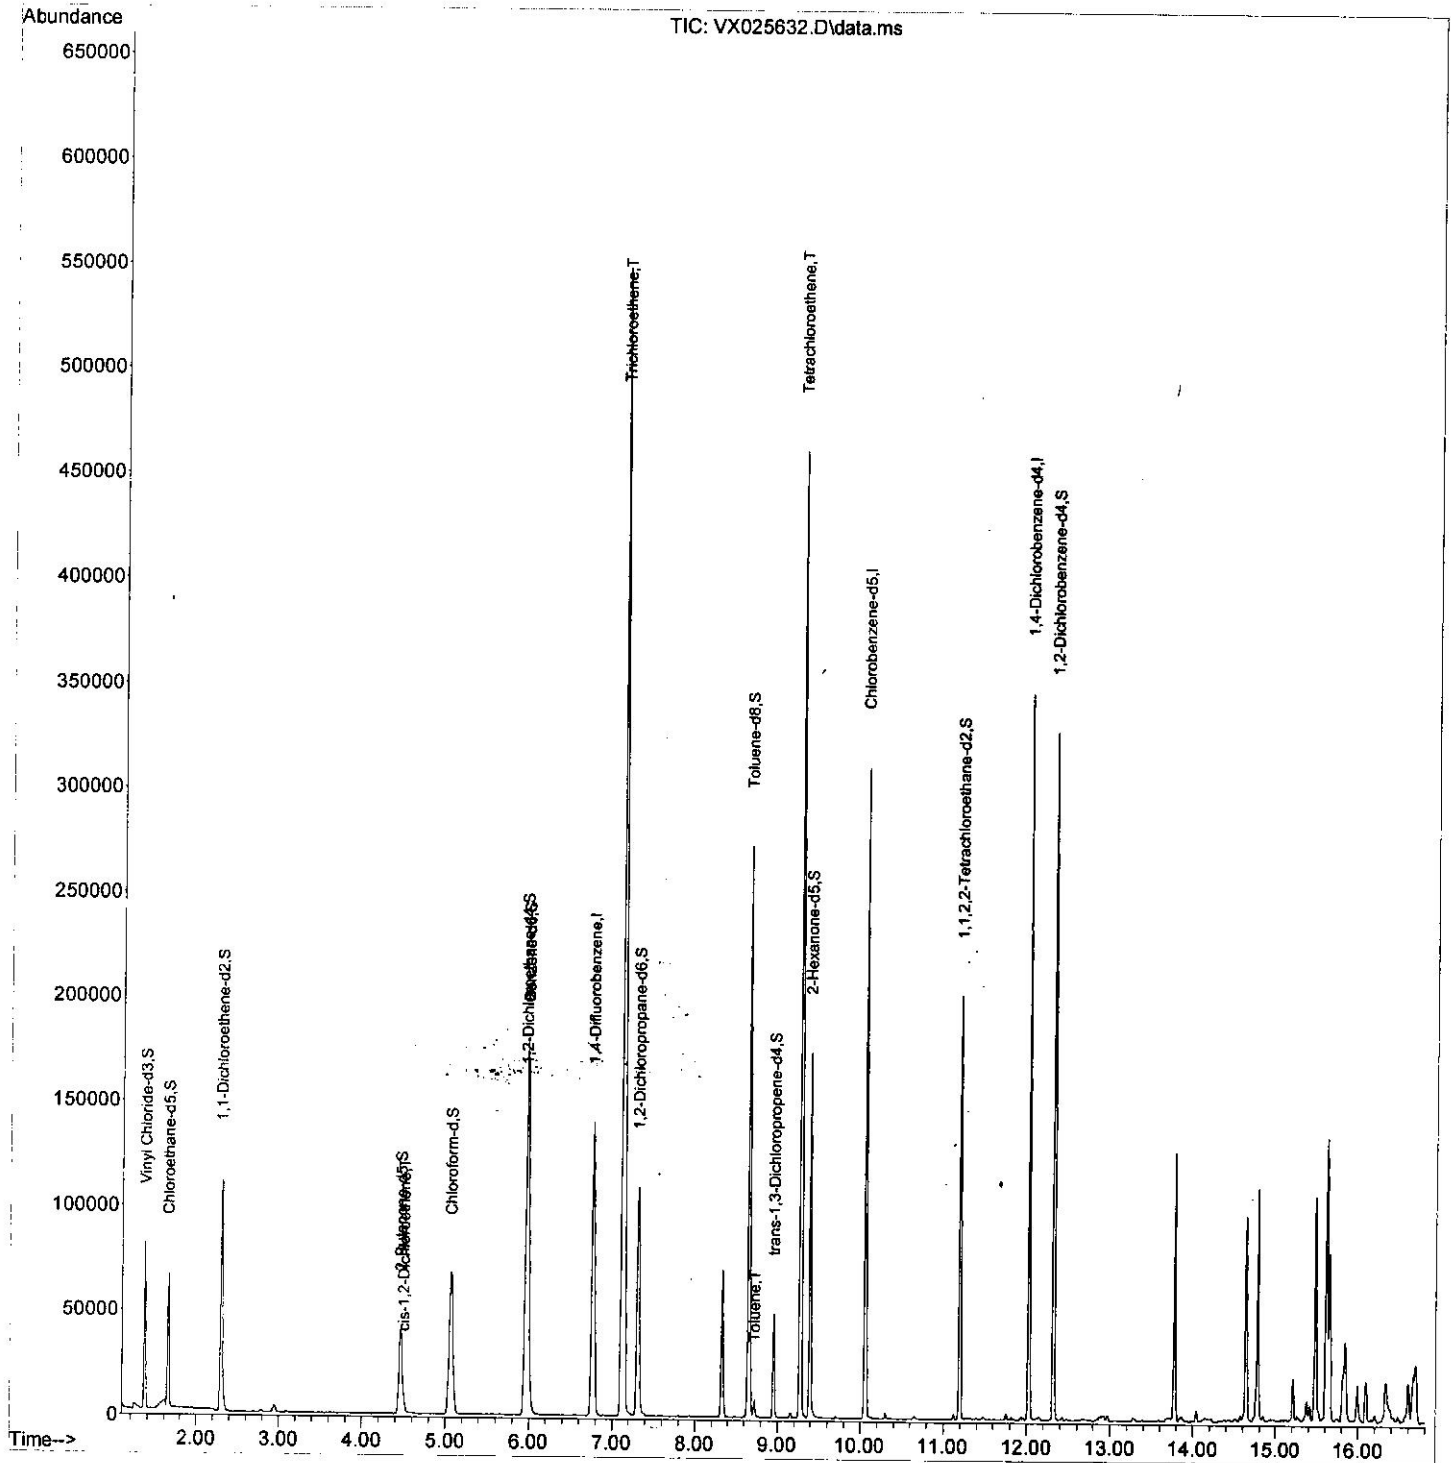

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
 Data File : VX025632.D
 Acq On : 08 Dec 2021 20:16
 Operator : JC/MD
 Sample : M4885-15MEDL 10X
 Misc : 3.06g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 Client Sampled :
 EW9M2MEDL

Quant Time: Dec 09 03:30:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 09 03:12:30 2021
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/15/2021
 Supervised By :Semsettin Yesilyurt 12/15/2021

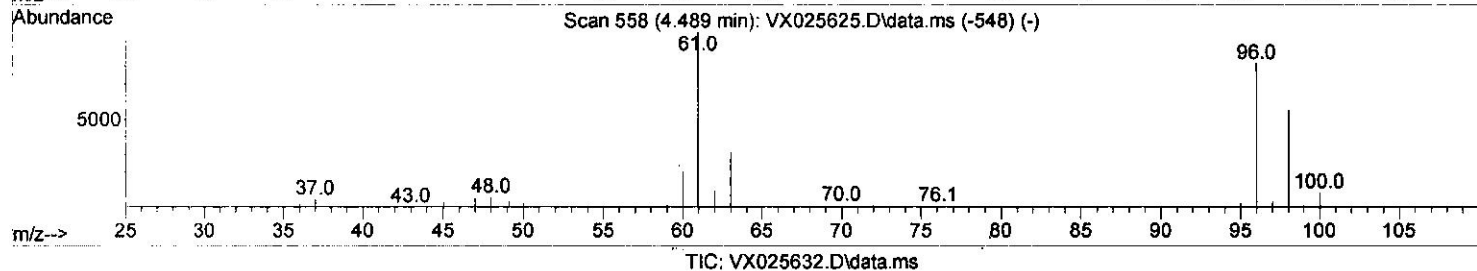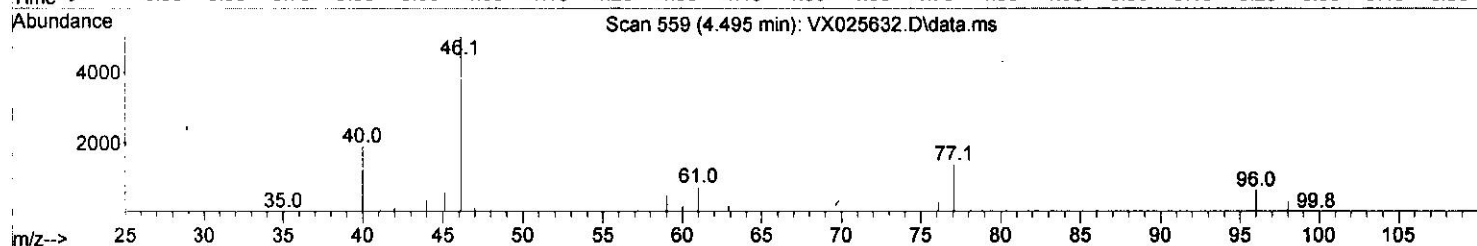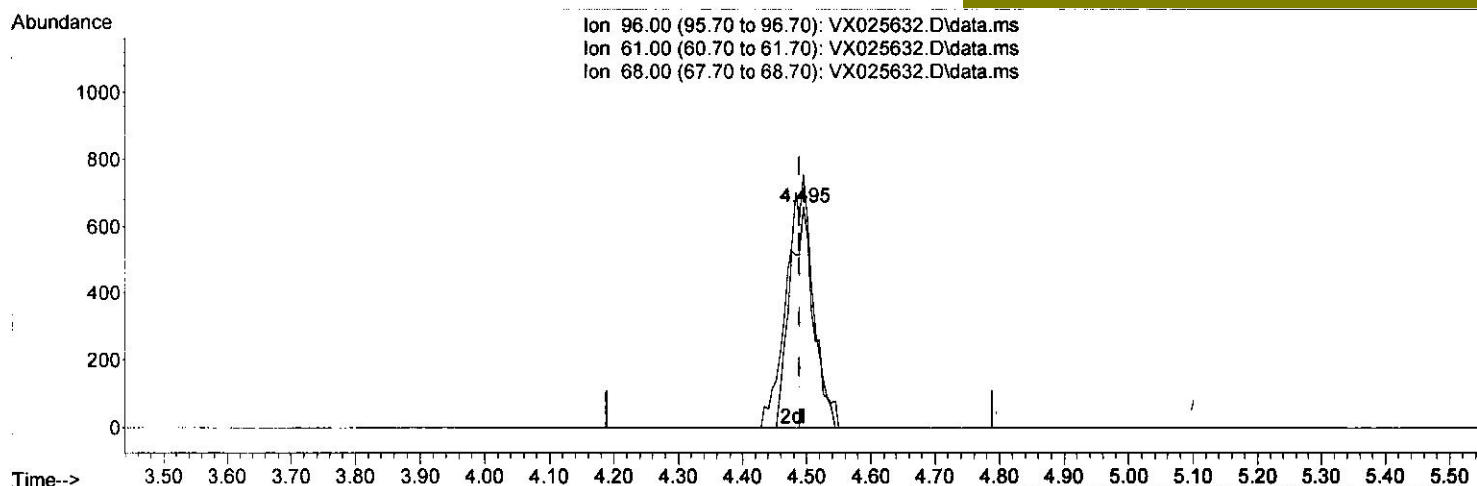

(20) cis-1,2-Dichloroethene (T)

4.495min (+ 0.006) 0.83 ug/L

response 852

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	117.50	114.44
68.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
 Data File : VX025632.D
 Acq On : 08 Dec 2021 20:16
 Operator : JC/MD
 Sample : M4885-15MEDL 10X
 Misc : 3.06g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 Client Sampled :
 EW9M2MEDL

Quant Time: Dec 09 03:30:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 09 03:12:30 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Mahesh Dadoda 12/15/2021
 Supervised By : Semsettin Yesilyurt 12/15/2021

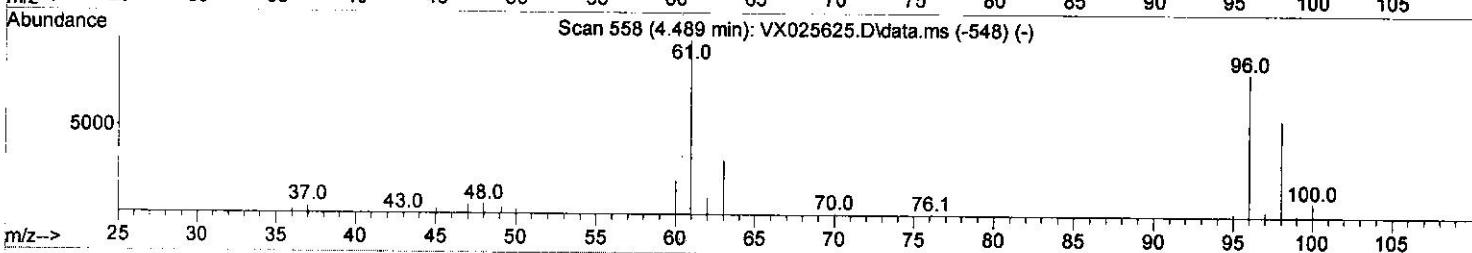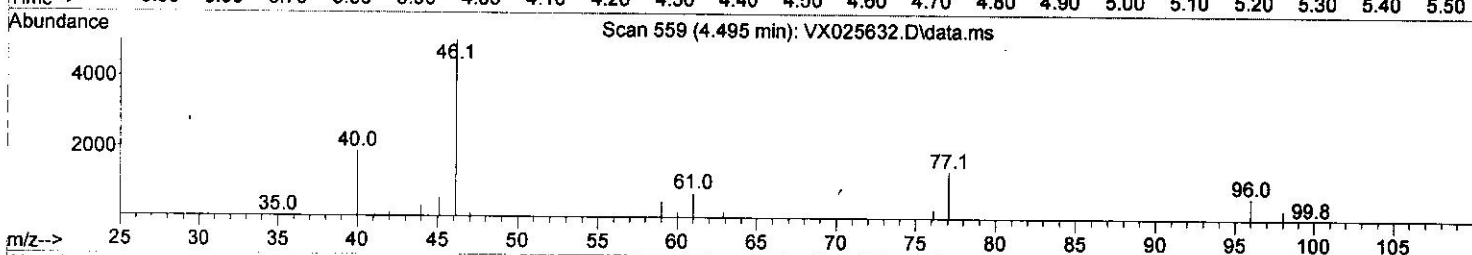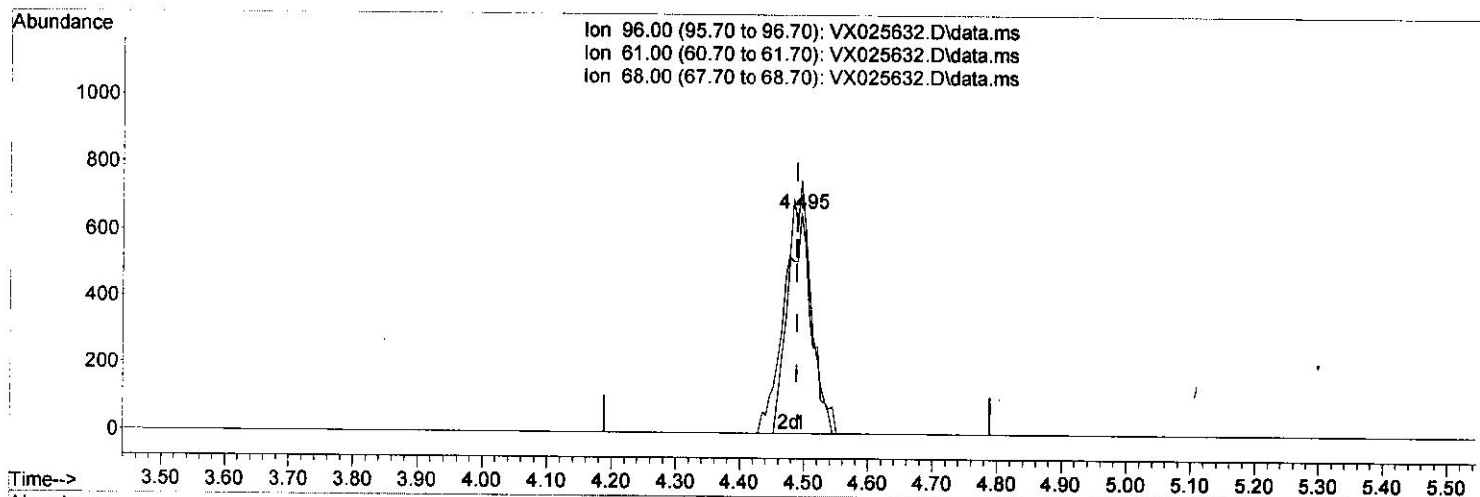

TIC: VX025632.D\data.ms

(20) cis-1,2-Dichloroethene (T)

4.495min (+ 0.006) 1.62 ug/L m

response 1670

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	117.50	114.44
68.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
 Data File : VX025632.D
 Acq On : 08 Dec 2021 20:16
 Operator : JC/MD
 Sample : M4885-15MEDL 10X
 Misc : 3.06g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 Client Sampled :
 EW9M2MEDL

Quant Time: Dec 09 03:30:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 09 03:12:30 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Mahesh Dadoda 12/15/2021
 Supervised By : Semsettin Yesilyurt 12/15/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	151484	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	140061	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	70927	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	47017	45.479	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	90.960%		
7) Chloroethane-d5	1.654	69	40659	47.653	ug/L	-0.01
Spiked Amount 50.000	Range 70 - 130		Recovery =	95.300%		
11) 1,1-Dichloroethene-d2	2.300	63	61562	37.347	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.700%		
21) 2-Butanone-d5	4.459	46	69168	89.879	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	89.880%		
24) Chloroform-d	5.062	84	83600	46.270	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.540%		
26) 1,2-Dichloroethane-d4	5.958	65	55788	49.536	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.080%		
32) Benzene-d6	5.977	84	179286	48.298	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.600%		
36) 1,2-Dichloropropane-d6	7.312	67	54069	47.045	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	94.100%		
41) Toluene-d8	8.653	98	165727	47.300	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.600%		
43) trans-1,3-Dichloroprop...	8.952	79	22074	38.202	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	76.400%		
47) 2-Hexanone-d5	9.385	63	50865	85.022	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	85.020%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	72704	44.761	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	89.520%		
66) 1,2-Dichlorobenzene-d4	12.323	152	67768	48.715	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.420%		
Target Compounds						
20) cis-1,2-Dichloroethene	4.495	96	1670m	1.618	ug/L	Qvalue
34) Trichloroethene	7.129	95	203535	206.814	ug/L	98
42) Toluene	8.720	91	5116	1.240	ug/L	94
46) Tetrachloroethene	9.275	164	87551	104.898	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed