

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
 Data File : VX025620.D
 Acq On : 08 Dec 2021 14:50
 Operator : JC/MD
 Sample : M4884-15ME
 Misc : 5.35g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW9K1ME

Quant Time: Dec 09 01:43:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 09 01:41:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	115606	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.061	117	102229	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	50739	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	35303	44.746	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	89.500%
7) Chloroethane-d5	1.648	69	18617	28.591	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	57.180%#
11) 1,1-Dichloroethene-d2	2.282	63	51484	40.927	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.860%
21) 2-Butanone-d5	4.495	46	53001	90.245	ug/L	0.05
Spiked Amount	100.000	Range	40 - 130	Recovery	=	90.250%
24) Chloroform-d	5.068	84	66234	48.035	ug/L	0.01
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.080%
26) 1,2-Dichloroethane-d4	5.958	65	44270	51.509	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.020%
32) Benzene-d6	5.971	84	146325	54.007	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.020%
36) 1,2-Dichloropropane-d6	7.312	67	42805	51.028	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.060%
41) Toluene-d8	8.653	98	134405	52.556	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.120%
43) trans-1,3-Dichloroprop...	8.958	79	15612	37.018	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.040%
47) 2-Hexanone-d5	9.403	63	38264	87.629	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	87.630%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	56303	47.491	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.980%
66) 1,2-Dichlorobenzene-d4	12.323	152	52265	52.519	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.040%
Target Compounds						Qvalue
34) Trichloroethene	7.123	95	23619	32.881	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
Data File : VX025620.D
Acq On : 08 Dec 2021 14:50
Operator : JC/MD
Sample : M4884-15ME
Misc : 5.35g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW9K1ME

Quant Time: Dec 09 01:43:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 09 01:41:02 2021
Response via : Initial Calibration

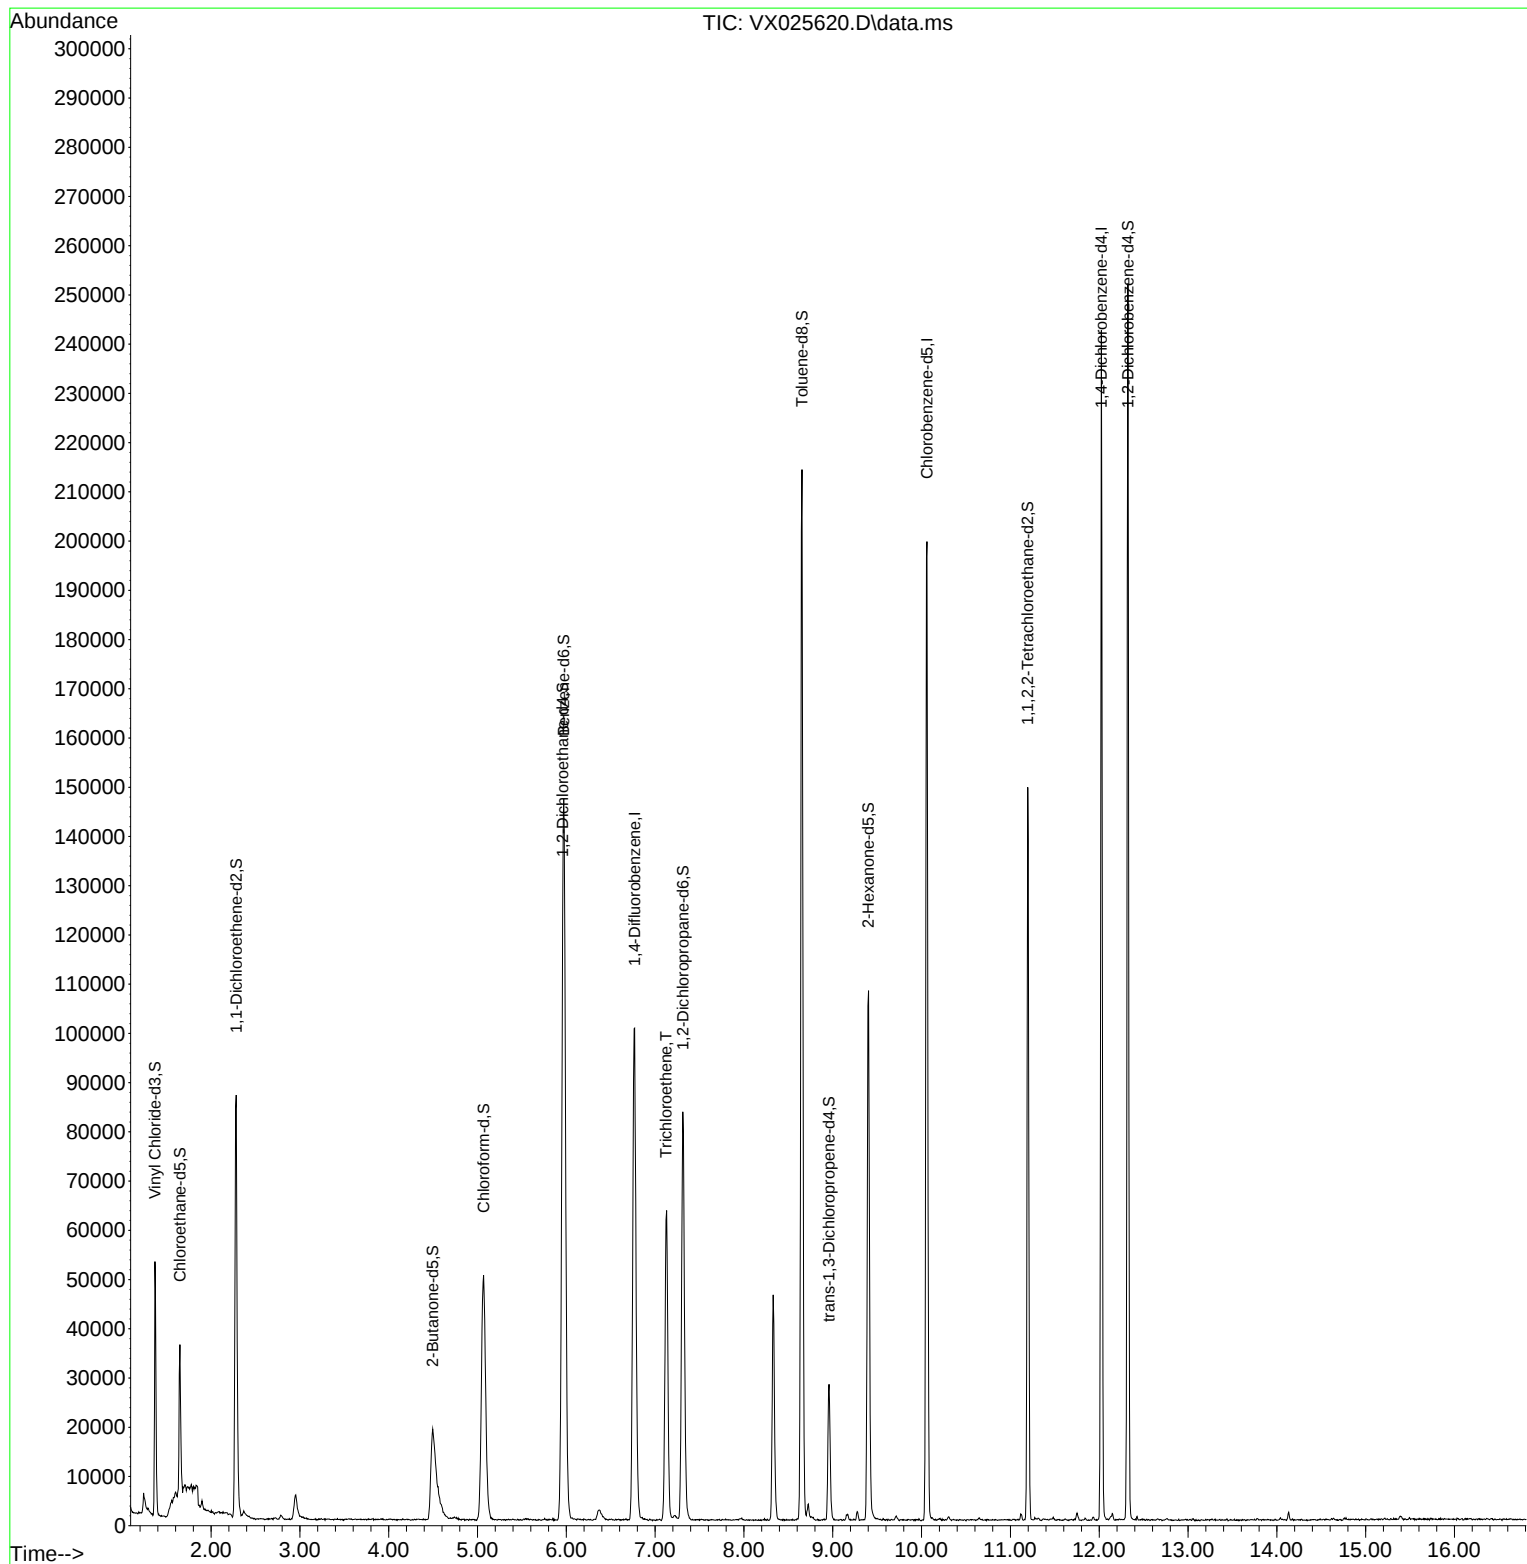

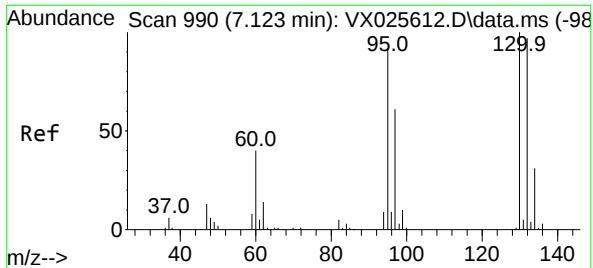

#34
 Trichloroethene
 Concen: 32.881 ug/L
 RT: 7.123 min Scan# 99
 Delta R.T. 0.000 min
 Lab File: VX025620.D
 Acq: 08 Dec 2021 14:50

Instrument :
 MSVOA_X
 ClientSampleId :
 EW9K1ME

Tgt Ion: 95 Resp: 23619

Ion	Ratio	Lower	Upper
95	100		
97	61.3	46.0	85.4
132	95.7	75.0	139.2
130	101.1	77.9	144.7

