

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
 Data File : VX025626.D
 Acq On : 08 Dec 2021 17:56
 Operator : JC/MD
 Sample : VX1208MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK646

Quant Time: Dec 09 03:12:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 09 03:12:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	118605	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	107568	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	50616	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	34762	42.947	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	85.900%
7) Chloroethane-d5	1.666	69	30653	45.884	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.760%
11) 1,1-Dichloroethene-d2	2.307	63	47028	36.439	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.880%
21) 2-Butanone-d5	4.453	46	61575	102.193	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	102.190%
24) Chloroform-d	5.062	84	68179	48.195	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.400%
26) 1,2-Dichloroethane-d4	5.958	65	44445	50.405	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.800%
32) Benzene-d6	5.977	84	138836	48.699	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.400%
36) 1,2-Dichloropropane-d6	7.312	67	43260	49.010	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.020%
41) Toluene-d8	8.653	98	127444	47.361	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.720%
43) trans-1,3-Dichloroprop...	8.952	79	17981	40.519	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.040%
47) 2-Hexanone-d5	9.385	63	43869	95.478	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.480%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	60177	48.240	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.480%
66) 1,2-Dichlorobenzene-d4	12.323	152	50195	50.561	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.120%
Target Compounds						
16) Methylene chloride	2.794	84	2251	3.056	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120821\
Data File : VX025626.D
Acq On : 08 Dec 2021 17:56
Operator : JC/MD
Sample : VX1208MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK646

Quant Time: Dec 09 03:12:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 09 03:12:30 2021
Response via : Initial Calibration

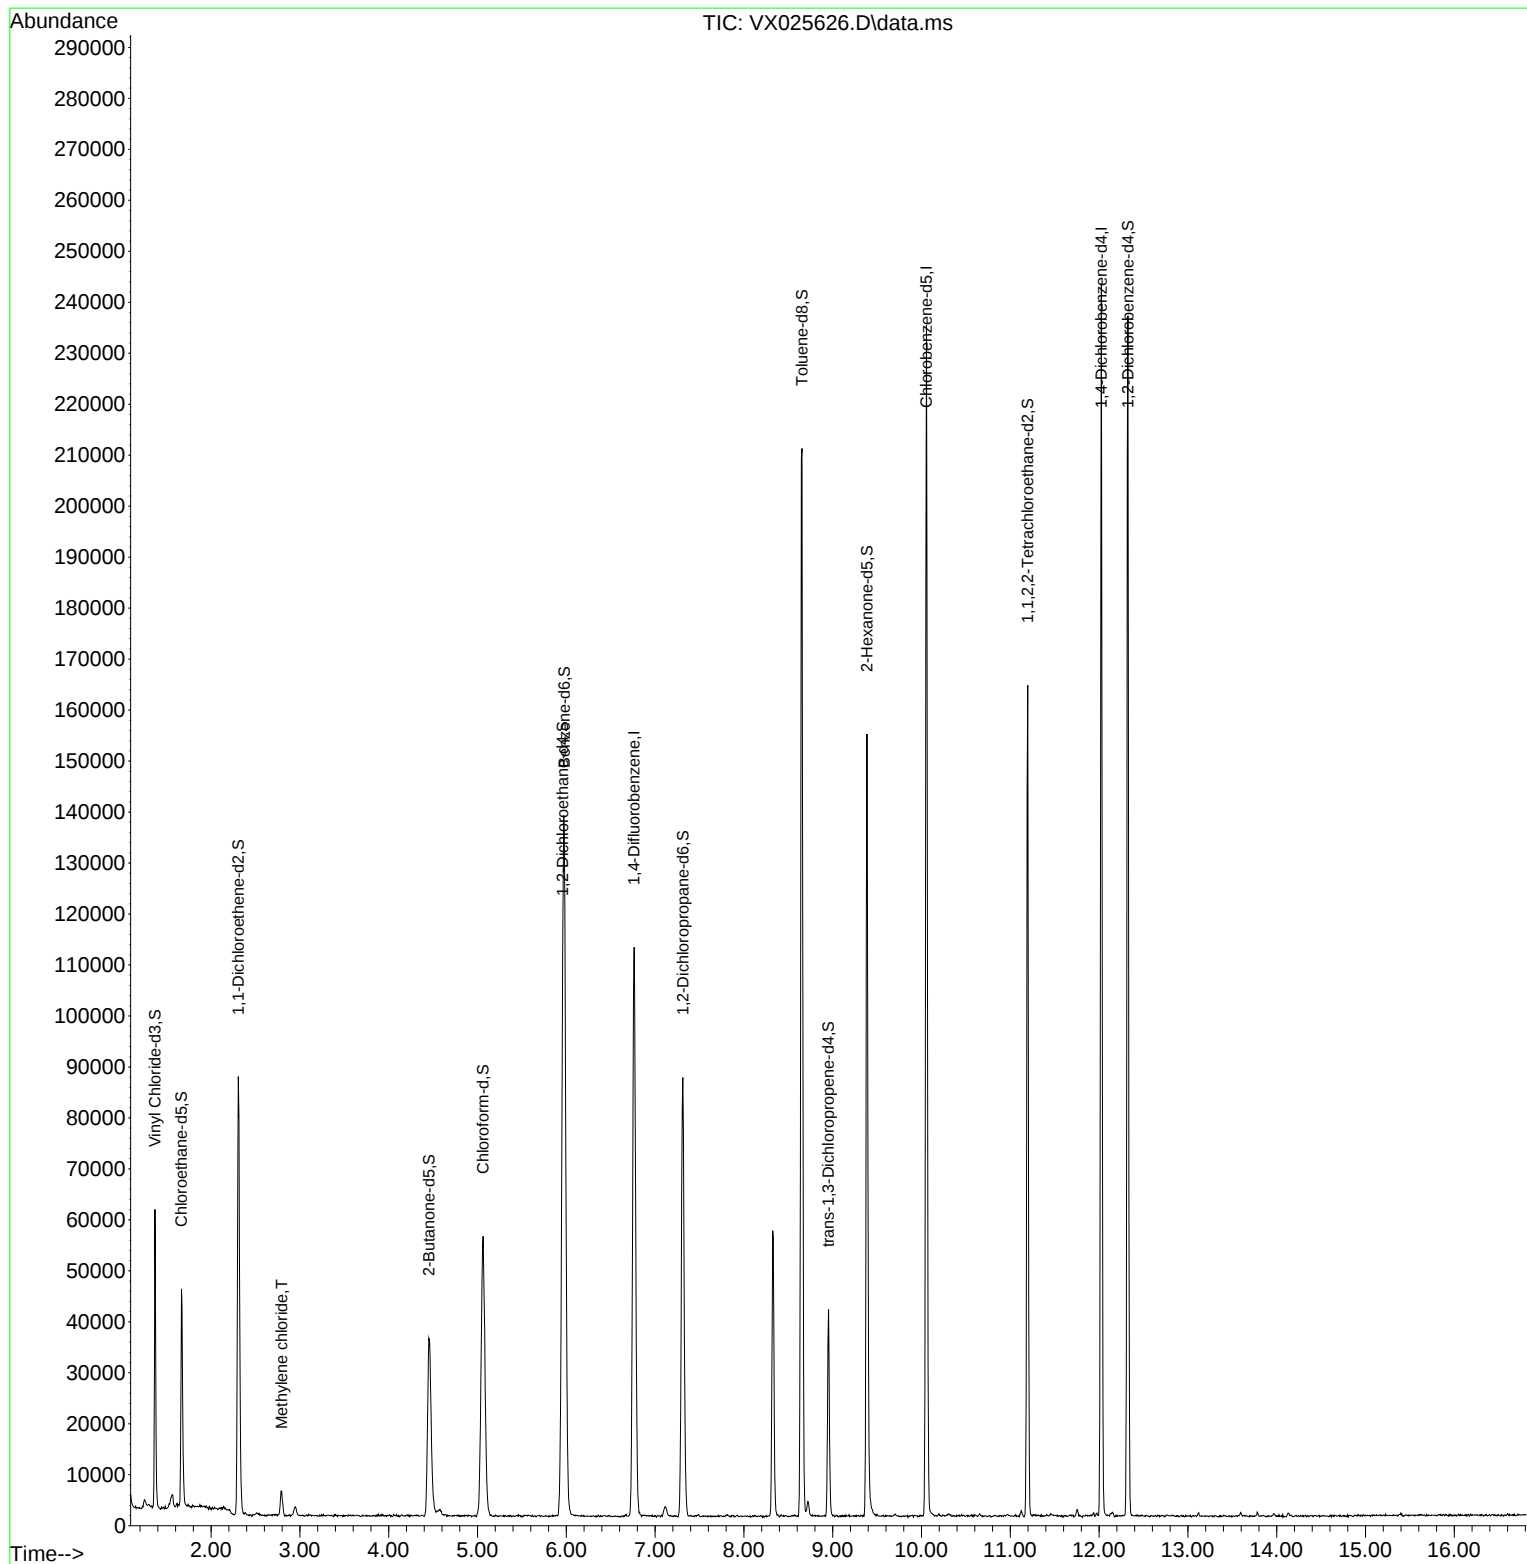

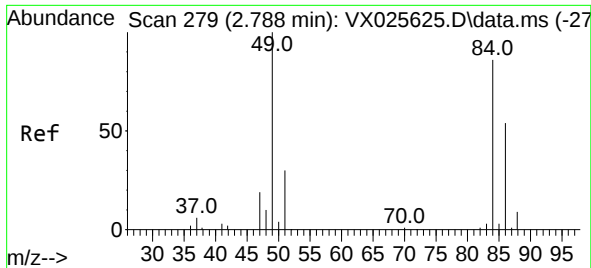

#16
Methylene chloride
Concen: 3.056 ug/L
RT: 2.794 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX025626.D
Acq: 08 Dec 2021 17:56

Instrument :
MSVOA_X
ClientSampleId :
VBLK646

Tgt Ion: 84 Resp: 2251

Ion	Ratio	Lower	Upper
84	100		
86	60.4	45.1	83.9
49	116.8	82.3	152.8

